

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031422\
 Data File : PD068551.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2022 14:18
 Operator : AR\AJ
 Sample : N1818-10MSD
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DBSF4MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/17/2022
 Supervised By : Ankita Jodhani 03/17/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 07:15:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 07:24:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.448	4.173	23124893	183.9E6	16.981	16.799
27)	SA Decachlor...	8.206	9.365	47453924	212.1E6	34.126	33.621
Target Compounds							
2)	A alpha-BHC	3.887	4.569	91149946	648.1E6	47.616	41.452
3)	MA gamma-BHC...	4.170	4.858	85341895	600.9E6	47.015	41.448m
4)	MA Heptachlor	4.469	5.386	79657365	555.8E6	44.468	40.379
5)	MB Aldrin	4.716	5.699	79123536	557.3E6	44.989	41.298
6)	B beta-BHC	4.421	5.022	37263045	281.2E6	44.717	44.035
7)	B delta-BHC	4.625	5.248	82469217	579.3E6	46.641	40.919
8)	B Heptachlo...	5.160	6.087	75049332	497.7E6	46.212	41.319
9)	A Endosulfan I	5.499	6.449	69822831	447.2E6	45.352	41.093
10)	B trans-Chl...	5.386	6.323	76952477	488.8E6	46.109	41.100
11)	B cis-Chlor...	5.446	6.398	75010309	475.3E6	45.694	41.437
12)	B 4,4'-DDE	5.612	6.548	147.4E6	885.1E6	99.100	86.640
13)	MA Dieldrin	5.743	6.708	160.6E6	946.3E6	96.130	85.168
14)	MA Endrin	6.001	6.928	134.5E6	716.8E6	95.114	84.777
15)	B Endosulfa...	6.275	7.132	135.2E6	757.6E6	93.193	84.660
16)	A 4,4'-DDD	6.128	7.039	122.0E6	700.7E6	92.849	83.510
17)	MA 4,4'-DDT	6.369	7.340	129.8E6	714.2E6	97.211	90.622m
18)	B Endrin al...	6.444	7.256	101.3E6	567.9E6	92.410	85.516
19)	B Endosulfa...	6.657	7.480	125.9E6	675.1E6	90.091	82.433
20)	A Methoxychlor	6.919	7.794	330.5E6	1528.3E6	466.895	436.279
21)	B Endrin ke...	7.149	7.956	157.5E6	750.2E6	98.724	87.859

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031422\
 Data File : PD068551.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2022 14:18
 Operator : AR\AJ
 Sample : N1818-10MSD
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 07:15:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 07:24:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

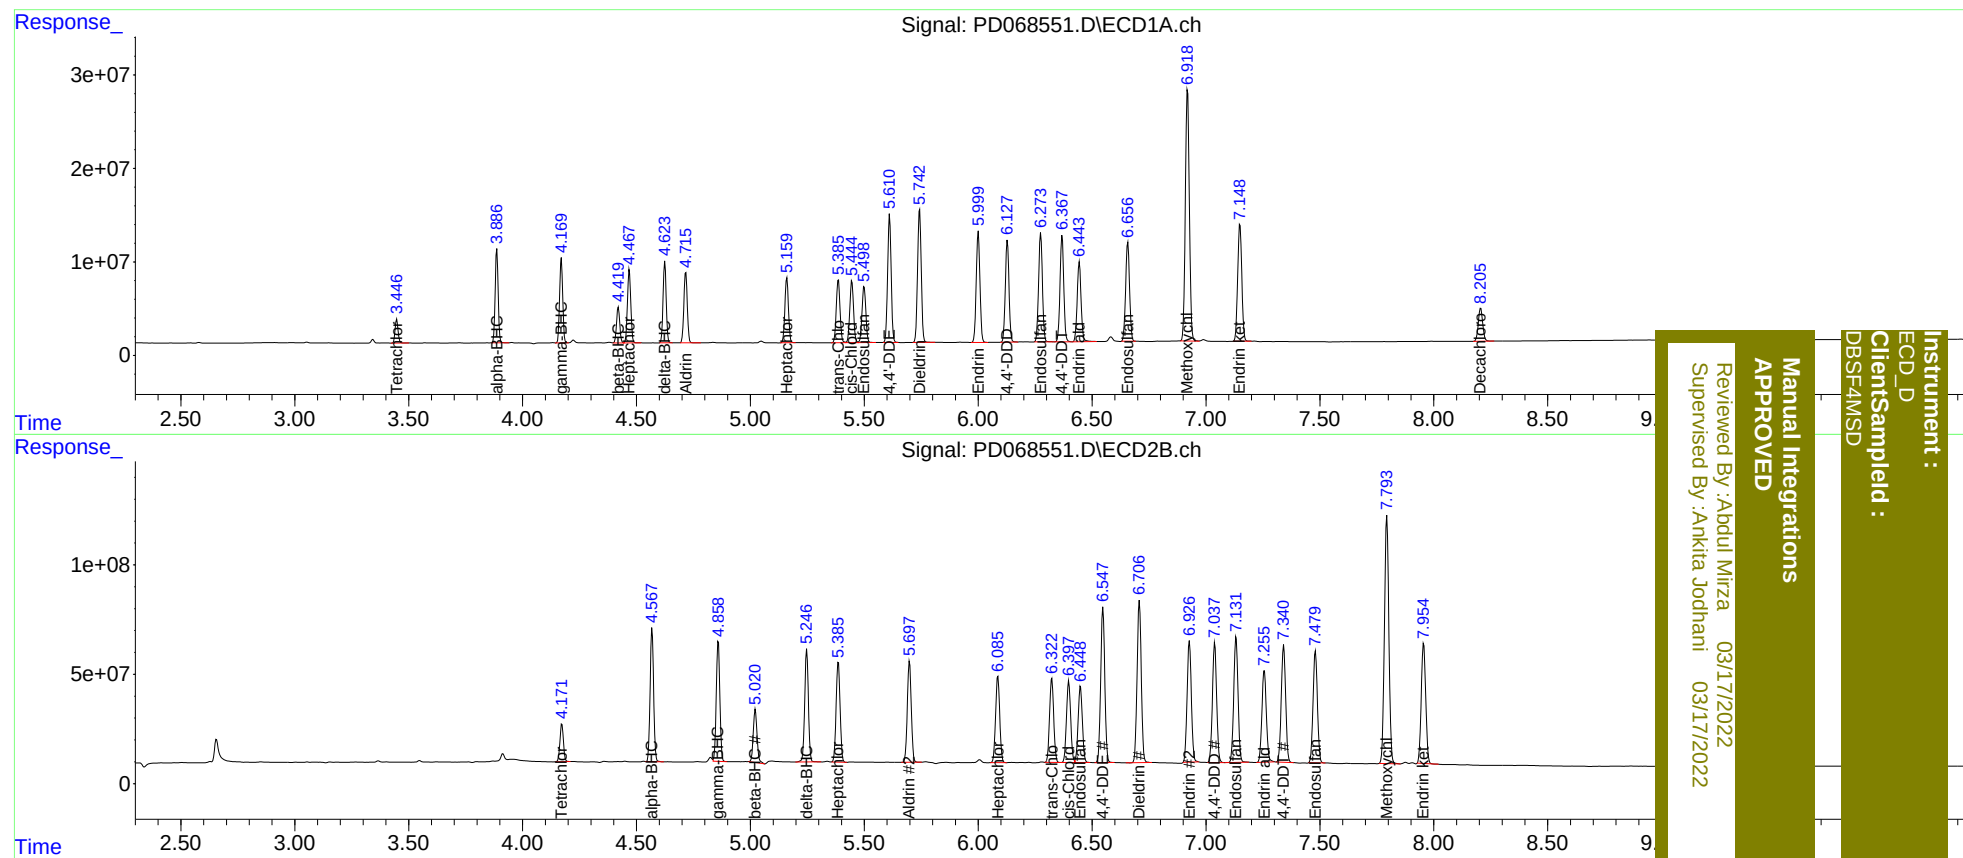

Reviewed By: Abdul Mirza 03/17/2022
 Supervised By: Ankita Jodhani 03/17/2022

Manual Integrations
 APPROVED

Instrument :
 ECD_D
 ClientSampled :
 DBSF4MSD