

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031422\
 Data File : PD068571.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2022 19:18
 Operator : AR\AJ
 Sample : N1820-04MS
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DBRZ5MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/17/2022
 Supervised By : Ankita Jodhani 03/17/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 07:19:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 07:24:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.447	4.173	25717442	200.6E6	18.885	18.323
2)	SA Decachlor...	8.206	9.366	49840475	219.9E6	35.842	34.872
Target Compounds							
2)	A alpha-BHC	3.886	4.569	94840100	655.5E6	49.544	41.924
3)	MA gamma-BHC...	4.170	4.859	89382204	611.9E6	49.240	42.208
4)	MA Heptachlor	4.468	5.387	84702714	562.0E6	47.285	40.832
5)	MB Aldrin	4.716	5.699	84859659	563.6E6	48.250	41.766
6)	B beta-BHC	4.420	5.022	38770004	274.8E6	46.525	43.023
7)	B delta-BHC	4.624	5.247	81923058	535.7E6	46.332	37.846
8)	B Heptachlo...	5.160	6.087	78686286	495.3E6	48.452	41.119
9)	A Endosulfan I	5.498	6.450	73026781	445.1E6	47.433	40.902
10)	B trans-Chl...	5.386	6.324	79899106	488.0E6	47.875	41.031
11)	B cis-Chlor...	5.445	6.399	78106175	473.3E6	47.580	41.267
12)	B 4,4'-DDE	5.611	6.548	153.2E6	885.8E6	102.992	86.700
13)	MA Dieldrin	5.742	6.708	167.0E6	944.0E6	99.979	84.956
14)	MA Endrin	6.000	6.928	141.0E6	734.3E6	99.716	86.849
15)	B Endosulfa...	6.274	7.133	139.0E6	750.2E6	95.845	83.836
16)	A 4,4'-DDD	6.127	7.039	126.0E6	704.0E6	95.877	83.910
17)	MA 4,4'-DDT	6.369	7.342	134.0E6	715.3E6	100.374	90.760
18)	B Endrin al...	6.444	7.257	104.5E6	563.0E6	95.293	84.788
19)	B Endosulfa...	6.656	7.482	131.4E6	672.5E6	94.003	82.105
20)	A Methoxychlor	6.920	7.795	351.4E6	1557.2E6	496.471	444.511
21)	B Endrin ke...	7.150	7.955	163.1E6	759.1E6	102.223	88.904m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031422\
Data File : PD068571.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2022 19:18
Operator : AR\AJ
Sample : N1820-04MS
Misc :
ALS Vial : 35 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 07:19:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 07:24:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

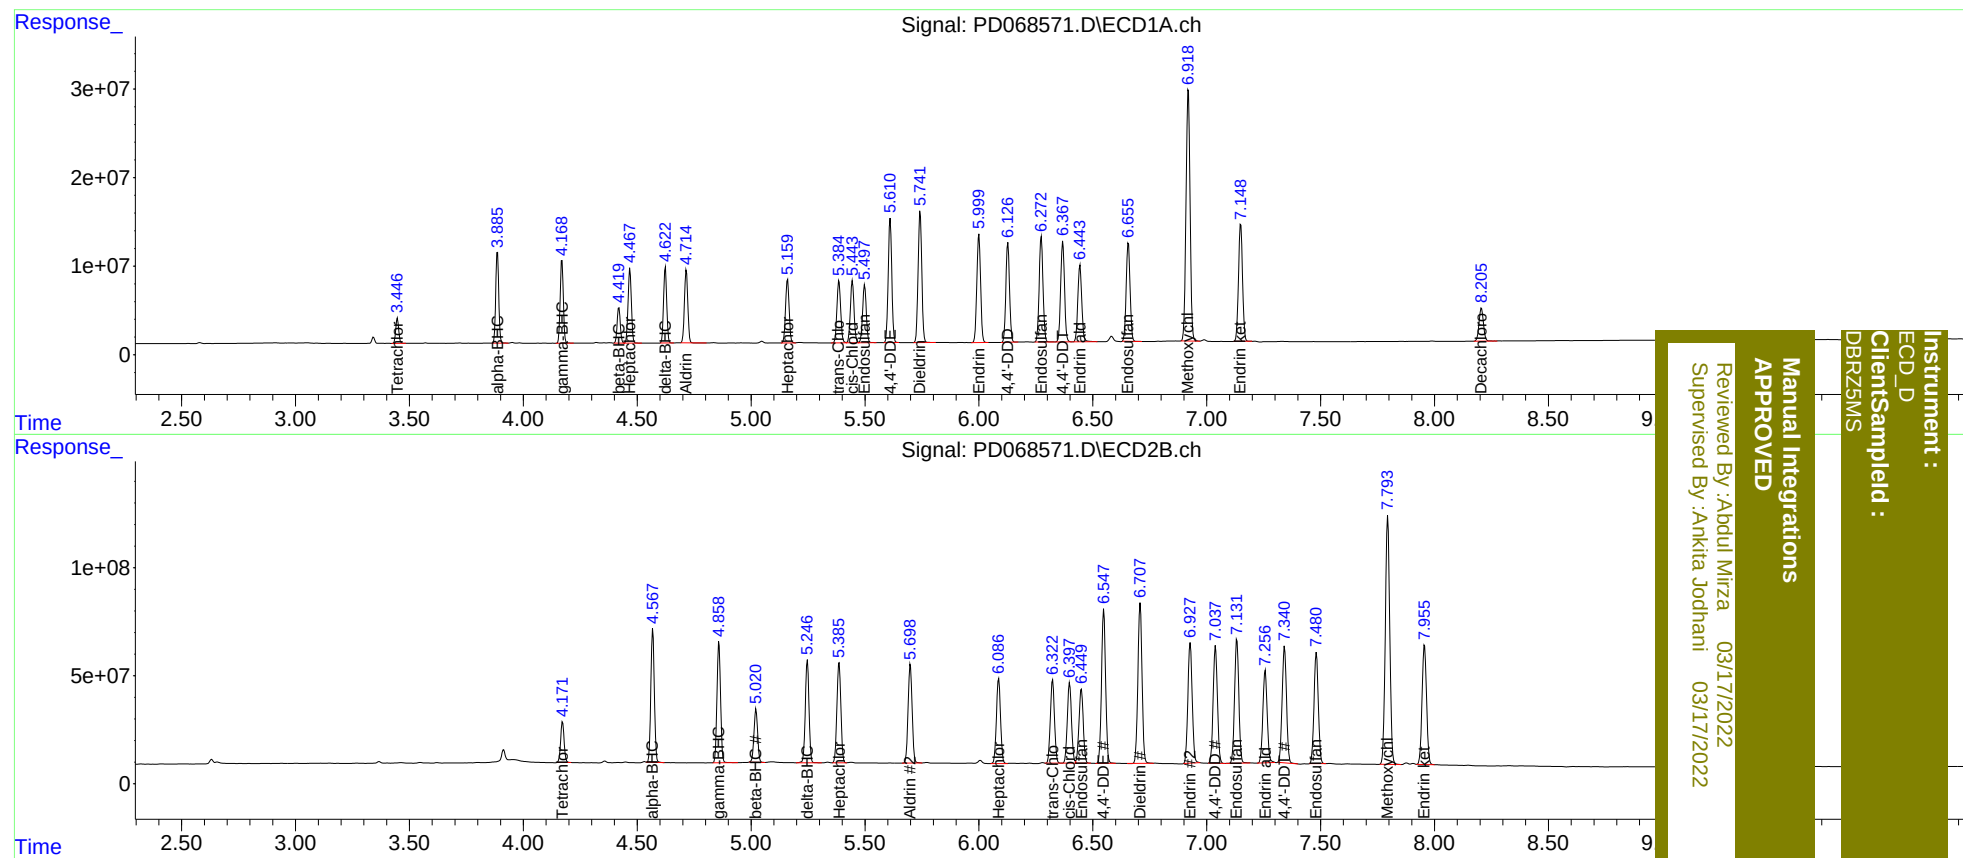

Reviewed By: Abdul Mirza 03/17/2022
Supervised By: Ankita Jodhani 03/17/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
DBRZ5MS