

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031422\
 Data File : PD068572.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2022 19:32
 Operator : AR\AJ
 Sample : N1820-05MSD
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DBRZ5MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/17/2022
 Supervised By : Ankita Jodhani 03/17/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 07:20:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 07:24:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.447	4.173	25987600	205.1E6	19.084	18.740
27)	SA Decachlor...	8.206	9.367	49725806	220.2E6	35.760	34.909
Target Compounds							
2)	A alpha-BHC	3.887	4.568	96180011	667.2E6	50.244	42.671
3)	MA gamma-BHC...	4.170	4.859	90313418	621.7E6	49.753	42.882
4)	MA Heptachlor	4.468	5.386	85429261	571.2E6	47.690	41.499
5)	MB Aldrin	4.716	5.699	85662692	572.0E6	48.707	42.386
6)	B beta-BHC	4.420	5.022	39108538	278.9E6	46.932	43.671
7)	B delta-BHC	4.624	5.247	82982241	543.4E6	46.931	38.384
8)	B Heptachlo...	5.160	6.087	79520005	502.1E6	48.965	41.688
9)	A Endosulfan I	5.498	6.450	73705687	450.7E6	47.874	41.416
10)	B trans-Chl...	5.386	6.324	80780118	493.4E6	48.403	41.487
11)	B cis-Chlor...	5.445	6.398	78986386	479.2E6	48.116	41.781
12)	B 4,4'-DDE	5.611	6.548	154.8E6	896.5E6	104.065	87.752
13)	MA Dieldrin	5.743	6.707	168.4E6	961.5E6	100.790	86.535
14)	MA Endrin	6.000	6.928	142.5E6	740.4E6	100.797	87.569
15)	B Endosulfa...	6.274	7.133	140.2E6	758.2E6	96.649	84.723
16)	A 4,4'-DDD	6.128	7.039	126.8E6	712.1E6	96.498	84.869
17)	MA 4,4'-DDT	6.369	7.342	134.1E6	722.3E6	100.383	91.651
18)	B Endrin al...	6.444	7.257	105.3E6	569.6E6	96.050	85.774
19)	B Endosulfa...	6.656	7.482	131.6E6	680.6E6	94.193	83.102
20)	A Methoxychlor	6.919	7.795	350.4E6	1573.6E6	494.977	449.199
21)	B Endrin ke...	7.149	7.955	163.9E6	765.1E6	102.735	89.609m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031422\
Data File : PD068572.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2022 19:32
Operator : AR\AJ
Sample : N1820-05MSD
Misc :
ALS Vial : 36 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 07:20:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 07:24:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

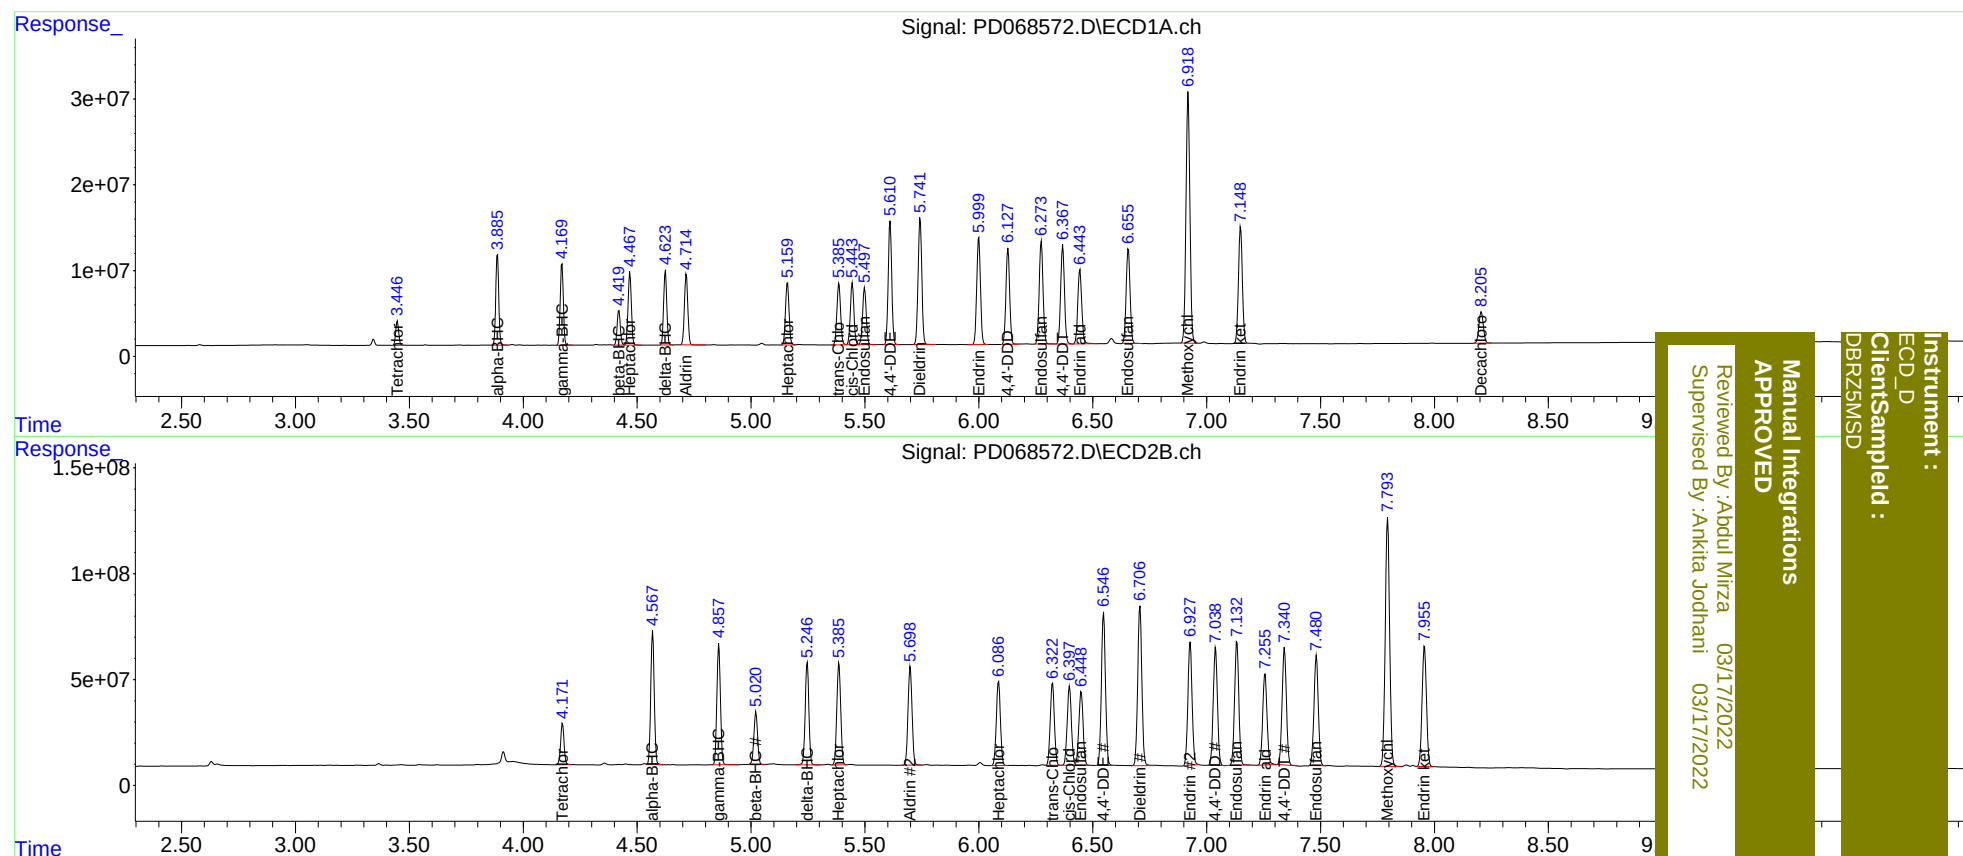

Reviewed By: Abdul Mirza 03/17/2022
Supervised By: Ankita Jodhani 03/17/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
DBRZ5MSD