

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031422\
 Data File : PD068540.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2022 10:41
 Operator : AR\AJ
 Sample : PB143211BS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS211

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/17/2022
 Supervised By : Ankita Jodhani 03/17/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 07:13:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 07:24:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.455	4.173	25615562	205.7E6	18.810	18.797
27)	SA Decachlor...	8.214	9.370	57274072	261.9E6	41.188	41.517
Target Compounds							
2)	A alpha-BHC	3.894	4.569	7915992	72714084	4.135	4.651
3)	MA gamma-BHC...	4.178	4.860	7756976	68550500	4.273	4.728
4)	MA Heptachlor	4.477	5.387	7788256	69103588	4.348	5.021
5)	MB Aldrin	4.724	5.700	7318153	61785516	4.161	4.579
6)	B beta-BHC	4.428	5.023	4067021	46736586	4.881	7.318 #
7)	B delta-BHC	4.632	5.248	6554853	61640271	3.707	4.354
8)	B Heptachlo...	5.169	6.088	7752767	65798907	4.774	5.463
9)	A Endosulfan I	5.508	6.451	7204163	54917709	4.679	5.046
10)	B trans-Chl...	5.395	6.325	8001504	59798173	4.794	5.028
11)	B cis-Chlor...	5.454	6.400	7885845	60094969	4.804	5.240
12)	B 4,4'-DDE	5.620	6.550	13913525	107.1E6	9.354	10.483
13)	MA Dieldrin	5.751	6.709	15123181	113.7E6	9.053	10.235
14)	MA Endrin	6.009	6.929	13208299	81857679	9.343	9.682
15)	B Endosulfa...	6.283	7.133	14345915	96929802	9.890	10.832m
16)	A 4,4'-DDD	6.137	7.041	12363560	86682889	9.406	10.331
17)	MA 4,4'-DDT	6.377	7.344	12628426	83784951	9.457	10.631
18)	B Endrin al...	6.453	7.258	10247836	67380387	9.345	10.147
19)	B Endosulfa...	6.665	7.483	14244084	88296859	10.192	10.781
20)	A Methoxychlor	6.928	7.797	36126654	187.7E6	51.039	53.585
21)	B Endrin ke...	7.159	7.959	16788492	98436241	10.522	11.528

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031422\
Data File : PD068540.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2022 10:41
Operator : AR\AJ
Sample : PB143211BS
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 07:13:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 07:24:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

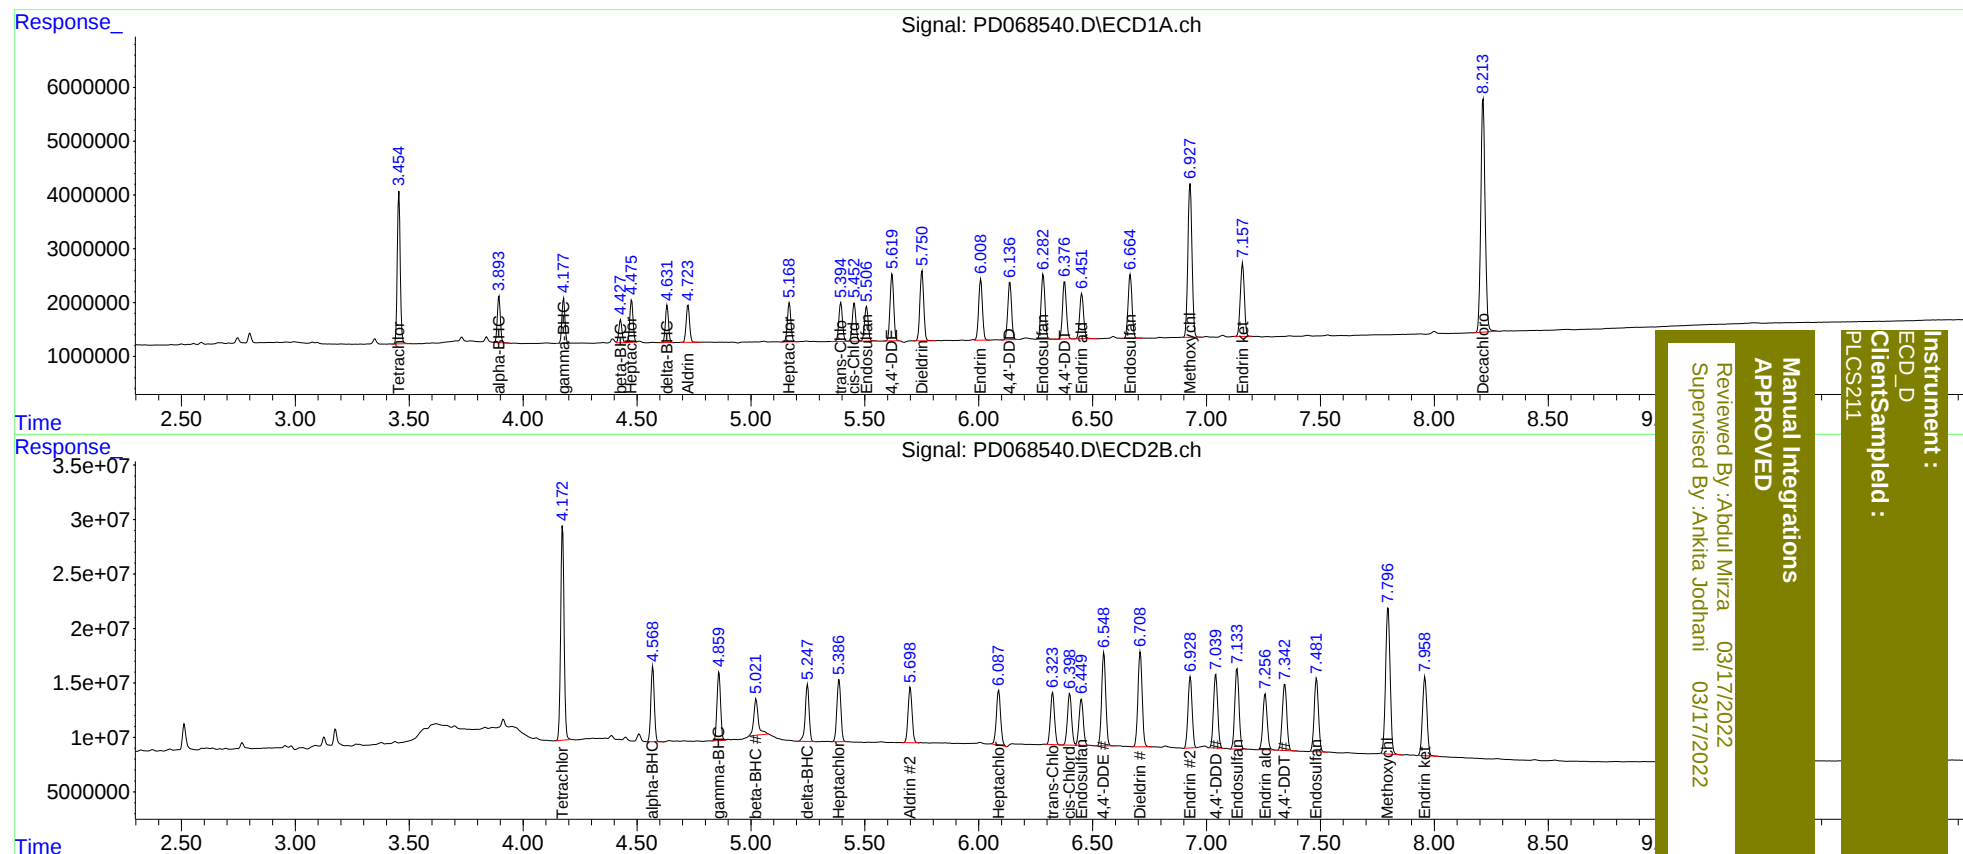

Reviewed By: Abdul Mirza 03/17/2022
Supervised By: Ankita Jodhani 03/17/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
PLCS211