

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031422\
 Data File : PD068584.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2022 22:34
 Operator : AR\AJ
 Sample : N1882-05MS
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DBRX6MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/17/2022
 Supervised By : Ankita Jodhani 03/17/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 07:22:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 07:24:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.448	4.173	21089849	169.6E6	15.487	15.492
27)	SA Decachlor...	8.206	9.365	37782640	172.1E6	27.171	27.290
Target Compounds							
2)	A alpha-BHC	3.887	4.569	93240332	662.9E6	48.708	42.400
3)	MA gamma-BHC...	4.170	4.859	87945894	616.1E6	48.449	42.494
4)	MA Heptachlor	4.469	5.386	82896405	564.3E6	46.276	41.000
5)	MB Aldrin	4.716	5.699	78624790	566.6E6	44.705	41.991
6)	B beta-BHC	4.420	5.022	38170914	285.1E6	45.806	44.642
7)	B delta-BHC	4.624	5.247	81189741	546.6E6	45.917	38.611
8)	B Heptachlo...	5.160	6.087	77092800	497.8E6	47.471	41.330
9)	A Endosulfan I	5.498	6.449	71684518	449.3E6	46.561	41.280
10)	B trans-Chl...	5.386	6.323	78884362	492.9E6	47.267	41.441
11)	B cis-Chlor...	5.445	6.398	76913970	476.3E6	46.854	41.528
12)	B 4,4'-DDE	5.611	6.548	150.6E6	893.9E6	101.258	87.501
13)	MA Dieldrin	5.742	6.708	164.5E6	948.9E6	98.503	85.395
14)	MA Endrin	6.000	6.928	138.5E6	731.7E6	97.965	86.541
15)	B Endosulfa...	6.274	7.132	138.0E6	756.5E6	95.110	84.537
16)	A 4,4'-DDD	6.128	7.038	125.0E6	708.0E6	95.072	84.377
17)	MA 4,4'-DDT	6.369	7.342	130.1E6	710.6E6	97.440	90.163
18)	B Endrin al...	6.444	7.256	103.2E6	566.7E6	94.094	85.339
19)	B Endosulfa...	6.656	7.480	128.9E6	679.6E6	92.210	82.979m
20)	A Methoxychlor	6.919	7.794	340.5E6	1551.4E6	481.011	442.854
21)	B Endrin ke...	7.149	7.955	160.3E6	759.2E6	100.460	88.910m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031422\
 Data File : PD068584.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2022 22:34
 Operator : AR\AJ
 Sample : N1882-05MS
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 07:22:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 07:24:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

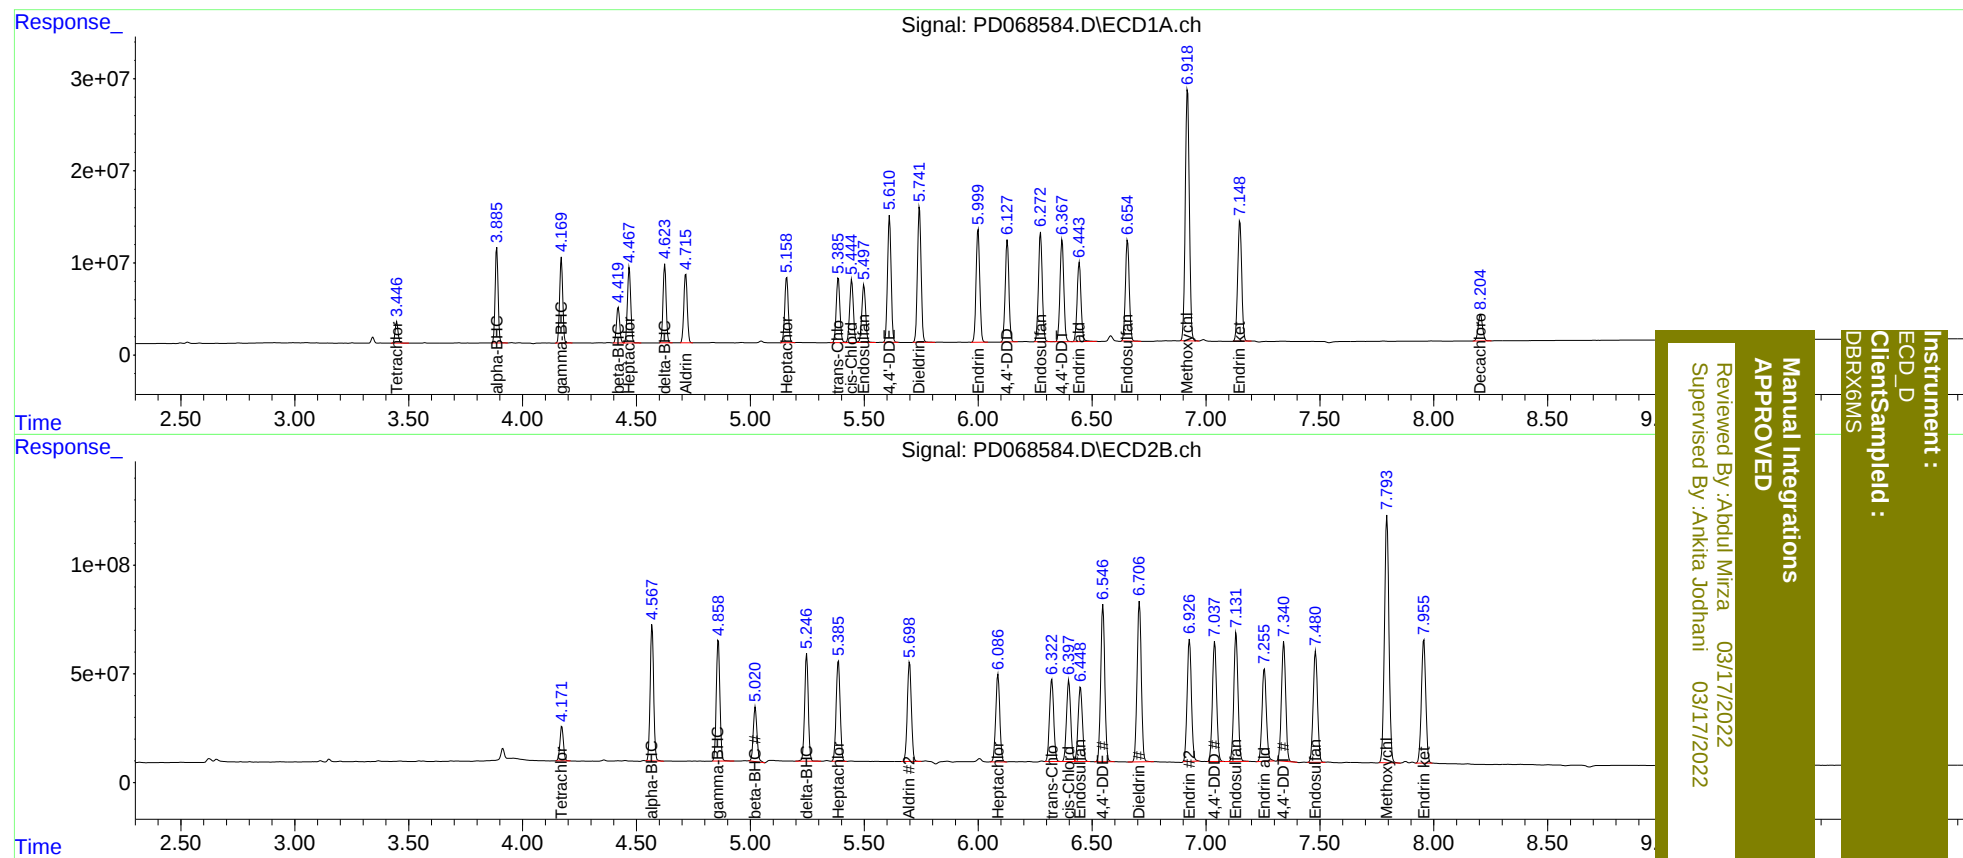

Reviewed By: Abdul Mirza 03/17/2022
 Supervised By: Ankita Jodhani 03/17/2022

Manual Integrations
 APPROVED

Instrument :
 ECD_D
 ClientSampled :
 DBRX6MS