

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031422\
 Data File : PD068585.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2022 22:48
 Operator : AR\AJ
 Sample : N1882-06MSD
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DBRX6MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/17/2022
 Supervised By : Ankita Jodhani 03/17/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 07:23:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 07:24:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.448	4.173	21311669	172.5E6	15.650	15.764
27)	SA Decachlor...	8.206	9.367	39014658	174.8E6	28.057	27.715
Target Compounds							
2)	A alpha-BHC	3.887	4.569	94975709	676.1E6	49.615	43.239
3)	MA gamma-BHC...	4.170	4.859	89616879	628.5E6	49.370	43.349
4)	MA Heptachlor	4.468	5.387	84407100	575.2E6	47.120	41.788
5)	MB Aldrin	4.716	5.699	80078873	576.3E6	45.532	42.704
6)	B beta-BHC	4.420	5.022	38840805	291.0E6	46.610	45.558
7)	B delta-BHC	4.624	5.247	83147627	554.7E6	47.025	39.182
8)	B Heptachlo...	5.160	6.087	78481022	507.6E6	48.325	42.139
9)	A Endosulfan I	5.499	6.450	72989796	458.0E6	47.409	42.081
10)	B trans-Chl...	5.386	6.323	80482811	502.2E6	48.225	42.227
11)	B cis-Chlor...	5.445	6.399	78458329	485.4E6	47.795	42.322
12)	B 4,4'-DDE	5.611	6.548	153.6E6	909.8E6	103.243	89.055
13)	MA Dieldrin	5.743	6.708	167.6E6	970.6E6	100.360	87.354
14)	MA Endrin	6.000	6.928	141.3E6	745.6E6	99.955	88.191
15)	B Endosulfa...	6.274	7.132	140.4E6	771.5E6	96.813	86.210
16)	A 4,4'-DDD	6.128	7.038	127.8E6	721.4E6	97.247	85.976
17)	MA 4,4'-DDT	6.369	7.341	132.4E6	730.5E6	99.170	92.681
18)	B Endrin al...	6.444	7.256	105.1E6	578.2E6	95.795	87.074
19)	B Endosulfa...	6.655	7.479	132.0E6	693.0E6	94.444m	84.618m
20)	A Methoxychlor	6.919	7.794	348.6E6	1582.7E6	492.458	451.806
21)	B Endrin ke...	7.149	7.956	163.8E6	771.9E6	102.660	90.397

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031422\
Data File : PD068585.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2022 22:48
Operator : AR\AJ
Sample : N1882-06MSD
Misc :
ALS Vial : 47 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 07:23:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 07:24:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

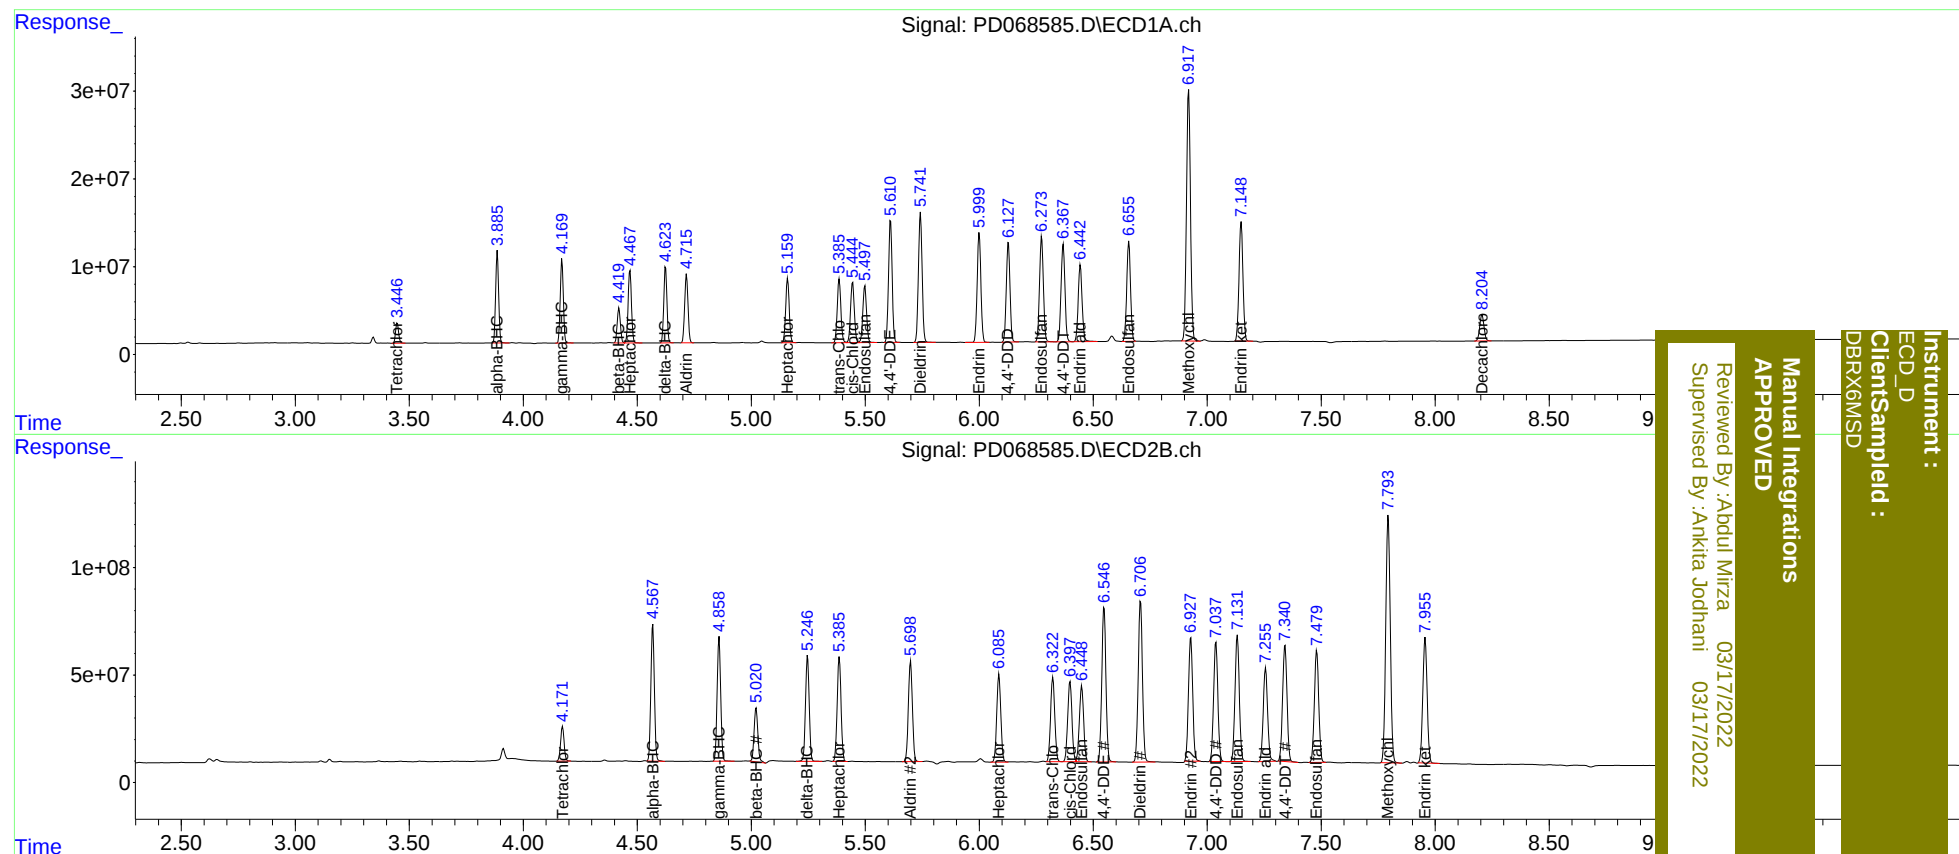

Reviewed By: Abdul Mirza 03/17/2022
Supervised By: Ankita Jodhani 03/17/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
DBRX6MSD