

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031423\
 Data File : PD074214.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2023 22:06
 Operator : AR\AJ
 Sample : PB151305BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 05:08:51 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031423.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 15 05:04:28 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.551	2.772	44349196	22073723	19.013	18.138
28)	SA Decachlor...	9.099	7.927	54431922	25141605	20.352	20.492
Target Compounds							
5)	MB Aldrin	5.296f	0.000	145535	0	0.043	N.D. #
7)	B delta-BHC	4.779	0.000	4274827	0	1.558	N.D. #
8)	B Heptachlo...	5.697	0.000	5422421	0	1.928	N.D. #
9)	A Endosulfan I	6.069f	0.000	28497	0	0.010	N.D. #
11)	B alpha-Chl...	6.069f	0.000	28497	0	0.009	N.D. #
14)	MA Endrin	0.000	5.660f	0	421821	N.D.	0.323 #
15)	B Endosulfa...	6.840f	0.000	306200	0	0.119	N.D. #
21)	B Endrin ke...	7.698f	0.000	885121	0	0.318	N.D. #
22)	Mirex	8.157	0.000	702188	0	0.331	N.D. #
24)	Chlordane-2	0.000	4.339	0	252152	N.D.	4.340 #
26)	Chlordane-4	6.069f	0.000	28497	0	0.048	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031423\
Data File : PD074214.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2023 22:06
Operator : AR\AJ
Sample : PB151305BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 05:08:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031423.M
Quant Title : GC Extractables
QLast Update : Wed Mar 15 05:04:28 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

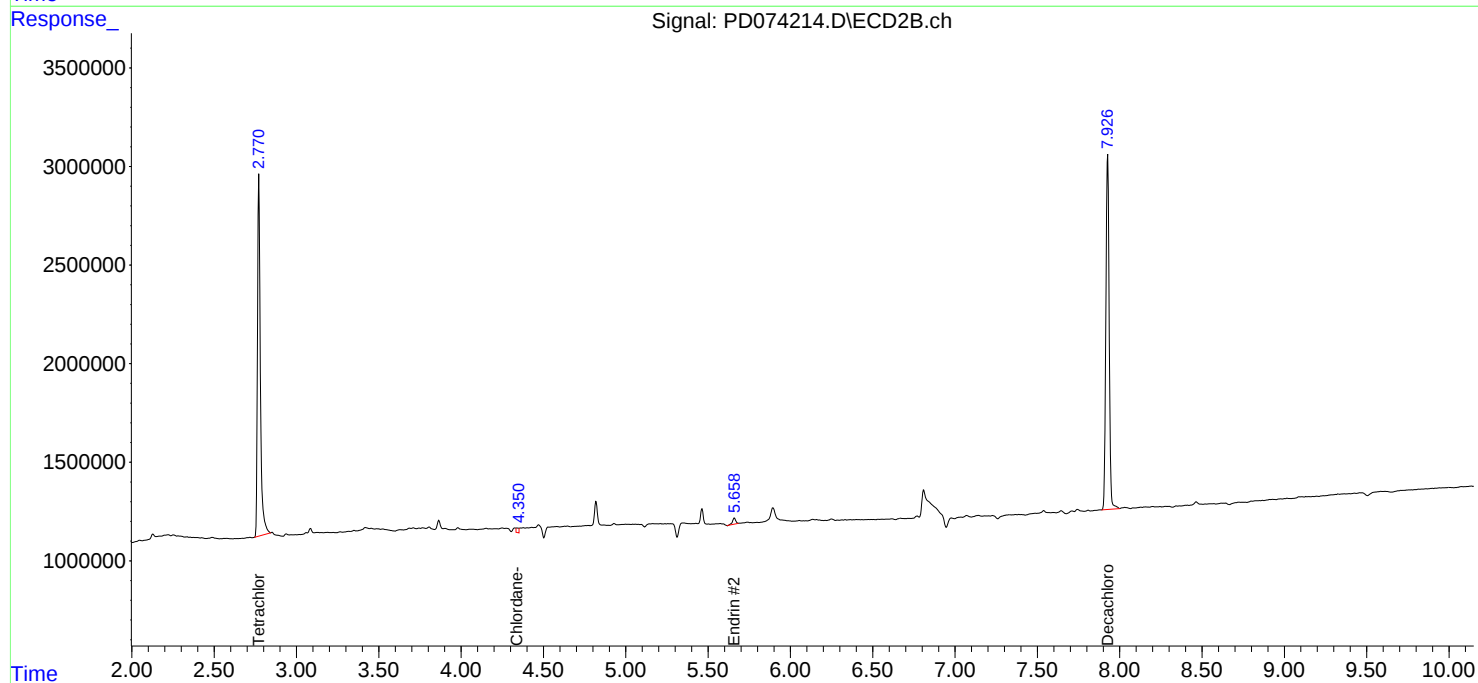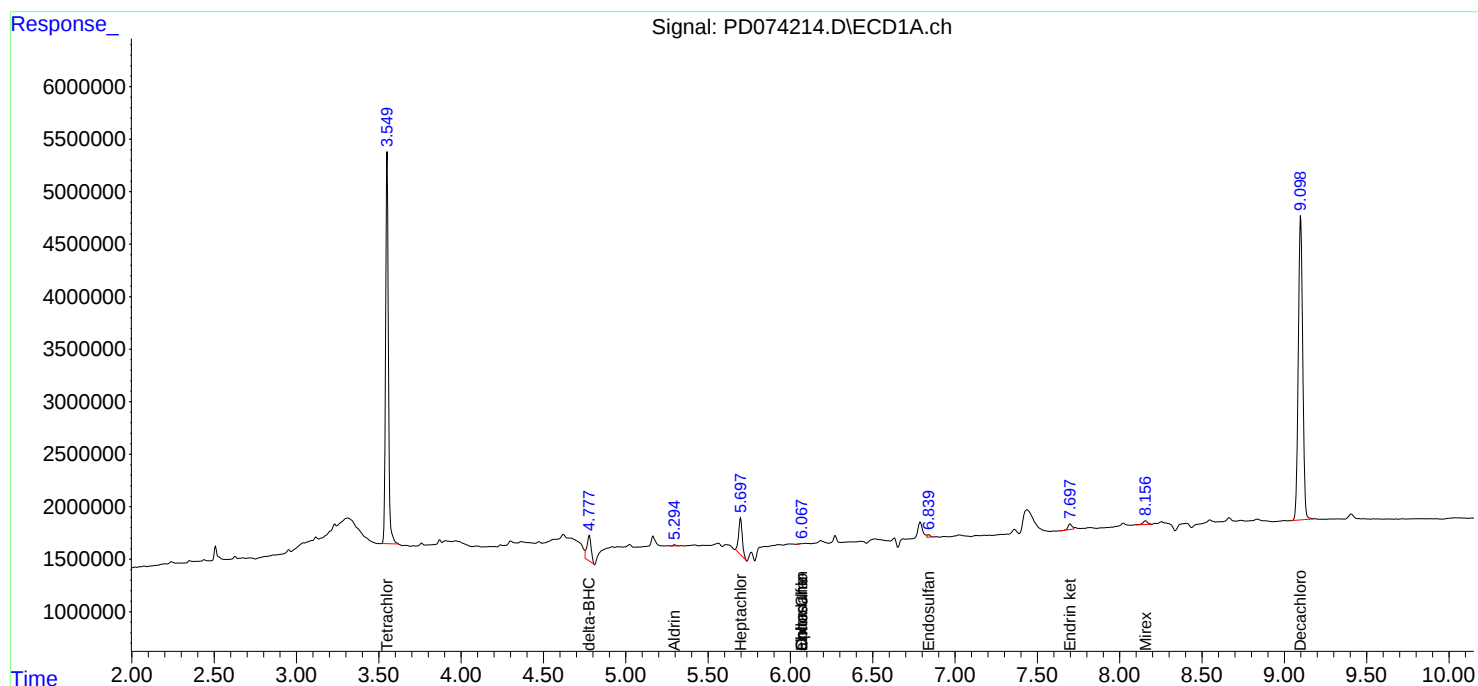


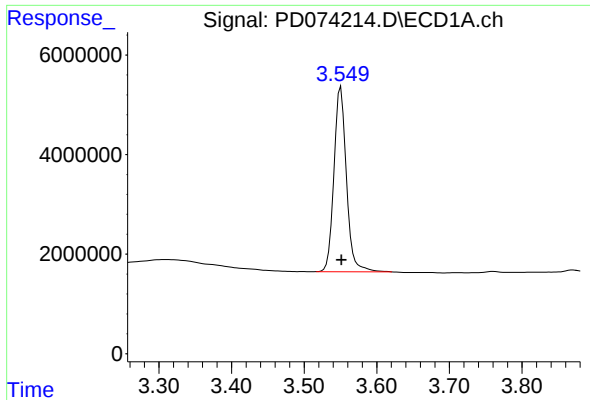

#1 Tetrachloro-m-xylene


R.T.: 3.551 min
Delta R.T.: 0.000 min
Response: 44349196
Conc: 19.01 ng/ml

Instrument :
ECD_D
ClientSampleId :

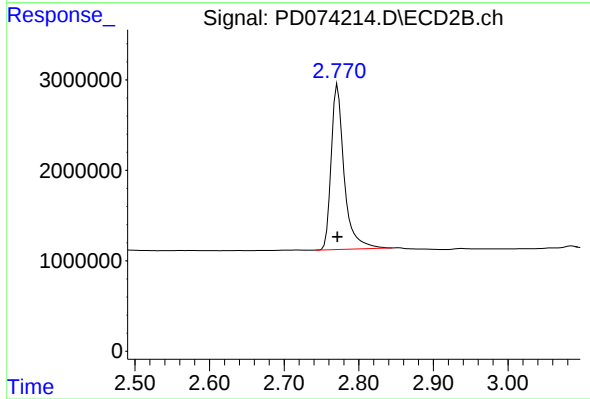


#1 Tetrachloro-m-xylene

R.T.: 2.772 min
Delta R.T.: 0.000 min
Response: 22073723
Conc: 18.14 ng/ml

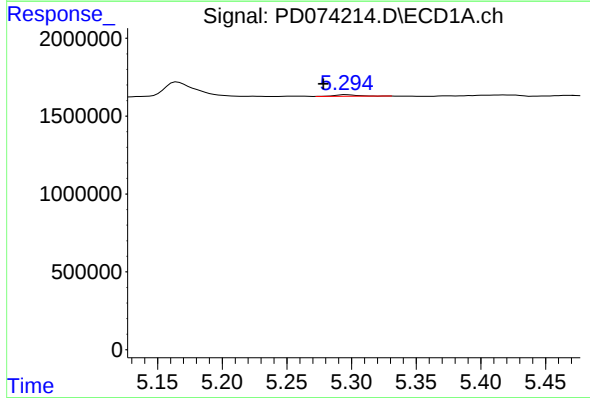


#5 Aldrin

R.T.: 5.296 min
Delta R.T.: 0.018 min
Response: 145535
Conc: 0.04 ng/ml

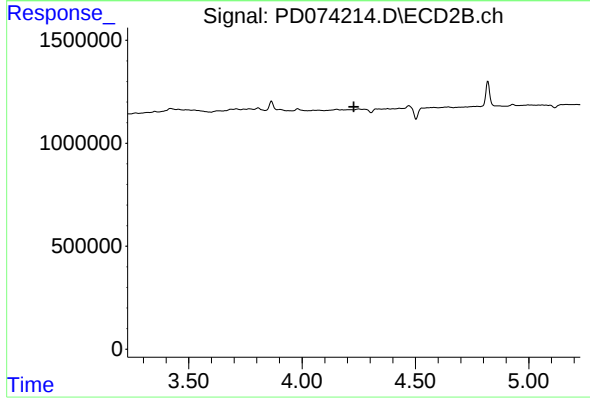

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 4.229 min
Response: 0
Conc: N.D.

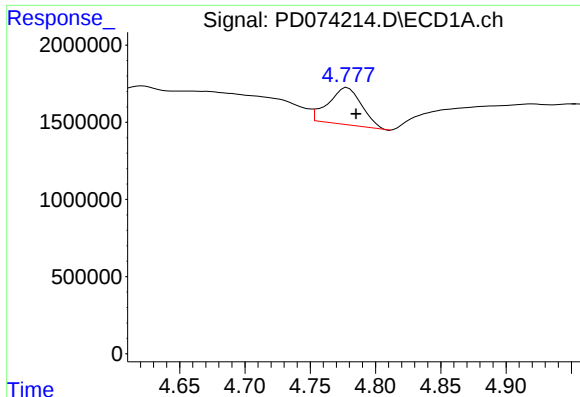

#7 delta-BHC


R.T.: 4.779 min
Delta R.T.: -0.007 min
Response: 4274827
Conc: 1.56 ng/ml

Instrument :
ECD_D
ClientSampleId :

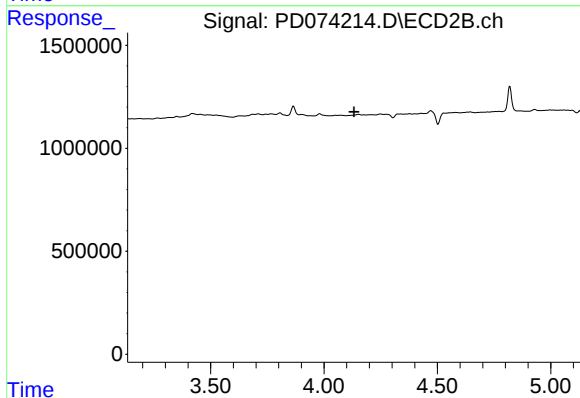


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.132 min
Response: 0
Conc: N.D.

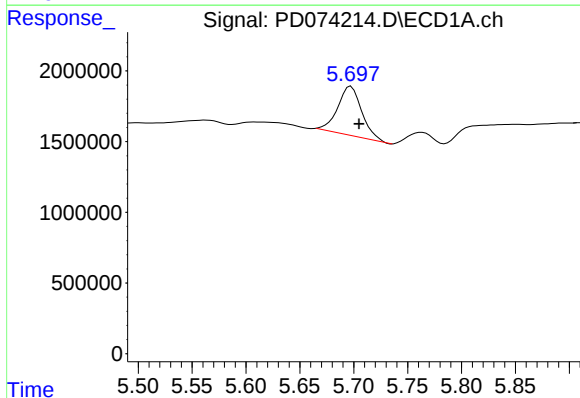


#8 Heptachlor epoxide

R.T.: 5.697 min
Delta R.T.: -0.008 min
Response: 5422421
Conc: 1.93 ng/ml

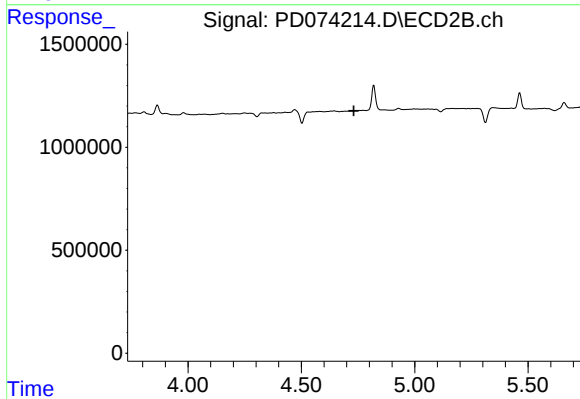

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.731 min
Response: 0
Conc: N.D.

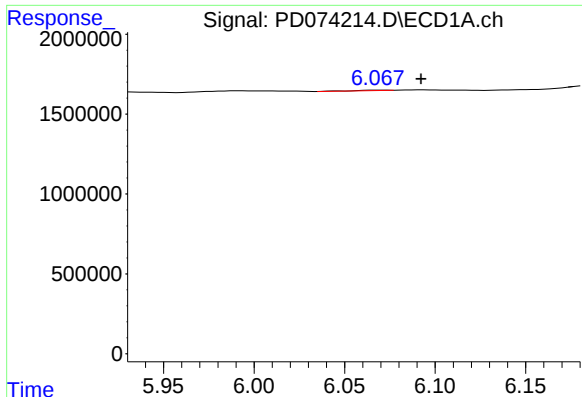

#9 Endosulfan I


R.T.: 6.069 min
Delta R.T.: -0.024 min
Response: 28497
Conc: 0.01 ng/ml

Instrument :
ECD_D
ClientSampleId :

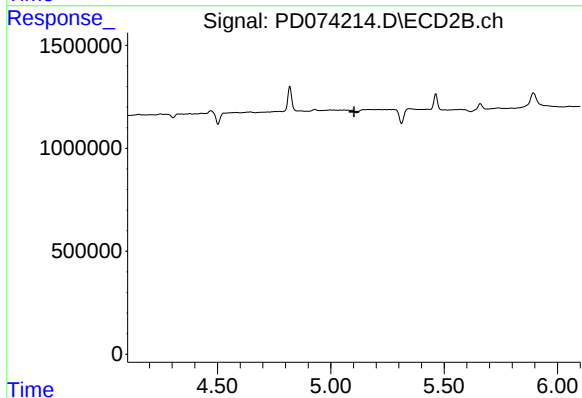


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.103 min
Response: 0
Conc: N.D.

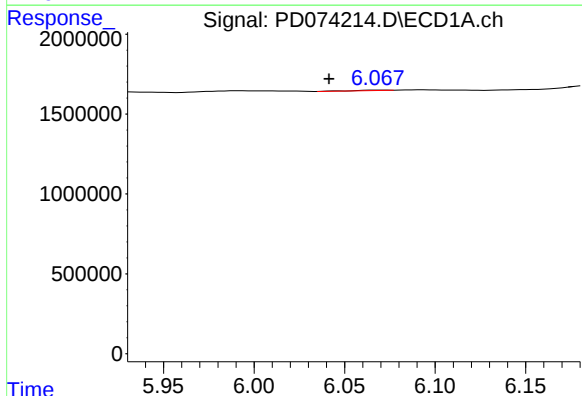


#11 alpha-Chlordane

R.T.: 6.069 min
Delta R.T.: 0.027 min
Response: 28497
Conc: 0.01 ng/ml

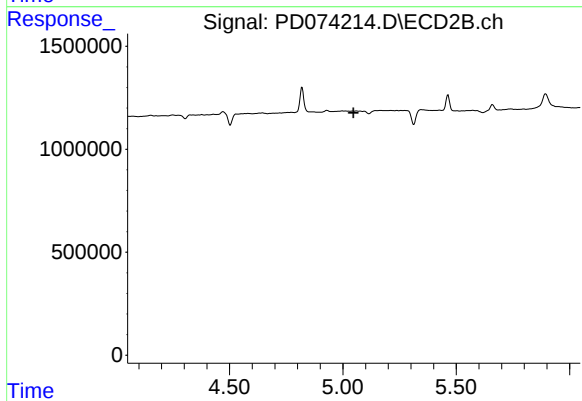

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.047 min
Response: 0
Conc: N.D.

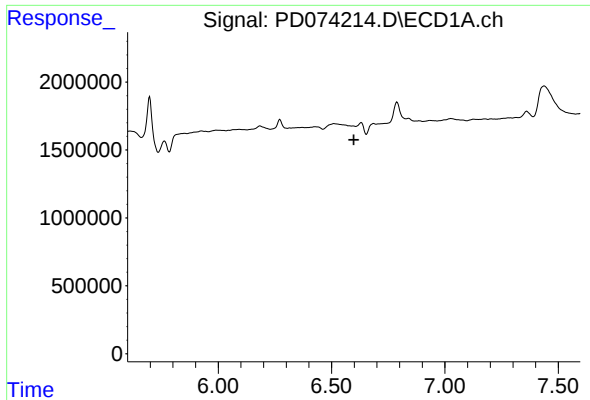

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.598 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

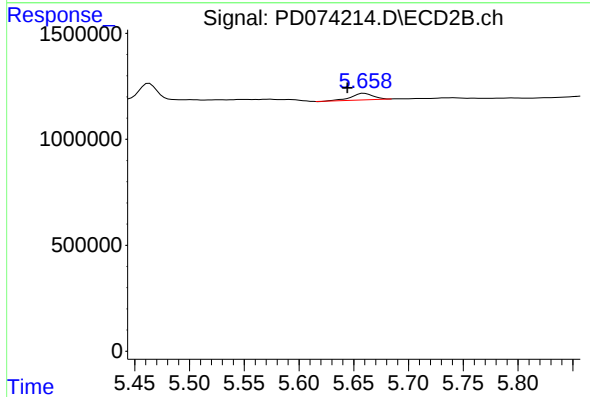


#14 Endrin

R.T.: 5.660 min
Delta R.T.: 0.016 min
Response: 421821
Conc: 0.32 ng/ml

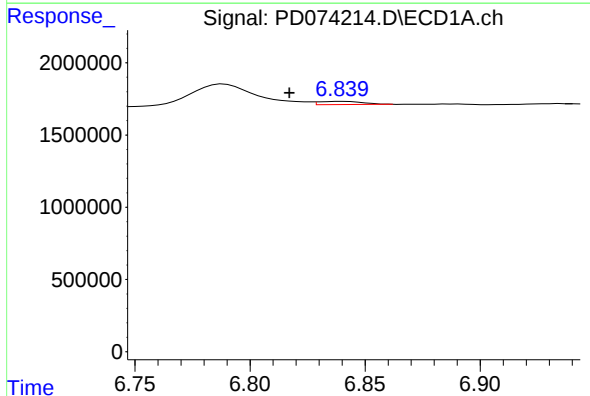


#15 Endosulfan II

R.T.: 6.840 min
Delta R.T.: 0.023 min
Response: 306200
Conc: 0.12 ng/ml

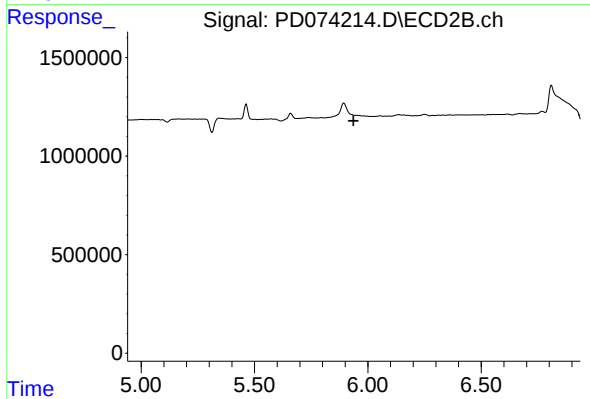

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.937 min
Response: 0
Conc: N.D.

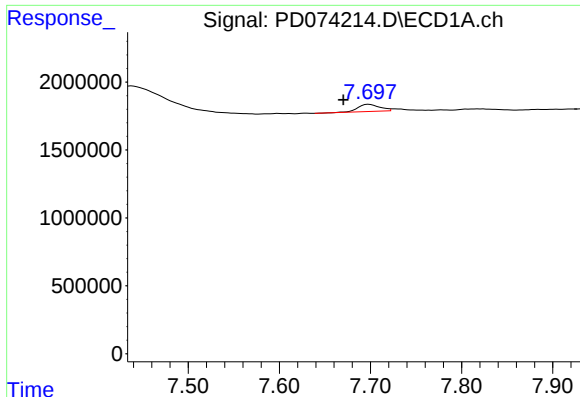

#21 Endrin ketone


R.T.: 7.698 min
Delta R.T.: 0.028 min
Response: 885121
Conc: 0.32 ng/ml

Instrument :
ECD_D
ClientSampleId :

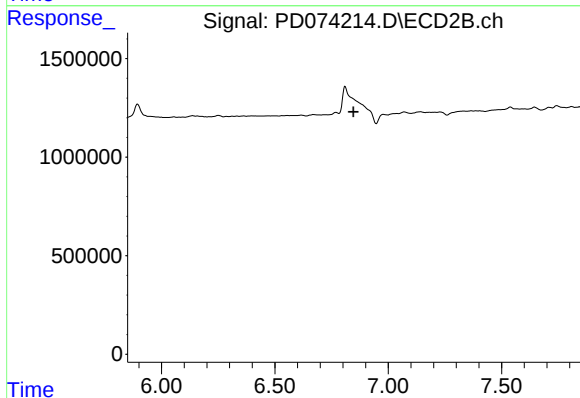


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.847 min
Response: 0
Conc: N.D.

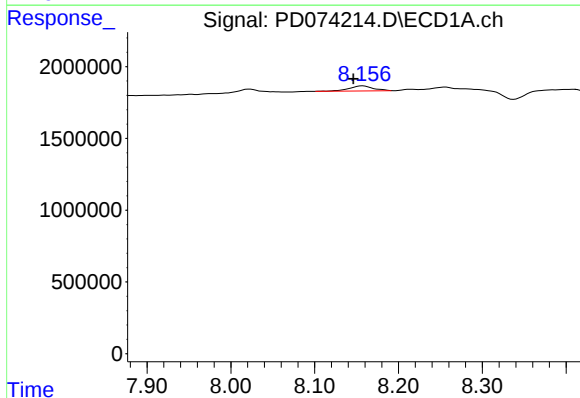


#22 Mirex

R.T.: 8.157 min
Delta R.T.: 0.011 min
Response: 702188
Conc: 0.33 ng/ml

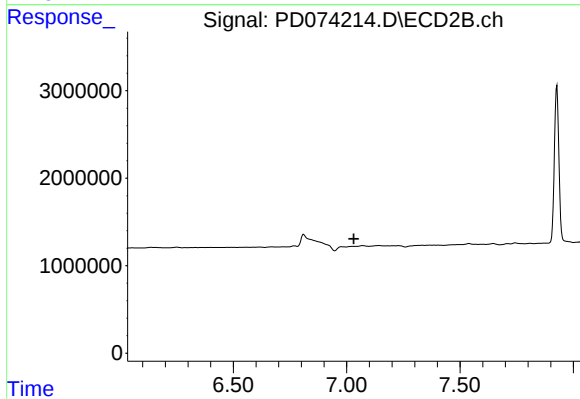

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 7.032 min
Response: 0
Conc: N.D.

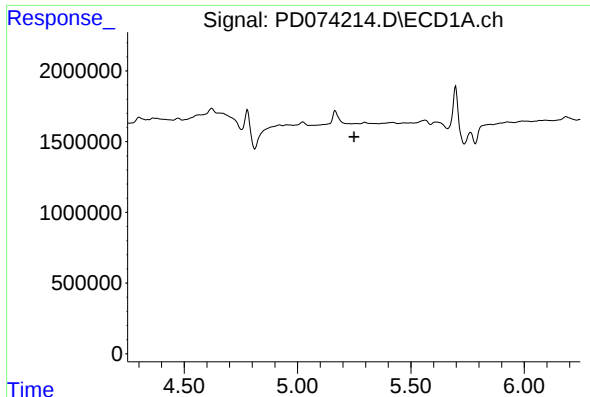

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.249 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

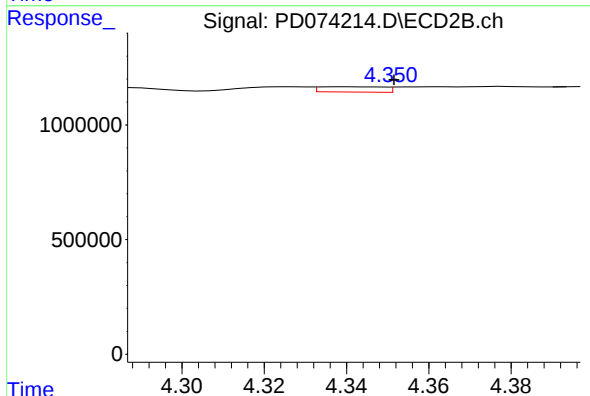


#24 Chlordane-2

R.T.: 4.339 min
Delta R.T.: -0.013 min
Response: 252152
Conc: 4.34 ng/ml

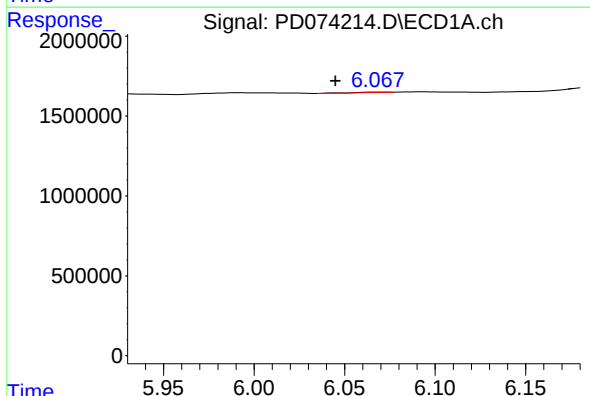


#26 Chlordane-4

R.T.: 6.069 min
Delta R.T.: 0.024 min
Response: 28497
Conc: 0.05 ng/ml

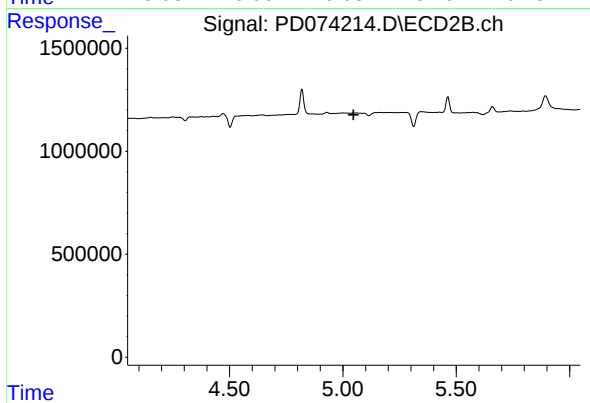

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.047 min
Response: 0
Conc: N.D.

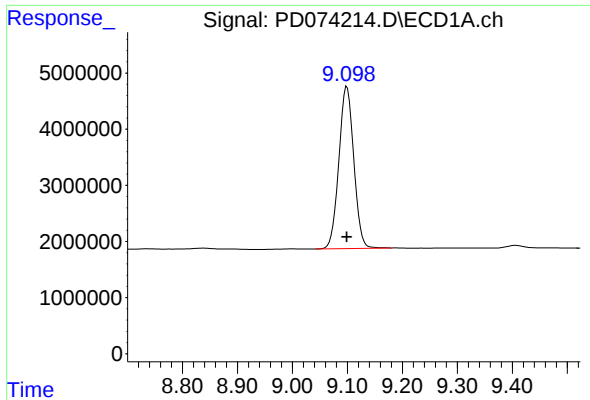

#28 Decachlorobiphenyl

R.T.: 9.099 min
Delta R.T.: 0.000 min
Response: 54431922
Conc: 20.35 ng/ml

Instrument :
ECD_D
ClientSampleId :

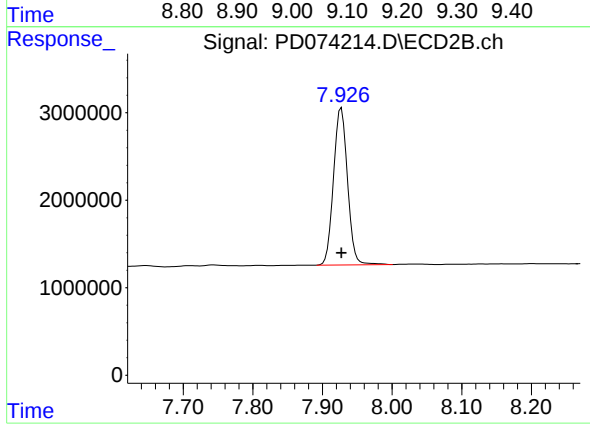

#28 Decachlorobiphenyl

R.T.: 7.927 min
Delta R.T.: 0.000 min
Response: 25141605
Conc: 20.49 ng/ml