

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031423\
 Data File : PD074191.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2023 15:35
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 05:07:26 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031423.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 15 05:04:28 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.551	2.772	52583649	27711685	22.543	22.770
28) SA Decachlor...	9.100	7.928	60222489	27472111	22.517	22.391
Target Compounds						
9) A Endosulfan I	6.093	5.104	30360972	15743256	10.679	10.939
10) B gamma-Chl...	5.962	4.983	31973849	17441849	10.653	11.233
12) B 4,4'-DDE	6.214	5.238	57921293	30205685	21.007	21.405
13) MA Dieldrin	6.369	5.369	63778266	32917871	21.620	21.892
19) B Endosulfa...	7.183	6.341	49662093	24208724	20.114	19.830
20) A Methoxychlor	7.524	6.622	142.7E6	69042927	101.990	102.040
21) B Endrin ke...	7.671	6.848	60906539	31908332	21.879	21.632



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031423\
Data File : PD074191.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2023 15:35
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 05:07:26 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031423.M
Quant Title : GC Extractables
QLast Update : Wed Mar 15 05:04:28 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

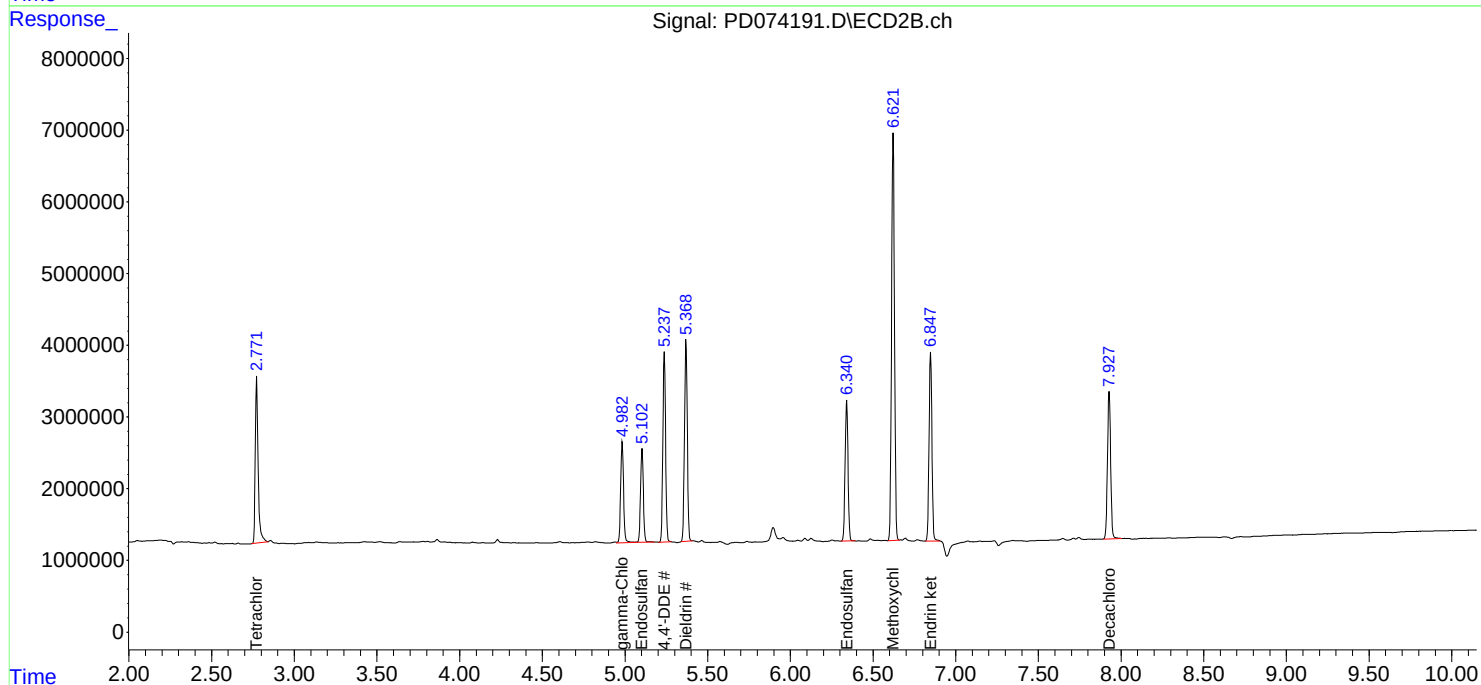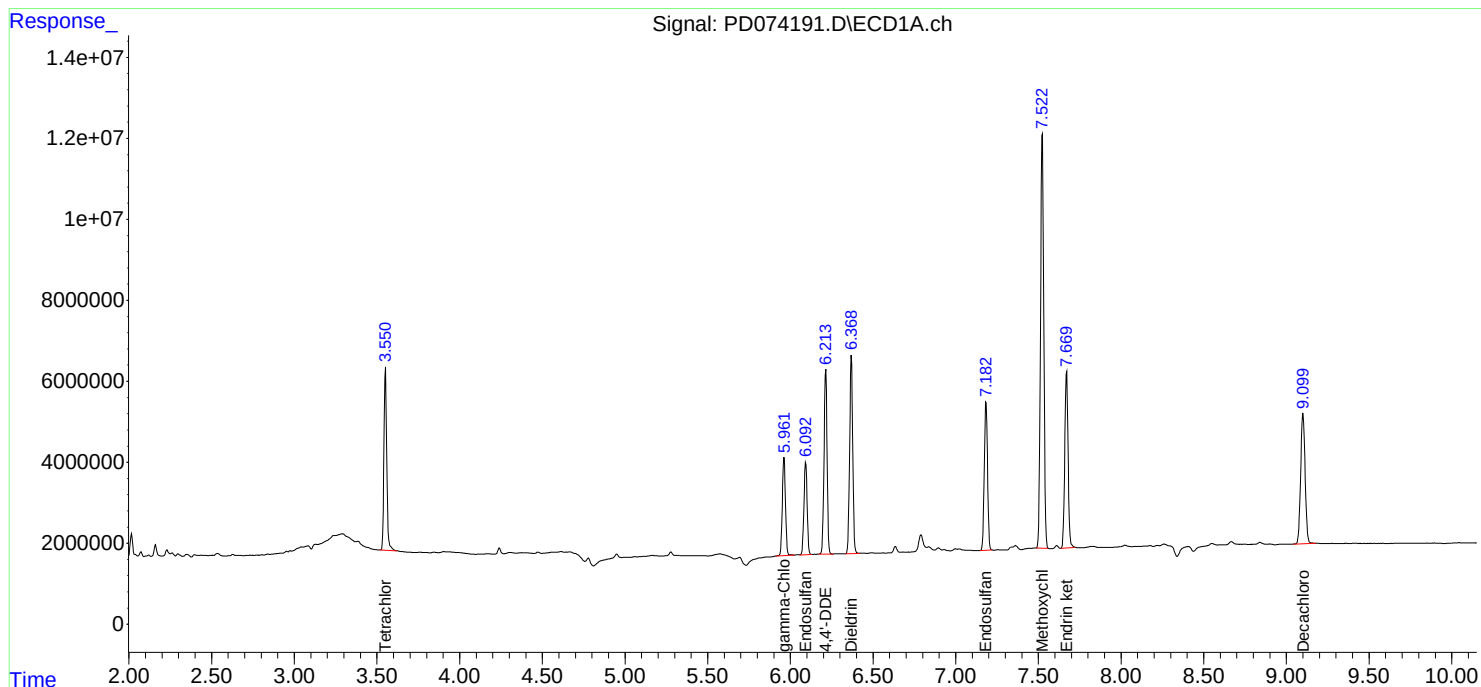


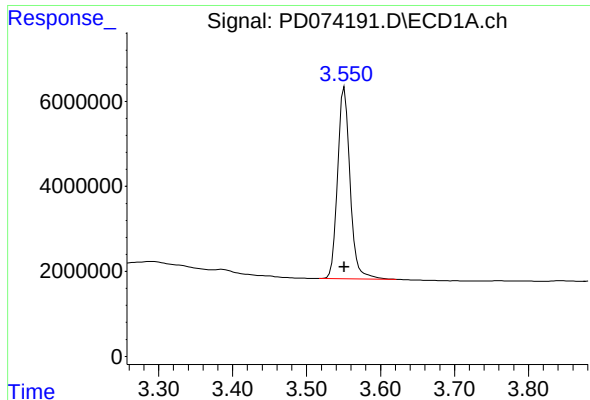

#1 Tetrachloro-m-xylene


R.T.: 3.551 min
Delta R.T.: 0.000 min
Response: 52583649
Conc: 22.54 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

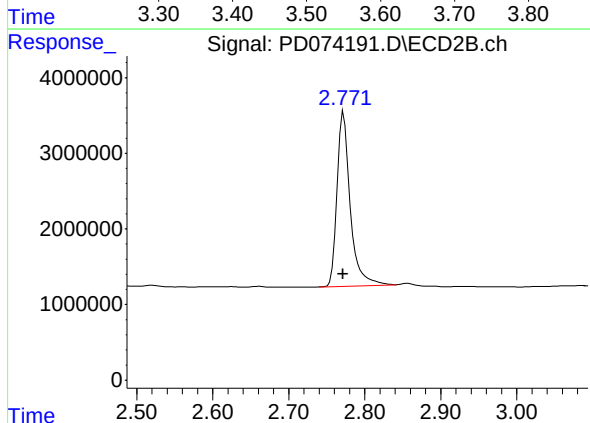


#1 Tetrachloro-m-xylene

R.T.: 2.772 min
Delta R.T.: 0.000 min
Response: 27711685
Conc: 22.77 ng/ml

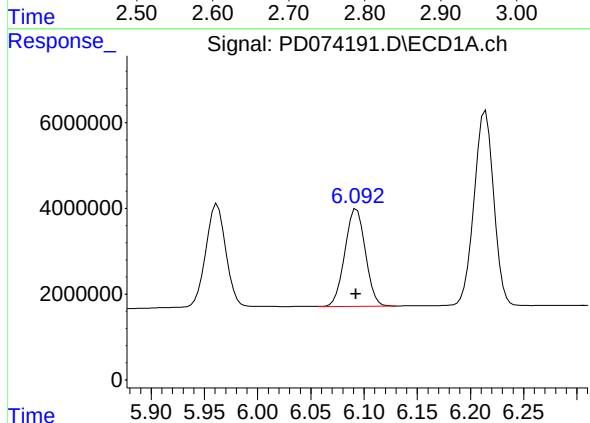


#9 Endosulfan I

R.T.: 6.093 min
Delta R.T.: 0.000 min
Response: 30360972
Conc: 10.68 ng/ml

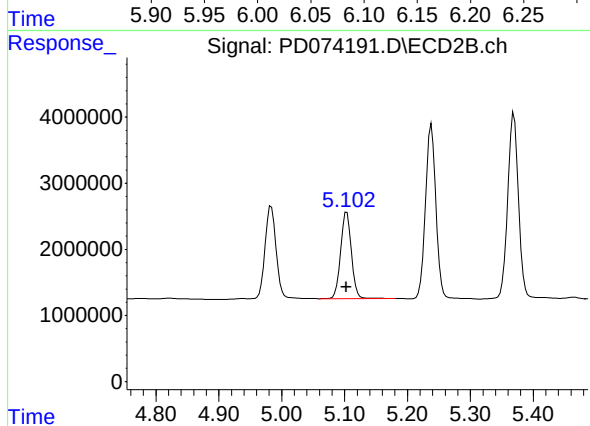

#9 Endosulfan I


R.T.: 5.104 min
Delta R.T.: 0.000 min
Response: 15743256
Conc: 10.94 ng/ml

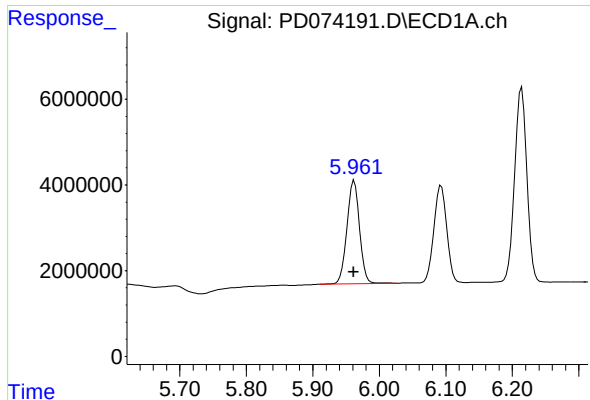

#10 gamma-Chlordane


R.T.: 5.962 min
Delta R.T.: 0.000 min
Response: 31973849
Conc: 10.65 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

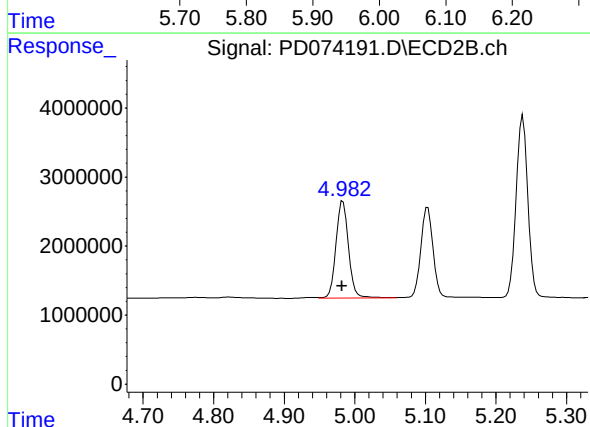


#10 gamma-Chlordane

R.T.: 4.983 min
Delta R.T.: 0.001 min
Response: 17441849
Conc: 11.23 ng/ml

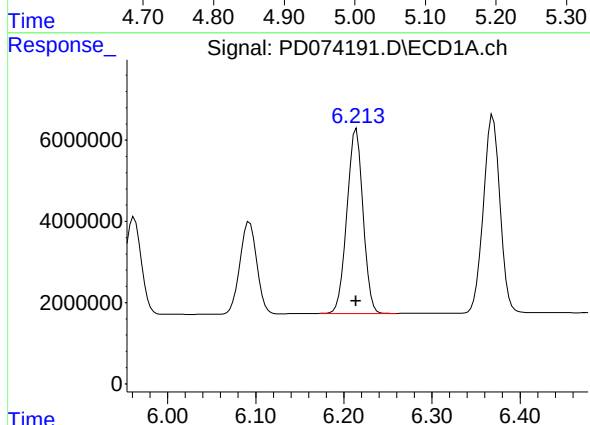


#12 4,4'-DDE

R.T.: 6.214 min
Delta R.T.: 0.000 min
Response: 57921293
Conc: 21.01 ng/ml

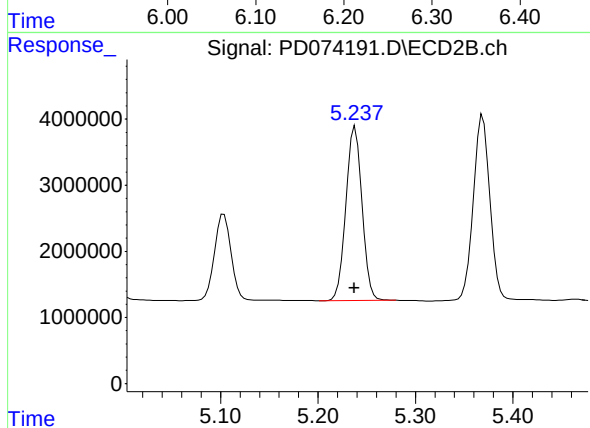

#12 4,4'-DDE


R.T.: 5.238 min
Delta R.T.: 0.001 min
Response: 30205685
Conc: 21.41 ng/ml

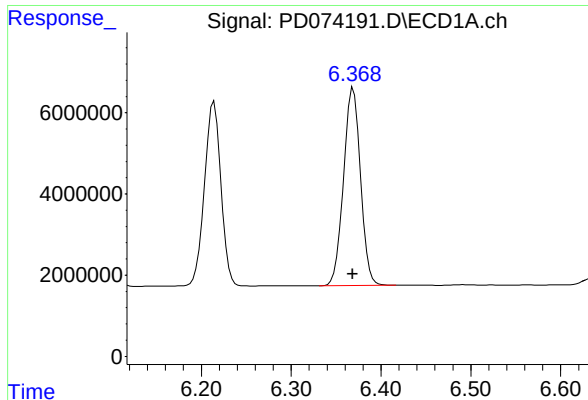

#13 Dieldrin


R.T.: 6.369 min
Delta R.T.: 0.000 min
Response: 63778266
Conc: 21.62 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

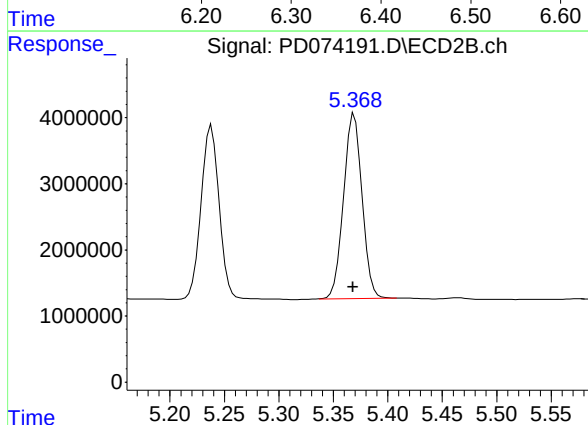


#13 Dieldrin

R.T.: 5.369 min
Delta R.T.: 0.001 min
Response: 32917871
Conc: 21.89 ng/ml

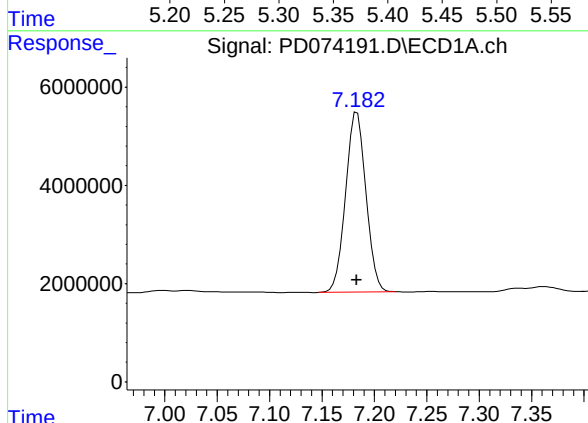


#19 Endosulfan Sulfate

R.T.: 7.183 min
Delta R.T.: 0.000 min
Response: 49662093
Conc: 20.11 ng/ml

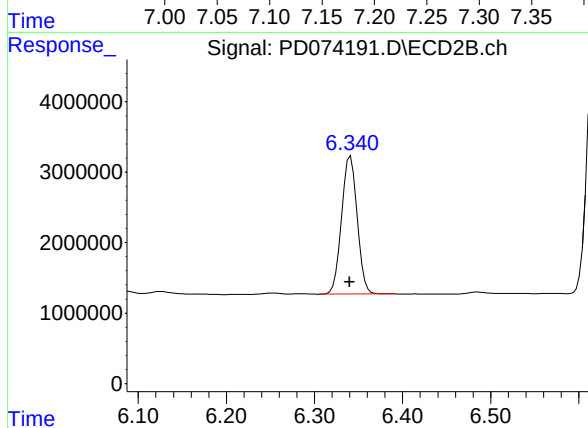

#19 Endosulfan Sulfate


R.T.: 6.341 min
Delta R.T.: 0.000 min
Response: 24208724
Conc: 19.83 ng/ml

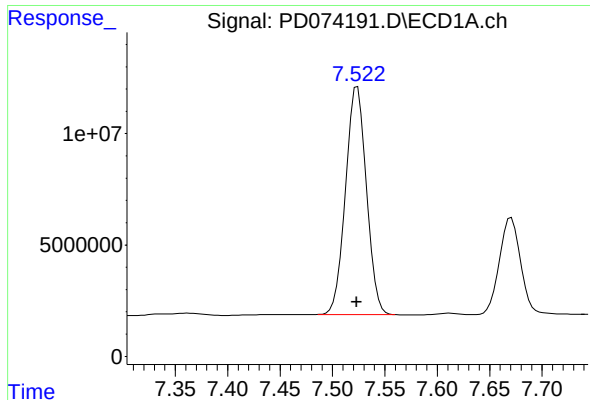

#20 Methoxychlor


R.T.: 7.524 min
Delta R.T.: 0.000 min
Response: 142703515
Conc: 101.99 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

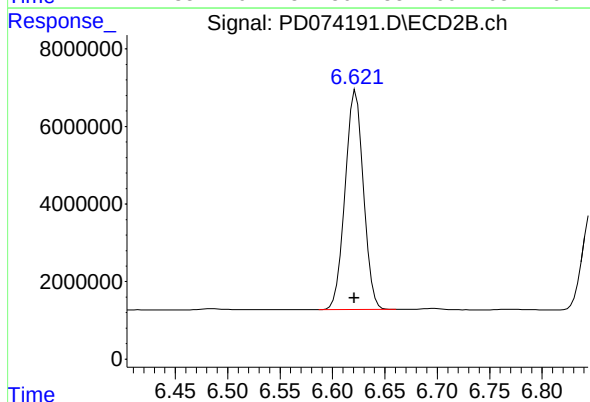


#20 Methoxychlor

R.T.: 6.622 min
Delta R.T.: 0.001 min
Response: 69042927
Conc: 102.04 ng/ml

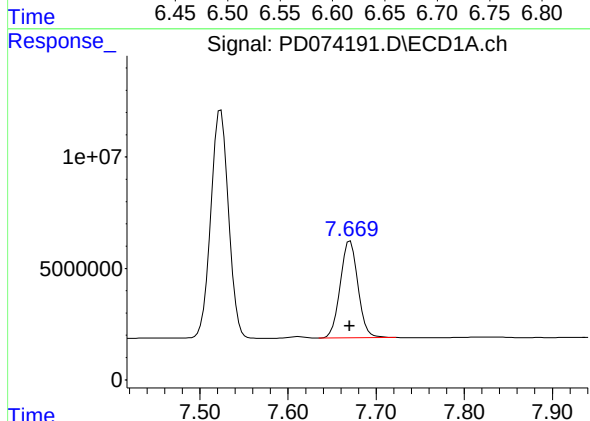


#21 Endrin ketone

R.T.: 7.671 min
Delta R.T.: 0.000 min
Response: 60906539
Conc: 21.88 ng/ml

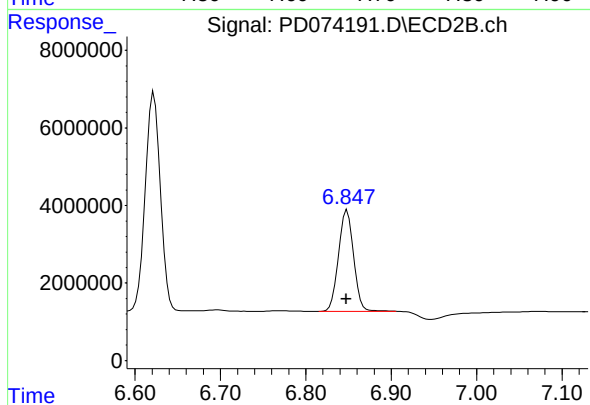

#21 Endrin ketone


R.T.: 6.848 min
Delta R.T.: 0.001 min
Response: 31908332
Conc: 21.63 ng/ml

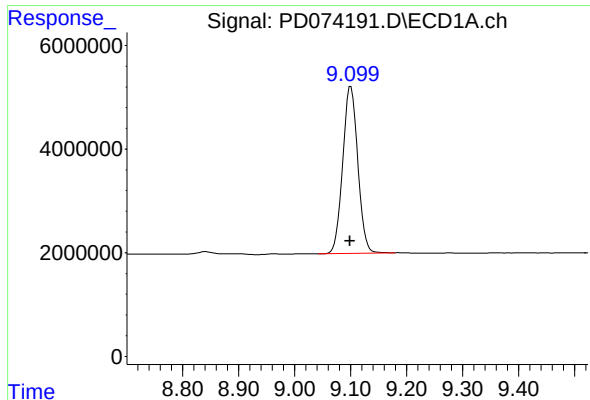

#28 Decachlorobiphenyl

R.T.: 9.100 min
Delta R.T.: 0.001 min
Response: 60222489
Conc: 22.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

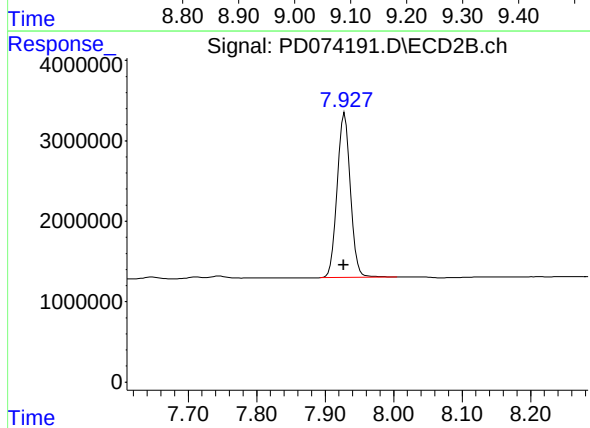

#28 Decachlorobiphenyl

R.T.: 7.928 min
Delta R.T.: 0.001 min
Response: 27472111
Conc: 22.39 ng/ml