

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031423\
 Data File : PD074198.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2023 17:10
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 04:28:02 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031423.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 15 04:27:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.550	2.771	171.2E6	111.1E6	74.471	74.428
28)	SA Decachlor...	9.100	7.927	182.3E6	87983762	74.233	74.355
Target Compounds							
23)	Chlordane-1	4.718	3.773	85641538	38027572	744.435	744.725
24)	Chlordane-2	5.249	4.351	89948629	42392307	743.517	748.609
25)	Chlordane-3	5.962	4.983	365.9E6	128.9E6	748.094	750.126
26)	Chlordane-4	6.045	5.046	441.0E6	122.5E6	746.906	746.147
27)	Chlordane-5	6.897	5.944	74802001	45591991	744.652	745.683



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031423\
Data File : PD074198.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2023 17:10
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 04:28:02 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031423.M
Quant Title : GC Extractables
QLast Update : Wed Mar 15 04:27:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

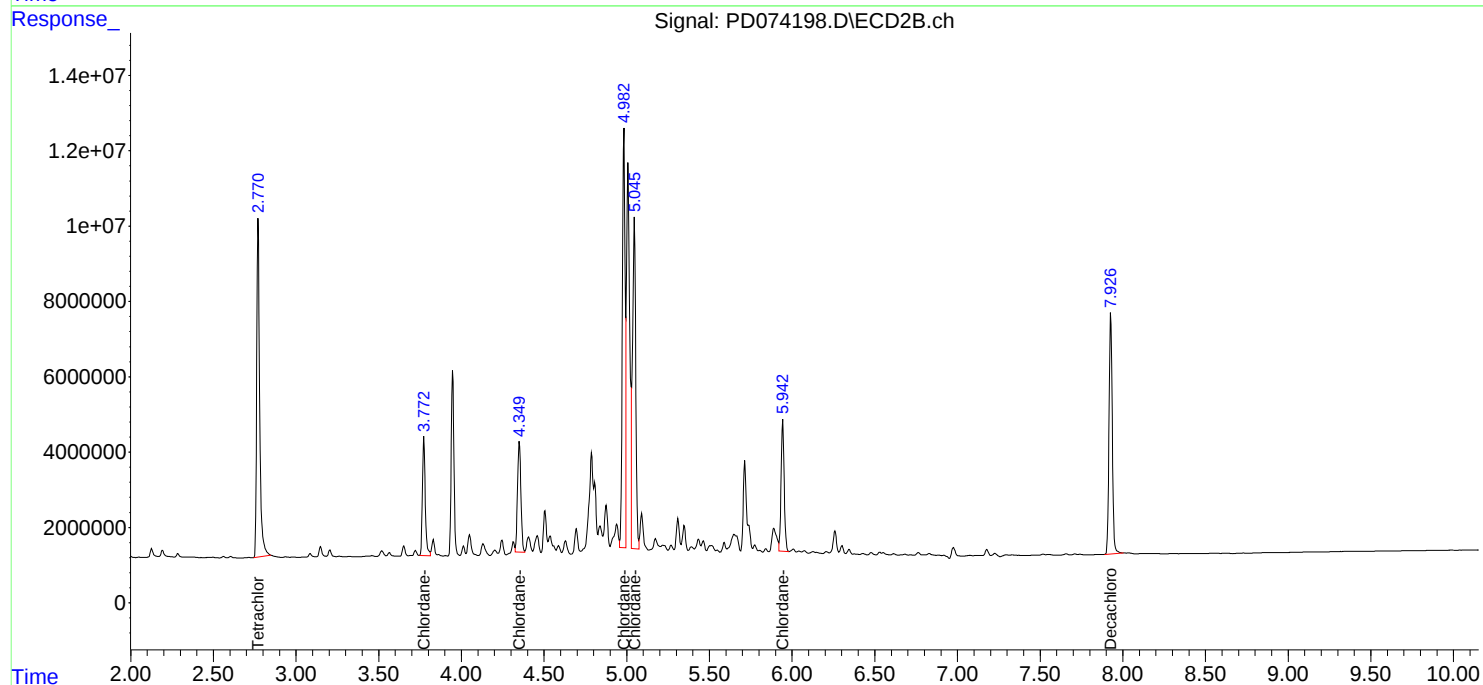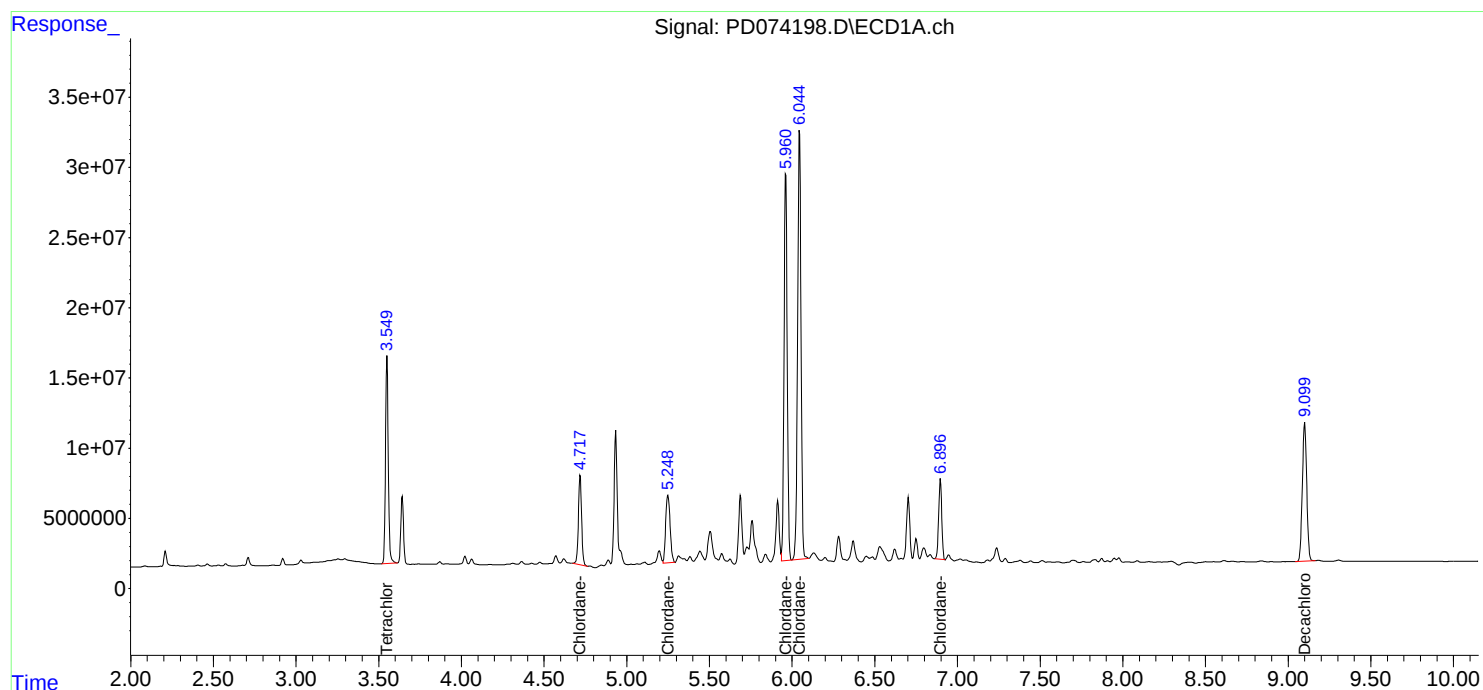


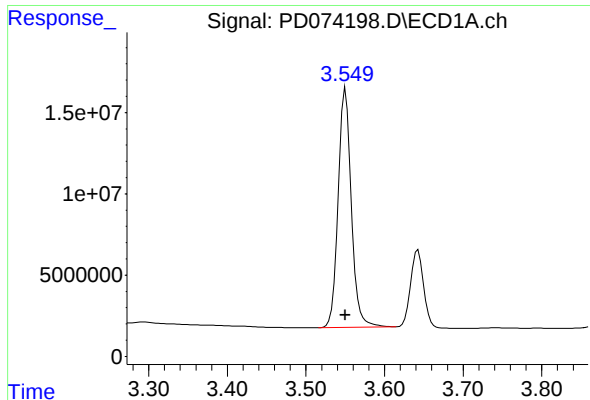

#1 Tetrachloro-m-xylene


R.T.: 3.550 min
Delta R.T.: 0.000 min
Response: 171170544
Conc: 74.47 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

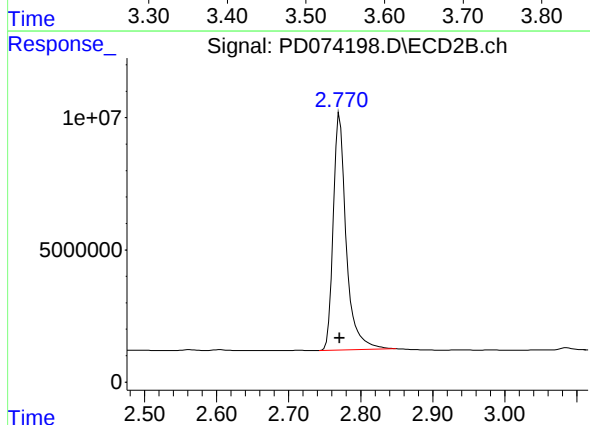


#1 Tetrachloro-m-xylene

R.T.: 2.771 min
Delta R.T.: 0.000 min
Response: 111092842
Conc: 74.43 ng/ml

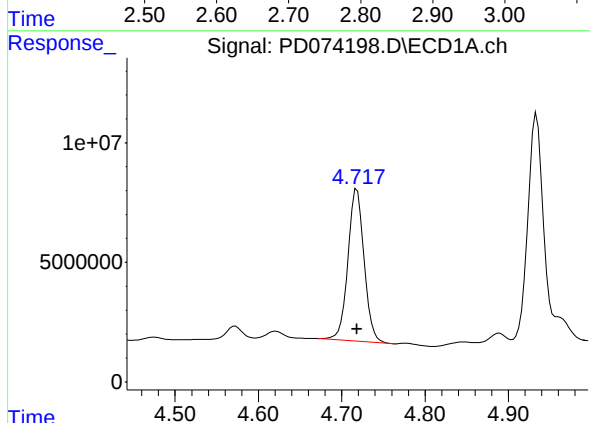


#23 Chlordane-1

R.T.: 4.718 min
Delta R.T.: 0.000 min
Response: 85641538
Conc: 744.43 ng/ml

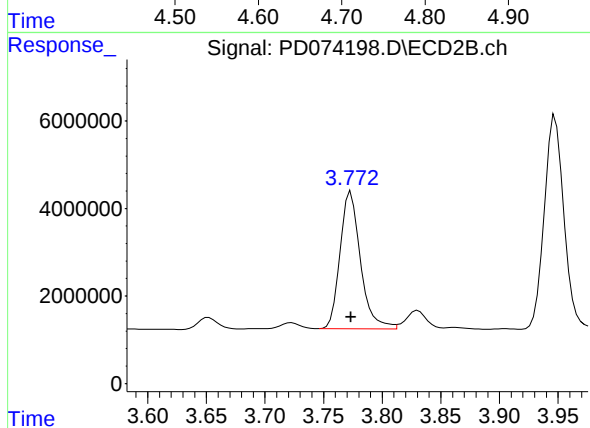

#23 Chlordane-1


R.T.: 3.773 min
Delta R.T.: 0.000 min
Response: 38027572
Conc: 744.72 ng/ml

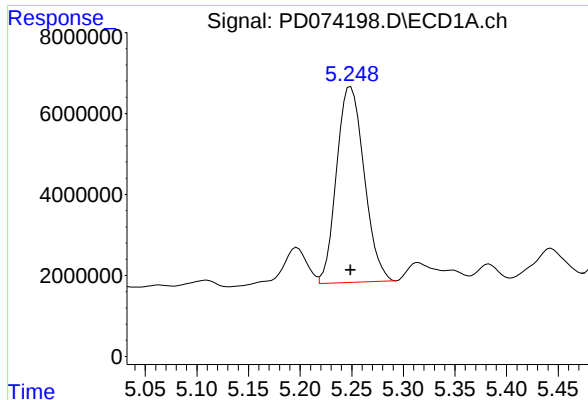

#24 Chlordane-2


R.T.: 5.249 min
Delta R.T.: 0.000 min
Response: 89948629
Conc: 743.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

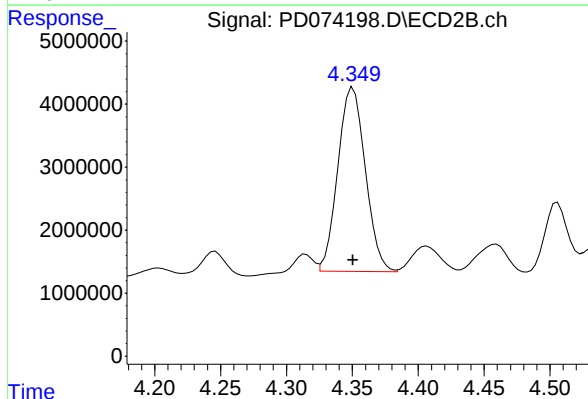


#24 Chlordane-2

R.T.: 4.351 min
Delta R.T.: 0.000 min
Response: 42392307
Conc: 748.61 ng/ml

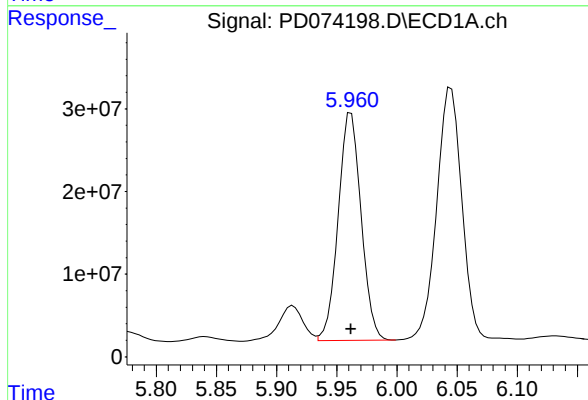


#25 Chlordane-3

R.T.: 5.962 min
Delta R.T.: 0.000 min
Response: 365901845
Conc: 748.09 ng/ml

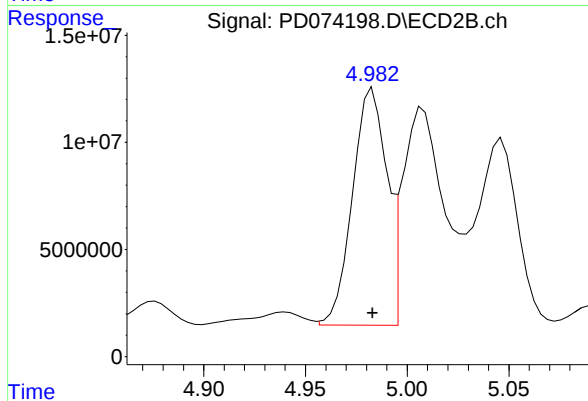

#25 Chlordane-3


R.T.: 4.983 min
Delta R.T.: 0.000 min
Response: 128948311
Conc: 750.13 ng/ml

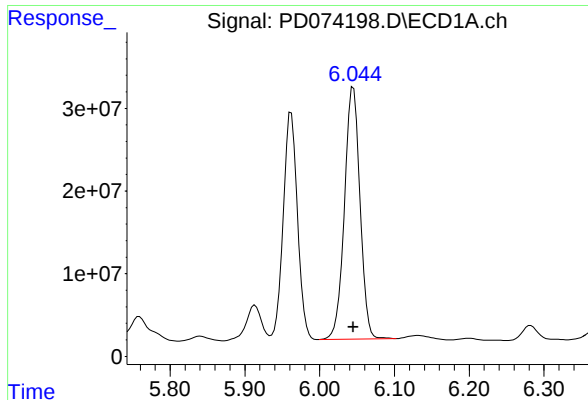

#26 Chlordane-4


R.T.: 6.045 min
Delta R.T.: 0.000 min
Response: 441009231
Conc: 746.91 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

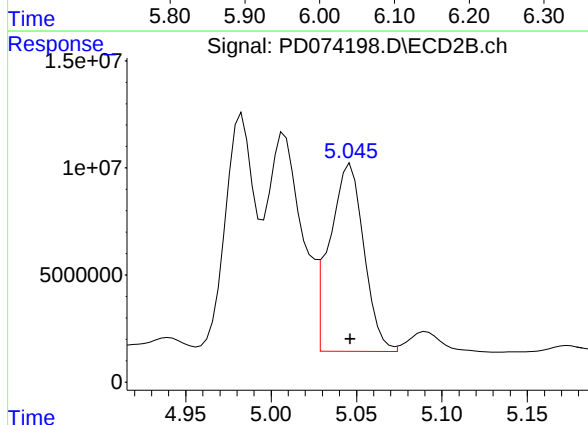


#26 Chlordane-4

R.T.: 5.046 min
Delta R.T.: 0.000 min
Response: 122485424
Conc: 746.15 ng/ml

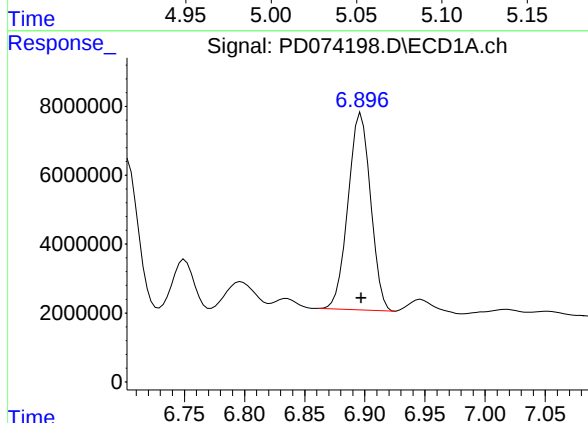


#27 Chlordane-5

R.T.: 6.897 min
Delta R.T.: 0.000 min
Response: 74802001
Conc: 744.65 ng/ml

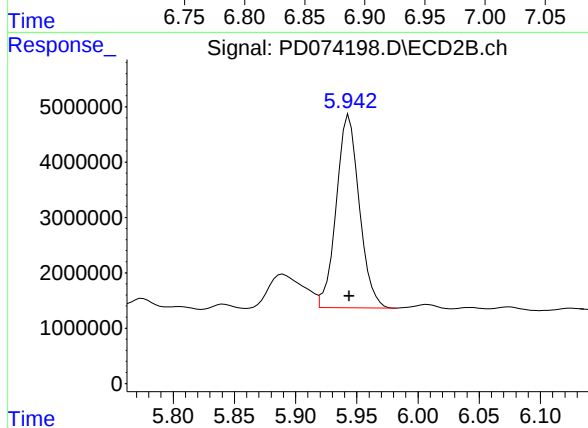

#27 Chlordane-5


R.T.: 5.944 min
Delta R.T.: 0.000 min
Response: 45591991
Conc: 745.68 ng/ml

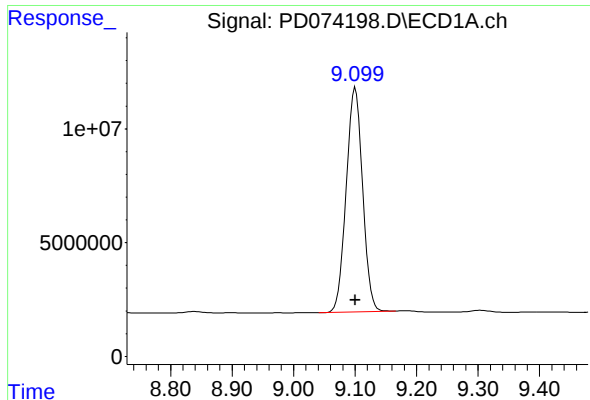

#28 Decachlorobiphenyl

R.T.: 9.100 min
Delta R.T.: 0.000 min
Response: 182291767
Conc: 74.23 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

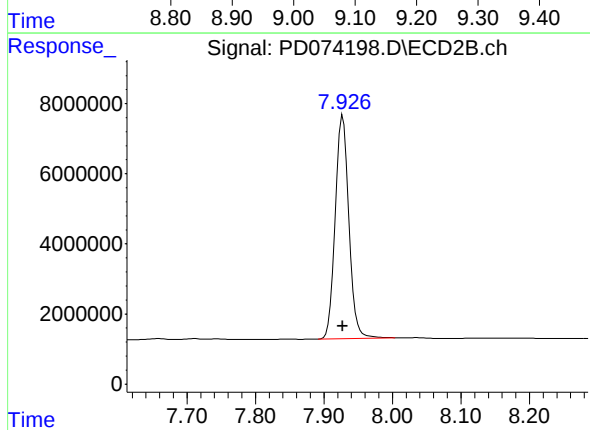

#28 Decachlorobiphenyl

R.T.: 7.927 min
Delta R.T.: 0.000 min
Response: 87983762
Conc: 74.36 ng/ml