

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031423\
 Data File : PD074199.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2023 17:23
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 04:12:55 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031423.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 15 04:06:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.551	2.771	115.5E6	75039362	50.000	50.000
28) SA Decachlor...	9.101	7.928	127.4E6	60809257	50.000	50.000
Target Compounds						
23) Chlordane-1	4.718	3.774	57887634	25647983	500.000	500.000
24) Chlordane-2	5.249	4.352	62390073	29049913	500.000	500.000
25) Chlordane-3	5.962	4.983	241.6E6	85519682	500.000	500.000
26) Chlordane-4	6.045	5.047	294.2E6	81649937	500.000	500.000
27) Chlordane-5	6.898	5.944	50592552	30785127	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031423\
Data File : PD074199.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2023 17:23
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 04:12:55 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031423.M
Quant Title : GC Extractables
QLast Update : Wed Mar 15 04:06:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

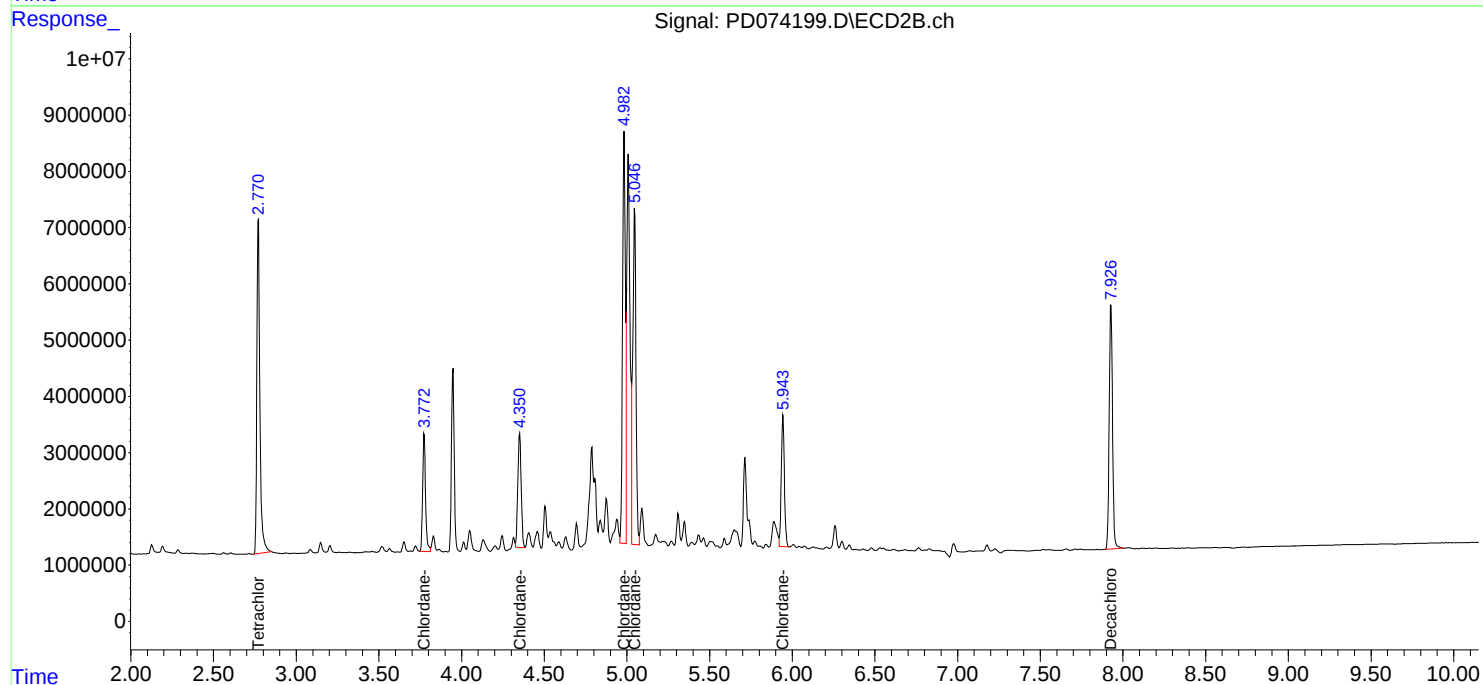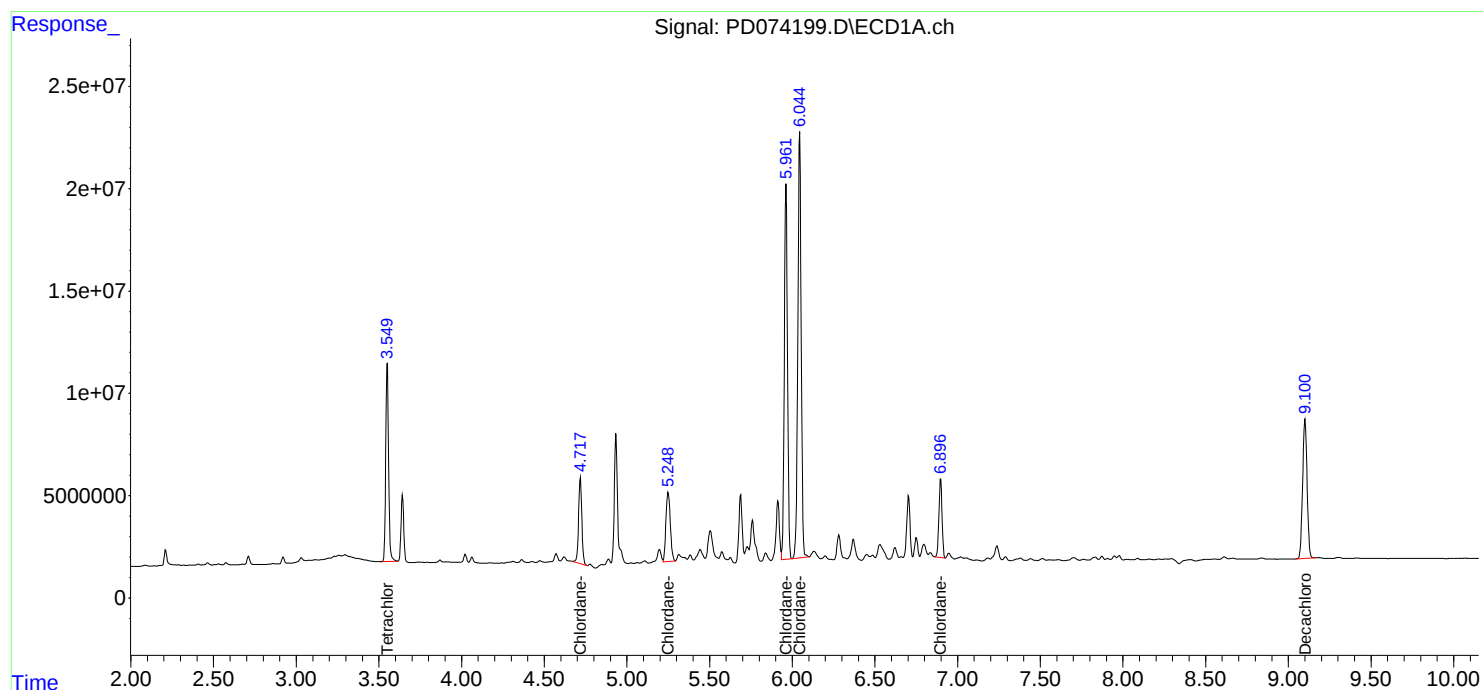


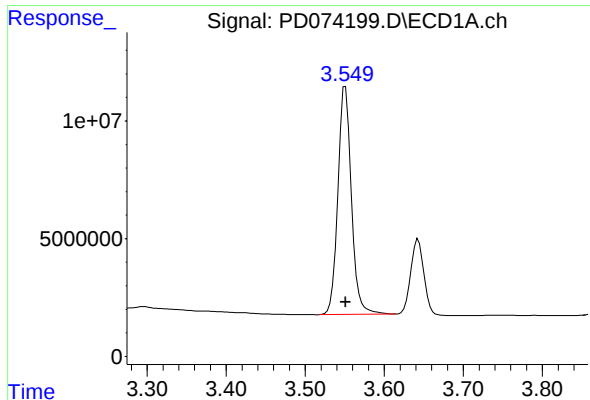

#1 Tetrachloro-m-xylene


R.T.: 3.551 min
Delta R.T.: 0.000 min
Response: 115485632
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

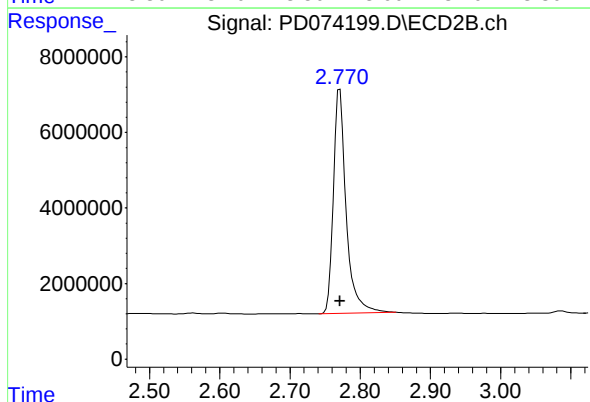


#1 Tetrachloro-m-xylene

R.T.: 2.771 min
Delta R.T.: 0.000 min
Response: 75039362
Conc: 50.00 ng/ml

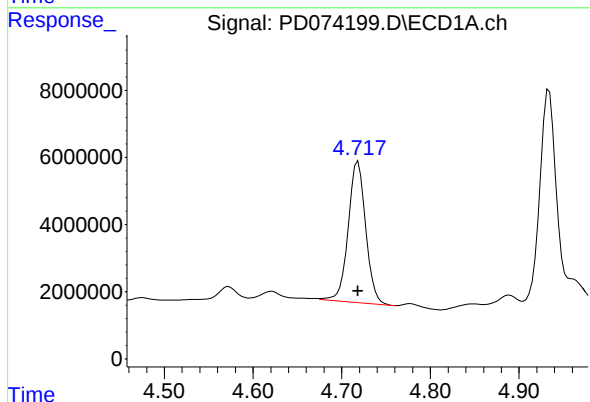


#23 Chlordane-1

R.T.: 4.718 min
Delta R.T.: 0.000 min
Response: 57887634
Conc: 500.00 ng/ml

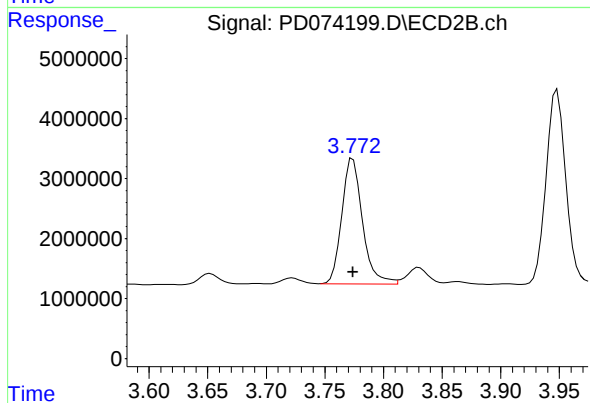

#23 Chlordane-1


R.T.: 3.774 min
Delta R.T.: 0.000 min
Response: 25647983
Conc: 500.00 ng/ml

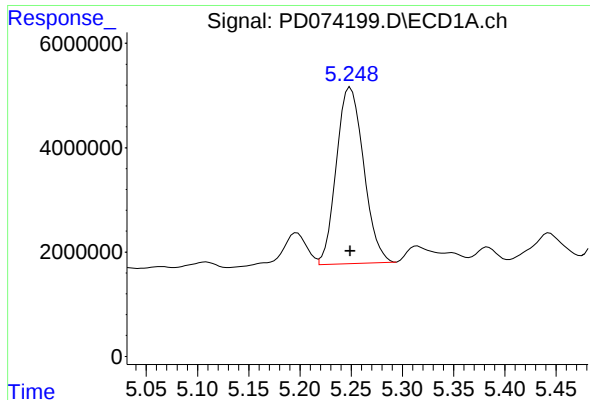

#24 Chlordane-2


R.T.: 5.249 min
Delta R.T.: 0.000 min
Response: 62390073
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

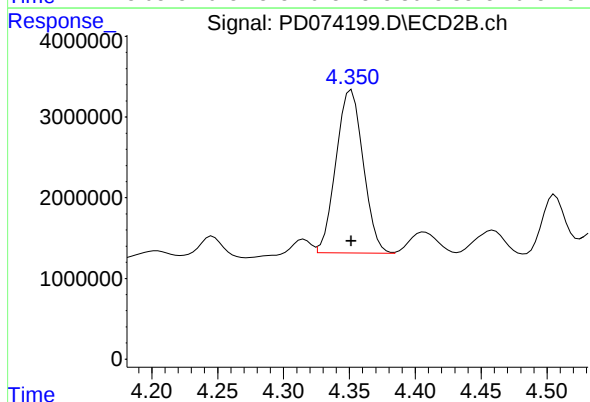


#24 Chlordane-2

R.T.: 4.352 min
Delta R.T.: 0.000 min
Response: 29049913
Conc: 500.00 ng/ml

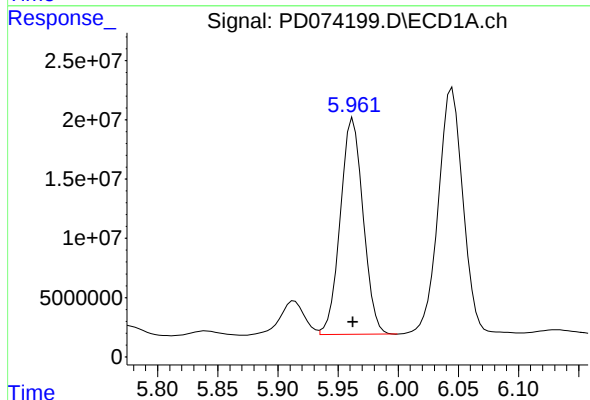


#25 Chlordane-3

R.T.: 5.962 min
Delta R.T.: 0.000 min
Response: 241592926
Conc: 500.00 ng/ml

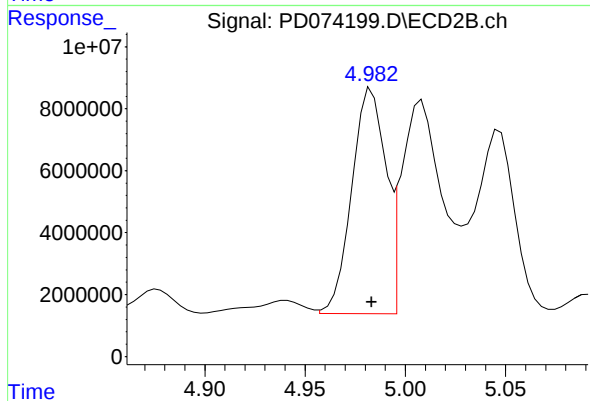

#25 Chlordane-3


R.T.: 4.983 min
Delta R.T.: 0.000 min
Response: 85519682
Conc: 500.00 ng/ml

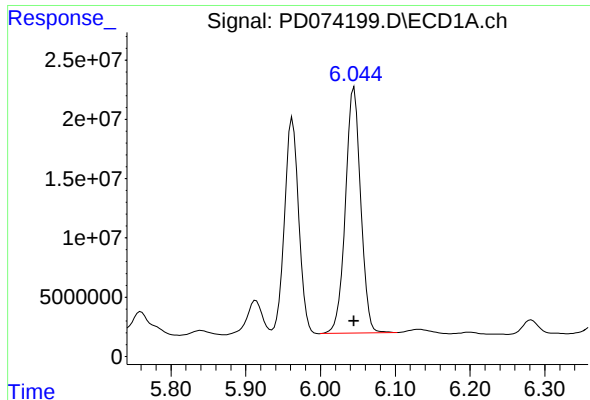

#26 Chlordane-4


R.T.: 6.045 min
Delta R.T.: 0.000 min
Response: 294216208
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

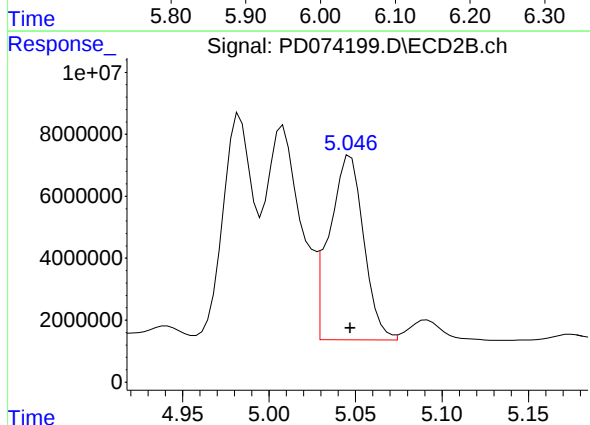


#26 Chlordane-4

R.T.: 5.047 min
Delta R.T.: 0.000 min
Response: 81649937
Conc: 500.00 ng/ml

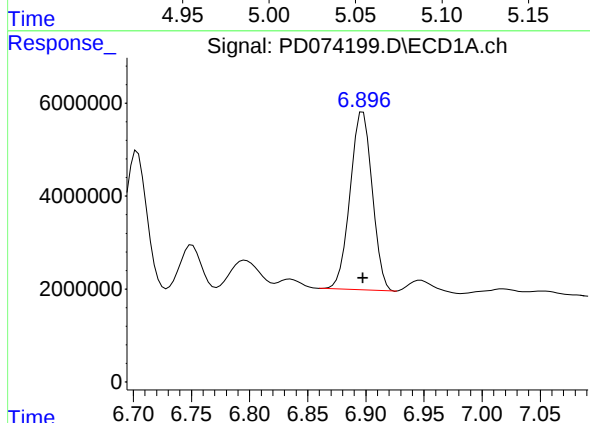


#27 Chlordane-5

R.T.: 6.898 min
Delta R.T.: 0.000 min
Response: 50592552
Conc: 500.00 ng/ml

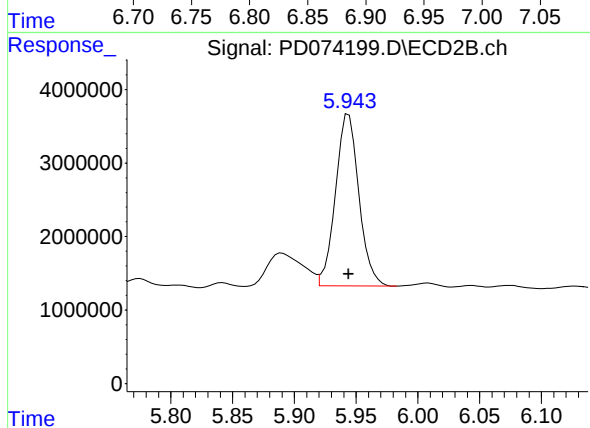

#27 Chlordane-5


R.T.: 5.944 min
Delta R.T.: 0.000 min
Response: 30785127
Conc: 500.00 ng/ml

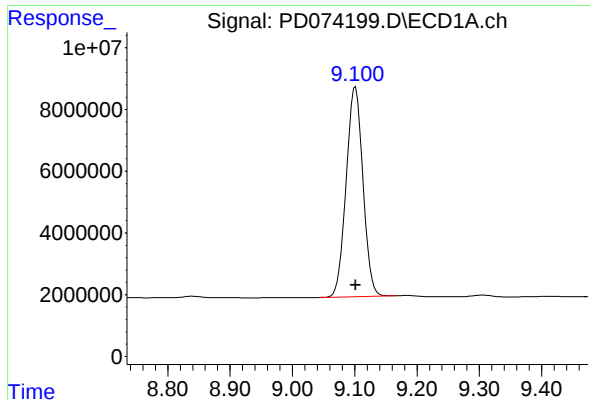

#28 Decachlorobiphenyl

R.T.: 9.101 min
Delta R.T.: 0.000 min
Response: 127432092
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

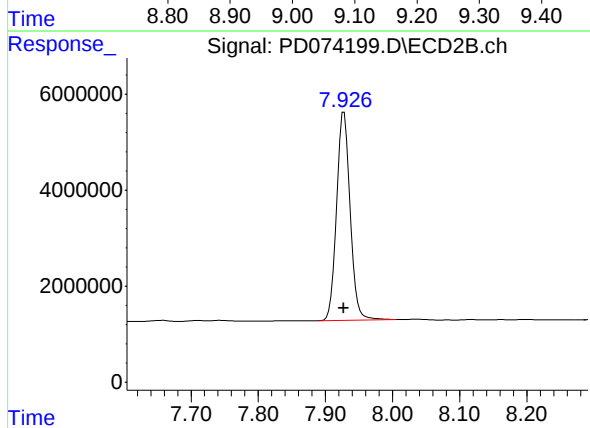

#28 Decachlorobiphenyl

R.T.: 7.928 min
Delta R.T.: 0.000 min
Response: 60809257
Conc: 50.00 ng/ml