

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031423\
 Data File : PD074200.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2023 17:37
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 04:31:41 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031423.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 15 04:31:34 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.551	2.771	56850223	36796104	13.839	13.824
28) SA Decachlor...	9.100	7.927	66924555	31352691	14.282	14.155
Target Compounds						
23) Chlordane-1	4.719	3.774	30472412	12703773	141.539	138.664
24) Chlordane-2	5.249	4.351	32281071	15124120	141.873	141.914
25) Chlordane-3	5.962	4.983	114.7E6	40901639	135.882	136.580
26) Chlordane-4	6.045	5.047	141.7E6	39528113	136.998	137.141
27) Chlordane-5	6.897	5.943	25169933	15301669	138.994	138.938



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031423\
Data File : PD074200.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2023 17:37
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 04:31:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031423.M
Quant Title : GC Extractables
QLast Update : Wed Mar 15 04:31:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

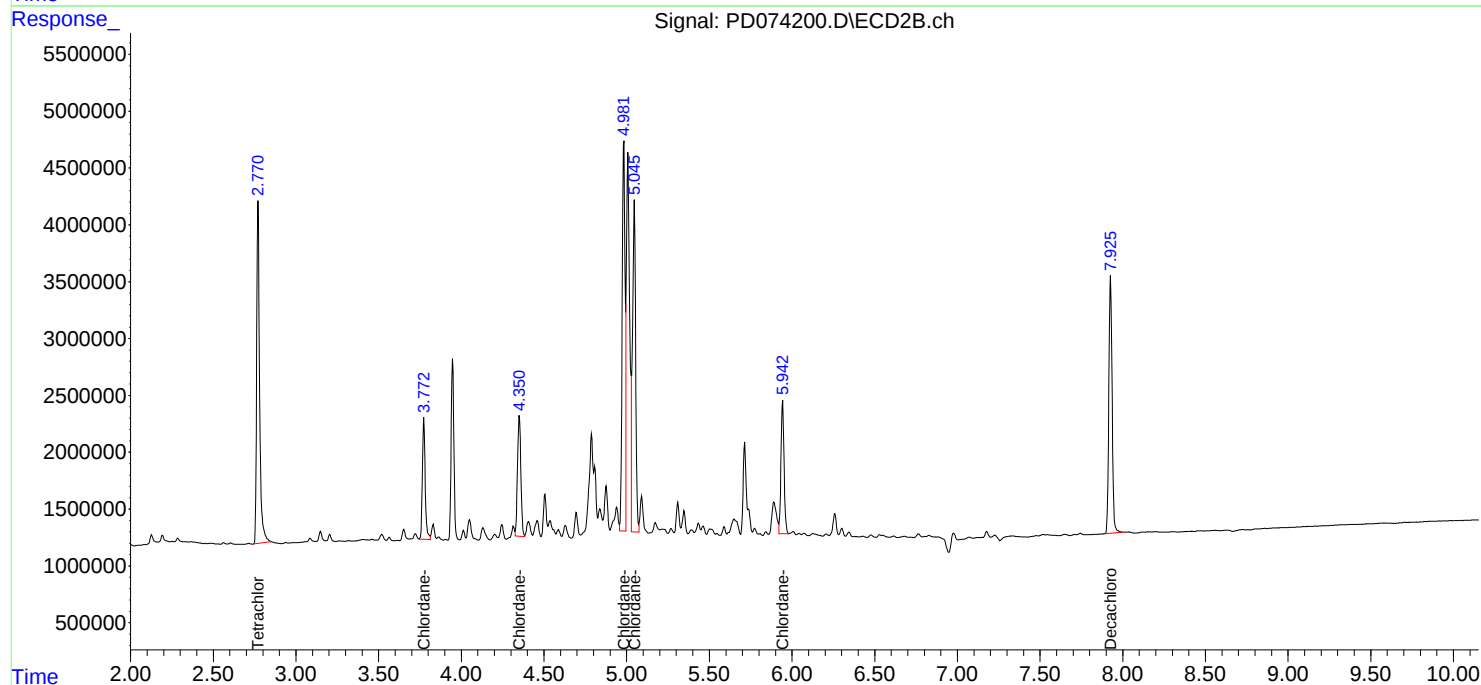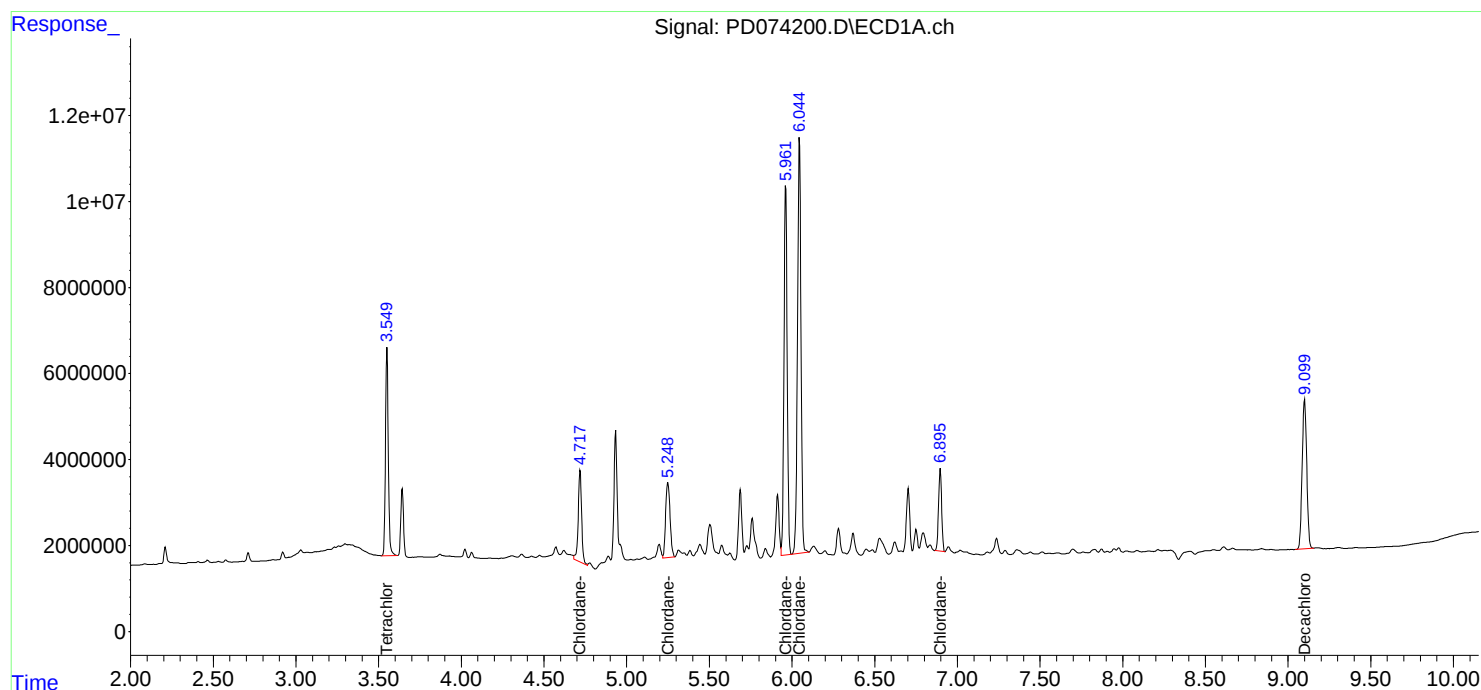


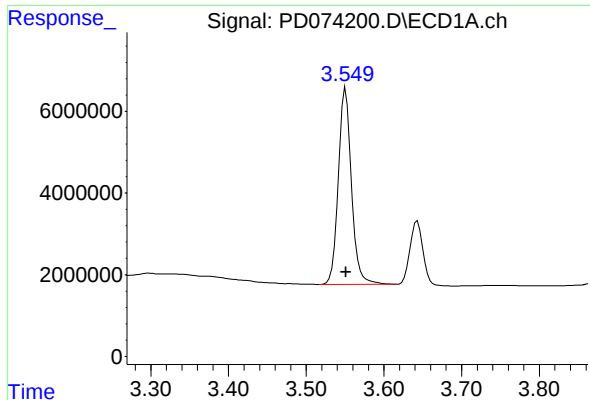

#1 Tetrachloro-m-xylene


R.T.: 3.551 min
Delta R.T.: 0.000 min
Response: 56850223
Conc: 13.84 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

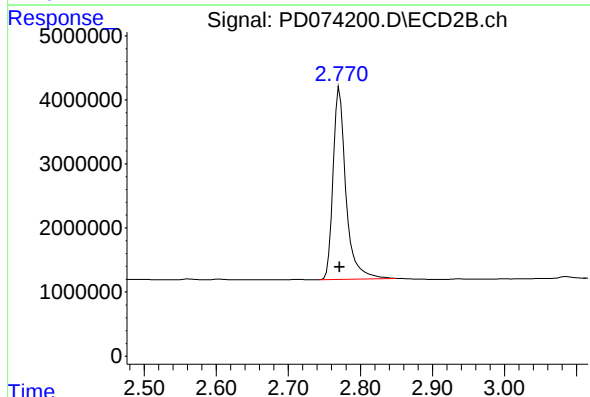


#1 Tetrachloro-m-xylene

R.T.: 2.771 min
Delta R.T.: 0.000 min
Response: 36796104
Conc: 13.82 ng/ml

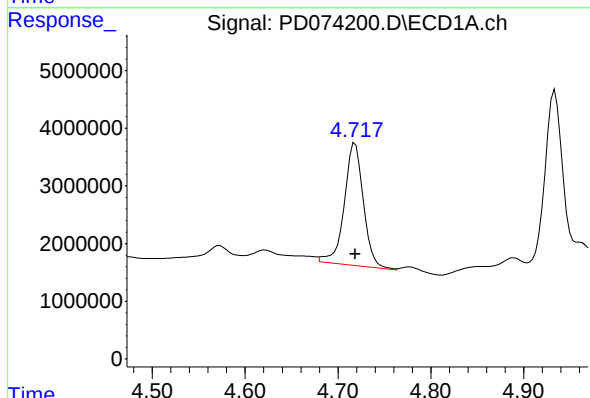


#23 Chlordane-1

R.T.: 4.719 min
Delta R.T.: 0.000 min
Response: 30472412
Conc: 141.54 ng/ml

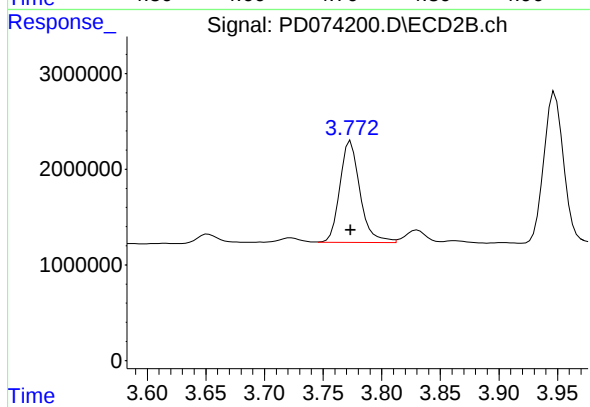

#23 Chlordane-1


R.T.: 3.774 min
Delta R.T.: 0.000 min
Response: 12703773
Conc: 138.66 ng/ml

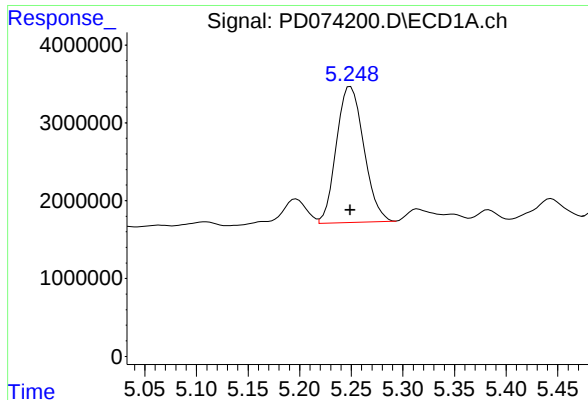

#24 Chlordane-2


R.T.: 5.249 min
Delta R.T.: 0.000 min
Response: 32281071
Conc: 141.87 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

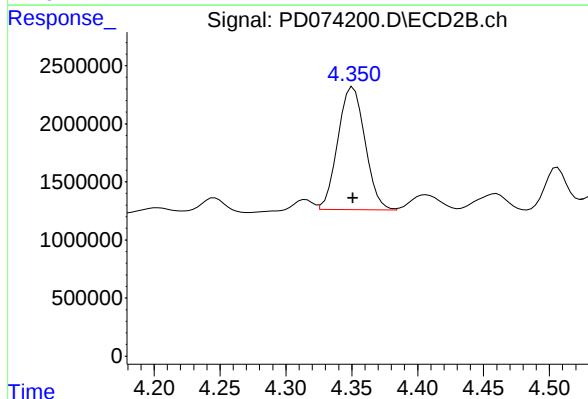


#24 Chlordane-2

R.T.: 4.351 min
Delta R.T.: 0.000 min
Response: 15124120
Conc: 141.91 ng/ml

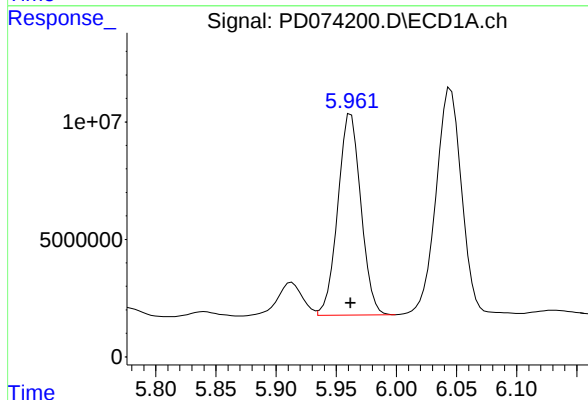


#25 Chlordane-3

R.T.: 5.962 min
Delta R.T.: 0.000 min
Response: 114665110
Conc: 135.88 ng/ml

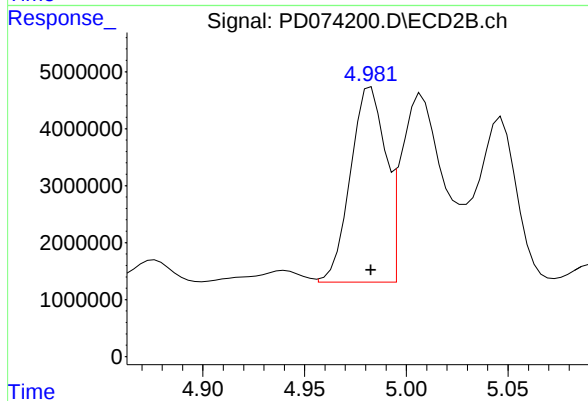

#25 Chlordane-3


R.T.: 4.983 min
Delta R.T.: 0.000 min
Response: 40901639
Conc: 136.58 ng/ml

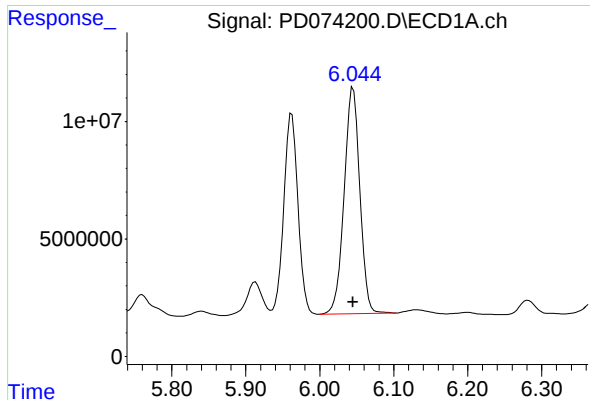

#26 Chlordane-4


R.T.: 6.045 min
Delta R.T.: 0.000 min
Response: 141743022
Conc: 137.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

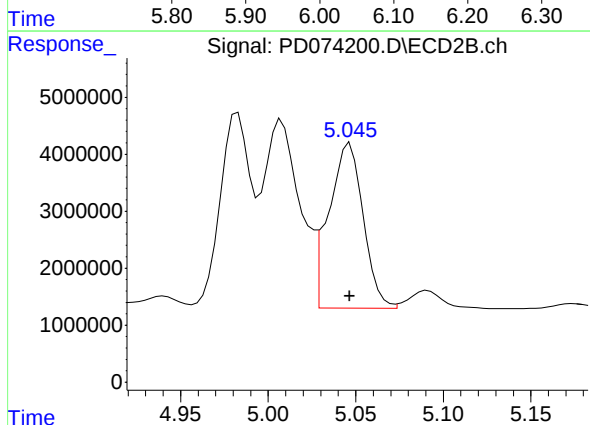


#26 Chlordane-4

R.T.: 5.047 min
Delta R.T.: 0.000 min
Response: 39528113
Conc: 137.14 ng/ml

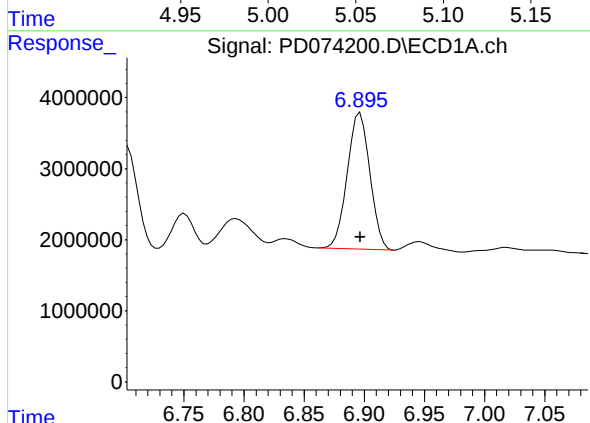


#27 Chlordane-5

R.T.: 6.897 min
Delta R.T.: 0.000 min
Response: 25169933
Conc: 138.99 ng/ml

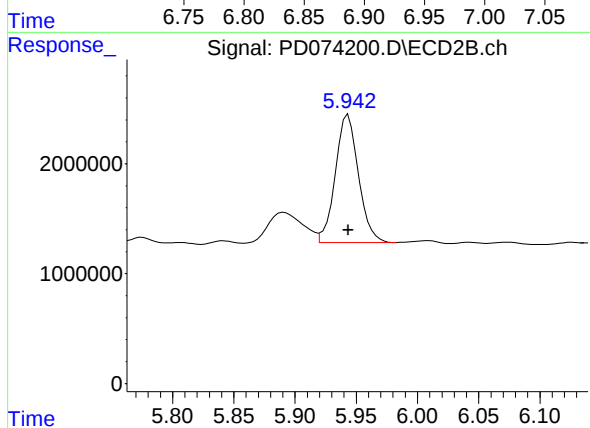

#27 Chlordane-5


R.T.: 5.943 min
Delta R.T.: 0.000 min
Response: 15301669
Conc: 138.94 ng/ml

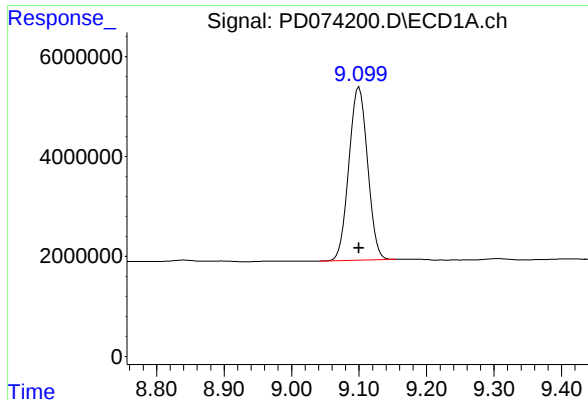

#28 Decachlorobiphenyl

R.T.: 9.100 min
Delta R.T.: 0.000 min
Response: 66924555
Conc: 14.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

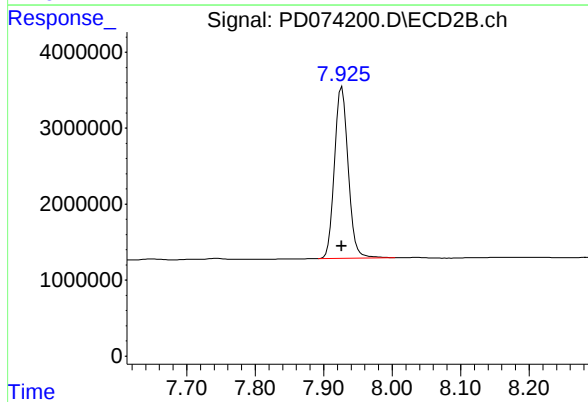

#28 Decachlorobiphenyl

R.T.: 7.927 min
Delta R.T.: 0.000 min
Response: 31352691
Conc: 14.16 ng/ml