

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031423\
 Data File : PD074201.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2023 17:50
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 04:33:18 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031423.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 15 04:33:09 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.550	2.771	11760675	7341496	5.104	4.948
28) SA Decachlor...	9.100	7.928	15484955	7240408	5.892	5.790
Target Compounds						
23) Chlordane-1	4.716	3.774	6065043	2615343	52.051m	51.019
24) Chlordane-2	5.249	4.352	7167618	3154959	56.402	53.751
25) Chlordane-3	5.962	4.983	22315689	8193196	47.034	48.585
26) Chlordane-4	6.045	5.046	28233802	8034194	48.629	49.516
27) Chlordane-5	6.897	5.944	4931405	3171840	49.249	51.480



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031423\
Data File : PD074201.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2023 17:50
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 04:33:18 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031423.M
Quant Title : GC Extractables
QLast Update : Wed Mar 15 04:33:09 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

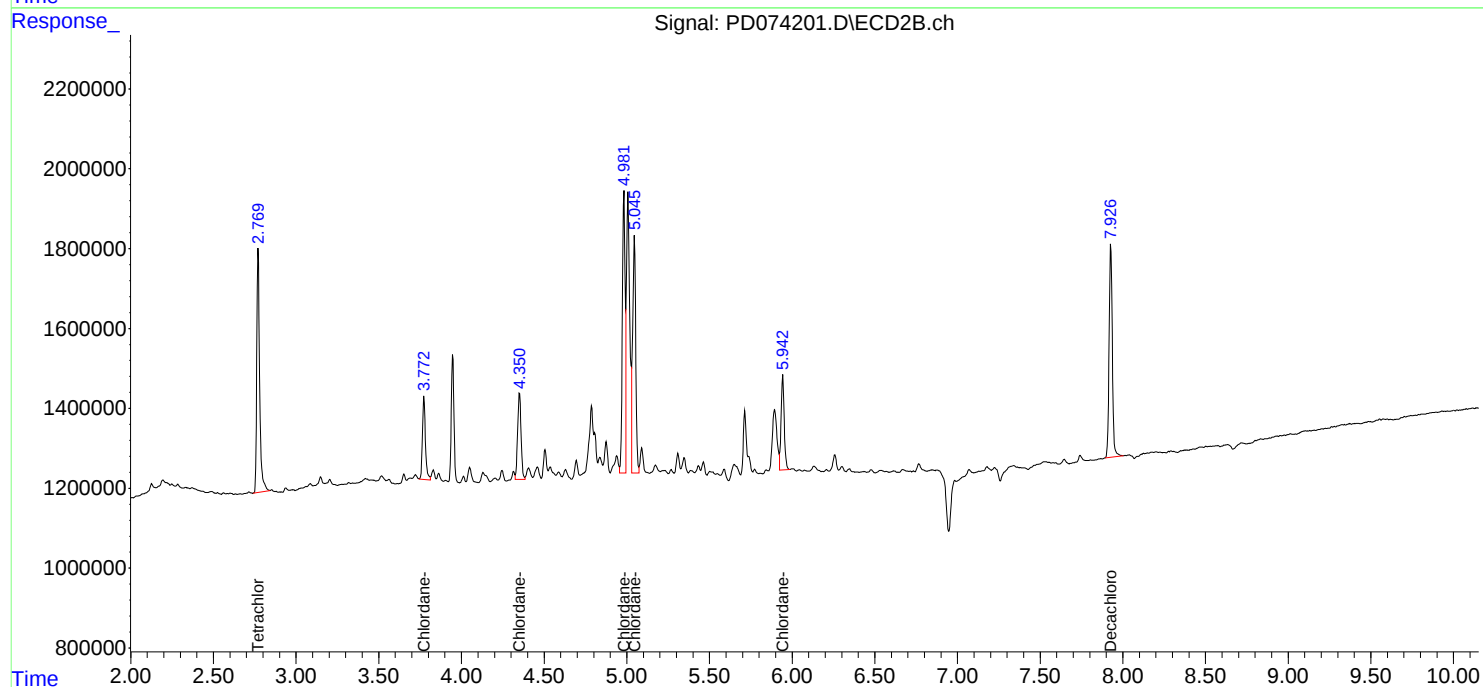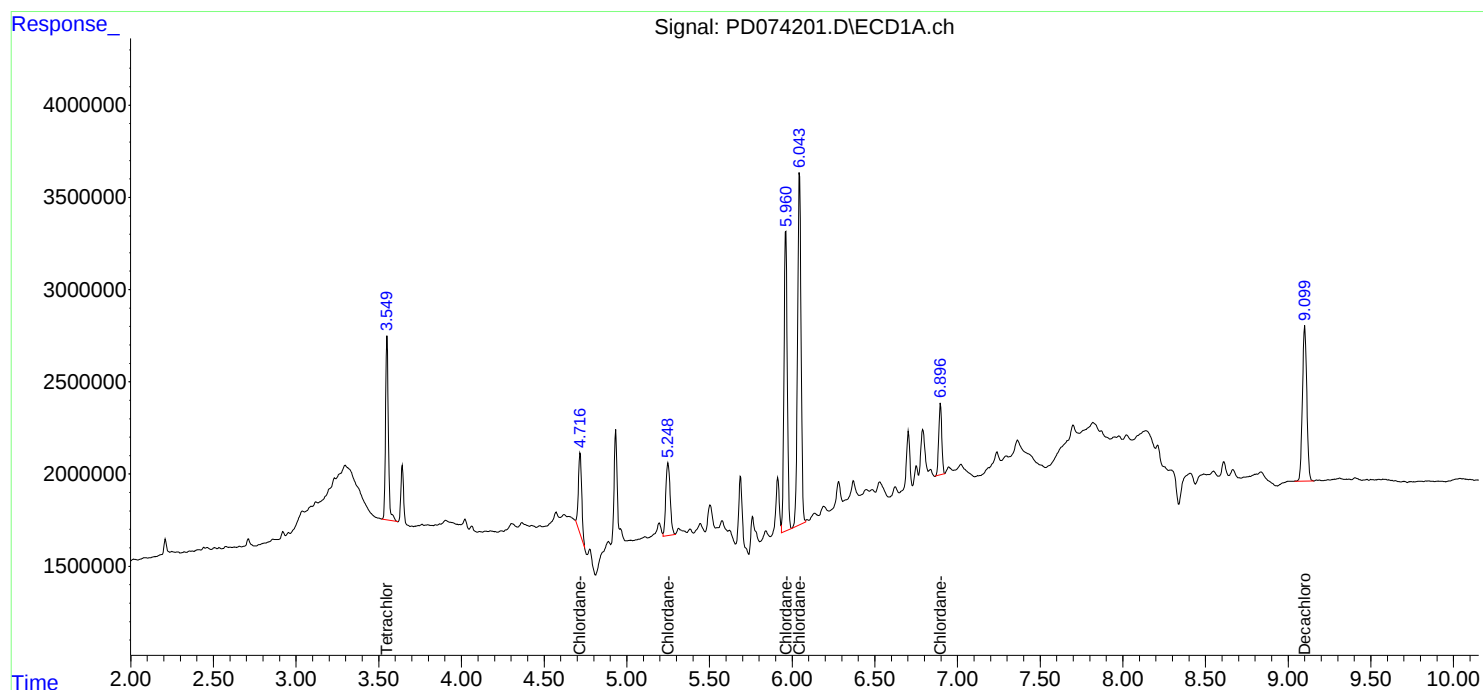


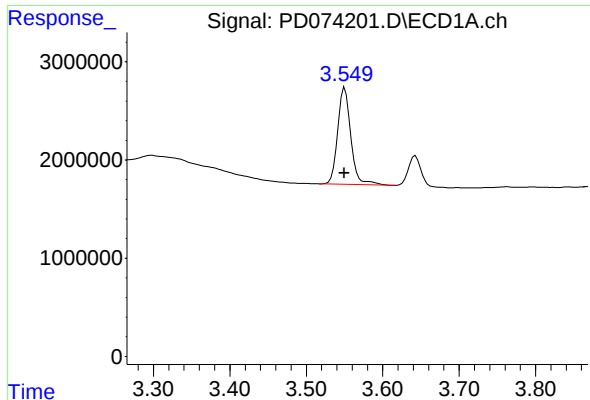

#1 Tetrachloro-m-xylene


R.T.: 3.550 min
Delta R.T.: 0.000 min
Response: 11760675
Conc: 5.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

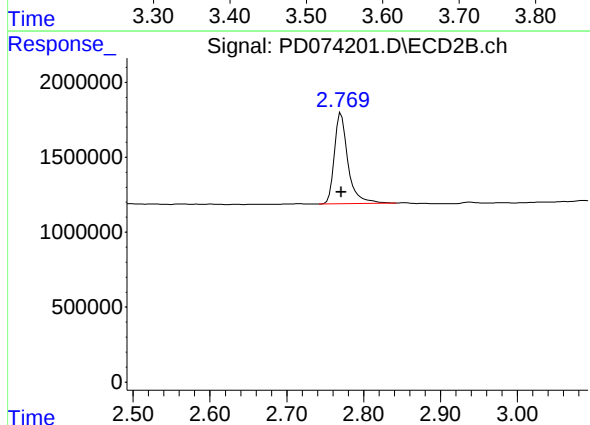


#1 Tetrachloro-m-xylene

R.T.: 2.771 min
Delta R.T.: 0.000 min
Response: 7341496
Conc: 4.95 ng/ml

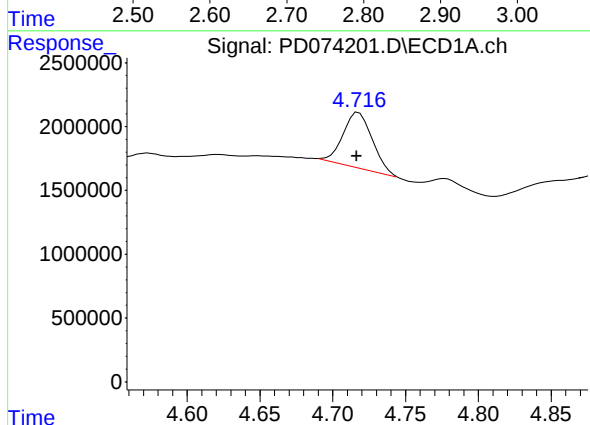


#23 Chlordane-1

R.T.: 4.716 min
Delta R.T.: 0.000 min
Response: 6065043
Conc: 52.05 ng/ml m

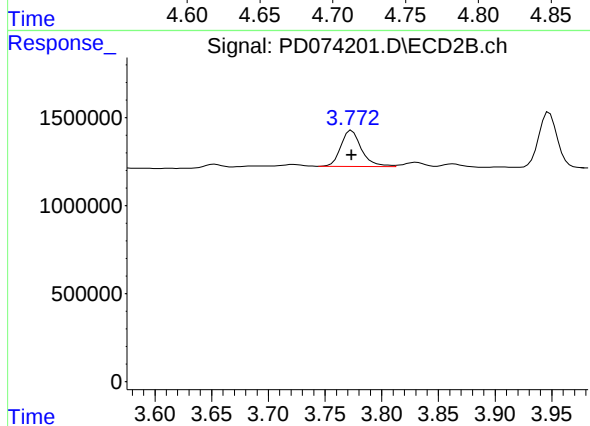

#23 Chlordane-1


R.T.: 3.774 min
Delta R.T.: 0.000 min
Response: 2615343
Conc: 51.02 ng/ml

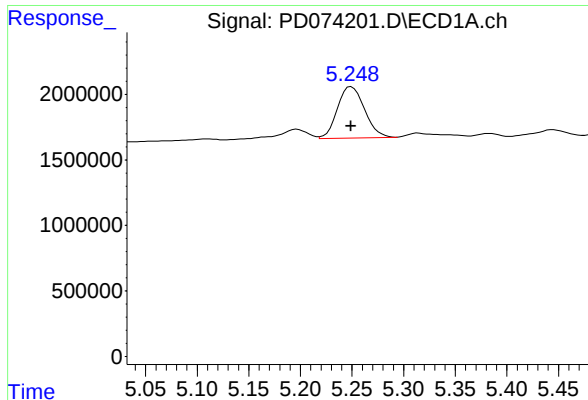

#24 Chlordane-2


R.T.: 5.249 min
Delta R.T.: 0.000 min
Response: 7167618
Conc: 56.40 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

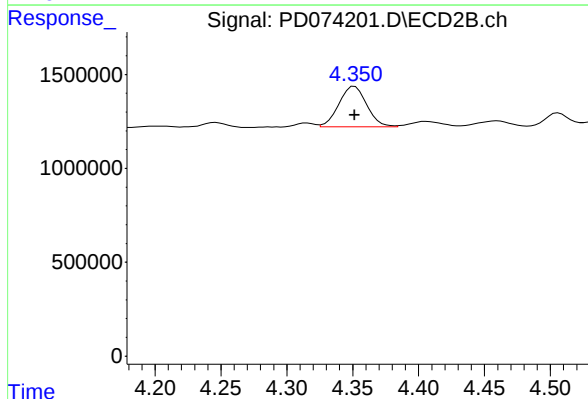


#24 Chlordane-2

R.T.: 4.352 min
Delta R.T.: 0.000 min
Response: 3154959
Conc: 53.75 ng/ml

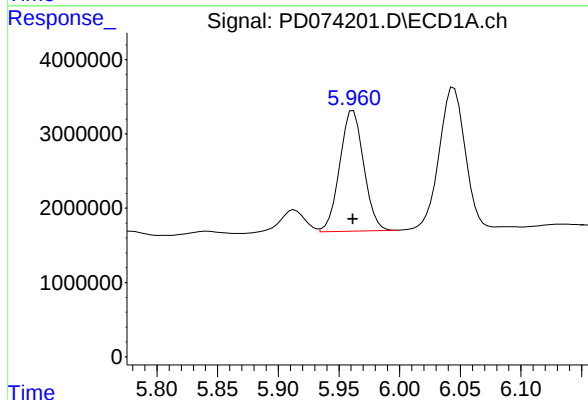


#25 Chlordane-3

R.T.: 5.962 min
Delta R.T.: 0.000 min
Response: 22315689
Conc: 47.03 ng/ml

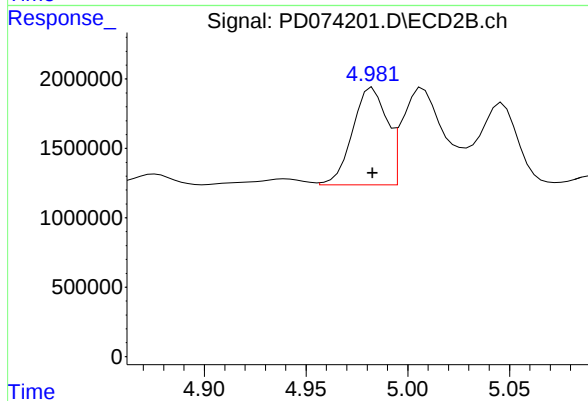

#25 Chlordane-3


R.T.: 4.983 min
Delta R.T.: 0.000 min
Response: 8193196
Conc: 48.59 ng/ml

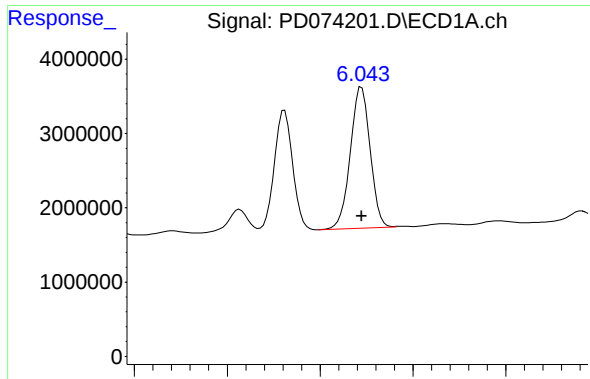

#26 Chlordane-4


R.T.: 6.045 min
Delta R.T.: 0.000 min
Response: 28233802
Conc: 48.63 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

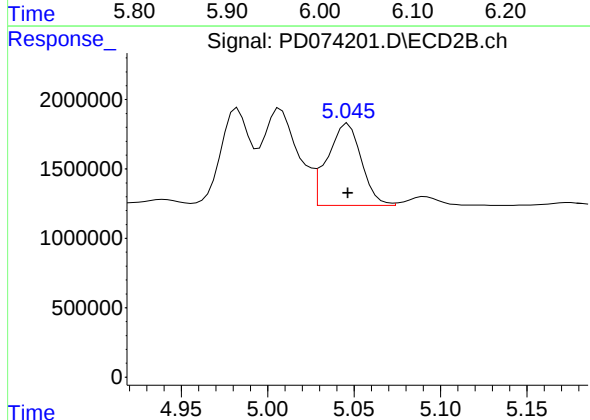


#26 Chlordane-4

R.T.: 5.046 min
Delta R.T.: 0.000 min
Response: 8034194
Conc: 49.52 ng/ml

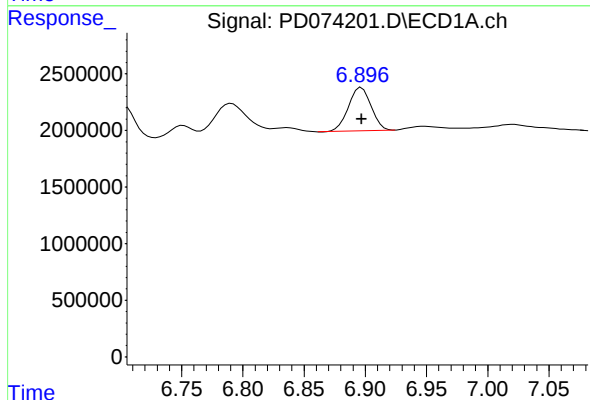


#27 Chlordane-5

R.T.: 6.897 min
Delta R.T.: 0.000 min
Response: 4931405
Conc: 49.25 ng/ml

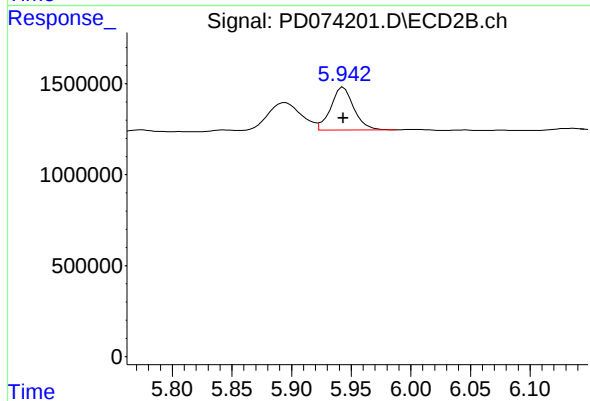

#27 Chlordane-5


R.T.: 5.944 min
Delta R.T.: 0.000 min
Response: 3171840
Conc: 51.48 ng/ml

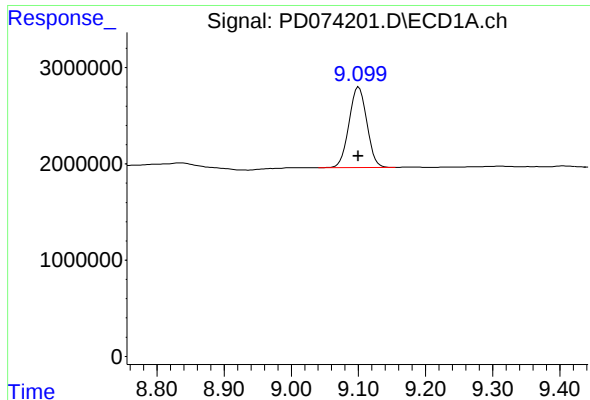

#28 Decachlorobiphenyl

R.T.: 9.100 min
Delta R.T.: 0.000 min
Response: 15484955
Conc: 5.89 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

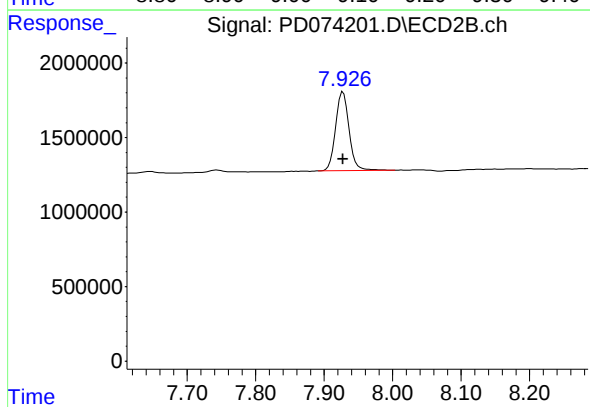

#28 Decachlorobiphenyl

R.T.: 7.928 min
Delta R.T.: 0.000 min
Response: 7240408
Conc: 5.79 ng/ml