

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031423\
 Data File : PD074208.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2023 19:51
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD031423CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 04:35:16 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031423.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 15 04:34:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.550	2.770	114.1E6	74656696	49.497	50.321
28)	SA Decachlor...	9.100	7.927	123.7E6	59912251	47.060	47.914
Target Compounds							
23)	Chlordane-1	4.718	3.773	66894110	28480716	574.096	555.592
24)	Chlordane-2	5.248	4.350	70751648	32461184	556.742	553.039
25)	Chlordane-3	5.961	4.982	278.1E6	95576161	586.096	566.762
26)	Chlordane-4	6.044	5.046	336.3E6	91572553	579.308	564.379
27)	Chlordane-5	6.896	5.943	57189684	34542894	571.138	560.639



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031423\
Data File : PD074208.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2023 19:51
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD031423CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 04:35:16 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031423.M
Quant Title : GC Extractables
QLast Update : Wed Mar 15 04:34:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

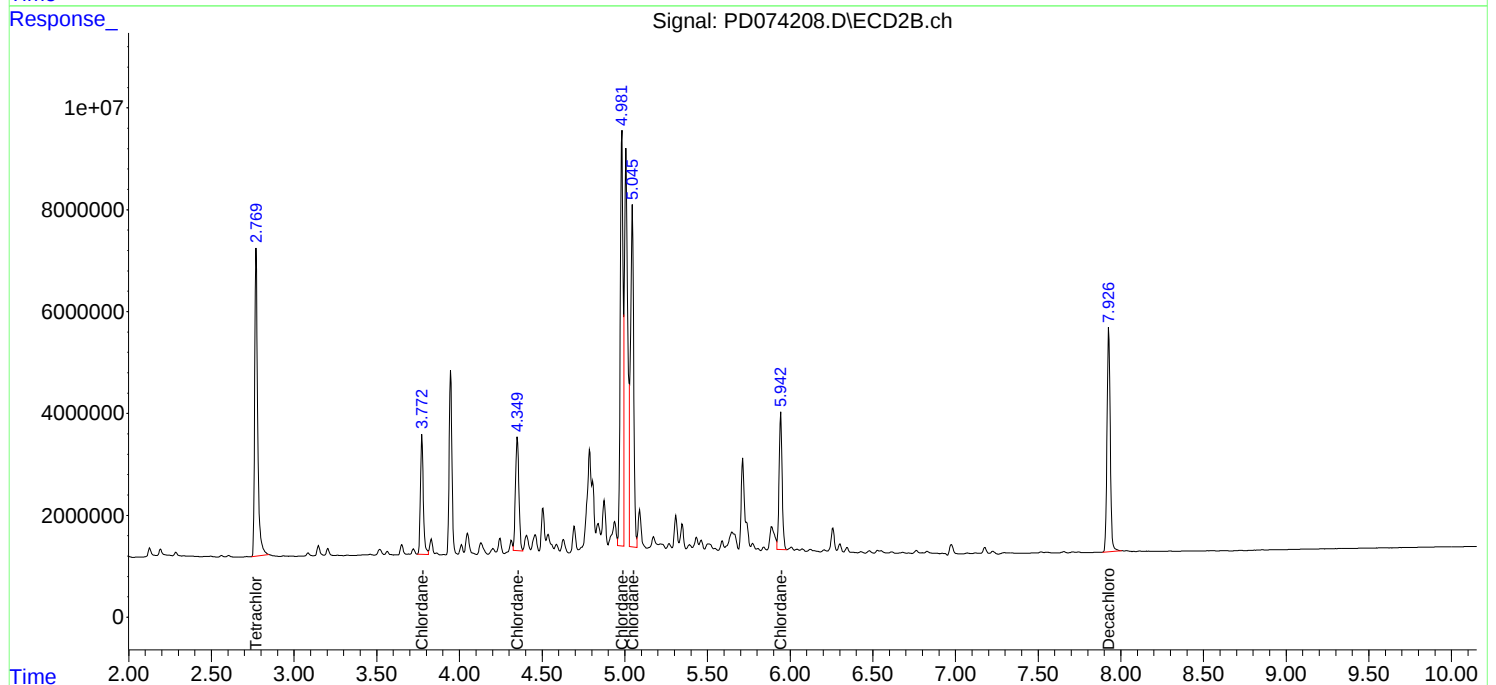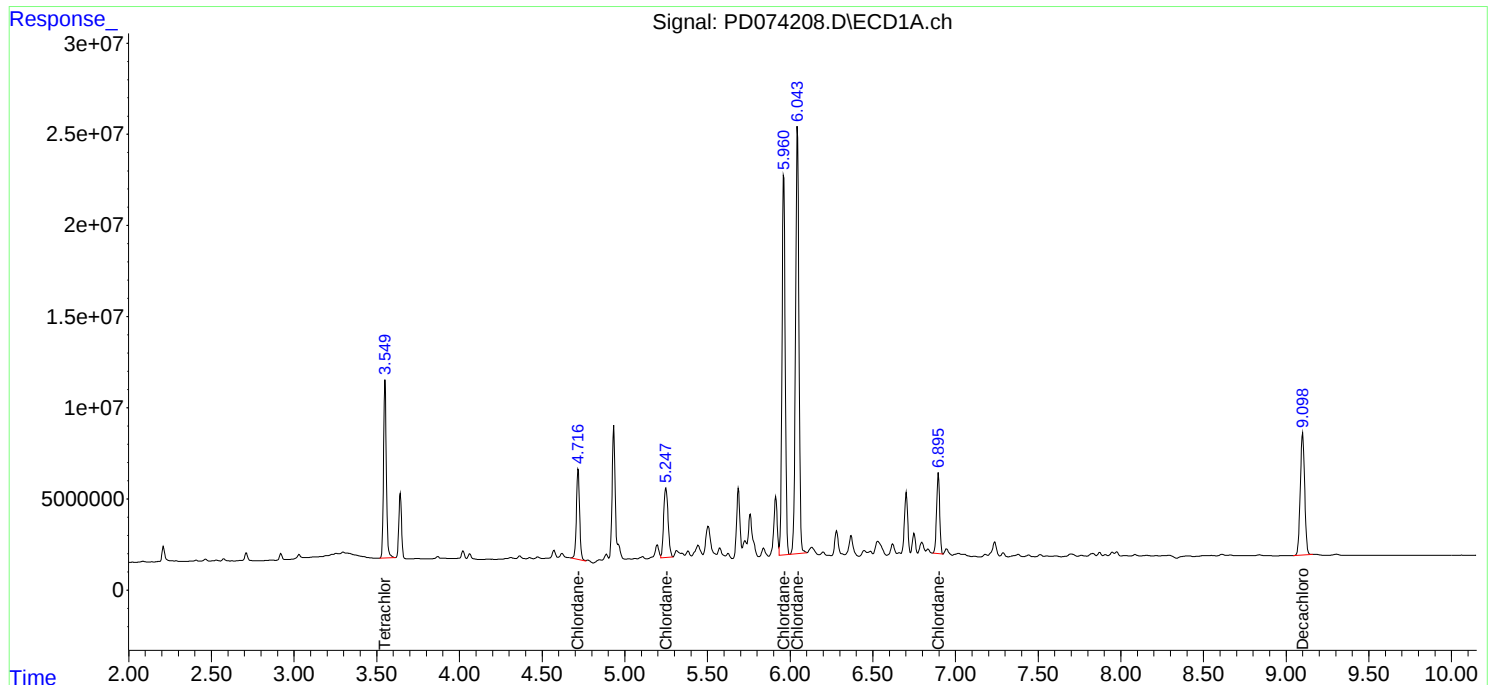


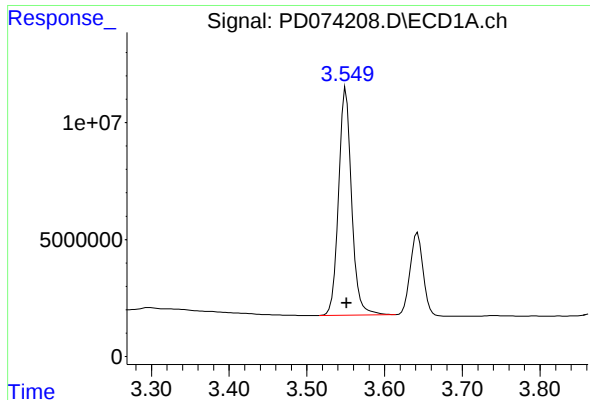

#1 Tetrachloro-m-xylene


R.T.: 3.550 min
Delta R.T.: 0.000 min
Response: 114057167
Conc: 49.50 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD031423CHLOR

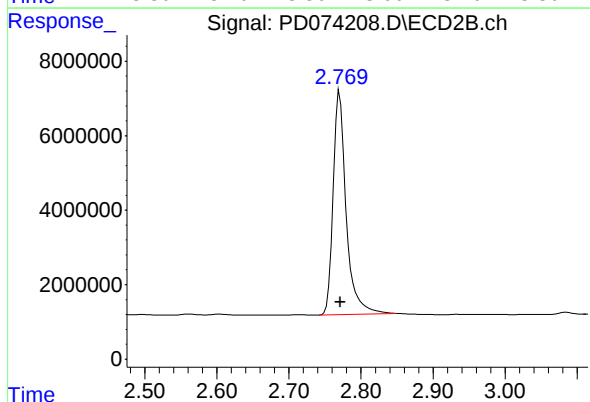


#1 Tetrachloro-m-xylene

R.T.: 2.770 min
Delta R.T.: 0.000 min
Response: 74656696
Conc: 50.32 ng/ml

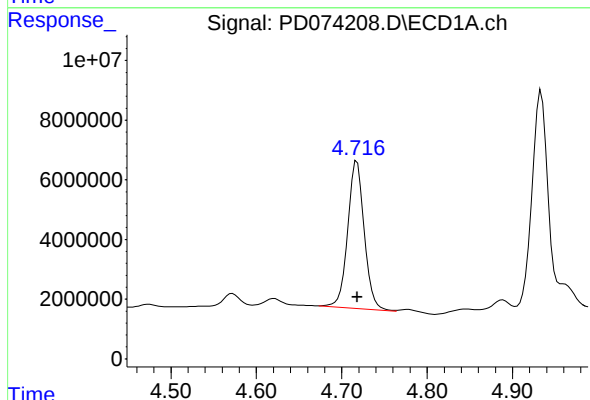


#23 Chlordane-1

R.T.: 4.718 min
Delta R.T.: 0.000 min
Response: 66894110
Conc: 574.10 ng/ml

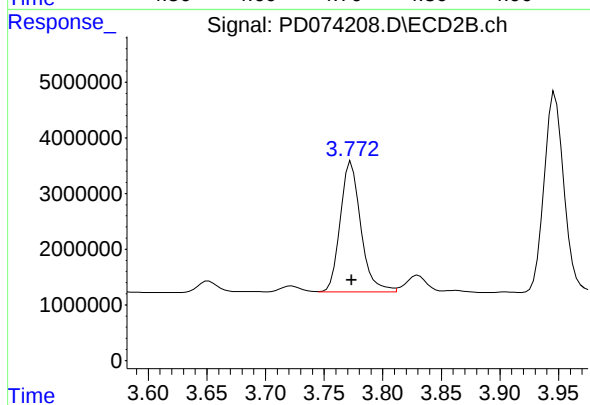

#23 Chlordane-1


R.T.: 3.773 min
Delta R.T.: 0.000 min
Response: 28480716
Conc: 555.59 ng/ml

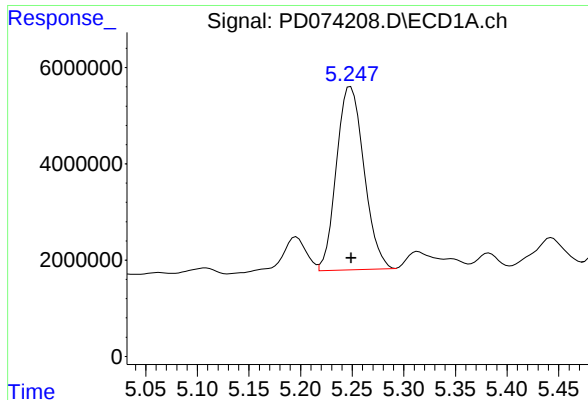

#24 Chlordane-2


R.T.: 5.248 min
Delta R.T.: 0.000 min
Response: 70751648
Conc: 556.74 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD031423CHLOR

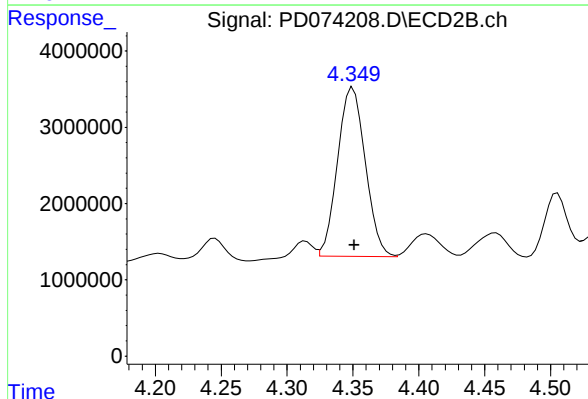


#24 Chlordane-2

R.T.: 4.350 min
Delta R.T.: 0.000 min
Response: 32461184
Conc: 553.04 ng/ml

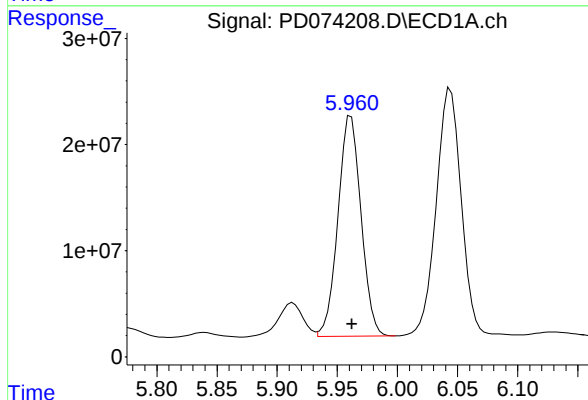


#25 Chlordane-3

R.T.: 5.961 min
Delta R.T.: 0.000 min
Response: 278080614
Conc: 586.10 ng/ml

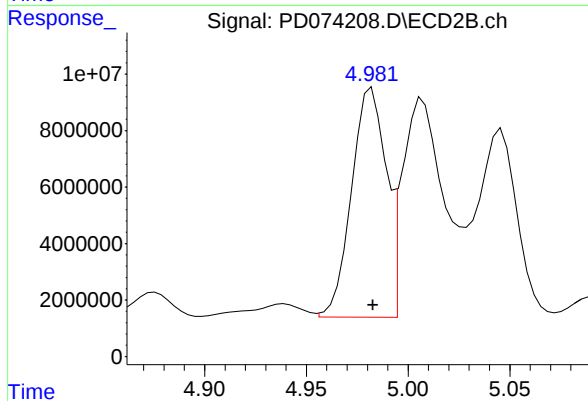

#25 Chlordane-3


R.T.: 4.982 min
Delta R.T.: 0.000 min
Response: 95576161
Conc: 566.76 ng/ml

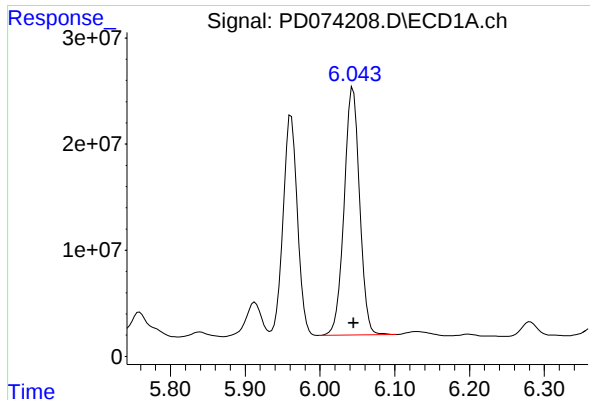

#26 Chlordane-4


R.T.: 6.044 min
Delta R.T.: -0.001 min
Response: 336345587
Conc: 579.31 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD031423CHLOR

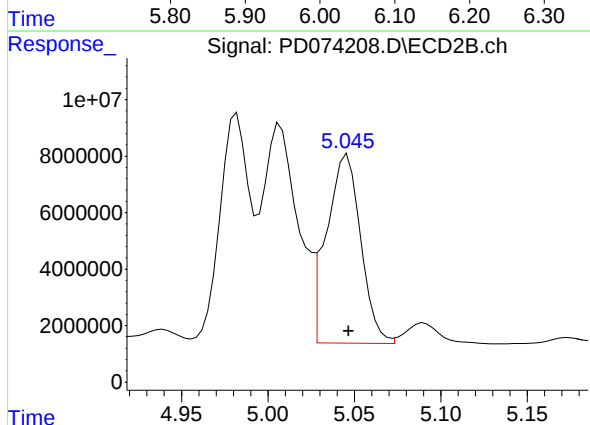


#26 Chlordane-4

R.T.: 5.046 min
Delta R.T.: 0.000 min
Response: 91572553
Conc: 564.38 ng/ml

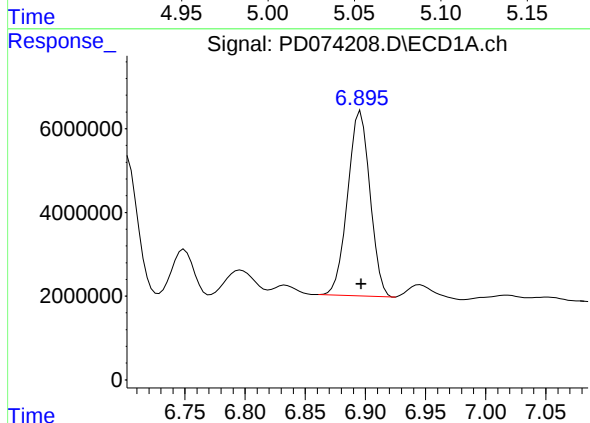


#27 Chlordane-5

R.T.: 6.896 min
Delta R.T.: 0.000 min
Response: 57189684
Conc: 571.14 ng/ml

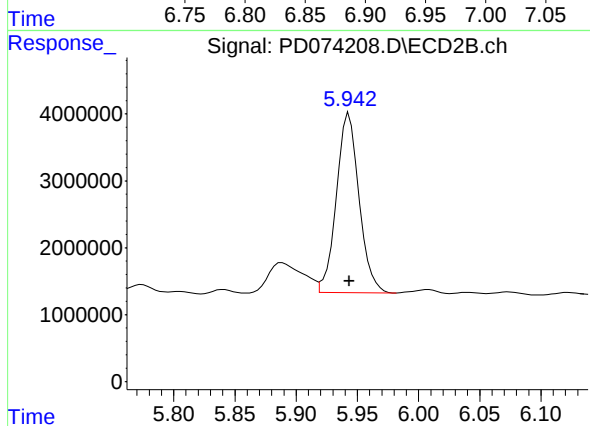

#27 Chlordane-5


R.T.: 5.943 min
Delta R.T.: 0.000 min
Response: 34542894
Conc: 560.64 ng/ml

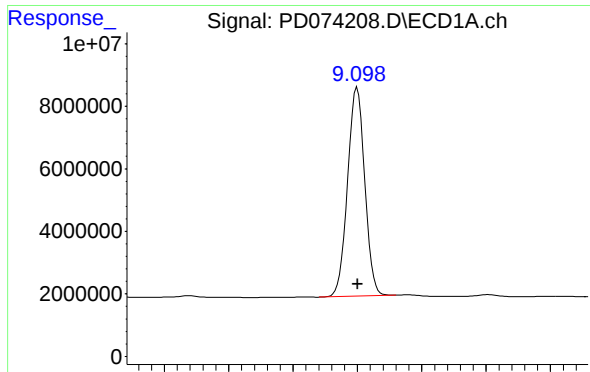

#28 Decachlorobiphenyl

R.T.: 9.100 min
Delta R.T.: 0.000 min
Response: 123682041
Conc: 47.06 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD031423CHLOR

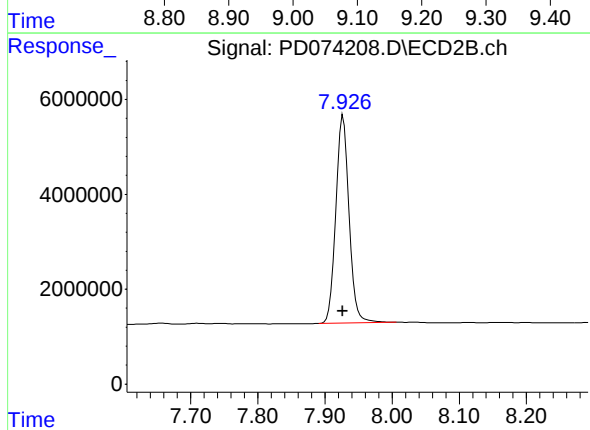

#28 Decachlorobiphenyl

R.T.: 7.927 min
Delta R.T.: 0.000 min
Response: 59912251
Conc: 47.91 ng/ml