

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031521\
 Data File : PD061596.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2021 19:40
 Operator : AR\AJ
 Sample : PTOXICC1000
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 02:53:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX031521.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 16 02:53:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.486	3.982	76658872	735.7E6	100.147	99.448
7) SA Decachlor...	8.258	9.039	104.7E6	769.8E6	98.626	97.478
Target Compounds						
2) Toxaphene-1	5.970	6.556	9912624	90067185	965.527	993.256
3) Toxaphene-2	6.237	7.063	7795641	73437810	960.970	981.587
4) Toxaphene-3	6.604	7.139	17141934	216.3E6	978.694	1006.365
5) Toxaphene-4	6.747	7.225	6015364	138.1E6	989.880	1010.831
6) Toxaphene-5	7.029	7.639	7137346	98010800	930.080	1008.070

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031521\
Data File : PD061596.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2021 19:40
Operator : AR\AJ
Sample : PTOXICC1000
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 02:53:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX031521.M
Quant Title : GC Extractables
QLast Update : Tue Mar 16 02:53:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

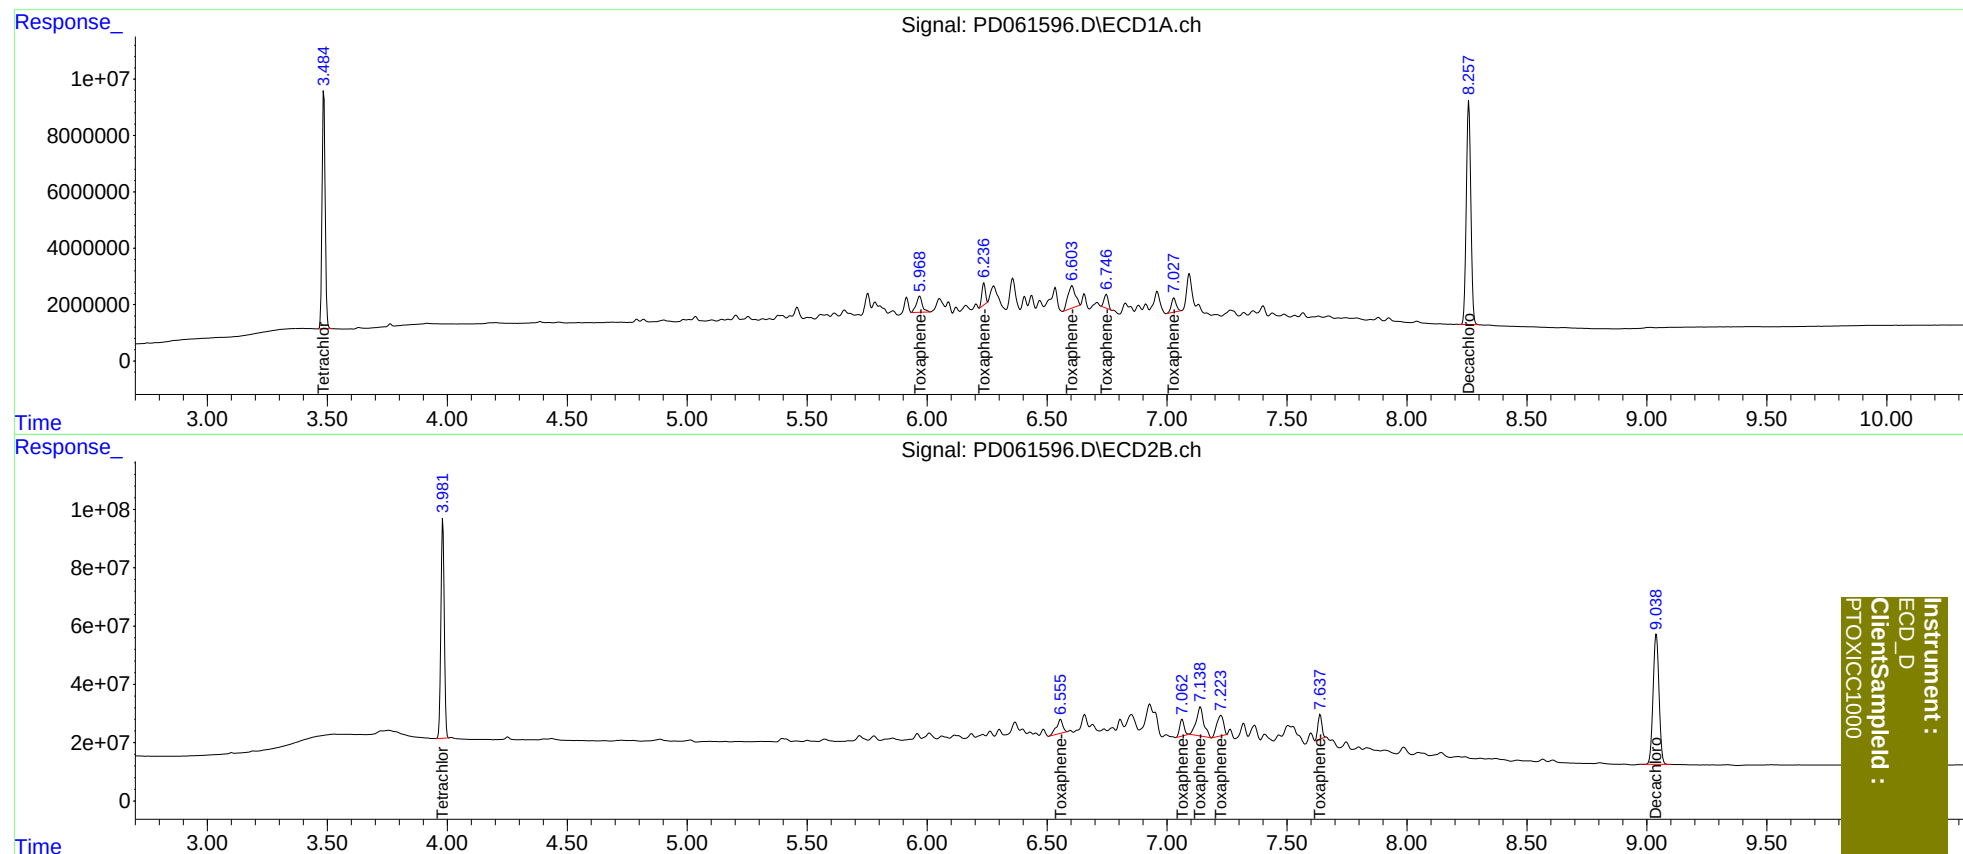

Instrument :
ECD_D
ClientSample :
PTOXICC1000