

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031521\
 Data File : PD061599.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2021 20:22
 Operator : AR\AJ
 Sample : PTOXICC250
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXICC250

Manual Integrations
 APPROVED

Ankita
 3/16/2021 11:14:12 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 02:57:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX031521.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 16 02:53:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.486	3.981	19226579	186.6E6	25.104	25.181
7) SA Decachlor...	8.258	9.039	27949401	208.3E6	25.914	26.072
Target Compounds						
2) Toxaphene-1	5.970	6.556	2468429	23629616	242.976	257.274
3) Toxaphene-2	6.238	7.061	2086328	19466371	255.443	257.307m
4) Toxaphene-3	6.605	7.139	4505940	56919075	253.858	260.353
5) Toxaphene-4	6.748	7.225	1577386	37984999	256.636	270.338
6) Toxaphene-5	7.031	7.638	1951511	24772539	255.303	254.793

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031521\
Data File : PD061599.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2021 20:22
Operator : AR\AJ
Sample : PTOXICC250
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 02:57:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX031521.M
Quant Title : GC Extractables
QLast Update : Tue Mar 16 02:53:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

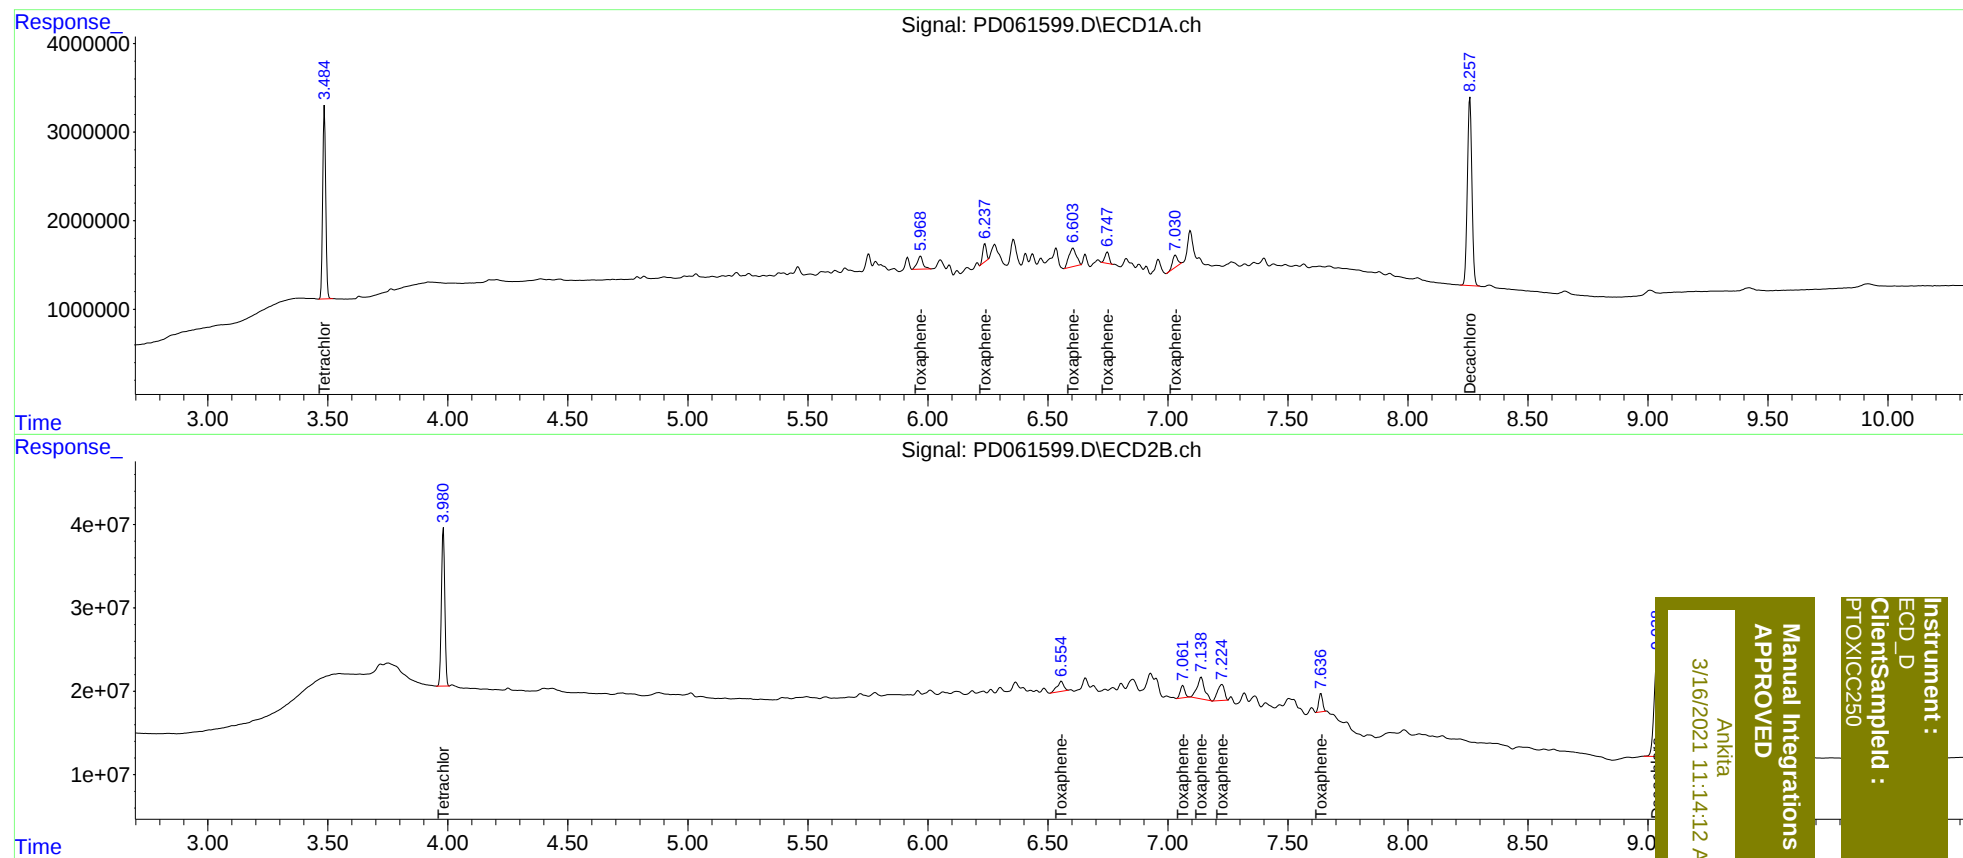

3/16/2021 11:14:12 AM

Manual Integrations
APPROVED

Ankita

Instrument :
ECD_D
Client Sampled :
PTOXICC250