

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031521\
 Data File : PD061618.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2021 00:47
 Operator : AR\AJ
 Sample : M1557-13
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PT-TXP-WP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 09:20:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX031521.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 16 03:01:54 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.486	3.982	18631179	184.9E6	24.135	24.775
7) SA Decachlor...	8.258	9.040	28038137	219.1E6	25.355	26.890
Target Compounds						
2) Toxaphene-1	5.969	6.556	54848232	504.2E6	5285.808	5369.160
3) Toxaphene-2	6.237	7.063	46892087	441.7E6	5773.728	5572.133
4) Toxaphene-3	6.604	7.139	114.1E6	1264.0E6	6551.034	5729.658
5) Toxaphene-4	6.748	7.226	39732619	784.1E6	6578.820	5690.510
6) Toxaphene-5	7.028	7.638	44701124	537.7E6	5789.059	5502.608

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031521\
Data File : PD061618.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2021 00:47
Operator : AR\AJ
Sample : M1557-13
Misc :
ALS Vial : 37 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 09:20:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX031521.M
Quant Title : GC Extractables
QLast Update : Tue Mar 16 03:01:54 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

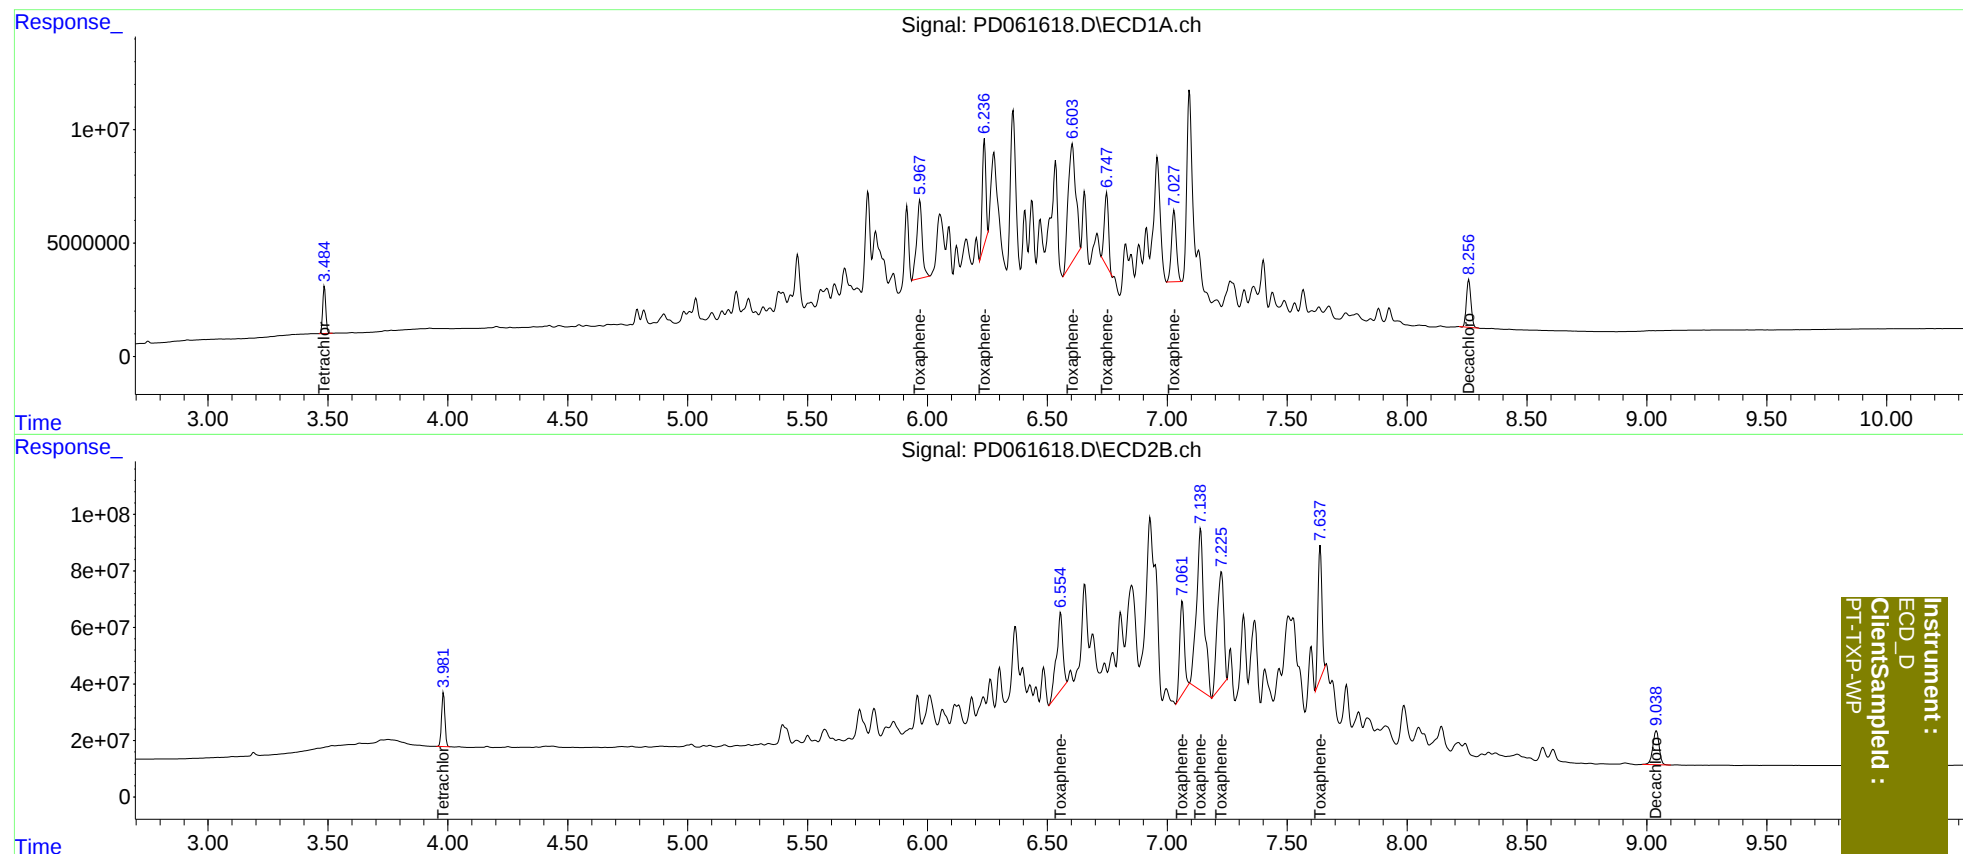

Instrument :
ECD_D
ClientSampled :
PT-TXP-WP