

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031521\
 Data File : PD061619.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2021 01:01
 Operator : AR\AJ
 Sample : M1557-13DL 10X
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PT-TXP-WPDL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 09:20:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX031521.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 16 03:01:54 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.486	3.982	1650909	16580961	2.139	2.222
7) SA Decachlor...	8.258	9.040	2800576	20607657	2.533	2.530
Target Compounds						
2) Toxaphene-1	5.969	6.556	5448971	47134977	525.126	501.889
3) Toxaphene-2	6.237	7.063	4445765	39491173	547.398	498.189
4) Toxaphene-3	6.604	7.139	9744905	117.8E6	559.421	534.056
5) Toxaphene-4	6.747	7.224	3368435	74351479	557.736	539.621
6) Toxaphene-5	7.029	7.638	4256042	51236151	551.182	524.372

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031521\
Data File : PD061619.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2021 01:01
Operator : AR\AJ
Sample : M1557-13DL 10X
Misc :
ALS Vial : 38 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 09:20:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX031521.M
Quant Title : GC Extractables
QLast Update : Tue Mar 16 03:01:54 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

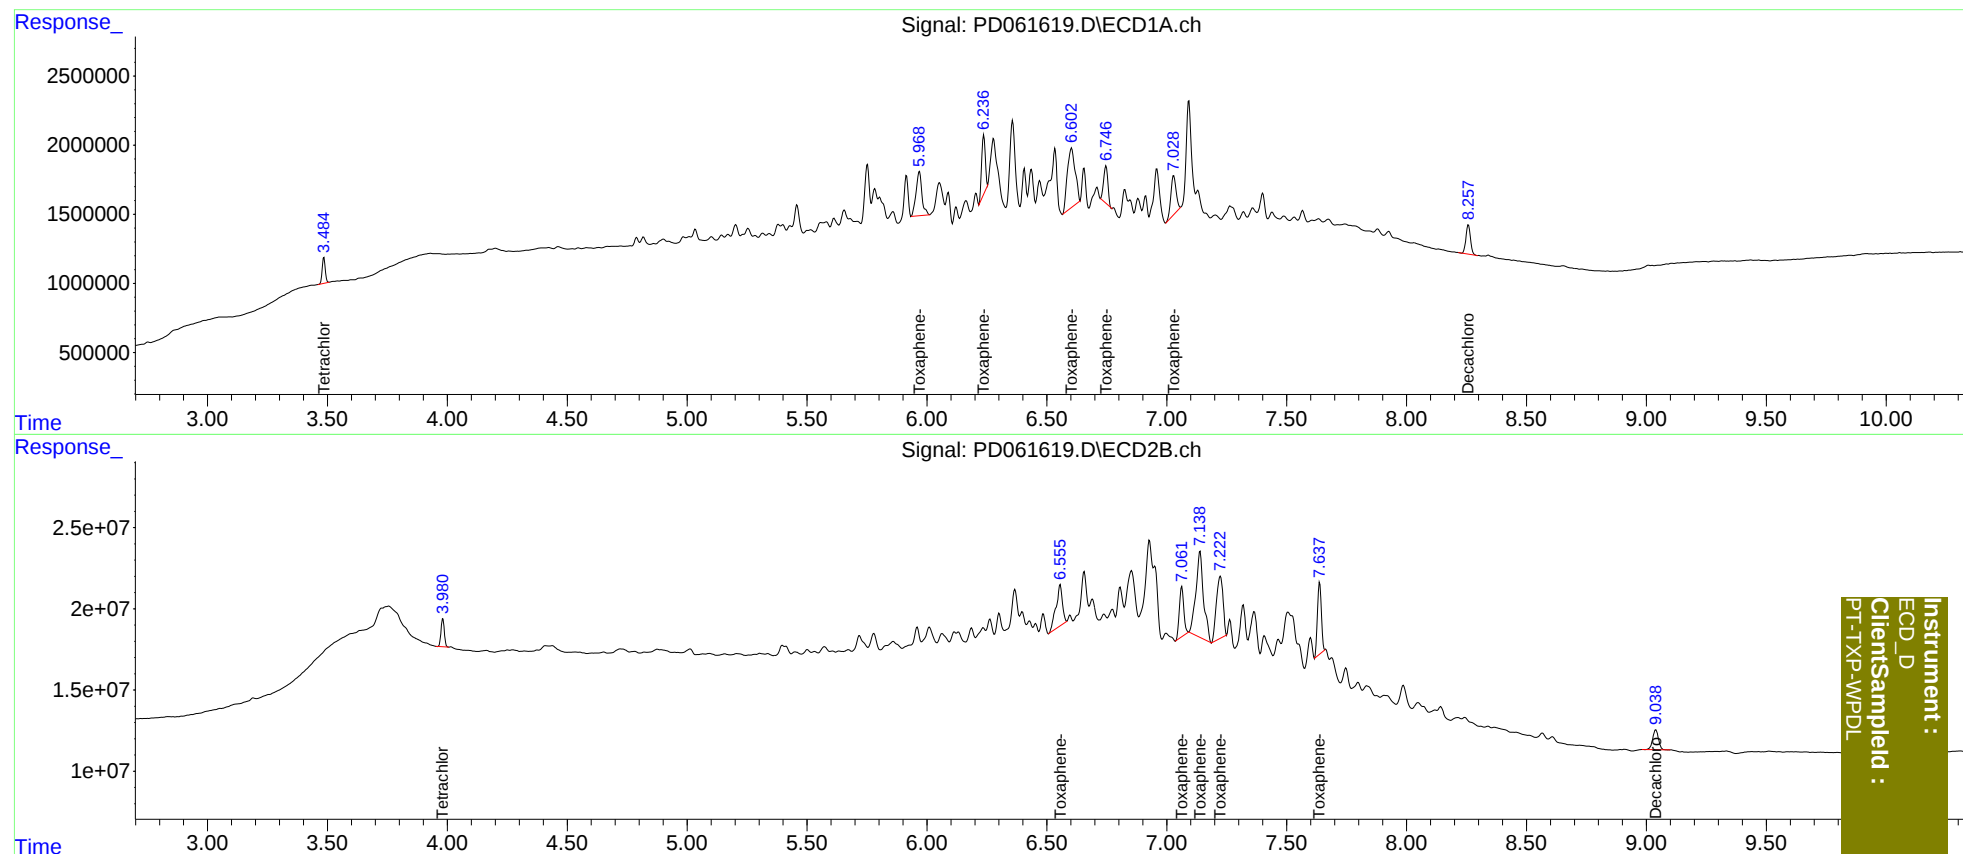

Instrument :
ECD_D
ClientSampled :
PT-TXP-WPDL