

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031521\
 Data File : PD061625.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2021 04:47
 Operator : AR\AJ
 Sample : PTOXCCC500
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 09:20:17 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX031521.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 16 03:01:54 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.485	3.981	39394132	390.1E6	51.032	52.268
7) SA Decachlor...	8.258	9.039	54945509	410.1E6	49.687	50.338
Target Compounds						
2) Toxaphene-1	5.970	6.555	5298603	47041780	510.634	500.896
3) Toxaphene-2	6.238	7.063	4332133	39807049	533.407	502.173
4) Toxaphene-3	6.605	7.139	9180567	109.5E6	527.024	496.350
5) Toxaphene-4	6.748	7.225	3078777	68757979	509.776	499.025
6) Toxaphene-5	7.030	7.638	3833054	48788387	496.403	499.321

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031521\
Data File : PD061625.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2021 04:47
Operator : AR\AJ
Sample : PTOXCCC500
Misc :
ALS Vial : 25 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 09:20:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX031521.M
Quant Title : GC Extractables
QLast Update : Tue Mar 16 03:01:54 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

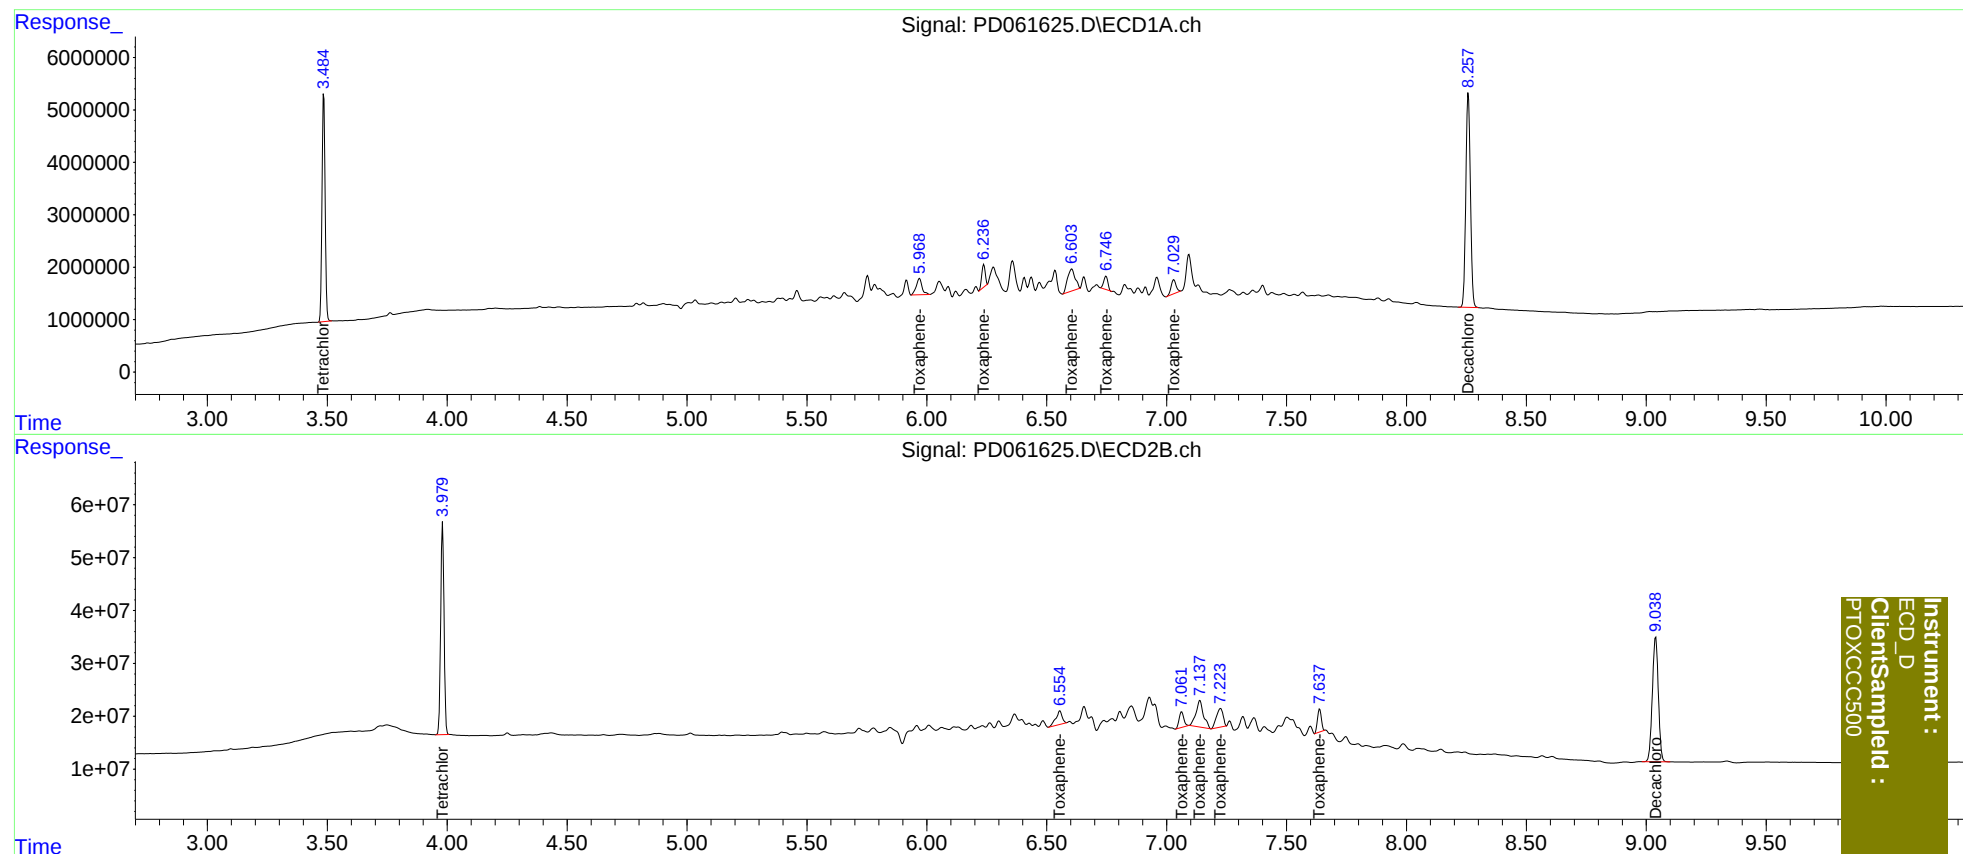

Instrument :
ECD_D
Client Sample :
PTOXC500