

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031521\
 Data File : PD061585.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2021 17:06
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 02:38:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031521.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 16 02:33:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	3.981	15647268	154.9E6	20.051	20.235
28)	SA Decachlor...	8.258	9.039	22369818	169.3E6	19.808	20.221
Target Compounds							
9)	A Endosulfan I	5.548	6.210	9861709	95366714	9.807	10.255
10)	B gamma-Chl...	5.435	6.087	10223339	102.8E6	9.567	9.953
12)	B 4,4'-DDE	5.657	6.316	20084146	205.0E6	19.283	20.463
13)	MA Dieldrin	5.793	6.466	20025217	203.1E6	19.529	20.177
19)	B Endosulfa...	6.707	7.239	18432008	170.1E6	19.011	19.544
20)	A Methoxychlor	6.962	7.562	38170666	354.6E6	98.133	92.650
21)	B Endrin ke...	7.201	7.710	21981833	170.2E6	18.950	18.673



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031521\
Data File : PD061585.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2021 17:06
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 02:38:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031521.M
Quant Title : GC Extractables
QLast Update : Tue Mar 16 02:33:48 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

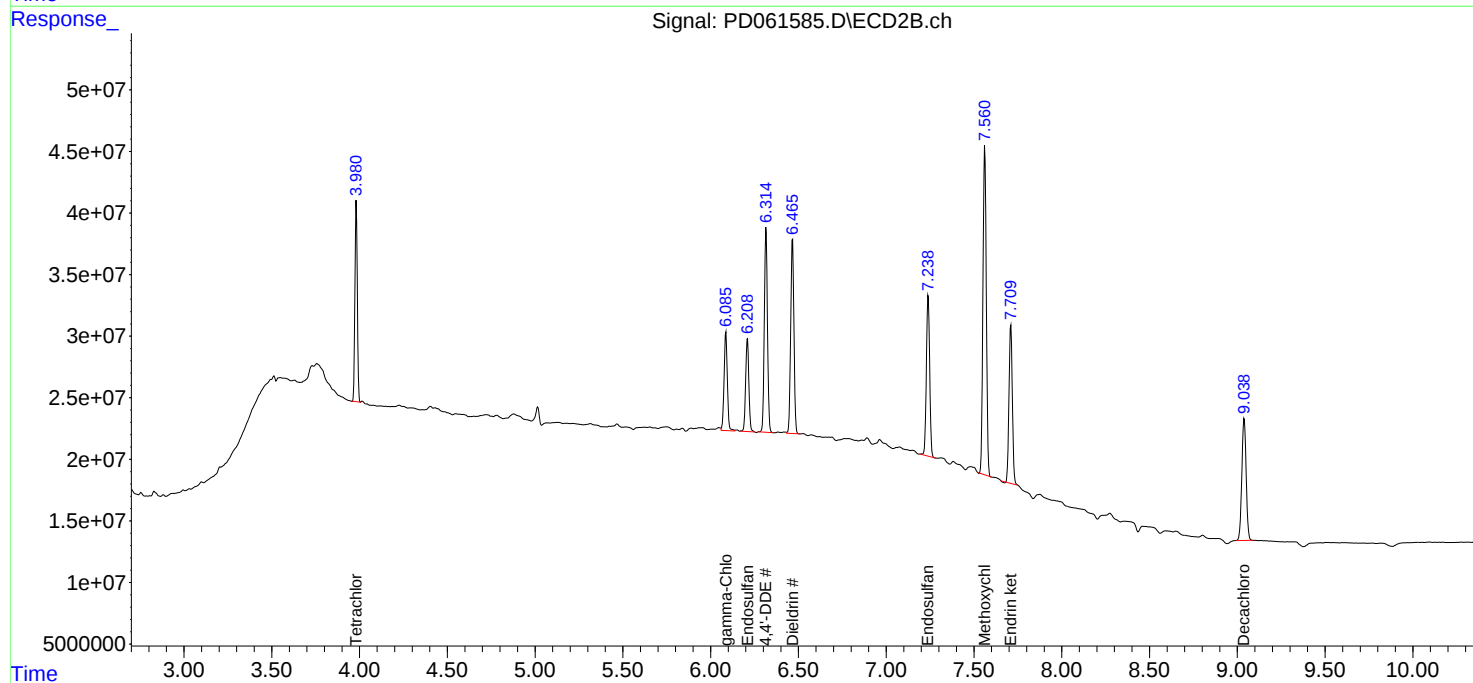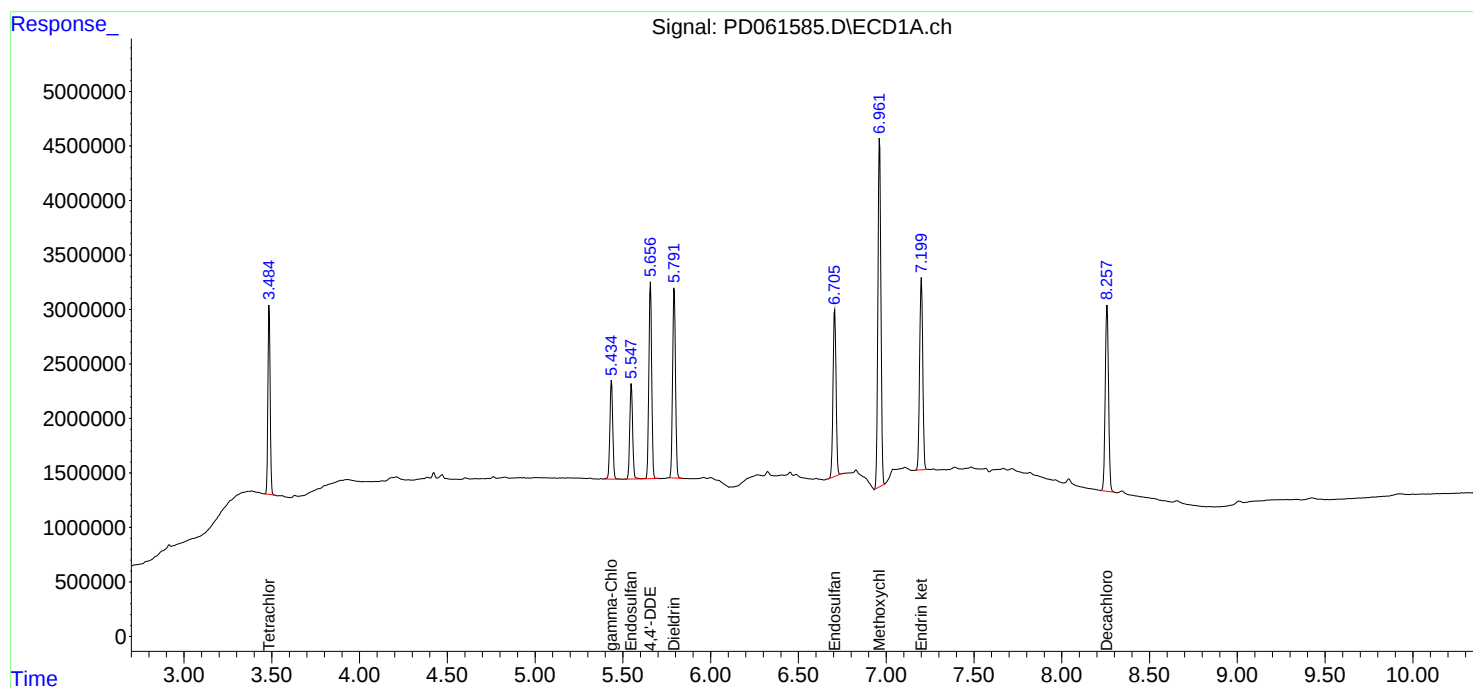


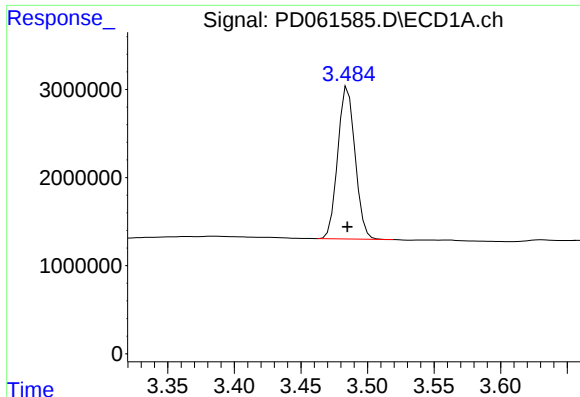

#1 Tetrachloro-m-xylene


R.T.: 3.485 min
Delta R.T.: 0.000 min
Response: 15647268
Conc: 20.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

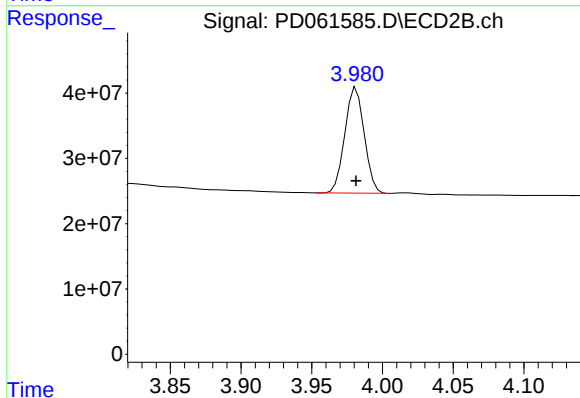


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 154882888
Conc: 20.24 ng/ml

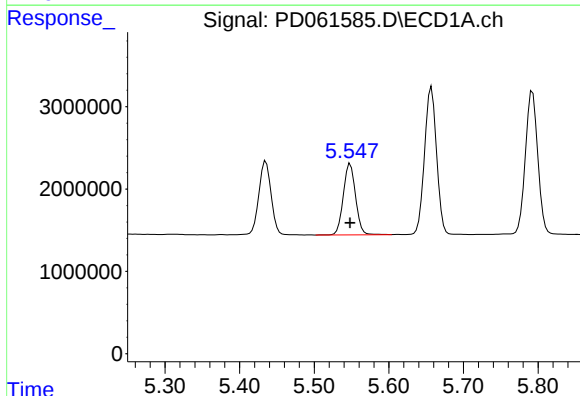


#9 Endosulfan I

R.T.: 5.548 min
Delta R.T.: 0.000 min
Response: 9861709
Conc: 9.81 ng/ml

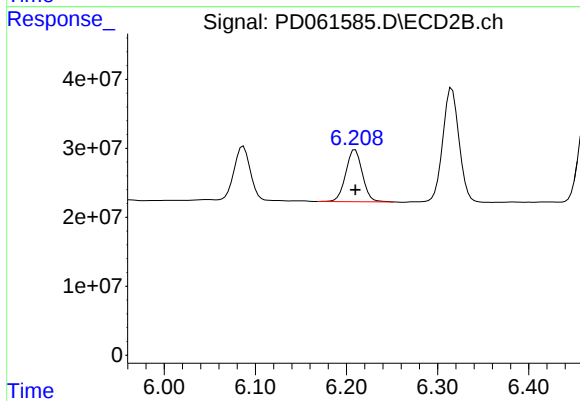

#9 Endosulfan I


R.T.: 6.210 min
Delta R.T.: 0.000 min
Response: 95366714
Conc: 10.25 ng/ml

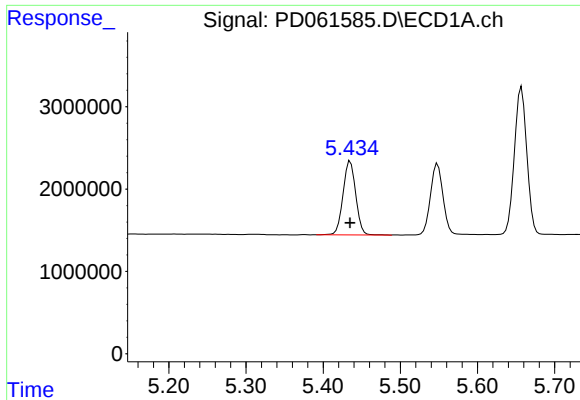

#10 gamma-Chlordane


R.T.: 5.435 min
Delta R.T.: 0.000 min
Response: 10223339
Conc: 9.57 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

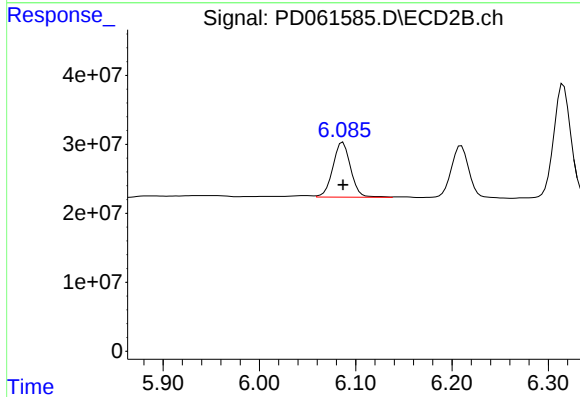


#10 gamma-Chlordane

R.T.: 6.087 min
Delta R.T.: 0.000 min
Response: 102848360
Conc: 9.95 ng/ml

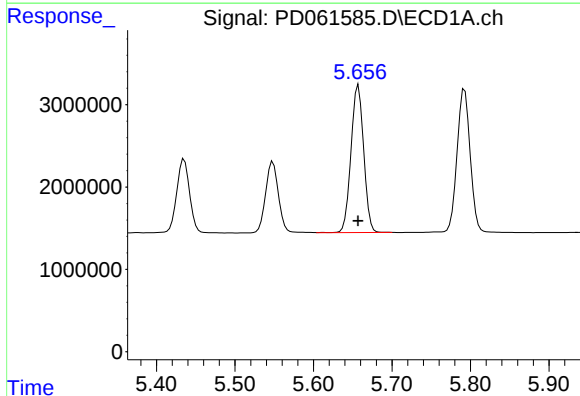


#12 4,4'-DDE

R.T.: 5.657 min
Delta R.T.: 0.000 min
Response: 20084146
Conc: 19.28 ng/ml

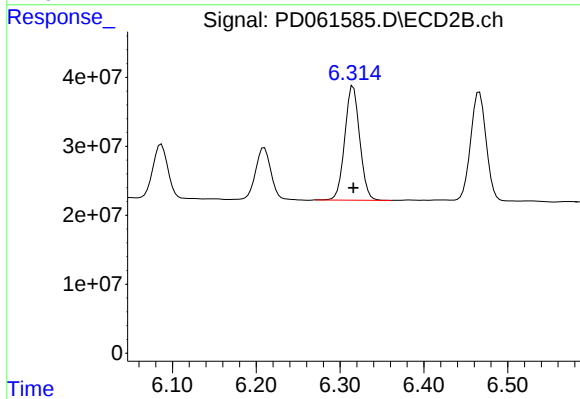

#12 4,4'-DDE


R.T.: 6.316 min
Delta R.T.: 0.000 min
Response: 205038415
Conc: 20.46 ng/ml

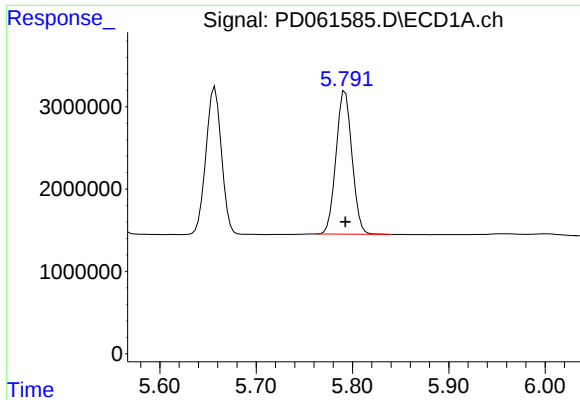

#13 Dieldrin


R.T.: 5.793 min
Delta R.T.: 0.000 min
Response: 20025217
Conc: 19.53 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

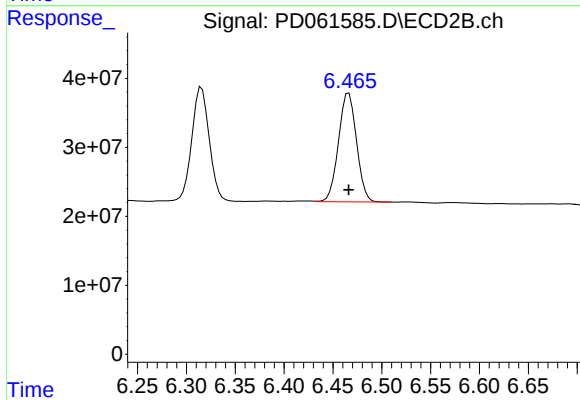


#13 Dieldrin

R.T.: 6.466 min
Delta R.T.: 0.000 min
Response: 203067287
Conc: 20.18 ng/ml

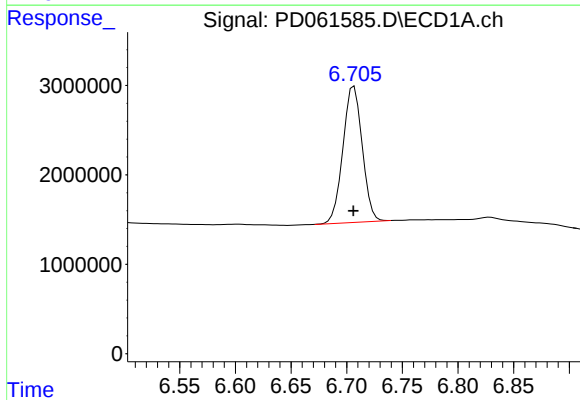


#19 Endosulfan Sulfate

R.T.: 6.707 min
Delta R.T.: 0.000 min
Response: 18432008
Conc: 19.01 ng/ml

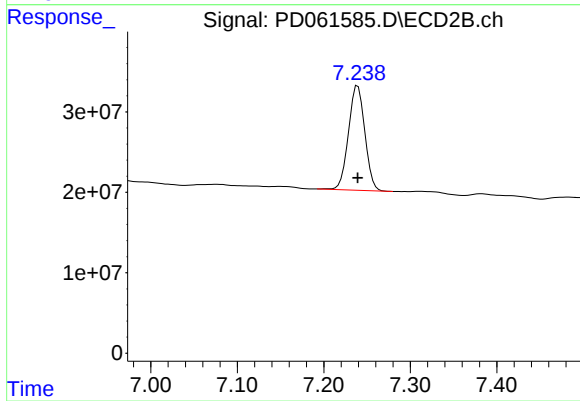

#19 Endosulfan Sulfate


R.T.: 7.239 min
Delta R.T.: 0.000 min
Response: 170050977
Conc: 19.54 ng/ml

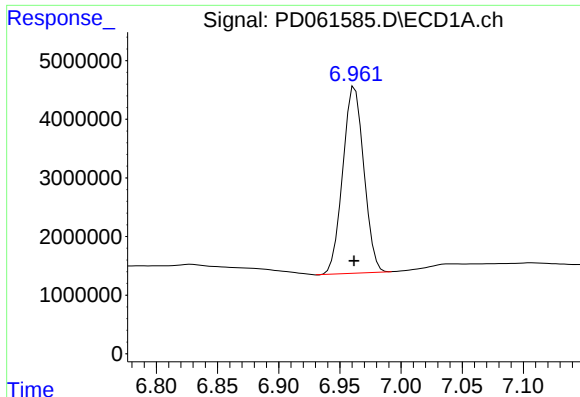

#20 Methoxychlor


R.T.: 6.962 min
Delta R.T.: 0.000 min
Response: 38170666
Conc: 98.13 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

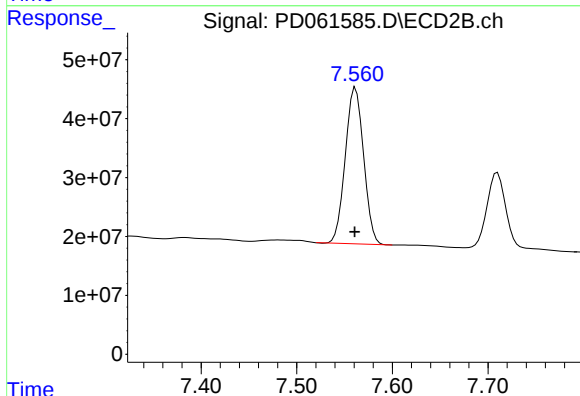


#20 Methoxychlor

R.T.: 7.562 min
Delta R.T.: 0.001 min
Response: 354597998
Conc: 92.65 ng/ml

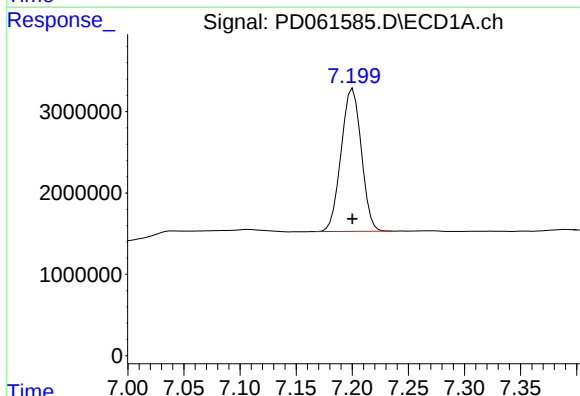


#21 Endrin ketone

R.T.: 7.201 min
Delta R.T.: 0.000 min
Response: 21981833
Conc: 18.95 ng/ml

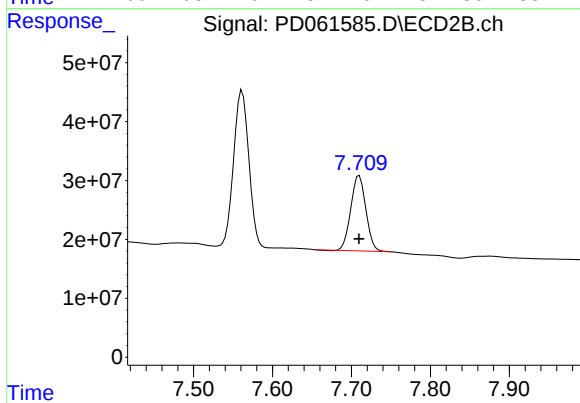

#21 Endrin ketone


R.T.: 7.710 min
Delta R.T.: 0.000 min
Response: 170162289
Conc: 18.67 ng/ml

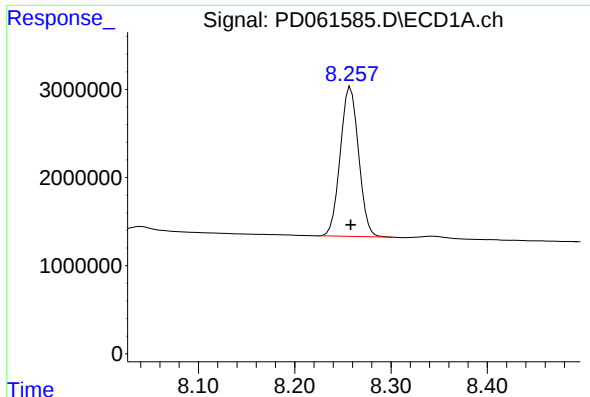

#28 Decachlorobiphenyl

R.T.: 8.258 min
Delta R.T.: 0.000 min
Response: 22369818
Conc: 19.81 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

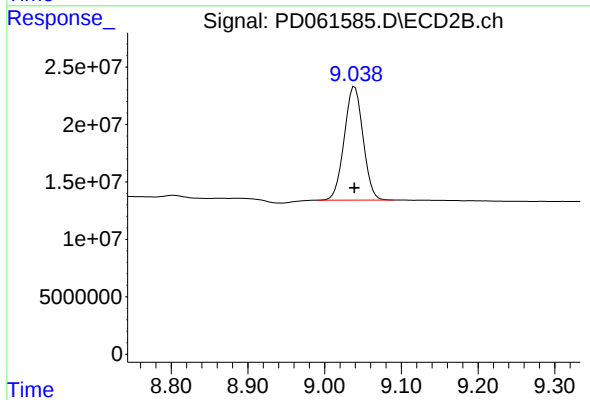

#28 Decachlorobiphenyl

R.T.: 9.039 min
Delta R.T.: 0.000 min
Response: 169295927
Conc: 20.22 ng/ml