

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031521\
 Data File : PD061593.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2021 18:58
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 01:52:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031521.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 16 01:52:25 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	3.982	43886901	371.6E6	50.000	50.000
28)	SA Decachlor...	8.257	9.039	54136797	399.4E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.360	4.975	14507995	161.9E6	500.000	500.000
24)	Chlordane-2	4.864	5.442	17444119	157.2E6	500.000	500.000
25)	Chlordane-3	5.435	6.087	53193312	713.6E6	500.000	500.000
26)	Chlordane-4	5.493	6.161	44128653	821.9E6	500.000	500.000
27)	Chlordane-5	6.333	6.965	19388899	156.5E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031521\
Data File : PD061593.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2021 18:58
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 01:52:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031521.M
Quant Title : GC Extractables
QLast Update : Tue Mar 16 01:52:25 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

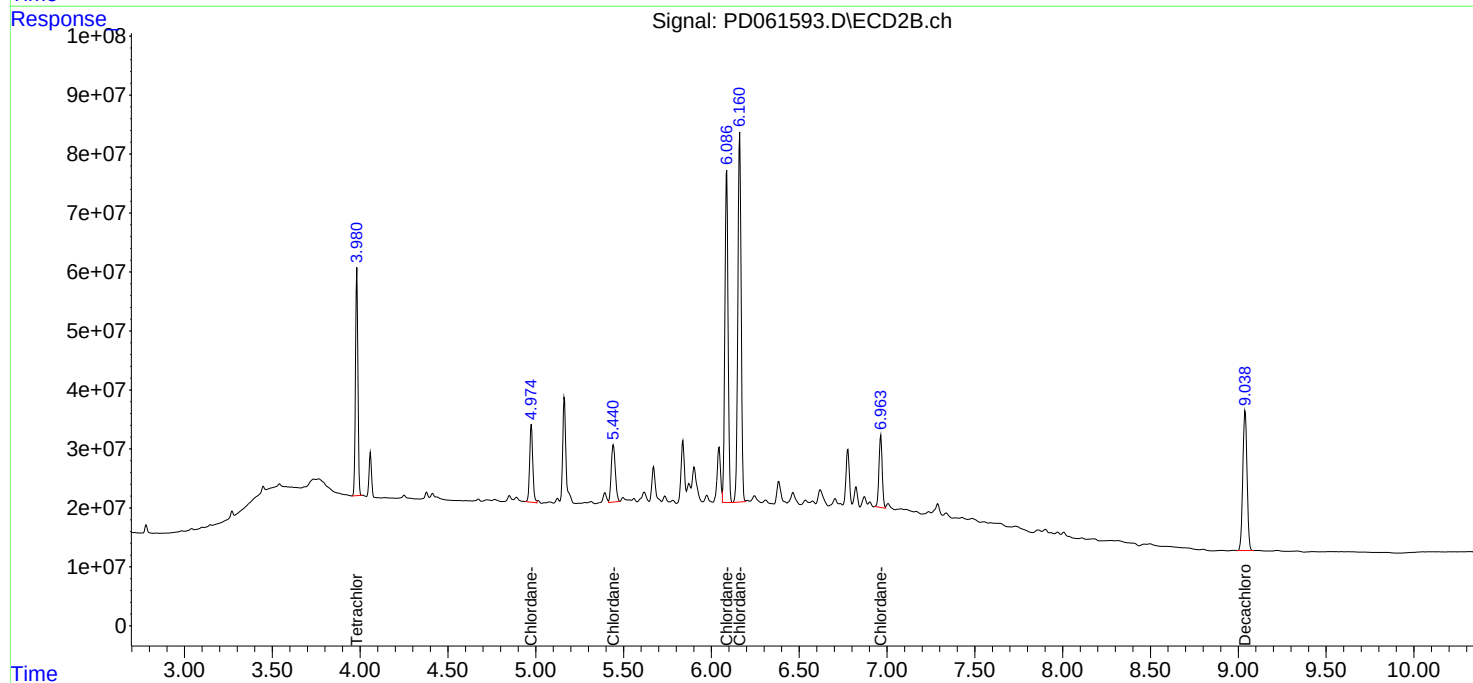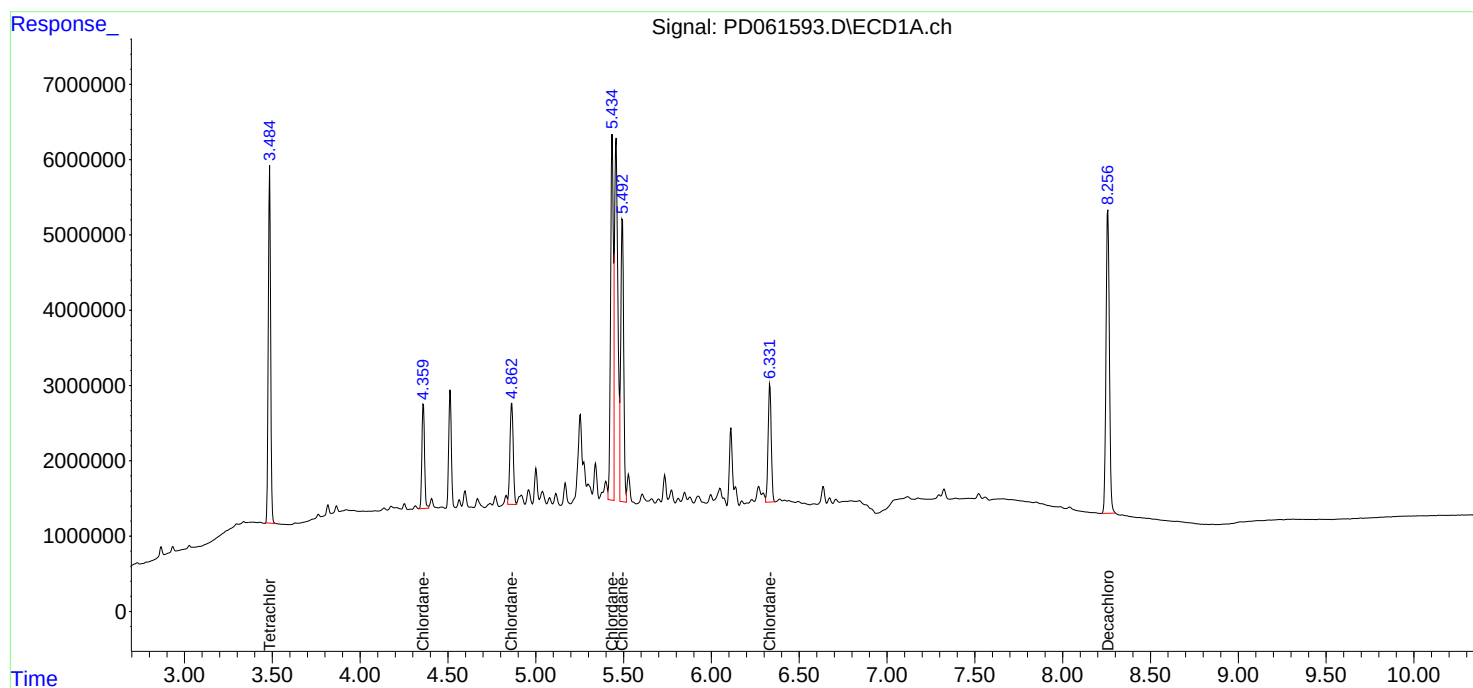


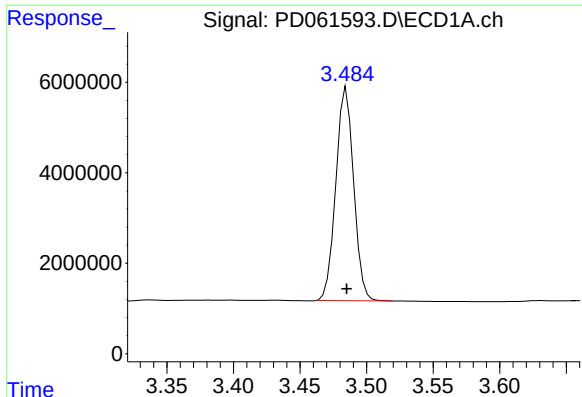

#1 Tetrachloro-m-xylene


R.T.: 3.485 min
Delta R.T.: 0.000 min
Response: 43886901
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

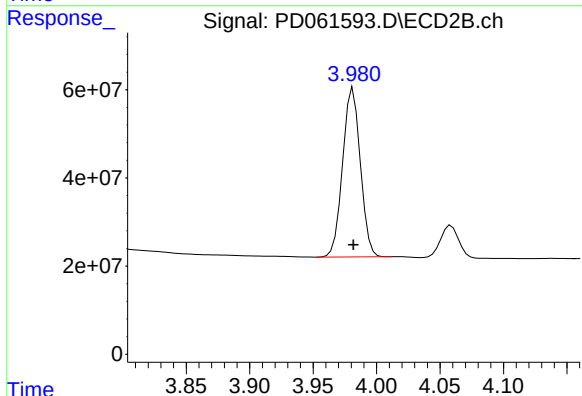


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 371551340
Conc: 50.00 ng/ml

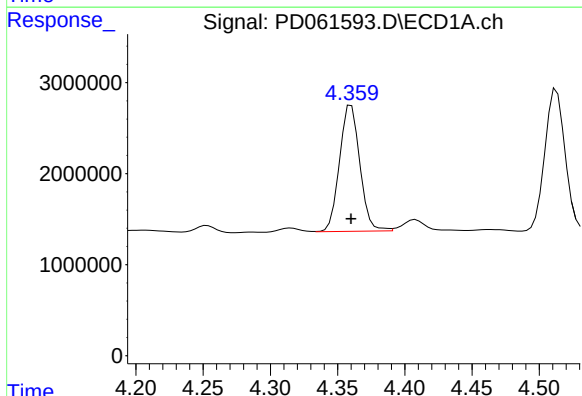


#23 Chlordane-1

R.T.: 4.360 min
Delta R.T.: 0.000 min
Response: 14507995
Conc: 500.00 ng/ml

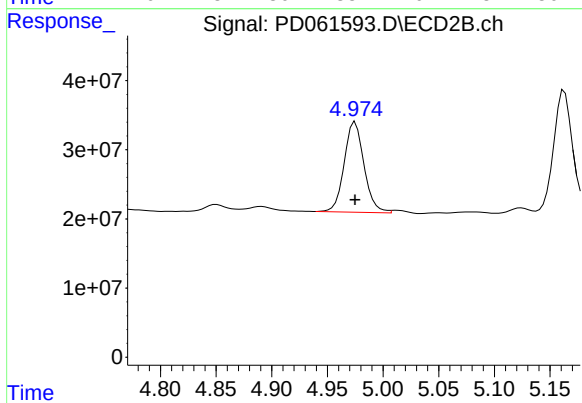

#23 Chlordane-1


R.T.: 4.975 min
Delta R.T.: 0.000 min
Response: 161871228
Conc: 500.00 ng/ml

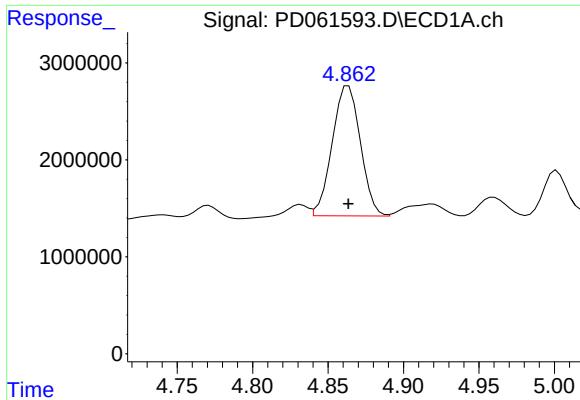

#24 Chlordane-2


R.T.: 4.864 min
Delta R.T.: 0.000 min
Response: 17444119
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

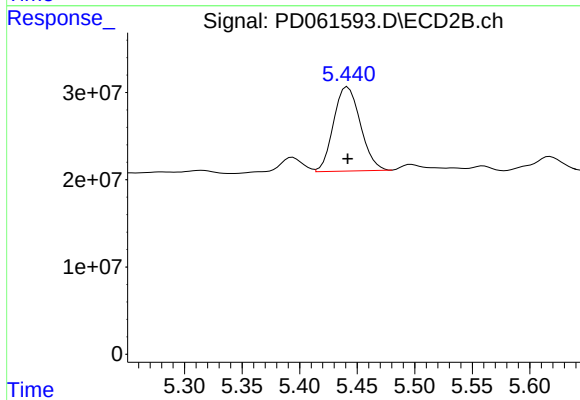


#24 Chlordane-2

R.T.: 5.442 min
Delta R.T.: 0.000 min
Response: 157189545
Conc: 500.00 ng/ml

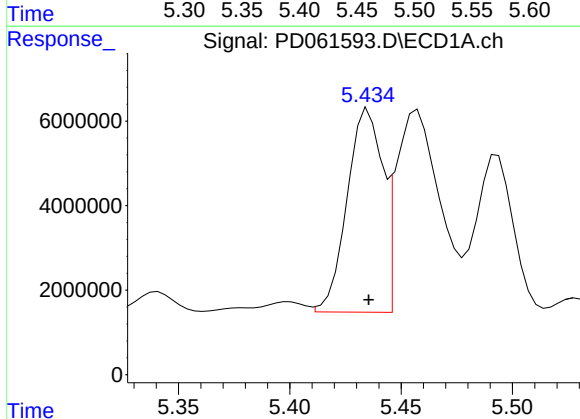


#25 Chlordane-3

R.T.: 5.435 min
Delta R.T.: 0.000 min
Response: 53193312
Conc: 500.00 ng/ml

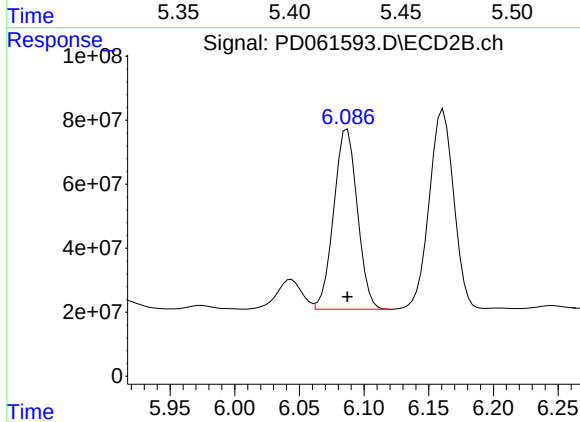

#25 Chlordane-3


R.T.: 6.087 min
Delta R.T.: 0.000 min
Response: 713614832
Conc: 500.00 ng/ml

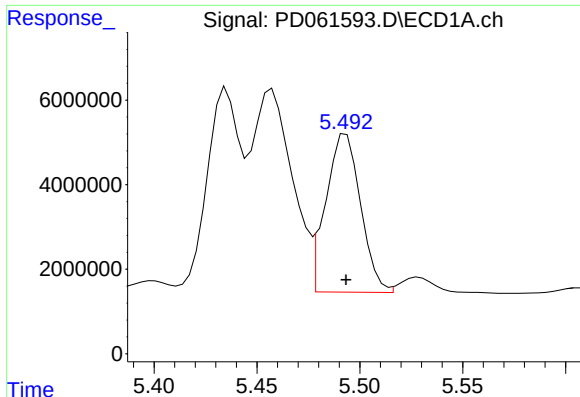

#26 Chlordane-4


R.T.: 5.493 min
Delta R.T.: 0.000 min
Response: 44128653
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

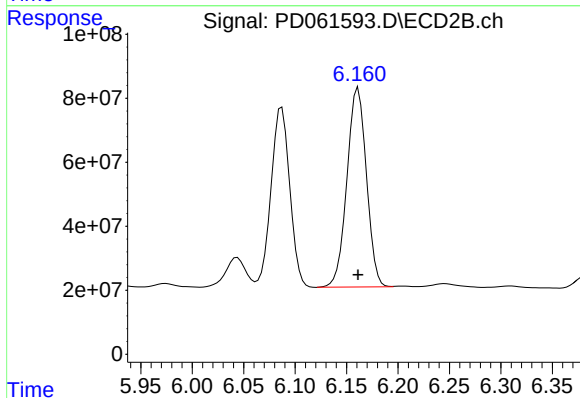


#26 Chlordane-4

R.T.: 6.161 min
Delta R.T.: 0.000 min
Response: 821917666
Conc: 500.00 ng/ml

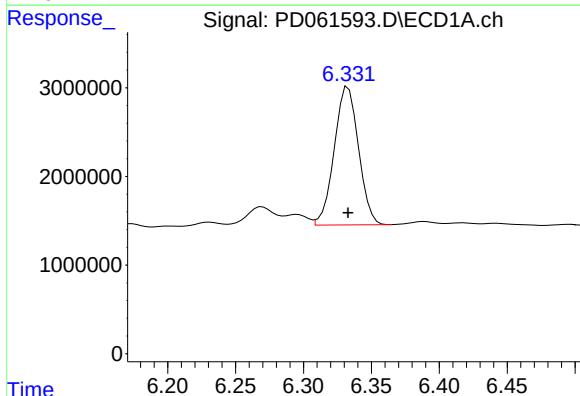


#27 Chlordane-5

R.T.: 6.333 min
Delta R.T.: 0.000 min
Response: 19388899
Conc: 500.00 ng/ml

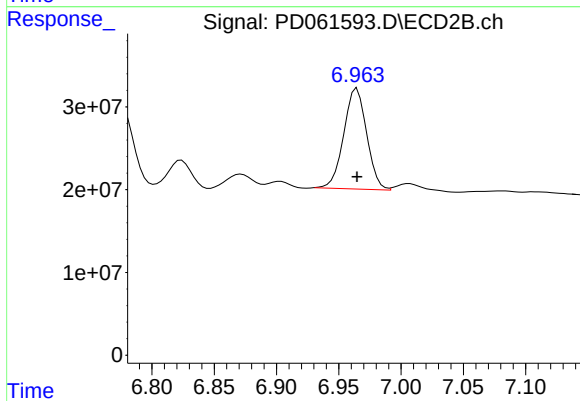

#27 Chlordane-5


R.T.: 6.965 min
Delta R.T.: 0.000 min
Response: 156546873
Conc: 500.00 ng/ml

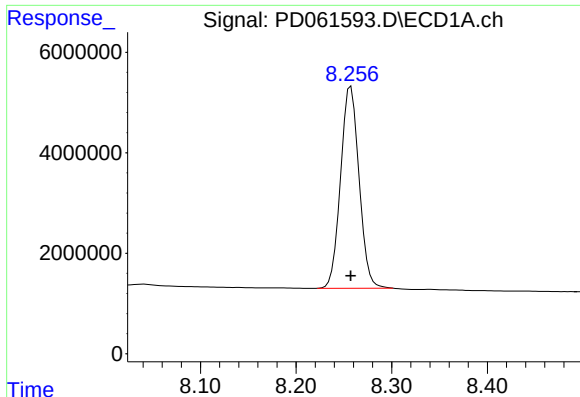

#28 Decachlorobiphenyl

R.T.: 8.257 min
Delta R.T.: 0.000 min
Response: 54136797
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

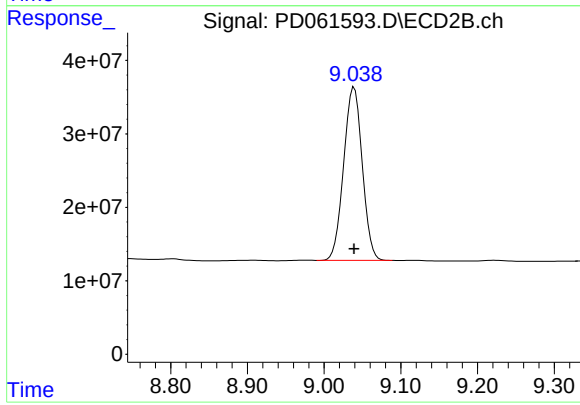

#28 Decachlorobiphenyl

R.T.: 9.039 min
Delta R.T.: 0.000 min
Response: 399369054
Conc: 50.00 ng/ml