

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031521\
 Data File : PD061602.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2021 21:04
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD031521CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 02:02:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031521.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 16 01:52:25 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	3.982	45473976	388.3E6	52.656	53.230
28)	SA Decachlor...	8.258	9.039	55685601	412.8E6	51.398	51.640
Target Compounds							
23)	Chlordane-1	4.361	4.974	15071716	172.4E6	530.522	555.436
24)	Chlordane-2	4.864	5.441	17939940	166.3E6	530.975	525.107
25)	Chlordane-3	5.436	6.087	54882716	741.4E6	527.217	527.811
26)	Chlordane-4	5.494	6.161	45437179	854.6E6	527.409	527.655
27)	Chlordane-5	6.334	6.966	20584724	160.9E6	540.647	527.601



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031521\
Data File : PD061602.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2021 21:04
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD031521CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 02:02:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031521.M
Quant Title : GC Extractables
QLast Update : Tue Mar 16 01:52:25 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

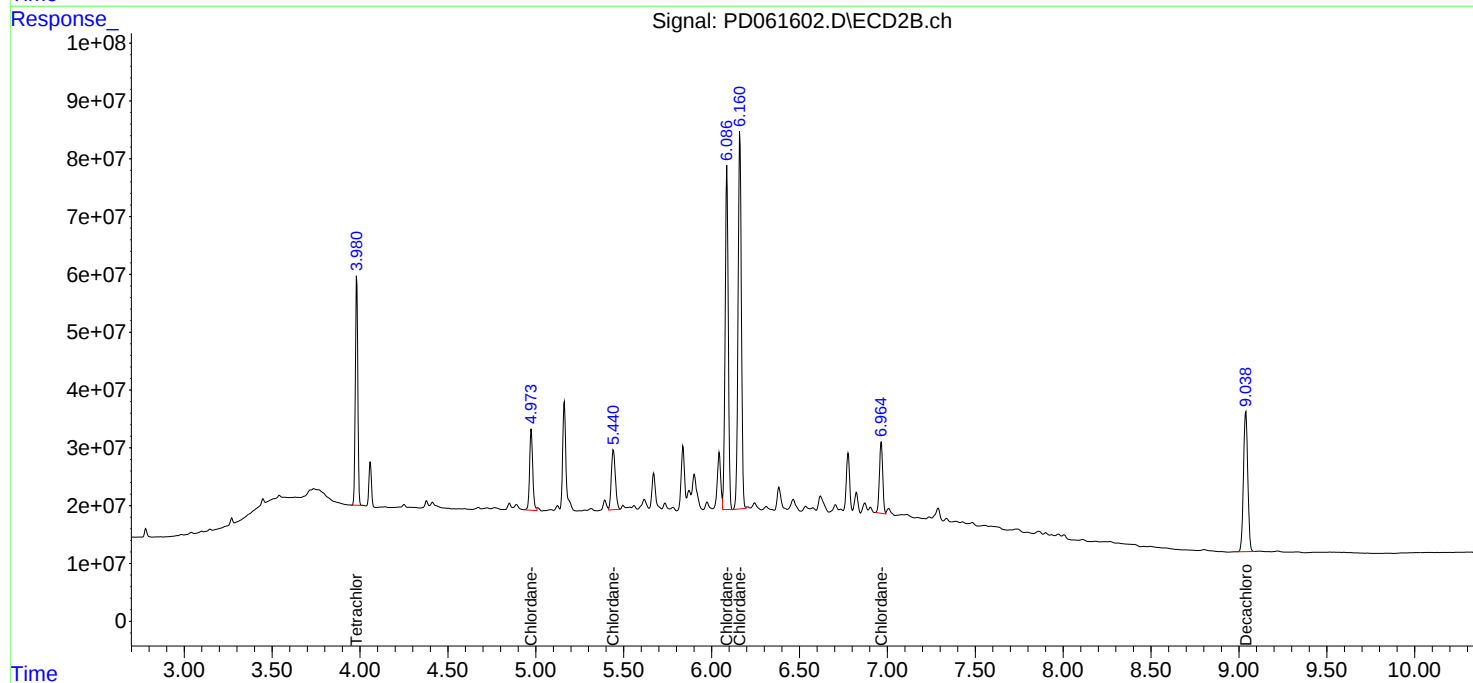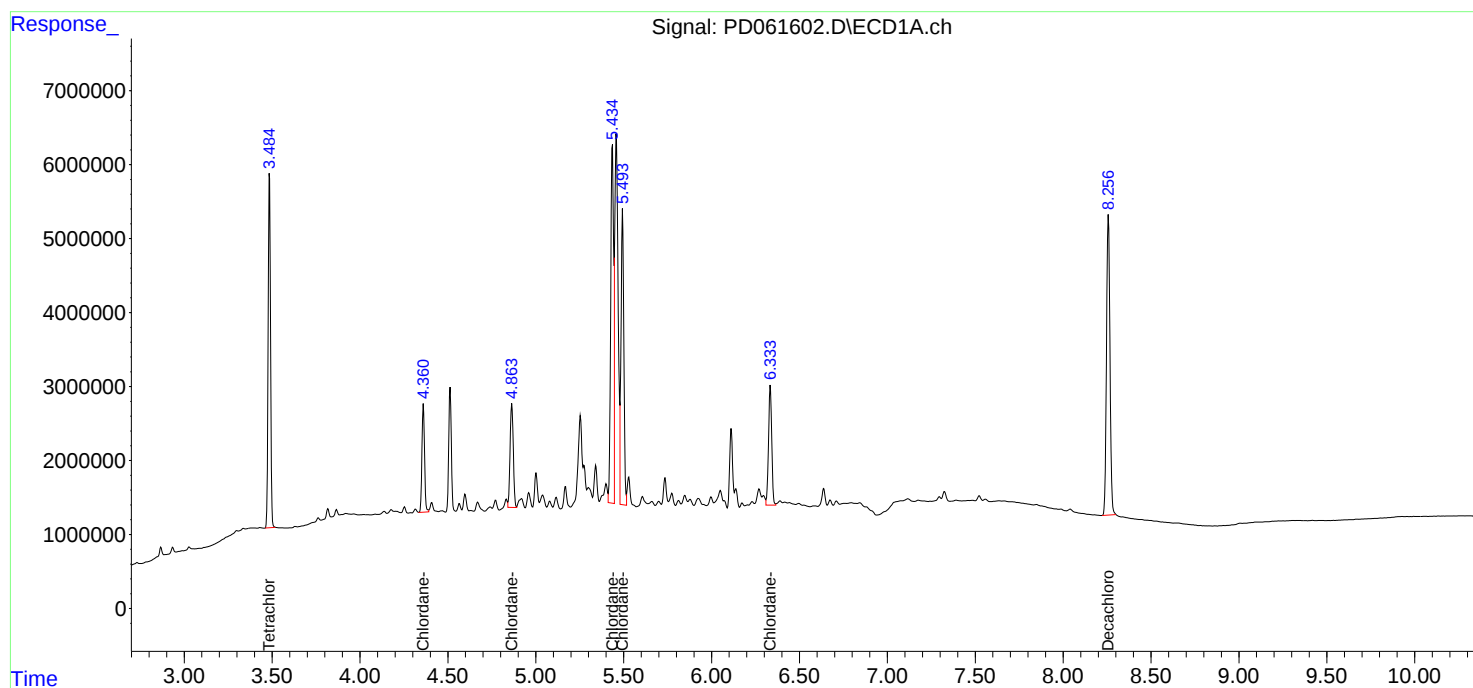


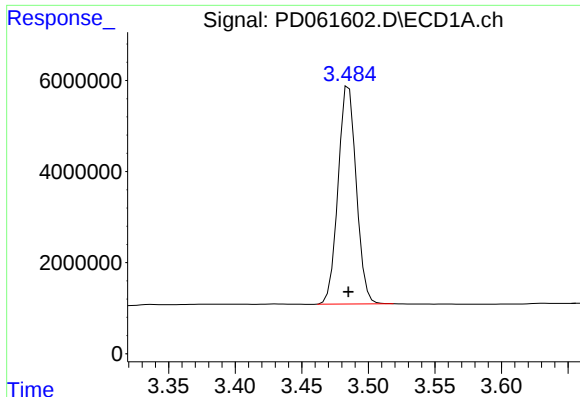

#1 Tetrachloro-m-xylene


R.T.: 3.485 min
Delta R.T.: 0.000 min
Response: 45473976
Conc: 52.66 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD031521CHLOR

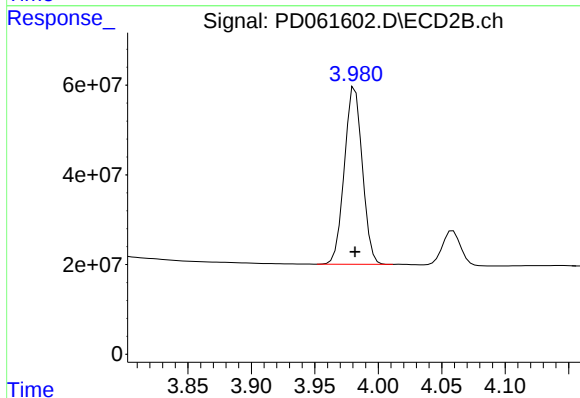


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 388267820
Conc: 53.23 ng/ml

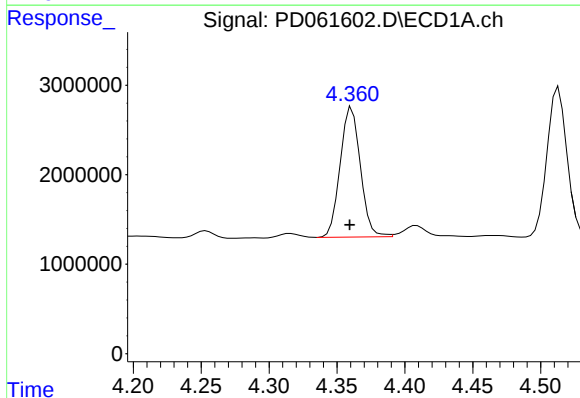


#23 Chlordane-1

R.T.: 4.361 min
Delta R.T.: 0.001 min
Response: 15071716
Conc: 530.52 ng/ml

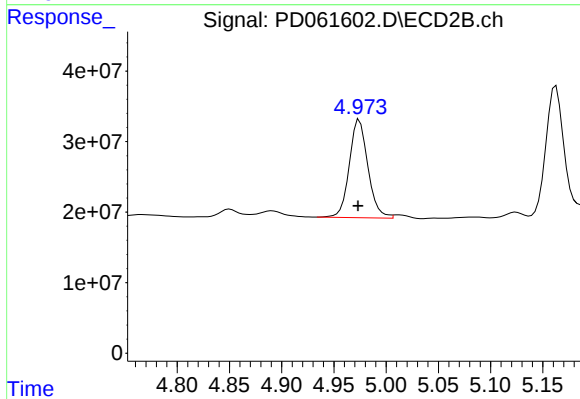

#23 Chlordane-1


R.T.: 4.974 min
Delta R.T.: 0.001 min
Response: 172379863
Conc: 555.44 ng/ml

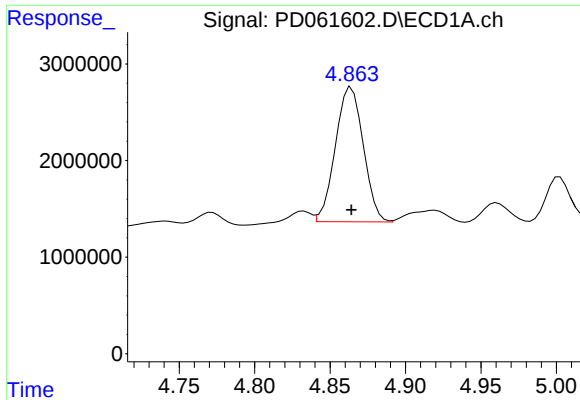

#24 Chlordane-2


R.T.: 4.864 min
Delta R.T.: 0.000 min
Response: 17939940
Conc: 530.98 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD031521CHLOR

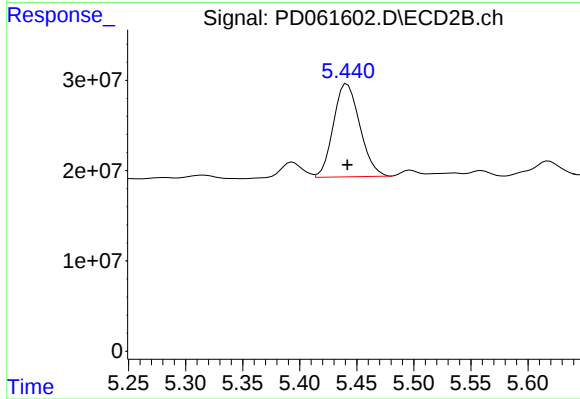


#24 Chlordane-2

R.T.: 5.441 min
Delta R.T.: 0.000 min
Response: 166269342
Conc: 525.11 ng/ml

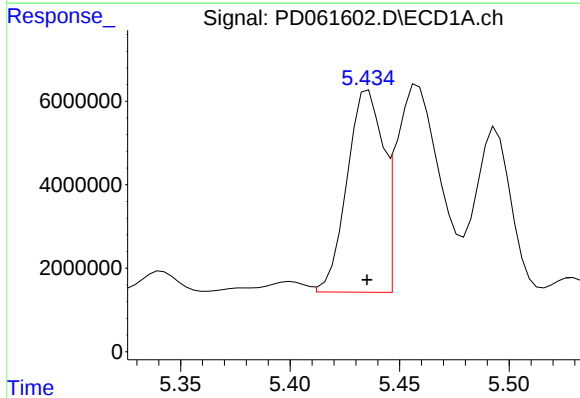


#25 Chlordane-3

R.T.: 5.436 min
Delta R.T.: 0.000 min
Response: 54882716
Conc: 527.22 ng/ml

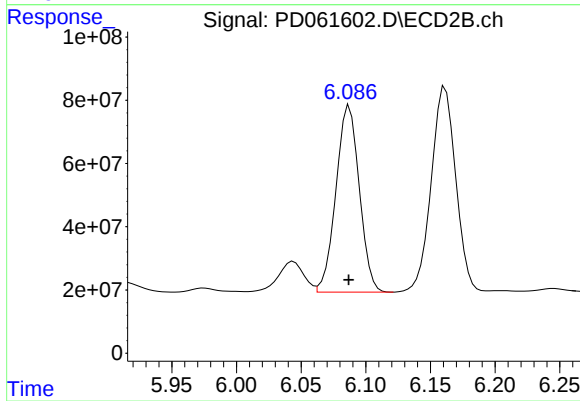

#25 Chlordane-3


R.T.: 6.087 min
Delta R.T.: 0.000 min
Response: 741426694
Conc: 527.81 ng/ml

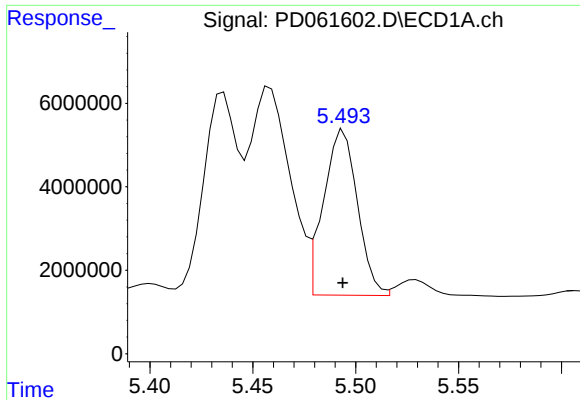

#26 Chlordane-4


R.T.: 5.494 min
Delta R.T.: 0.000 min
Response: 45437179
Conc: 527.41 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD031521CHLOR

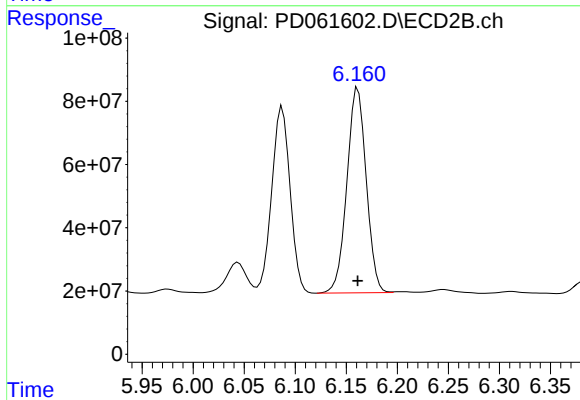


#26 Chlordane-4

R.T.: 6.161 min
Delta R.T.: 0.000 min
Response: 854629787
Conc: 527.66 ng/ml

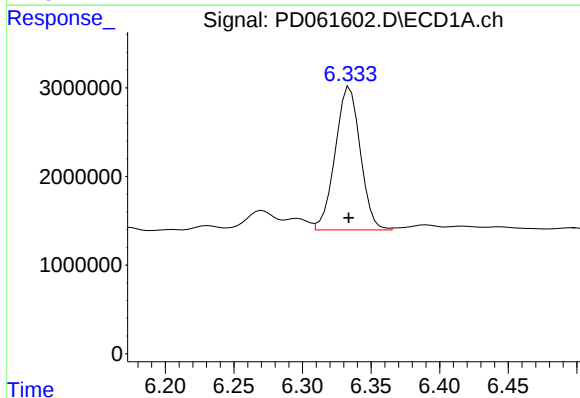


#27 Chlordane-5

R.T.: 6.334 min
Delta R.T.: 0.000 min
Response: 20584724
Conc: 540.65 ng/ml

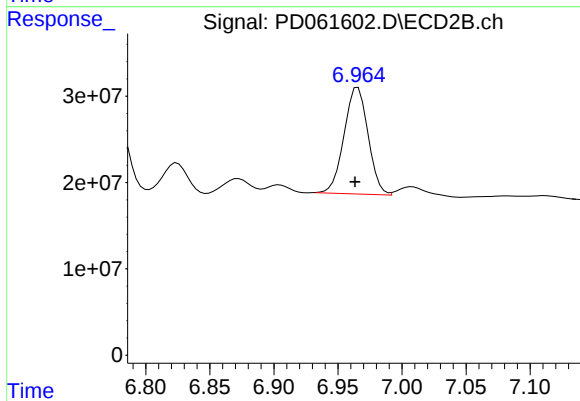

#27 Chlordane-5


R.T.: 6.966 min
Delta R.T.: 0.002 min
Response: 160874609
Conc: 527.60 ng/ml

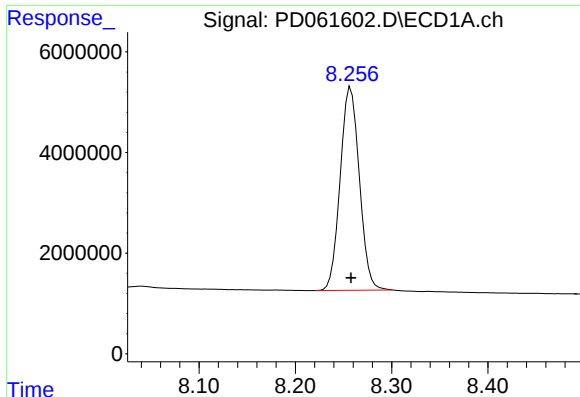

#28 Decachlorobiphenyl

R.T.: 8.258 min
Delta R.T.: 0.000 min
Response: 55685601
Conc: 51.40 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD031521CHLOR

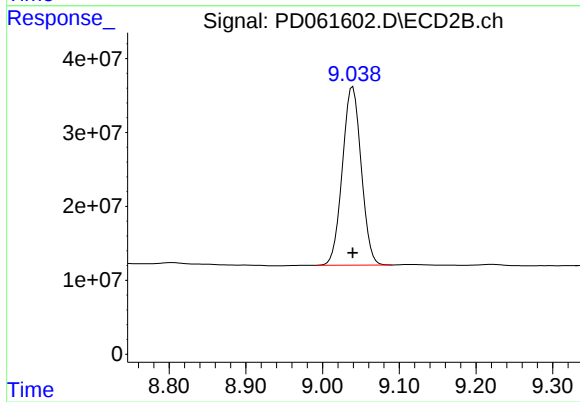

#28 Decachlorobiphenyl

R.T.: 9.039 min
Delta R.T.: 0.000 min
Response: 412761196
Conc: 51.64 ng/ml