

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031521\
 Data File : PD061614.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2021 23:52
 Operator : AR\AJ
 Sample : PB135087BS
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB135087BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 09:00:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031521.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 16 02:33:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	3.982	16587534	148.5E6	21.256	19.395
28)	SA Decachlor...	8.258	9.039	21943495	164.3E6	19.430	19.622
Target Compounds							
23)	Chlordane-1	4.361	4.975	5689822	65910058	200.281	212.373
24)	Chlordane-2	4.864	5.442	7086378	64932083	209.738	205.067
25)	Chlordane-3	5.435	6.087	20012405	277.8E6	192.244	197.758
26)	Chlordane-4	5.494	6.162	16908363	322.6E6	196.263	199.160
27)	Chlordane-5	6.333	6.965	7417576	59341201	194.819	194.614



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031521\
Data File : PD061614.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2021 23:52
Operator : AR\AJ
Sample : PB135087BS
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PB135087BS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 09:00:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031521.M
Quant Title : GC Extractables
QLast Update : Tue Mar 16 02:33:48 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

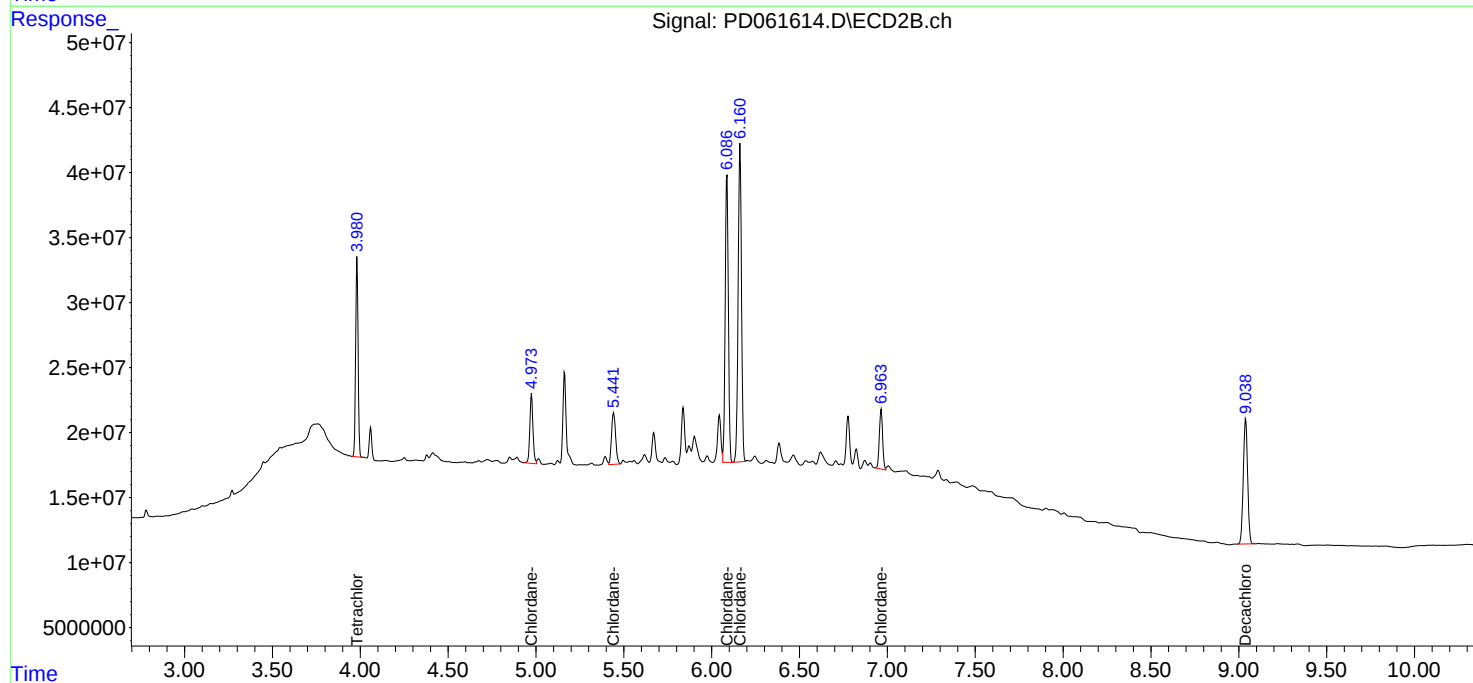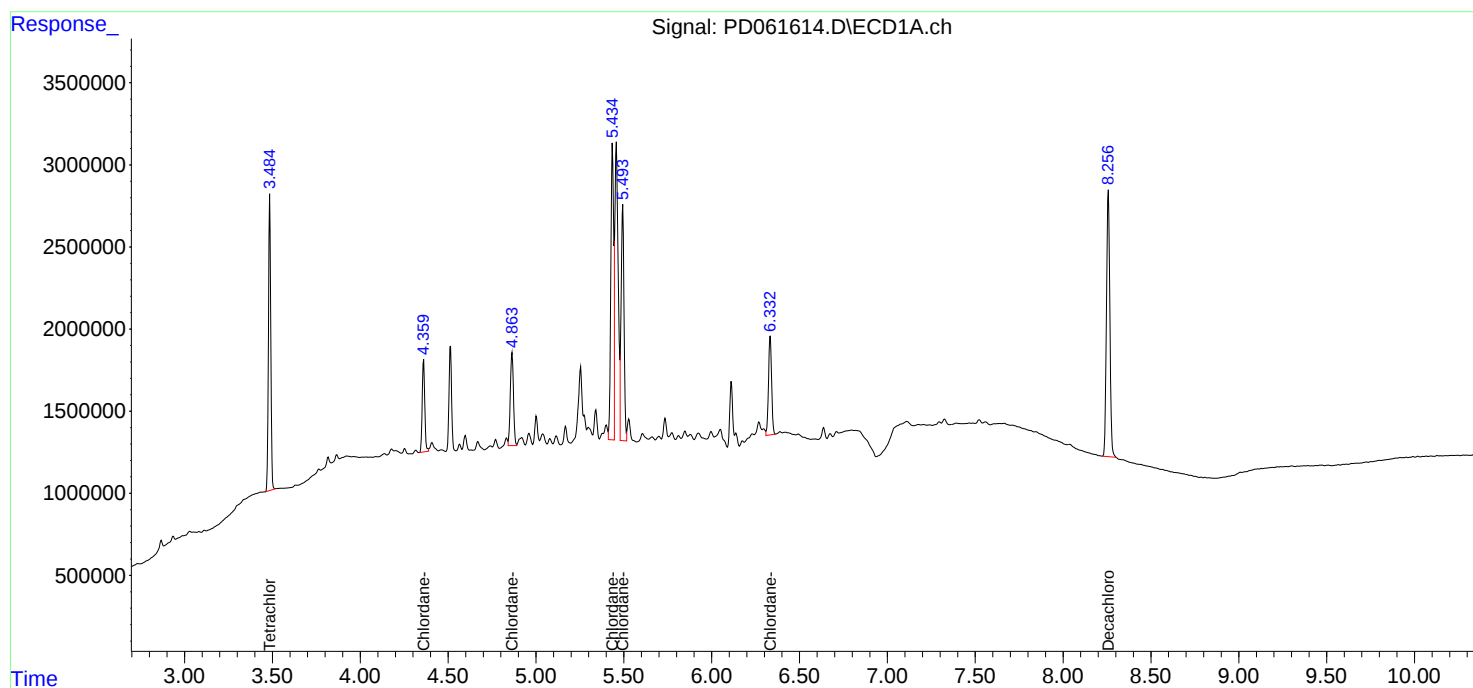


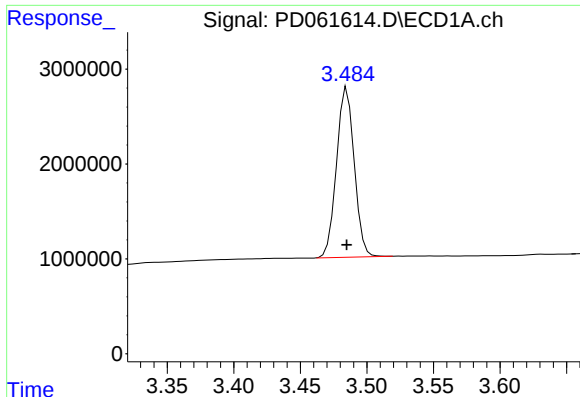

#1 Tetrachloro-m-xylene


R.T.: 3.485 min
Delta R.T.: 0.000 min
Response: 16587534
Conc: 21.26 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB135087BS

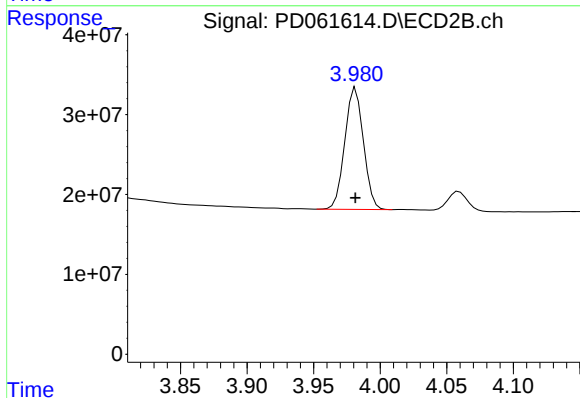


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 148454099
Conc: 19.40 ng/ml

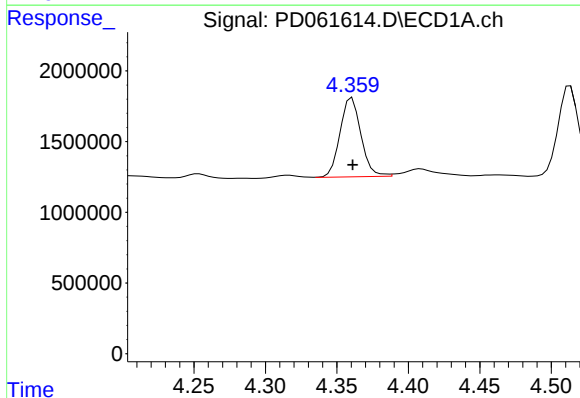


#23 Chlordane-1

R.T.: 4.361 min
Delta R.T.: 0.000 min
Response: 5689822
Conc: 200.28 ng/ml

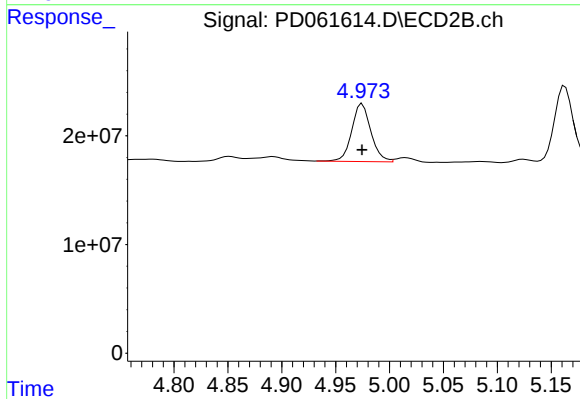

#23 Chlordane-1


R.T.: 4.975 min
Delta R.T.: 0.000 min
Response: 65910058
Conc: 212.37 ng/ml

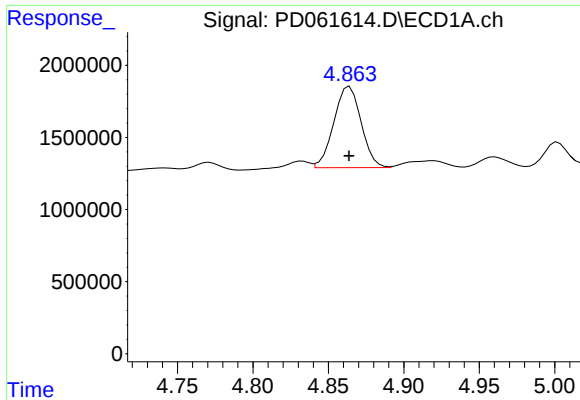

#24 Chlordane-2


R.T.: 4.864 min
Delta R.T.: 0.000 min
Response: 7086378
Conc: 209.74 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB135087BS

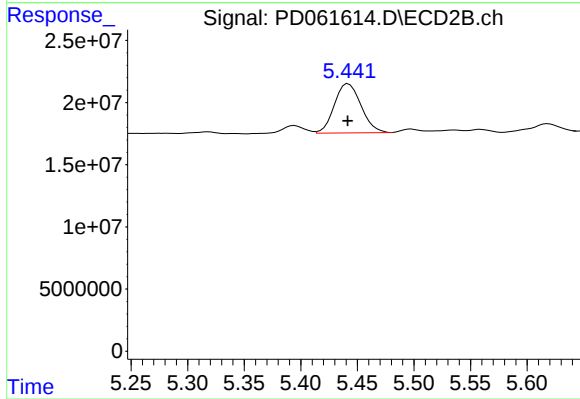


#24 Chlordane-2

R.T.: 5.442 min
Delta R.T.: 0.000 min
Response: 64932083
Conc: 205.07 ng/ml

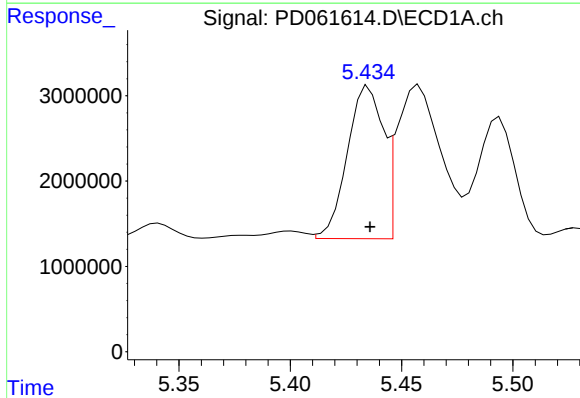


#25 Chlordane-3

R.T.: 5.435 min
Delta R.T.: 0.000 min
Response: 20012405
Conc: 192.24 ng/ml

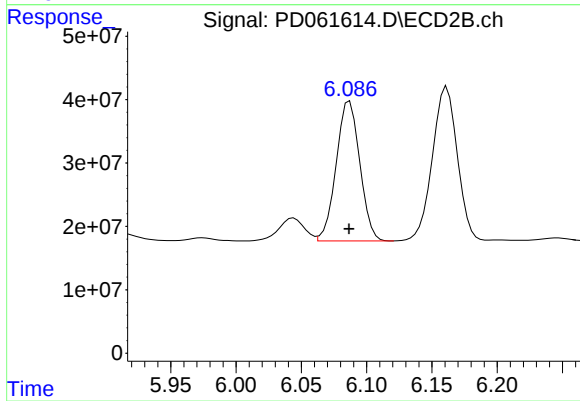

#25 Chlordane-3


R.T.: 6.087 min
Delta R.T.: 0.000 min
Response: 277794386
Conc: 197.76 ng/ml

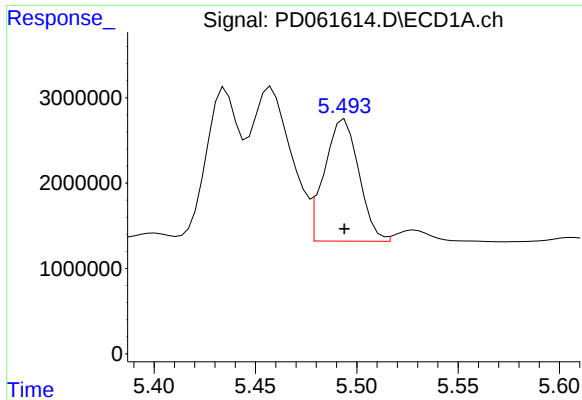

#26 Chlordane-4


R.T.: 5.494 min
Delta R.T.: 0.000 min
Response: 16908363
Conc: 196.26 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB135087BS

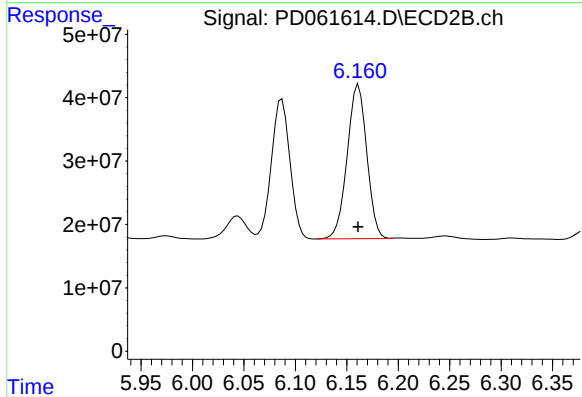


#26 Chlordane-4

R.T.: 6.162 min
Delta R.T.: 0.000 min
Response: 322573945
Conc: 199.16 ng/ml

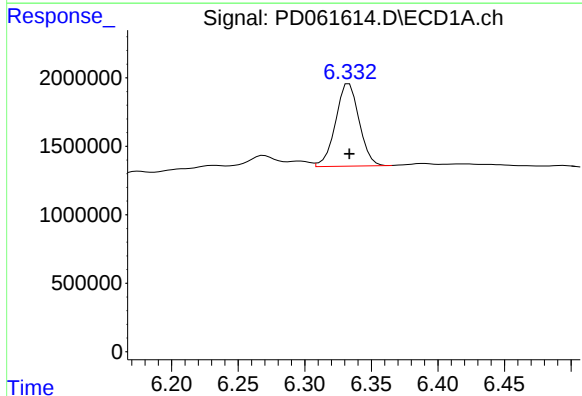


#27 Chlordane-5

R.T.: 6.333 min
Delta R.T.: 0.000 min
Response: 7417576
Conc: 194.82 ng/ml

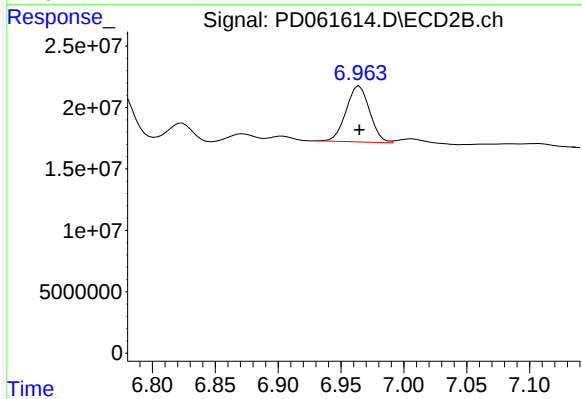

#27 Chlordane-5


R.T.: 6.965 min
Delta R.T.: 0.000 min
Response: 59341201
Conc: 194.61 ng/ml

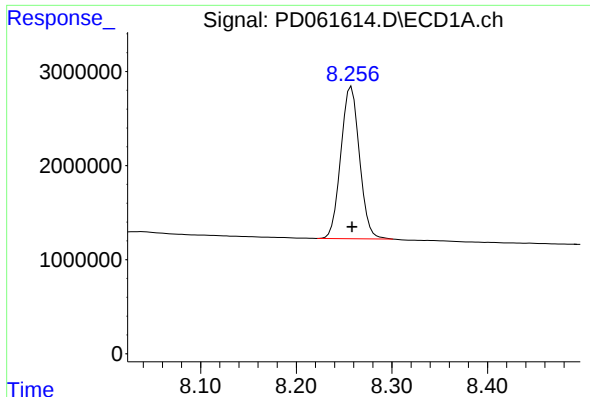

#28 Decachlorobiphenyl

R.T.: 8.258 min
Delta R.T.: 0.000 min
Response: 21943495
Conc: 19.43 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB135087BS

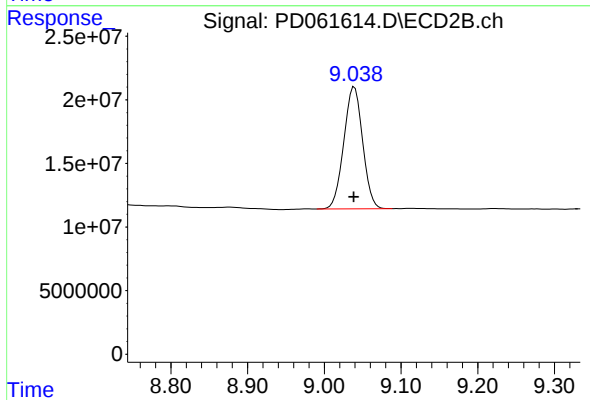

#28 Decachlorobiphenyl

R.T.: 9.039 min
Delta R.T.: 0.000 min
Response: 164281672
Conc: 19.62 ng/ml