

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031521\
 Data File : PD061615.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2021 00:06
 Operator : AR\AJ
 Sample : M1557-11
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PT-CHLR-WP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 09:00:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031521.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 16 02:33:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.484	3.981	25274943	178.8E6	32.389	23.366 #
28)	SA Decachlor...	8.257	9.038	26553326	198.5E6	23.512	23.706
Target Compounds							
23)	Chlordane-1	4.361	4.975	24932981	288.9E6	877.637	931.006
24)	Chlordane-2	4.864	5.442	29351172	274.3E6	868.718	866.321
25)	Chlordane-3	5.435	6.087	103.2E6	1180.4E6	991.222	840.335
26)	Chlordane-4	5.494	6.161	83309413	1321.0E6	967.008	815.615
27)	Chlordane-5	6.333	6.965	29984009	248.2E6	787.514	814.086



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031521\
Data File : PD061615.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2021 00:06
Operator : AR\AJ
Sample : M1557-11
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PT-CHLR-WP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 09:00:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031521.M
Quant Title : GC Extractables
QLast Update : Tue Mar 16 02:33:48 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

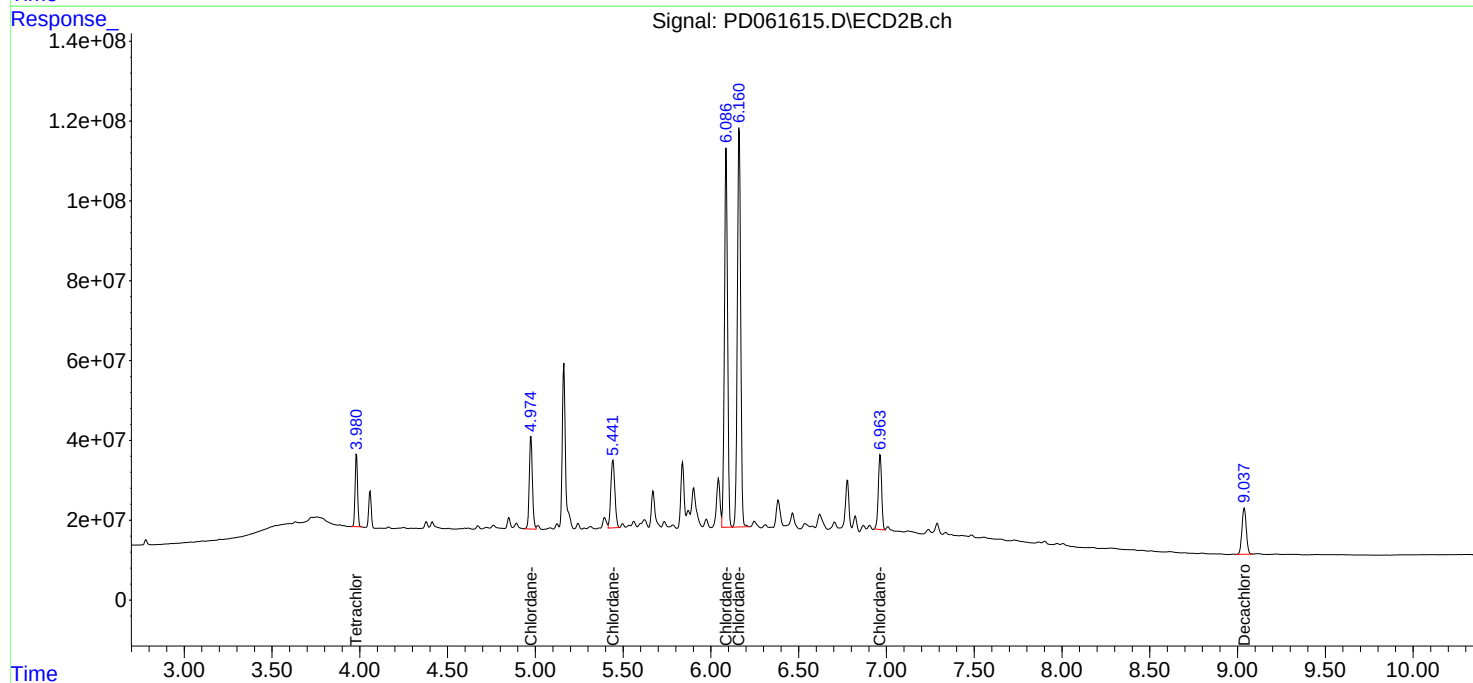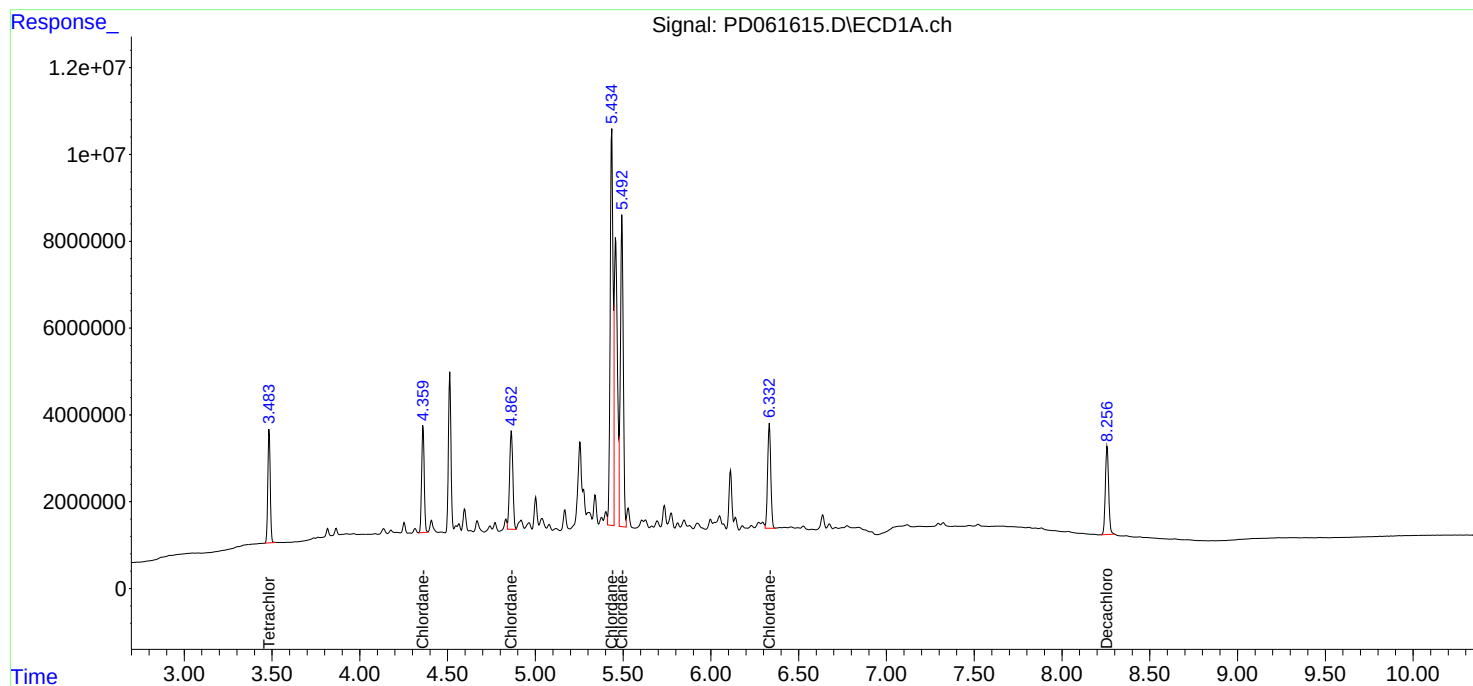


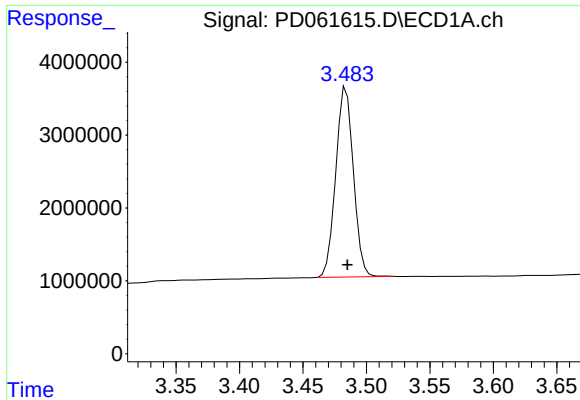

#1 Tetrachloro-m-xylene


R.T.: 3.484 min
Delta R.T.: 0.000 min
Response: 25274943
Conc: 32.39 ng/ml

Instrument :
ECD_D
ClientSampleId :
PT-CHLR-WP

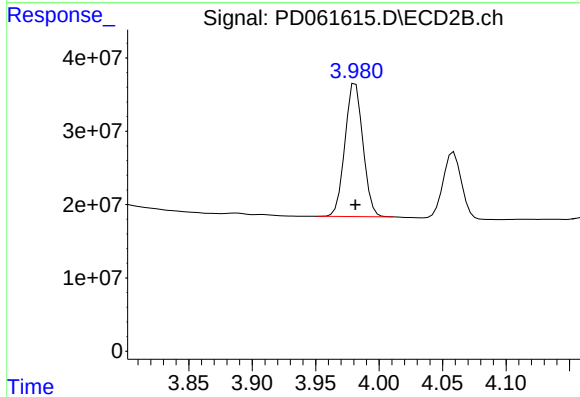


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 178843225
Conc: 23.37 ng/ml

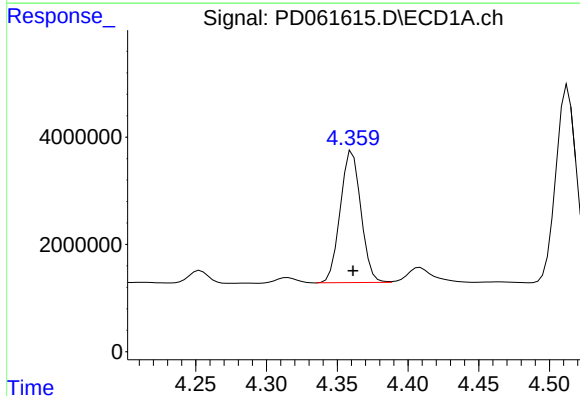


#23 Chlordane-1

R.T.: 4.361 min
Delta R.T.: 0.000 min
Response: 24932981
Conc: 877.64 ng/ml

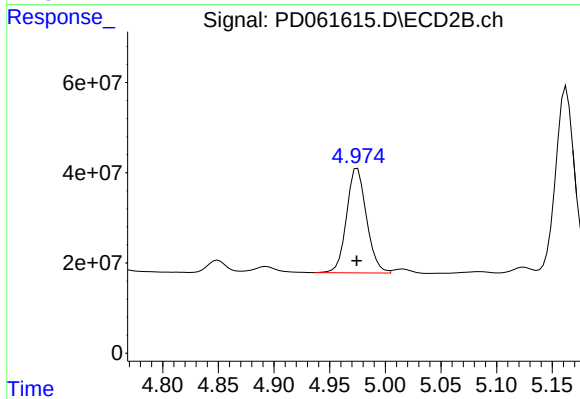

#23 Chlordane-1


R.T.: 4.975 min
Delta R.T.: 0.000 min
Response: 288938027
Conc: 931.01 ng/ml

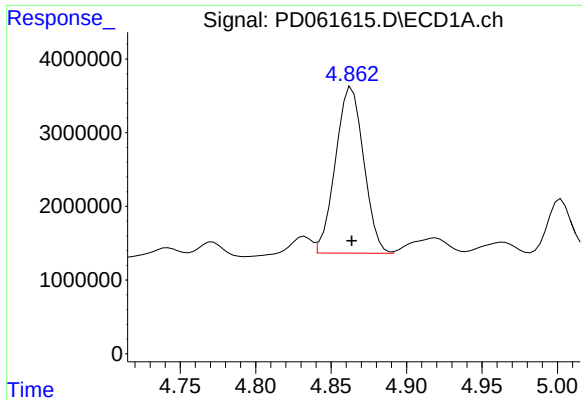

#24 Chlordane-2


R.T.: 4.864 min
Delta R.T.: 0.000 min
Response: 29351172
Conc: 868.72 ng/ml

Instrument :
ECD_D
ClientSampleId :
PT-CHLR-WP

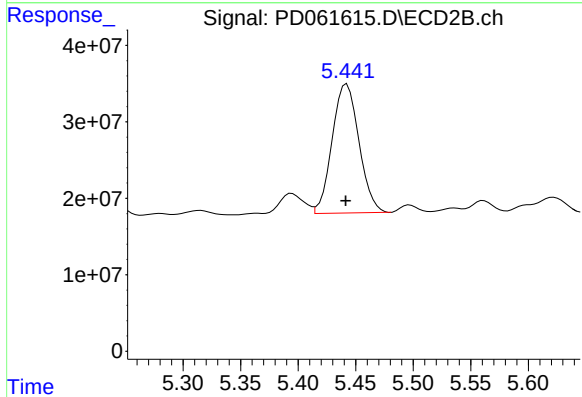


#24 Chlordane-2

R.T.: 5.442 min
Delta R.T.: 0.000 min
Response: 274311051
Conc: 866.32 ng/ml

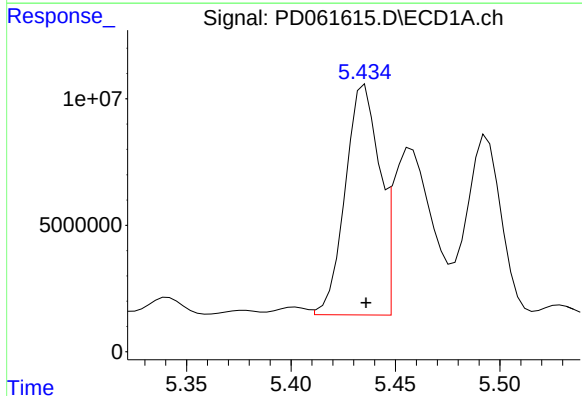


#25 Chlordane-3

R.T.: 5.435 min
Delta R.T.: 0.000 min
Response: 103185060
Conc: 991.22 ng/ml

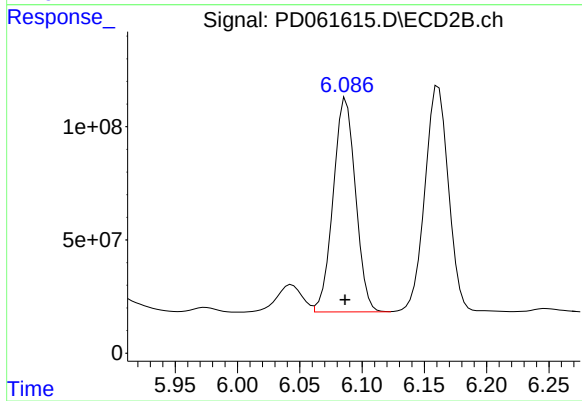

#25 Chlordane-3


R.T.: 6.087 min
Delta R.T.: 0.000 min
Response: 1180436868
Conc: 840.34 ng/ml

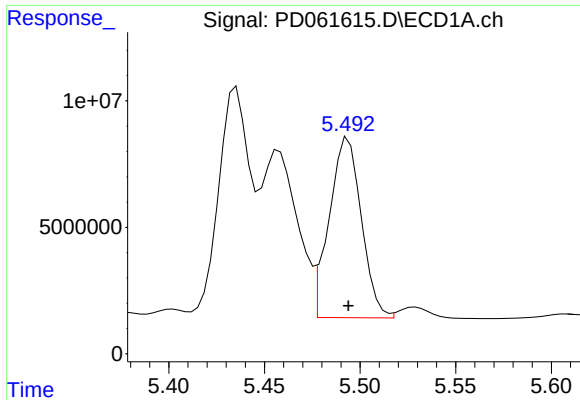

#26 Chlordane-4


R.T.: 5.494 min
Delta R.T.: 0.000 min
Response: 83309413
Conc: 967.01 ng/ml

Instrument :
ECD_D
ClientSampleId :
PT-CHLR-WP

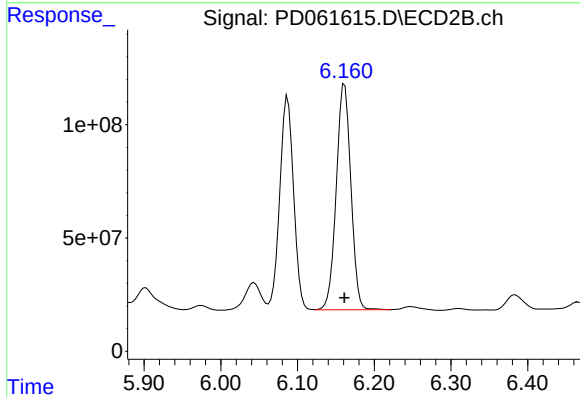


#26 Chlordane-4

R.T.: 6.161 min
Delta R.T.: 0.000 min
Response: 1321030196
Conc: 815.61 ng/ml

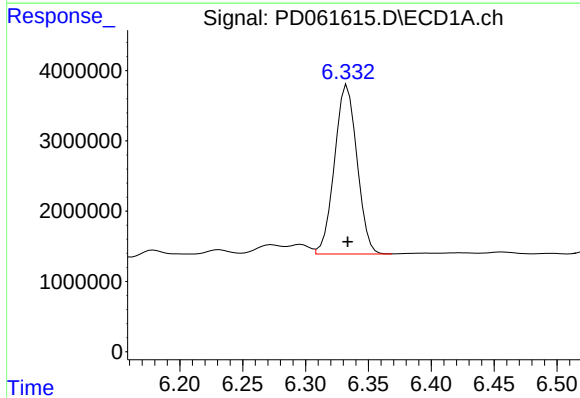


#27 Chlordane-5

R.T.: 6.333 min
Delta R.T.: 0.000 min
Response: 29984009
Conc: 787.51 ng/ml

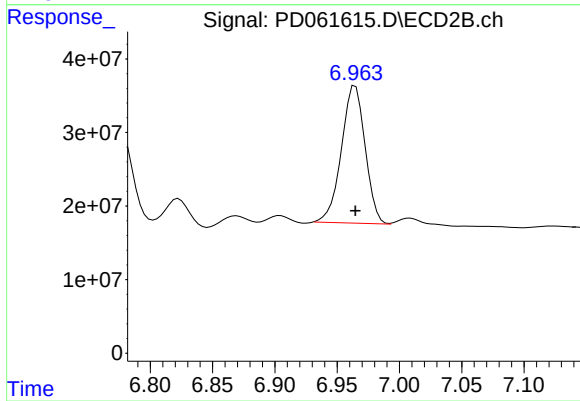

#27 Chlordane-5


R.T.: 6.965 min
Delta R.T.: 0.000 min
Response: 248228693
Conc: 814.09 ng/ml

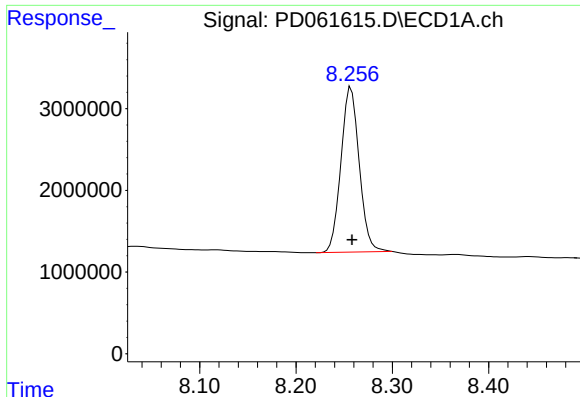

#28 Decachlorobiphenyl

R.T.: 8.257 min
Delta R.T.: 0.000 min
Response: 26553326
Conc: 23.51 ng/ml

Instrument :
ECD_D
ClientSampleId :
PT-CHLR-WP

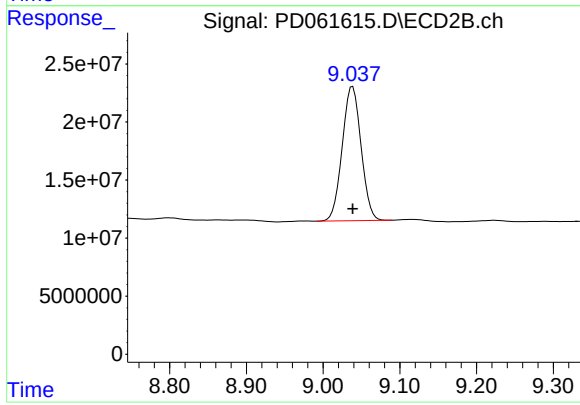

#28 Decachlorobiphenyl

R.T.: 9.038 min
Delta R.T.: 0.000 min
Response: 198472341
Conc: 23.71 ng/ml