

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031521\
 Data File : PD061621.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2021 01:29
 Operator : AR\AJ
 Sample : M1557-13DL 10X
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PT-TXP-WPDL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 04:09:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031521.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 16 02:33:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	3.982	45710418	388.7E6	58.576	50.782
28)	SA Decachlor...	8.258	9.040	55984230	410.4E6	49.572	49.013
Target Compounds							
23)	Chlordane-1	4.361	4.975	15378108	170.4E6	541.307	548.926
24)	Chlordane-2	4.864	5.442	18292067	165.4E6	541.397	522.441
25)	Chlordane-3	5.436	6.087	56226434	742.0E6	540.125	528.195
26)	Chlordane-4	5.494	6.162	45965308	854.8E6	533.539	527.750
27)	Chlordane-5	6.334	6.965	20759621	161.3E6	545.240	529.067



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031521\
Data File : PD061621.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2021 01:29
Operator : AR\AJ
Sample : M1557-13DL 10X
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PT-TXP-WPDL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 04:09:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031521.M
Quant Title : GC Extractables
QLast Update : Tue Mar 16 02:33:48 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

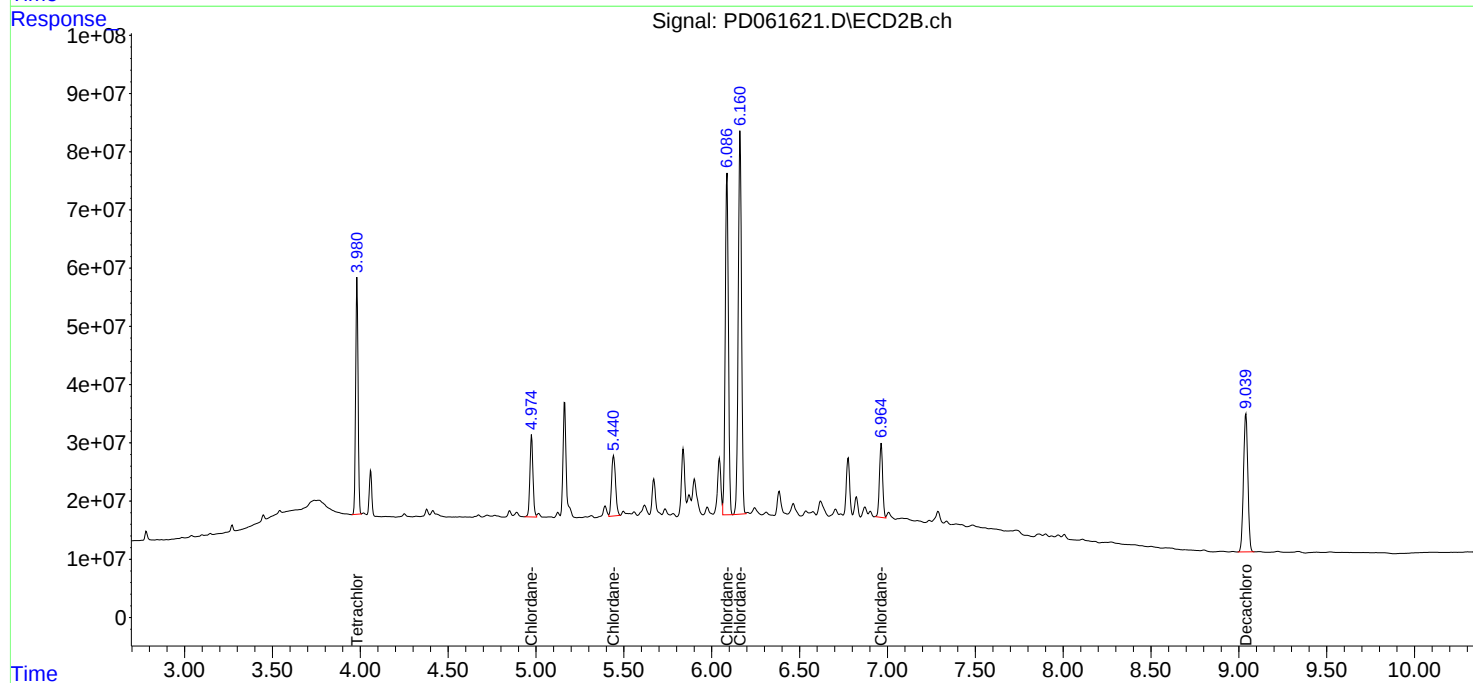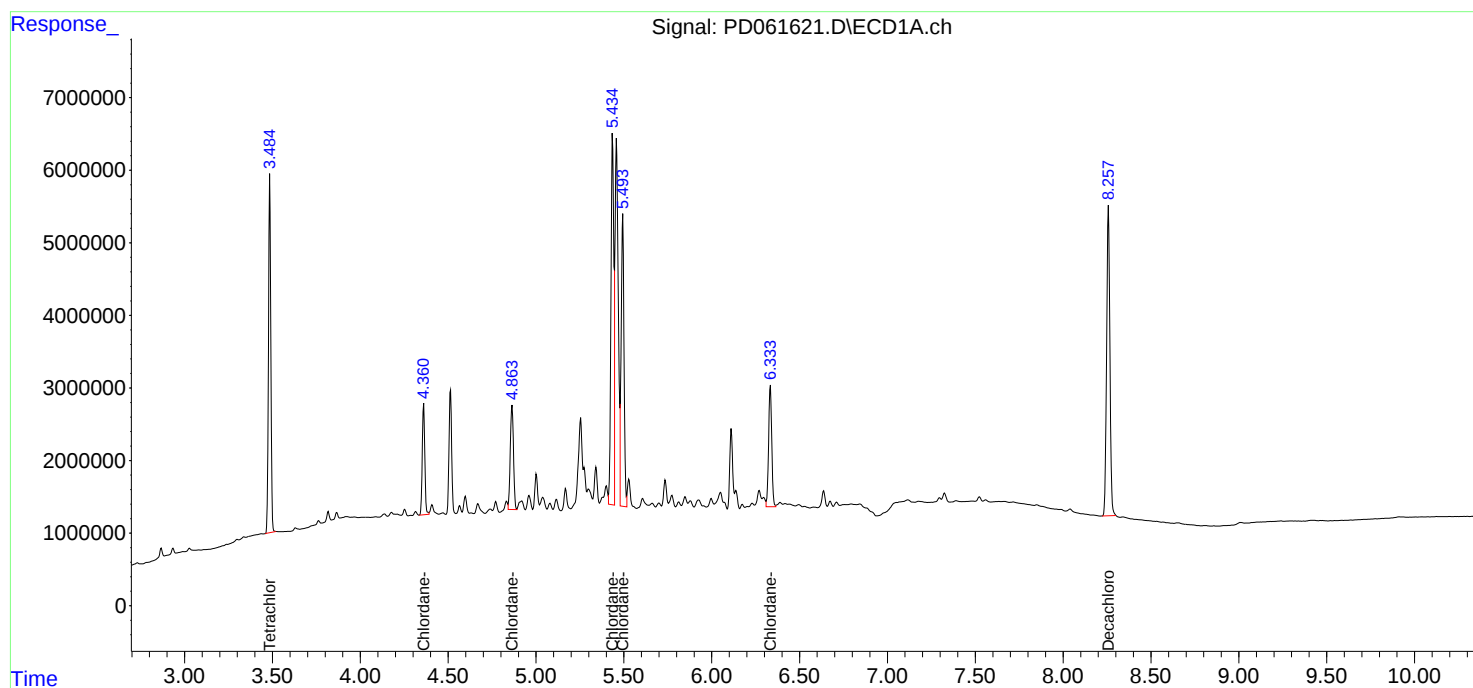


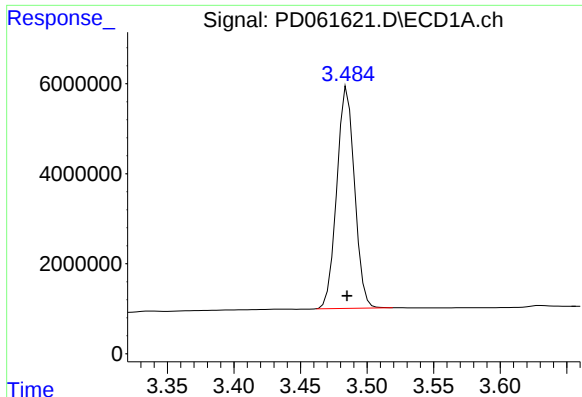

#1 Tetrachloro-m-xylene


R.T.: 3.485 min
Delta R.T.: 0.000 min
Response: 45710418
Conc: 58.58 ng/ml

Instrument :
ECD_D
ClientSampleId :
PT-TXP-WPDL

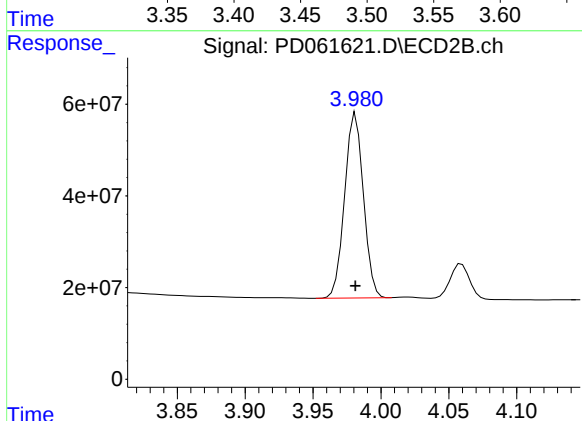


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 388689427
Conc: 50.78 ng/ml

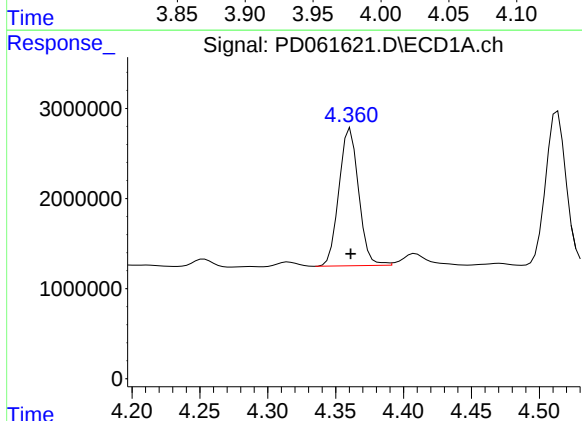


#23 Chlordane-1

R.T.: 4.361 min
Delta R.T.: 0.000 min
Response: 15378108
Conc: 541.31 ng/ml

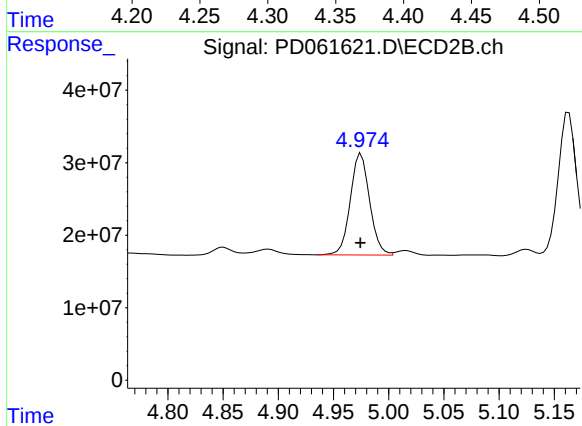

#23 Chlordane-1


R.T.: 4.975 min
Delta R.T.: 0.000 min
Response: 170359292
Conc: 548.93 ng/ml

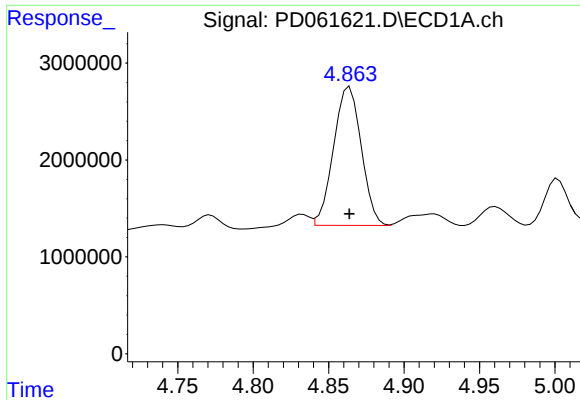

#24 Chlordane-2


R.T.: 4.864 min
Delta R.T.: 0.000 min
Response: 18292067
Conc: 541.40 ng/ml

Instrument :
ECD_D
ClientSampleId :
PT-TXP-WPDL

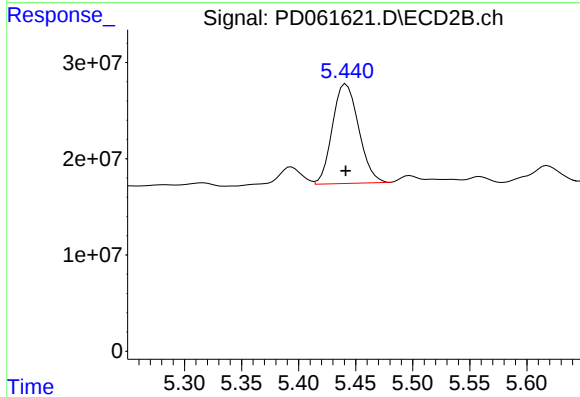


#24 Chlordane-2

R.T.: 5.442 min
Delta R.T.: 0.000 min
Response: 165425176
Conc: 522.44 ng/ml

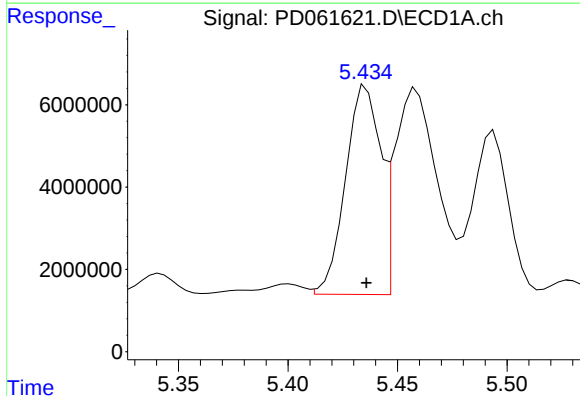


#25 Chlordane-3

R.T.: 5.436 min
Delta R.T.: 0.000 min
Response: 56226434
Conc: 540.13 ng/ml

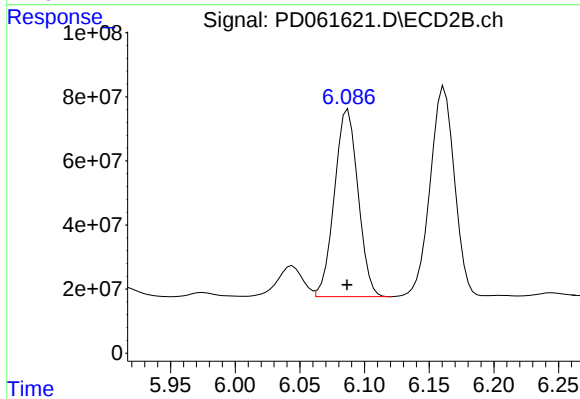

#25 Chlordane-3


R.T.: 6.087 min
Delta R.T.: 0.000 min
Response: 741966661
Conc: 528.20 ng/ml

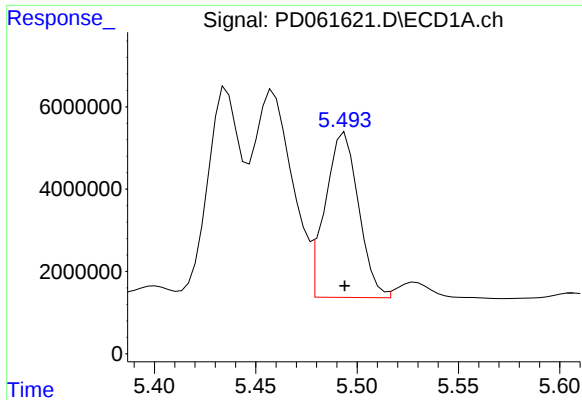

#26 Chlordane-4


R.T.: 5.494 min
Delta R.T.: 0.000 min
Response: 45965308
Conc: 533.54 ng/ml

Instrument :
ECD_D
ClientSampleId :
PT-TXP-WPDL

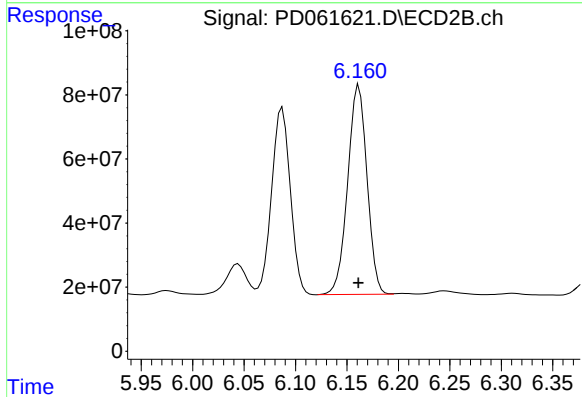


#26 Chlordane-4

R.T.: 6.162 min
Delta R.T.: 0.000 min
Response: 854783301
Conc: 527.75 ng/ml

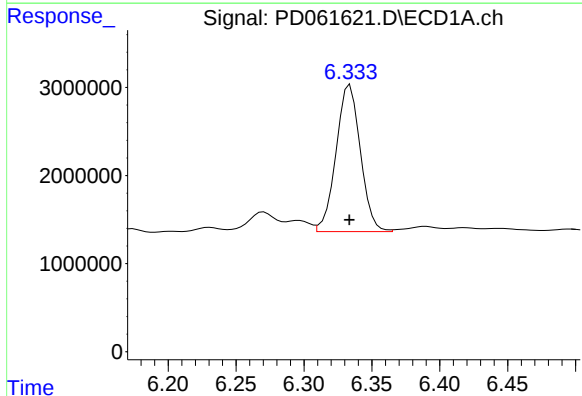


#27 Chlordane-5

R.T.: 6.334 min
Delta R.T.: 0.000 min
Response: 20759621
Conc: 545.24 ng/ml

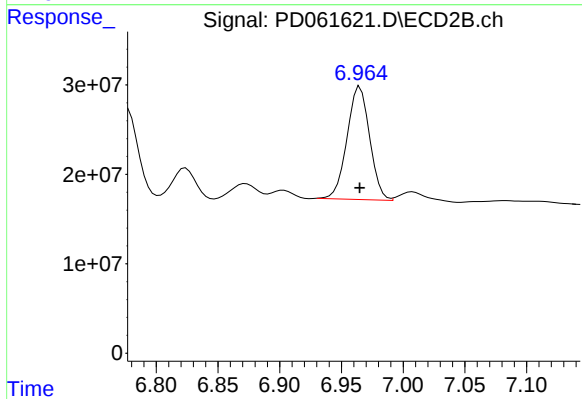

#27 Chlordane-5


R.T.: 6.965 min
Delta R.T.: 0.000 min
Response: 161321582
Conc: 529.07 ng/ml

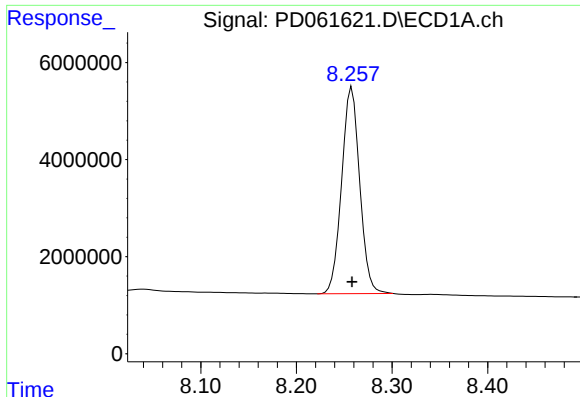

#28 Decachlorobiphenyl

R.T.: 8.258 min
Delta R.T.: 0.000 min
Response: 55984230
Conc: 49.57 ng/ml

Instrument :
ECD_D
ClientSampleId :
PT-TXP-WPDL

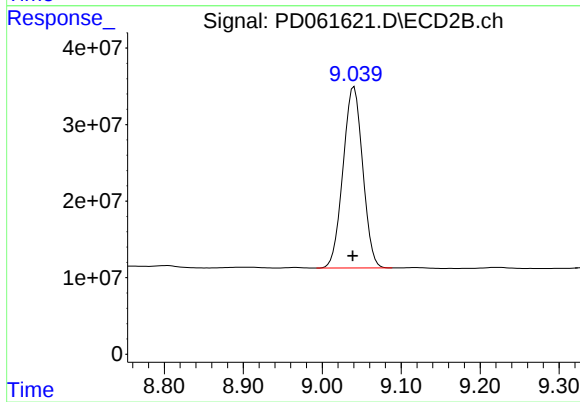

#28 Decachlorobiphenyl

R.T.: 9.040 min
Delta R.T.: 0.002 min
Response: 410352072
Conc: 49.01 ng/ml