

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031621\
 Data File : PD061642.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2021 13:46
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 05:56:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031521.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 16 02:33:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.486	3.982	43231381	371.1E6	55.399	48.485
28)	SA Decachlor...	8.258	9.039	52586495	384.9E6	46.564	45.969
Target Compounds							
23)	Chlordane-1	4.361	4.975	14589856	161.5E6	513.561	520.459
24)	Chlordane-2	4.865	5.442	17747678	157.8E6	525.285	498.253
25)	Chlordane-3	5.436	6.087	53145183	704.0E6	510.526	501.192
26)	Chlordane-4	5.495	6.162	43741457	806.7E6	507.726	498.037
27)	Chlordane-5	6.333	6.965	20266915	149.6E6	532.300	490.577



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031621\
Data File : PD061642.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2021 13:46
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 05:56:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031521.M
Quant Title : GC Extractables
QLast Update : Tue Mar 16 02:33:48 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

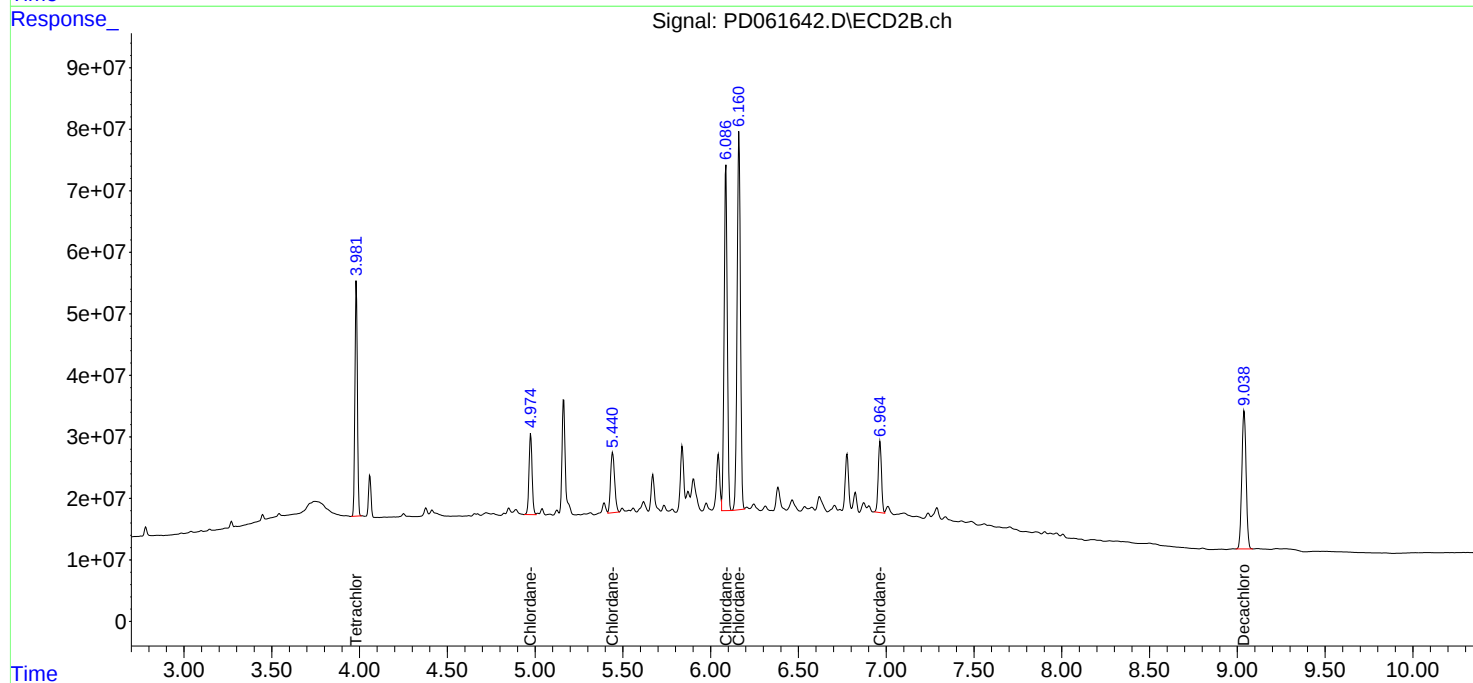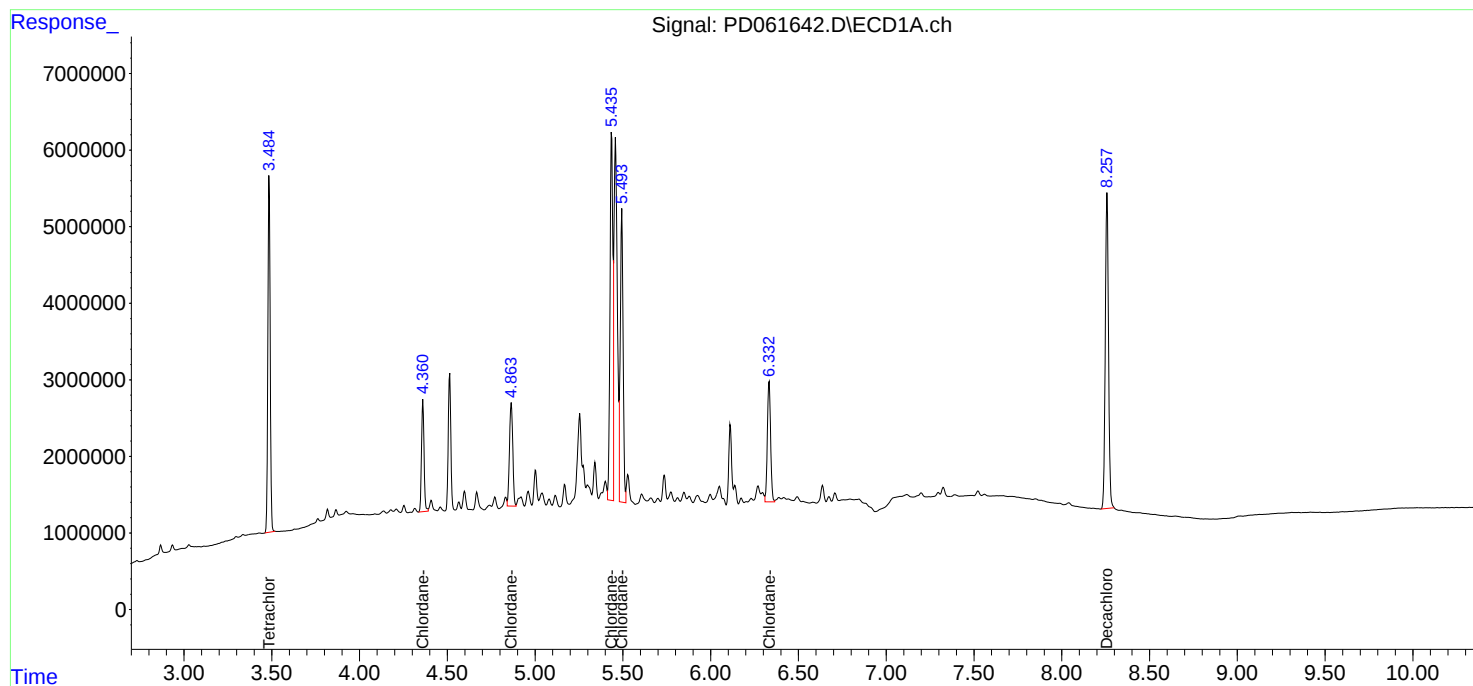


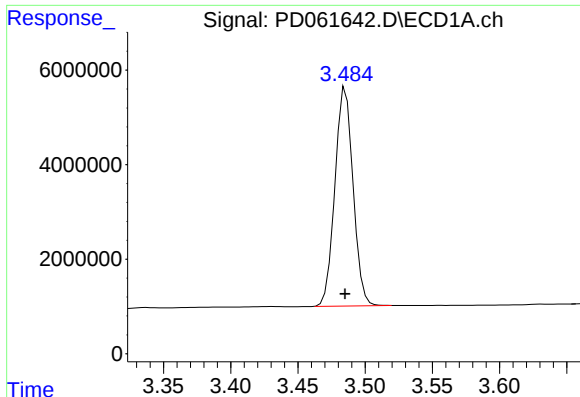

#1 Tetrachloro-m-xylene


R.T.: 3.486 min
Delta R.T.: 0.000 min
Response: 43231381
Conc: 55.40 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

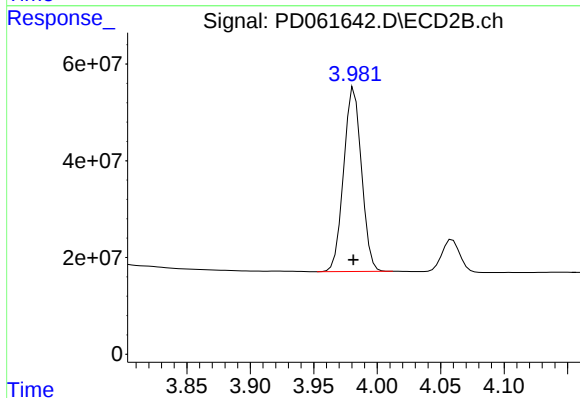


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 371109841
Conc: 48.49 ng/ml

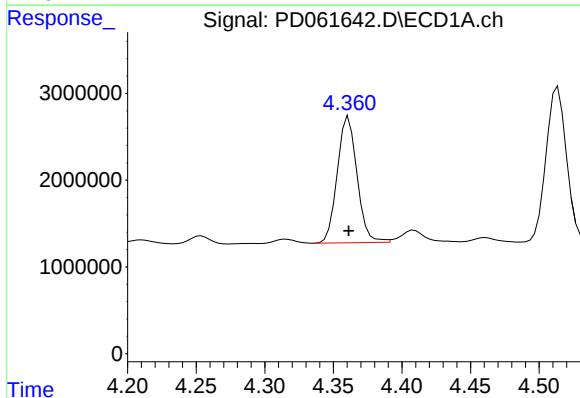


#23 Chlordane-1

R.T.: 4.361 min
Delta R.T.: 0.000 min
Response: 14589856
Conc: 513.56 ng/ml

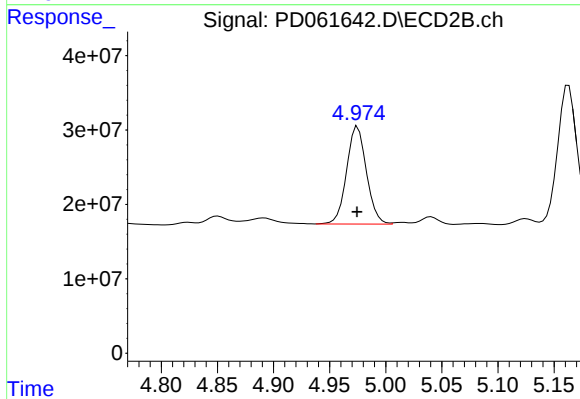

#23 Chlordane-1


R.T.: 4.975 min
Delta R.T.: 0.000 min
Response: 161524491
Conc: 520.46 ng/ml

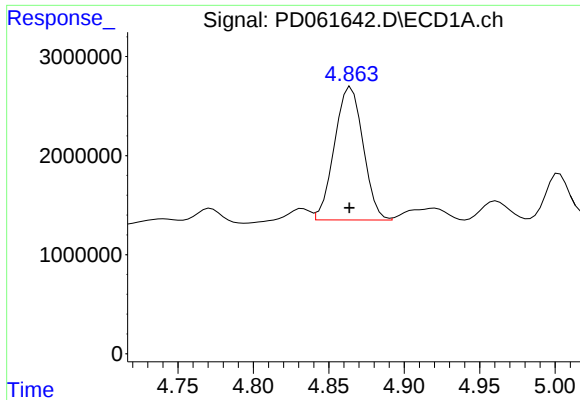

#24 Chlordane-2


R.T.: 4.865 min
Delta R.T.: 0.001 min
Response: 17747678
Conc: 525.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

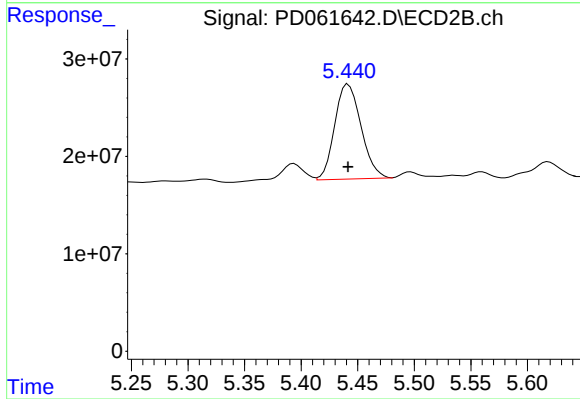


#24 Chlordane-2

R.T.: 5.442 min
Delta R.T.: 0.000 min
Response: 157766367
Conc: 498.25 ng/ml

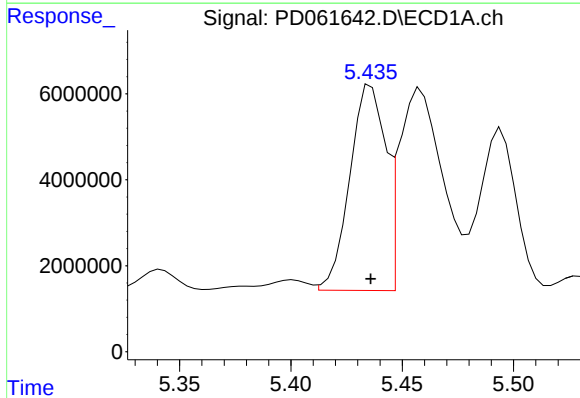


#25 Chlordane-3

R.T.: 5.436 min
Delta R.T.: 0.000 min
Response: 53145183
Conc: 510.53 ng/ml

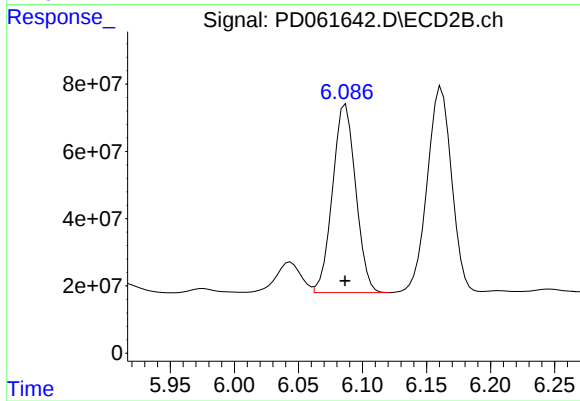

#25 Chlordane-3


R.T.: 6.087 min
Delta R.T.: 0.000 min
Response: 704034995
Conc: 501.19 ng/ml

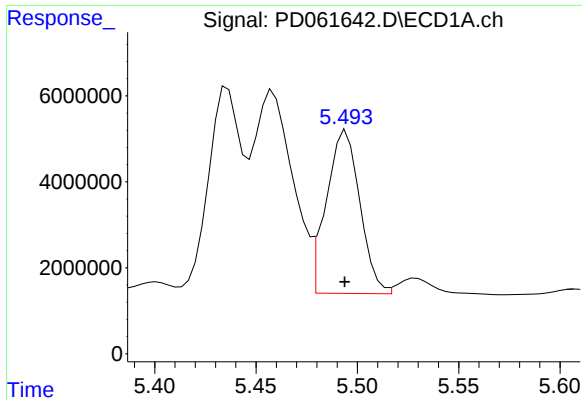

#26 Chlordane-4


R.T.: 5.495 min
Delta R.T.: 0.000 min
Response: 43741457
Conc: 507.73 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

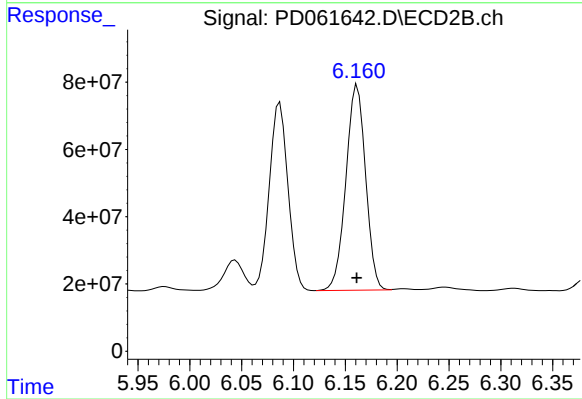


#26 Chlordane-4

R.T.: 6.162 min
Delta R.T.: 0.000 min
Response: 806657456
Conc: 498.04 ng/ml

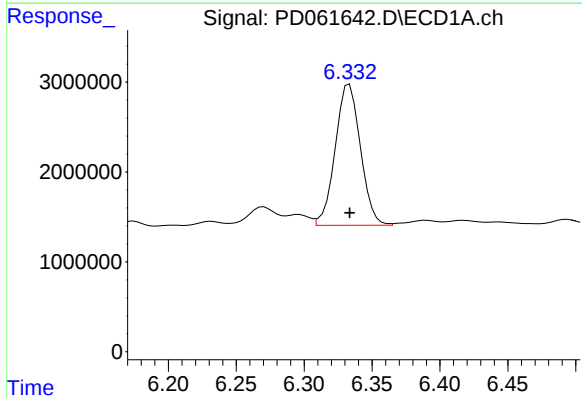


#27 Chlordane-5

R.T.: 6.333 min
Delta R.T.: 0.000 min
Response: 20266915
Conc: 532.30 ng/ml

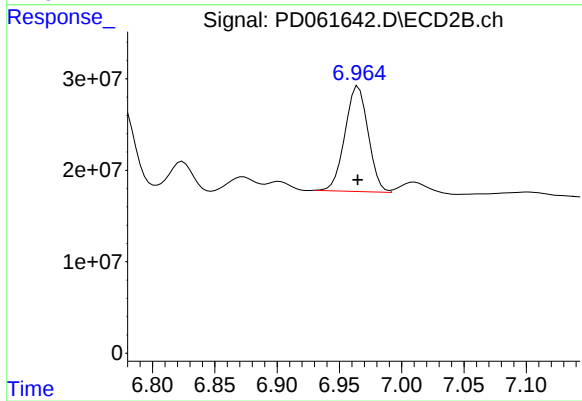

#27 Chlordane-5


R.T.: 6.965 min
Delta R.T.: 0.000 min
Response: 149585409
Conc: 490.58 ng/ml

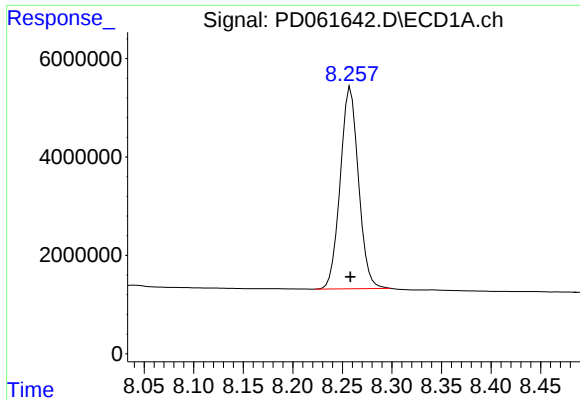

#28 Decachlorobiphenyl

R.T.: 8.258 min
Delta R.T.: 0.000 min
Response: 52586495
Conc: 46.56 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

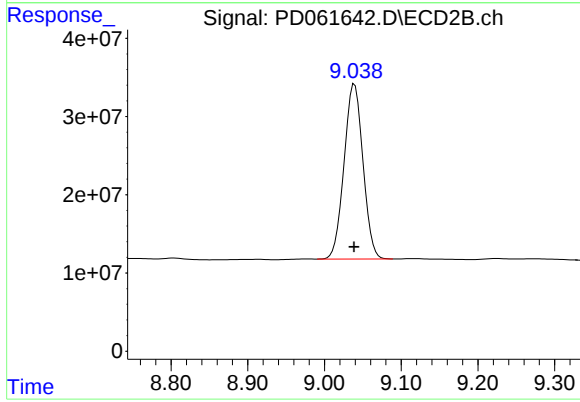

#28 Decachlorobiphenyl

R.T.: 9.039 min
Delta R.T.: 0.000 min
Response: 384866346
Conc: 45.97 ng/ml