

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031622\
 Data File : PD068638.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2022 09:01
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 01:49:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 07:24:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds


Target Compounds						
6) B	beta-BHC	0.000	5.051f	0	365141	N.D. <MDL
8) B	Heptachlo...	0.000	6.075	0	80808605	N.D. 6.709
9) A	Endosulfan I	0.000	6.452	0	1783867	N.D. 0.164
10) B	trans-Chl...	0.000	6.287f	0	4798361	N.D. 0.403
11) B	cis-Chlor...	0.000	6.452f	0	1783867	N.D. 0.156
12) B	4,4'-DDE	0.000	6.619f	0	5302104	N.D. 0.519
14) MA	Endrin	6.015	6.999f	744627	863089	0.527 0.102 #
15) B	Endosulfa...	6.229f	7.091f	2130196	3003955	1.469 0.336 #
16) A	4,4'-DDD	0.000	6.999f	0	863089	N.D. 0.103
20) A	Methoxychlor	0.000	7.744f	0	20861821	N.D. 5.955
22)	Toxaphene-1	0.000	6.619	0	5302104	N.D. 124.603
23)	Toxaphene-2	6.229f	0.000	2130196	0	198.633 N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031622\
Data File : PD068638.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2022 09:01
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 01:49:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 07:24:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

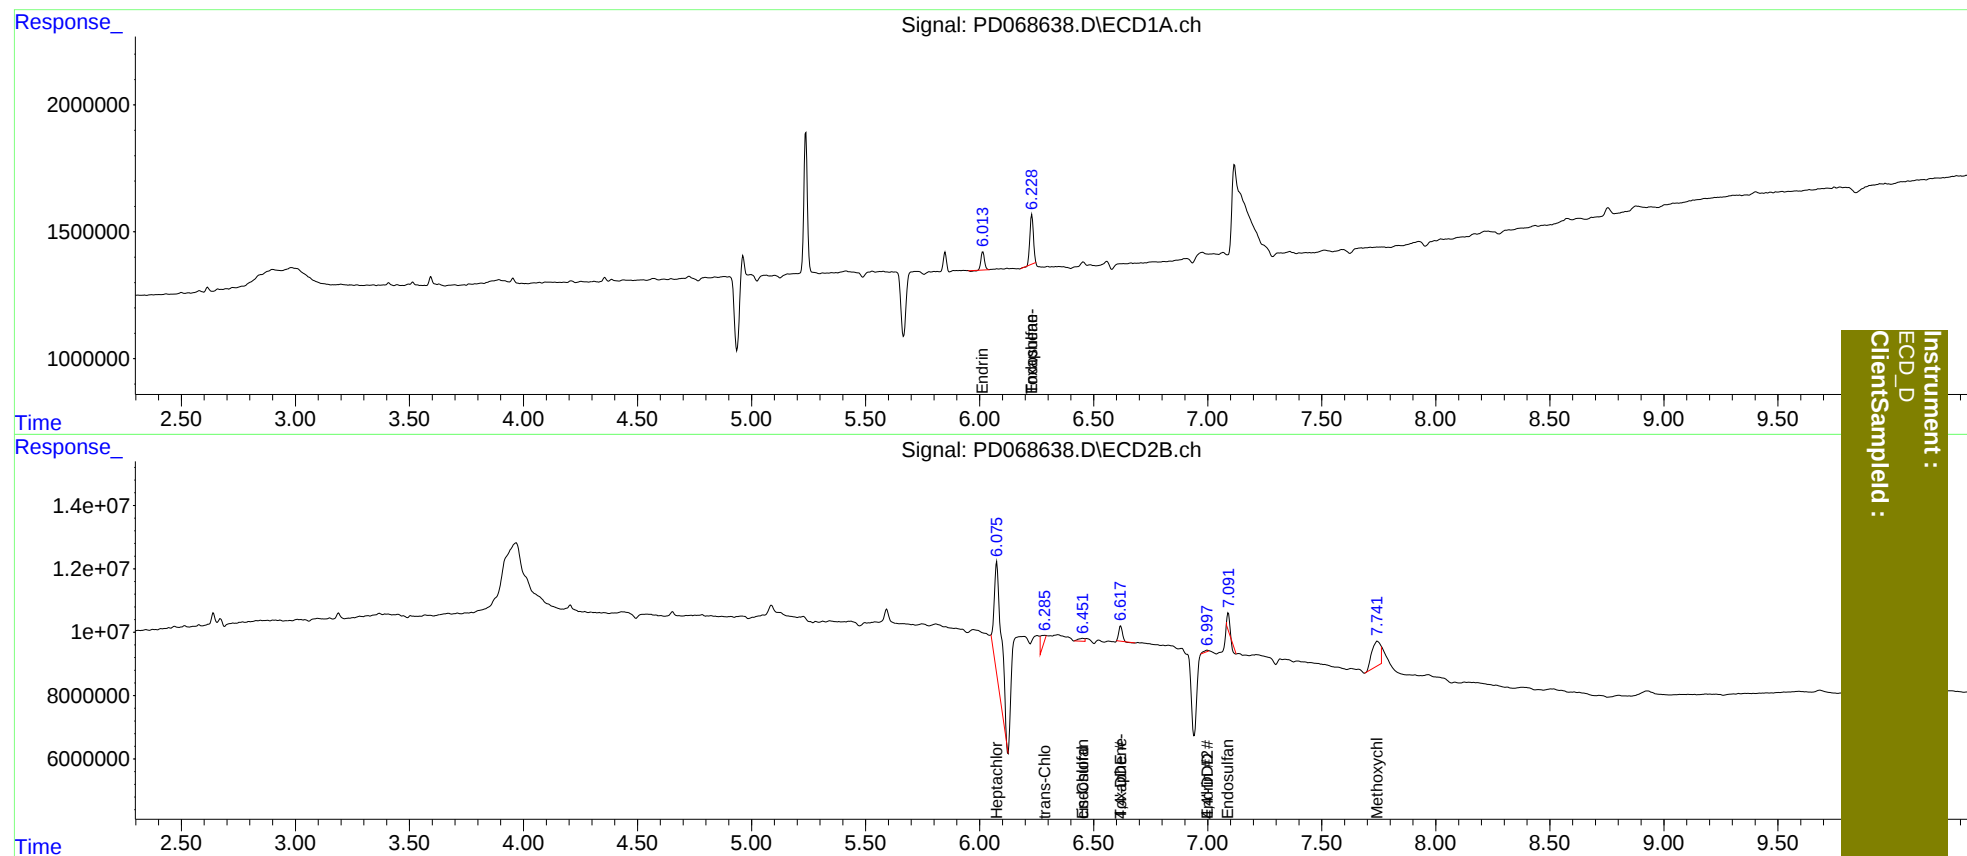


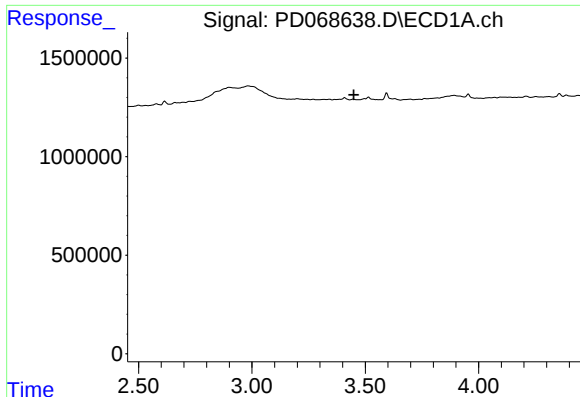

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.449 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

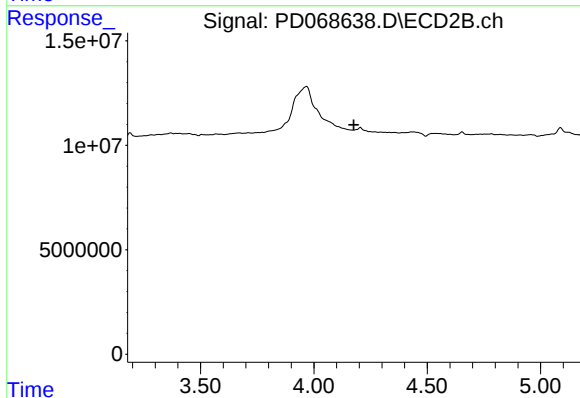


#1 Tetrachloro-m-xylene

R.T.: 4.206 min
Delta R.T.: 0.030 min
Response: -264523
Conc: N.D.

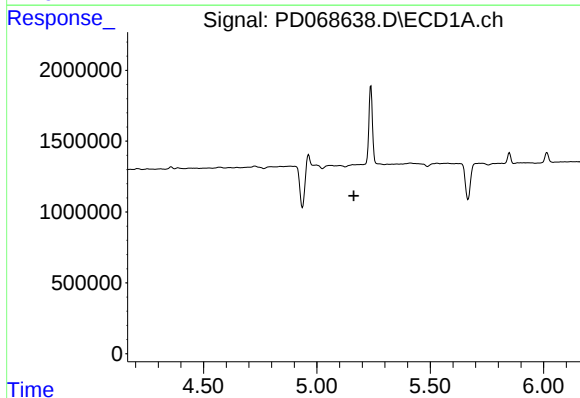


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.163 min
Response: 0
Conc: N.D.

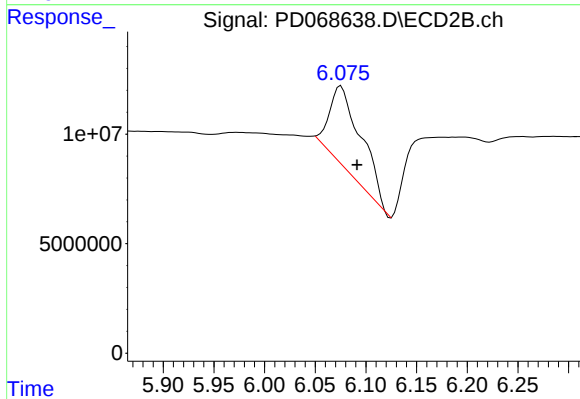

#8 Heptachlor epoxide


R.T.: 6.075 min
Delta R.T.: -0.016 min
Response: 80808605
Conc: 6.71 ng/ml

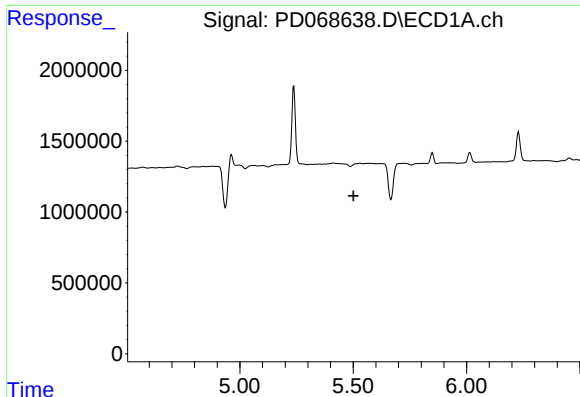

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.502 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

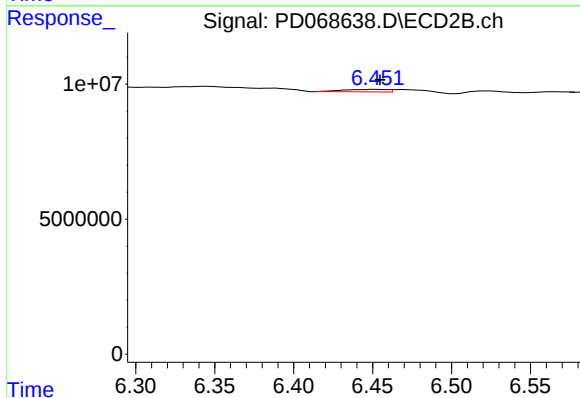


#9 Endosulfan I

R.T.: 6.452 min
Delta R.T.: -0.003 min
Response: 1783867
Conc: 0.16 ng/ml

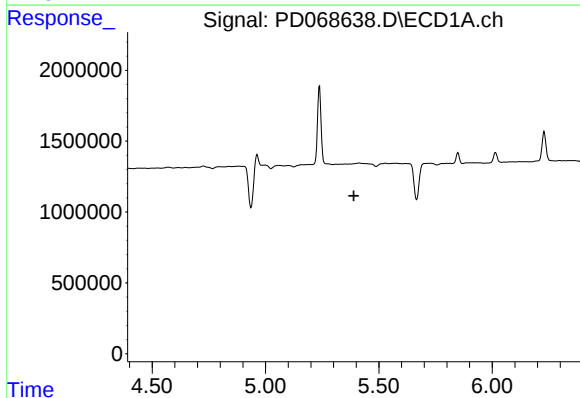


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.389 min
Response: 0
Conc: N.D.

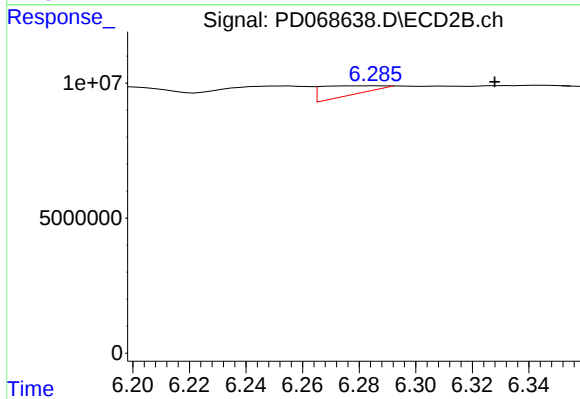

#10 trans-Chlordane


R.T.: 6.287 min
Delta R.T.: -0.041 min
Response: 4798361
Conc: 0.40 ng/ml

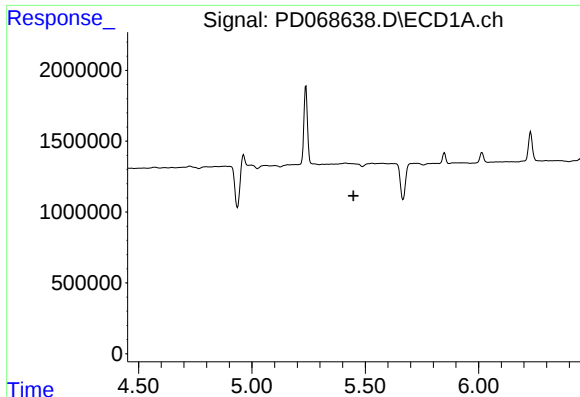

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.448 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

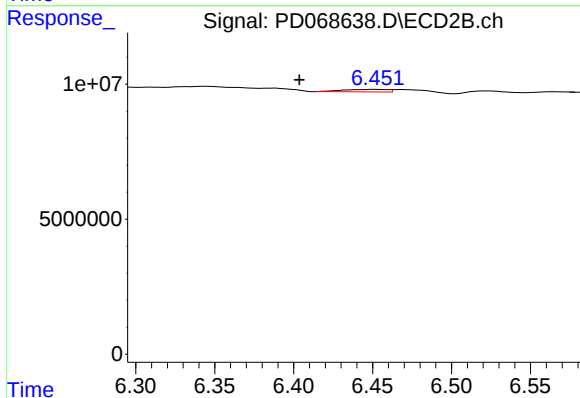


#11 cis-Chlordane

R.T.: 6.452 min
Delta R.T.: 0.048 min
Response: 1783867
Conc: 0.16 ng/ml

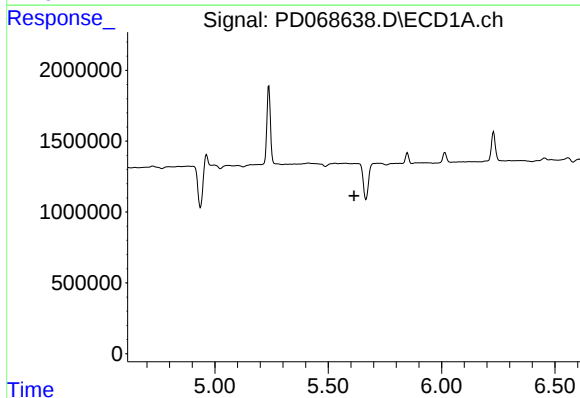


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.614 min
Response: 0
Conc: N.D.

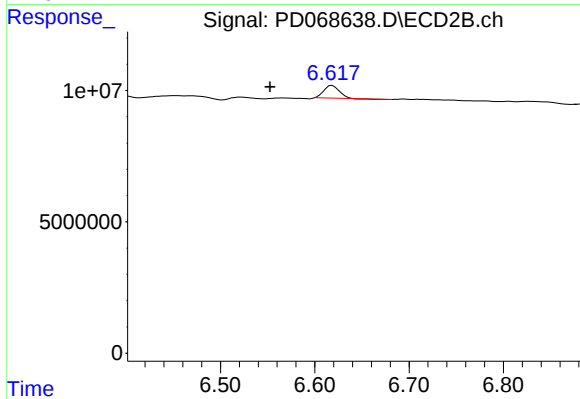

#12 4,4'-DDE


R.T.: 6.619 min
Delta R.T.: 0.066 min
Response: 5302104
Conc: 0.52 ng/ml

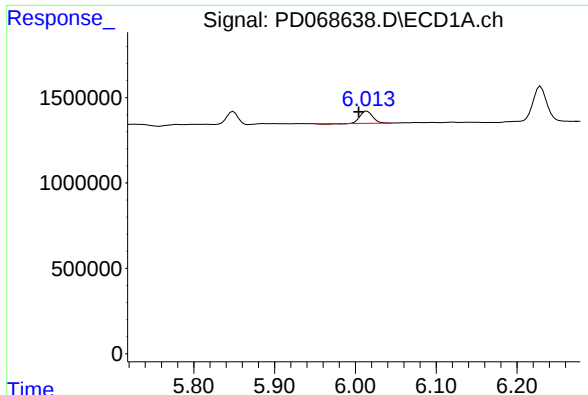

#14 Endrin


R.T.: 6.015 min
Delta R.T.: 0.010 min
Response: 744627
Conc: 0.53 ng/ml

Instrument :
ECD_D
ClientSampleId :

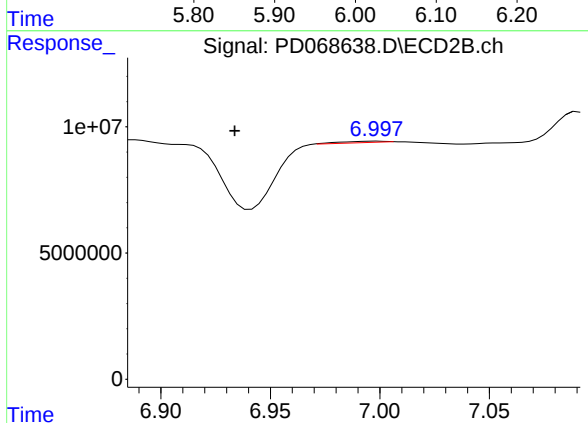


#14 Endrin

R.T.: 6.999 min
Delta R.T.: 0.065 min
Response: 863089
Conc: 0.10 ng/ml

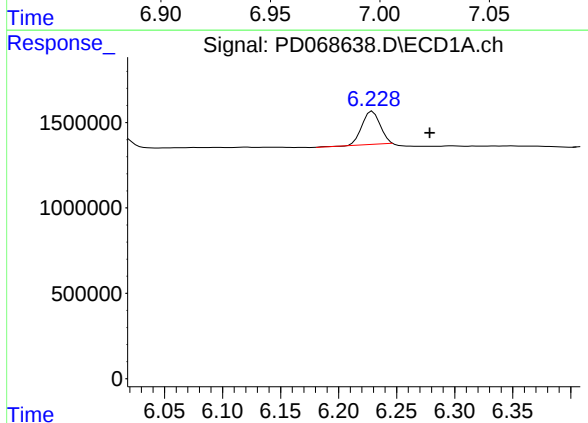


#15 Endosulfan II

R.T.: 6.229 min
Delta R.T.: -0.049 min
Response: 2130196
Conc: 1.47 ng/ml

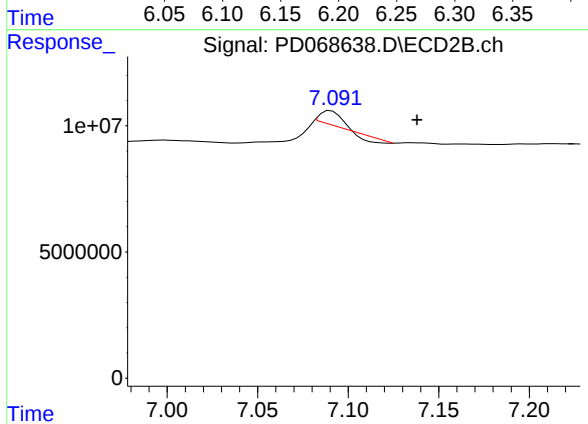

#15 Endosulfan II


R.T.: 7.091 min
Delta R.T.: -0.047 min
Response: 3003955
Conc: 0.34 ng/ml

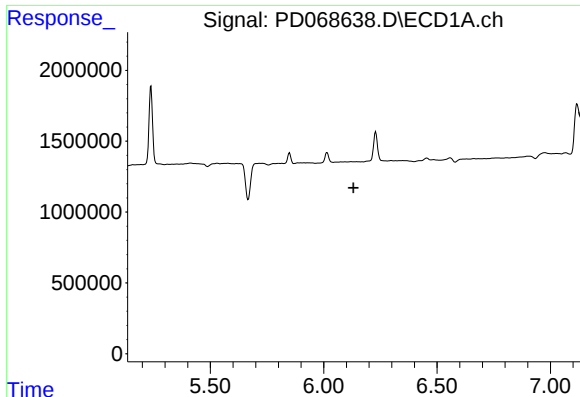

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.132 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

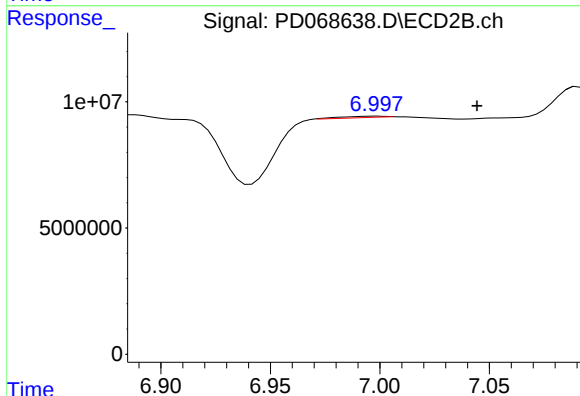


#16 4,4'-DDD

R.T.: 6.999 min
Delta R.T.: -0.046 min
Response: 863089
Conc: 0.10 ng/ml

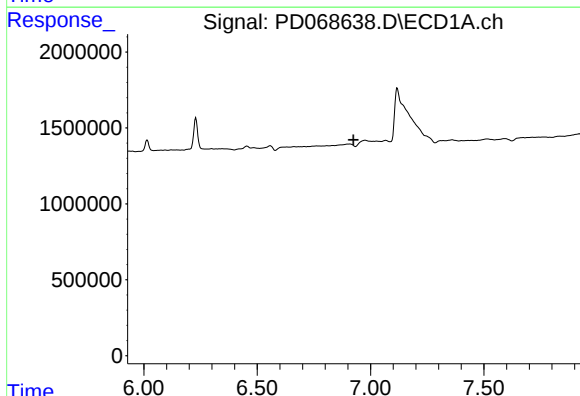


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 6.925 min
Response: 0
Conc: N.D.

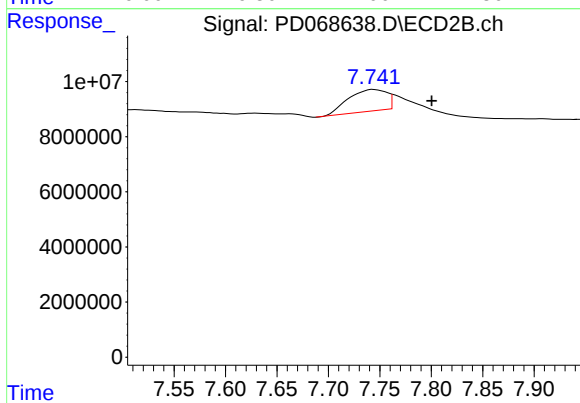

#20 Methoxychlor


R.T.: 7.744 min
Delta R.T.: -0.057 min
Response: 20861821
Conc: 5.96 ng/ml

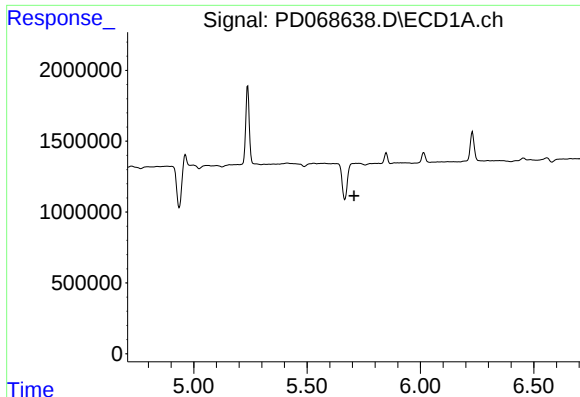

#22 Toxaphene-1


R.T.: 0.000 min
Exp R.T.: 5.708 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

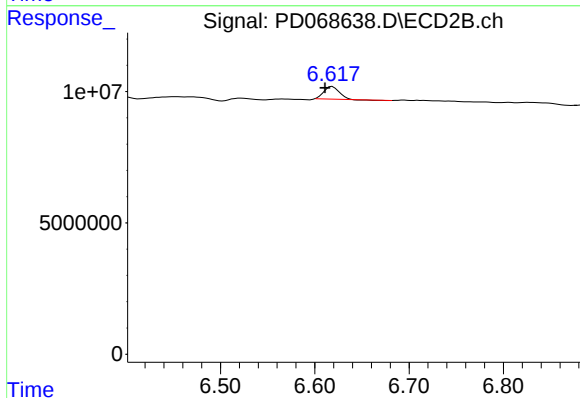


#22 Toxaphene-1

R.T.: 6.619 min
Delta R.T.: 0.008 min
Response: 5302104
Conc: 124.60 ng/ml

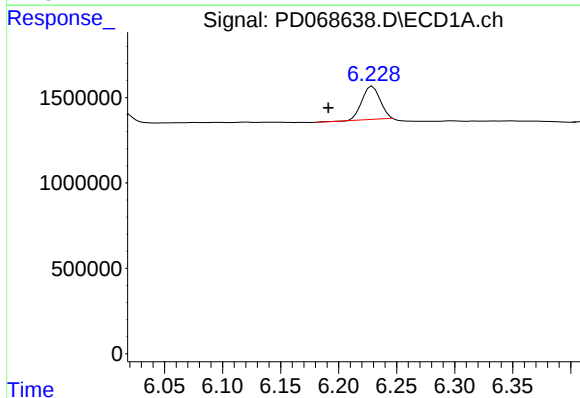


#23 Toxaphene-2

R.T.: 6.229 min
Delta R.T.: 0.038 min
Response: 2130196
Conc: 198.63 ng/ml

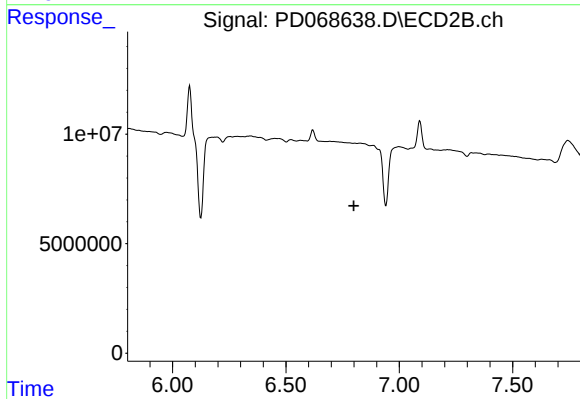

#23 Toxaphene-2


R.T.: 0.000 min
Exp R.T.: 6.799 min
Response: 0
Conc: N.D.

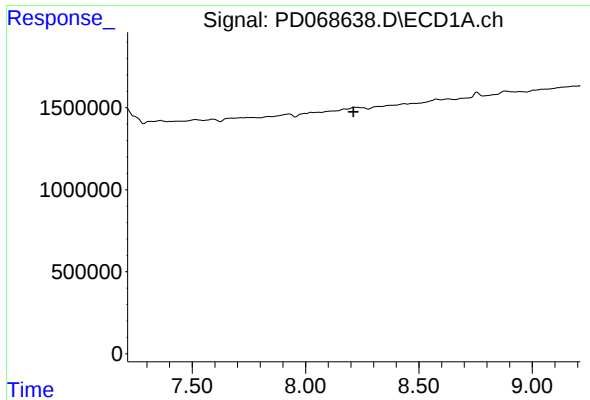

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.212 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

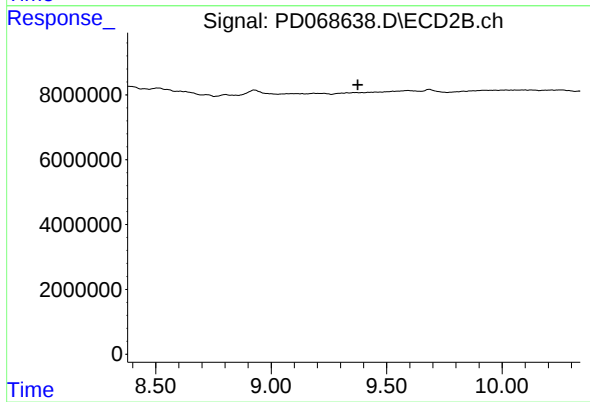

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.375 min
Response: 0
Conc: N.D.