

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031622\
 Data File : PD068641.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2022 11:57
 Operator : AR\AJ
 Sample : PB143352BS
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS352

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/17/2022
 Supervised By : Ankita Jodhani 03/17/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 01:50:30 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 07:24:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.457	4.176	20619096	171.4E6	15.141	15.660
27)	SA Decachlor...	8.217	9.373	43545762	203.3E6	31.316	32.227
Target Compounds							
2)	A alpha-BHC	3.896	4.572	6829813	64116473	3.568	4.101
3)	MA gamma-BHC...	4.180	4.863	9401429	83035425	5.179	5.727
4)	MA Heptachlor	4.479	5.390	8503334	71999727	4.747	5.231
5)	MB Aldrin	4.727	5.703	8313111	70258701	4.727	5.207
6)	B beta-BHC	4.431	5.026	4291279	41550341	5.150	6.506 #
7)	B delta-BHC	4.635	5.251	6595325	60156876	3.730	4.250
8)	B Heptachlo...	5.171	6.091	6827808	59235395	4.204	4.918
9)	A Endosulfan I	5.510	6.454	6726900	50867267	4.369	4.674
10)	B trans-Chl...	5.397	6.327	7181924	54568692	4.303	4.588m
11)	B cis-Chlor...	5.456	6.403	7204025	54633257	4.388	4.763
12)	B 4,4'-DDE	5.623	6.553	12492177	100.2E6	8.398	9.806
13)	MA Dieldrin	5.754	6.712	14442213	109.8E6	8.646	9.880
14)	MA Endrin	6.012	6.932	12181733	75410959	8.616	8.919
15)	B Endosulfa...	6.284	7.136	12994306	86726454	8.959m	9.691m
16)	A 4,4'-DDD	6.140	7.042	11066891	78662939	8.420	9.375m
17)	MA 4,4'-DDT	6.380	7.347	9895730	68325908	7.410	8.669
18)	B Endrin al...	6.456	7.261	11474561	74100437	10.464	11.159
19)	B Endosulfa...	6.669	7.487	11757037	75165870	8.412	9.178
20)	A Methoxychlor	6.932	7.799	30254650	164.9E6	42.743	47.076
21)	B Endrin ke...	7.162	7.961	14305815	85397524	8.966	10.001

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031622\
Data File : PD068641.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2022 11:57
Operator : AR\AJ
Sample : PB143352BS
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 01:50:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 07:24:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

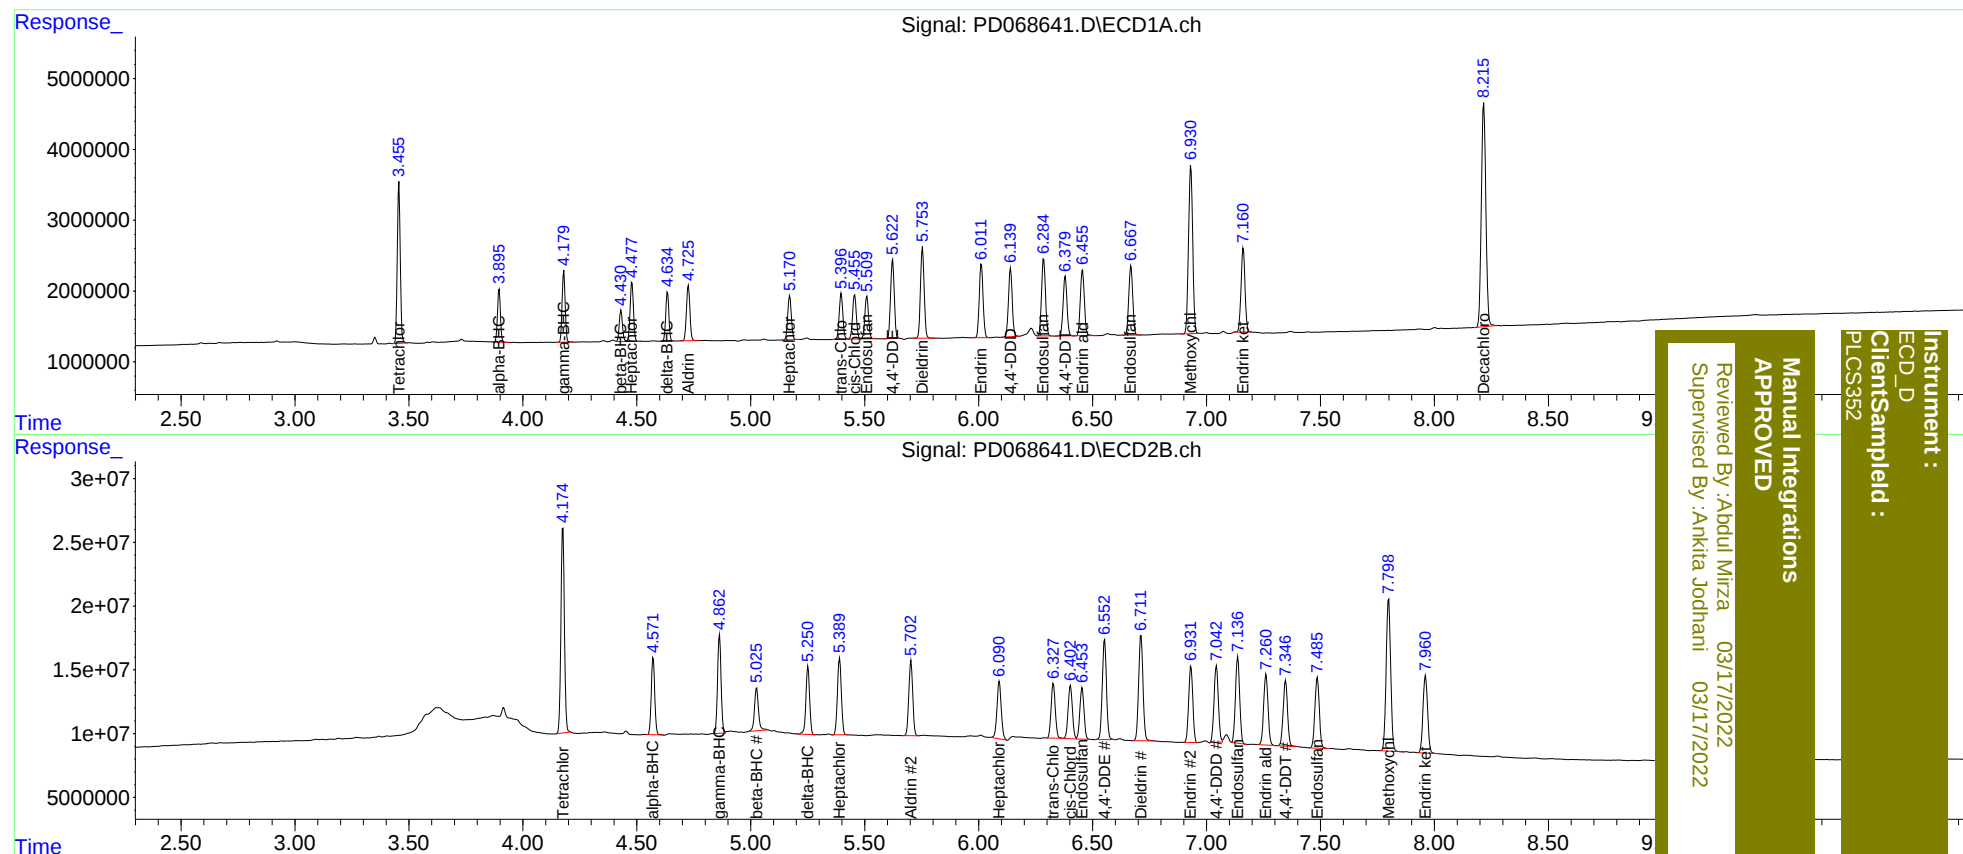

Instrument :
ECD_D
ClientSampled :
PLCS352

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/17/2022
Supervised By :Ankita Jodhani 03/17/2022