

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031623\
 Data File : PD074250.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2023 11:10
 Operator : AR\AJ
 Sample : PB151456BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 21:36:54 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 14 03:05:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.551	2.771	44191803	22250470	17.788	17.686
27)	SA Decachlor...	9.098	7.926	98276766	47070776	35.907	39.311
Target Compounds							
6)	B beta-BHC	4.571f	3.865f	189129	253382	0.112	0.313 #
7)	B delta-BHC	4.779	0.000	2490751	0	0.684	N.D. #
8)	B Heptachlo...	5.698	0.000	1175319	0	0.358	N.D. #
9)	A Endosulfan I	6.104	0.000	350277	0	0.117	N.D. #
11)	B cis-Chlor...	6.104f	0.000	350277	0	0.107	N.D. #
15)	B Endosulfa...	6.790	0.000	266986	0	<MDL	N.D. #
16)	A 4,4'-DDD	6.790f	0.000	266986	0	0.113	N.D. #
20)	A Methoxychlor	7.452f	0.000	180198	0	0.131	N.D. #
21)	B Endrin ke...	7.698	0.000	680909	0	0.230	N.D. #
23)	Toxaphene-2	6.505f	0.000	259196	0	8.740	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031623\
Data File : PD074250.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2023 11:10
Operator : AR\AJ
Sample : PB151456BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 21:36:54 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 14 03:05:06 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

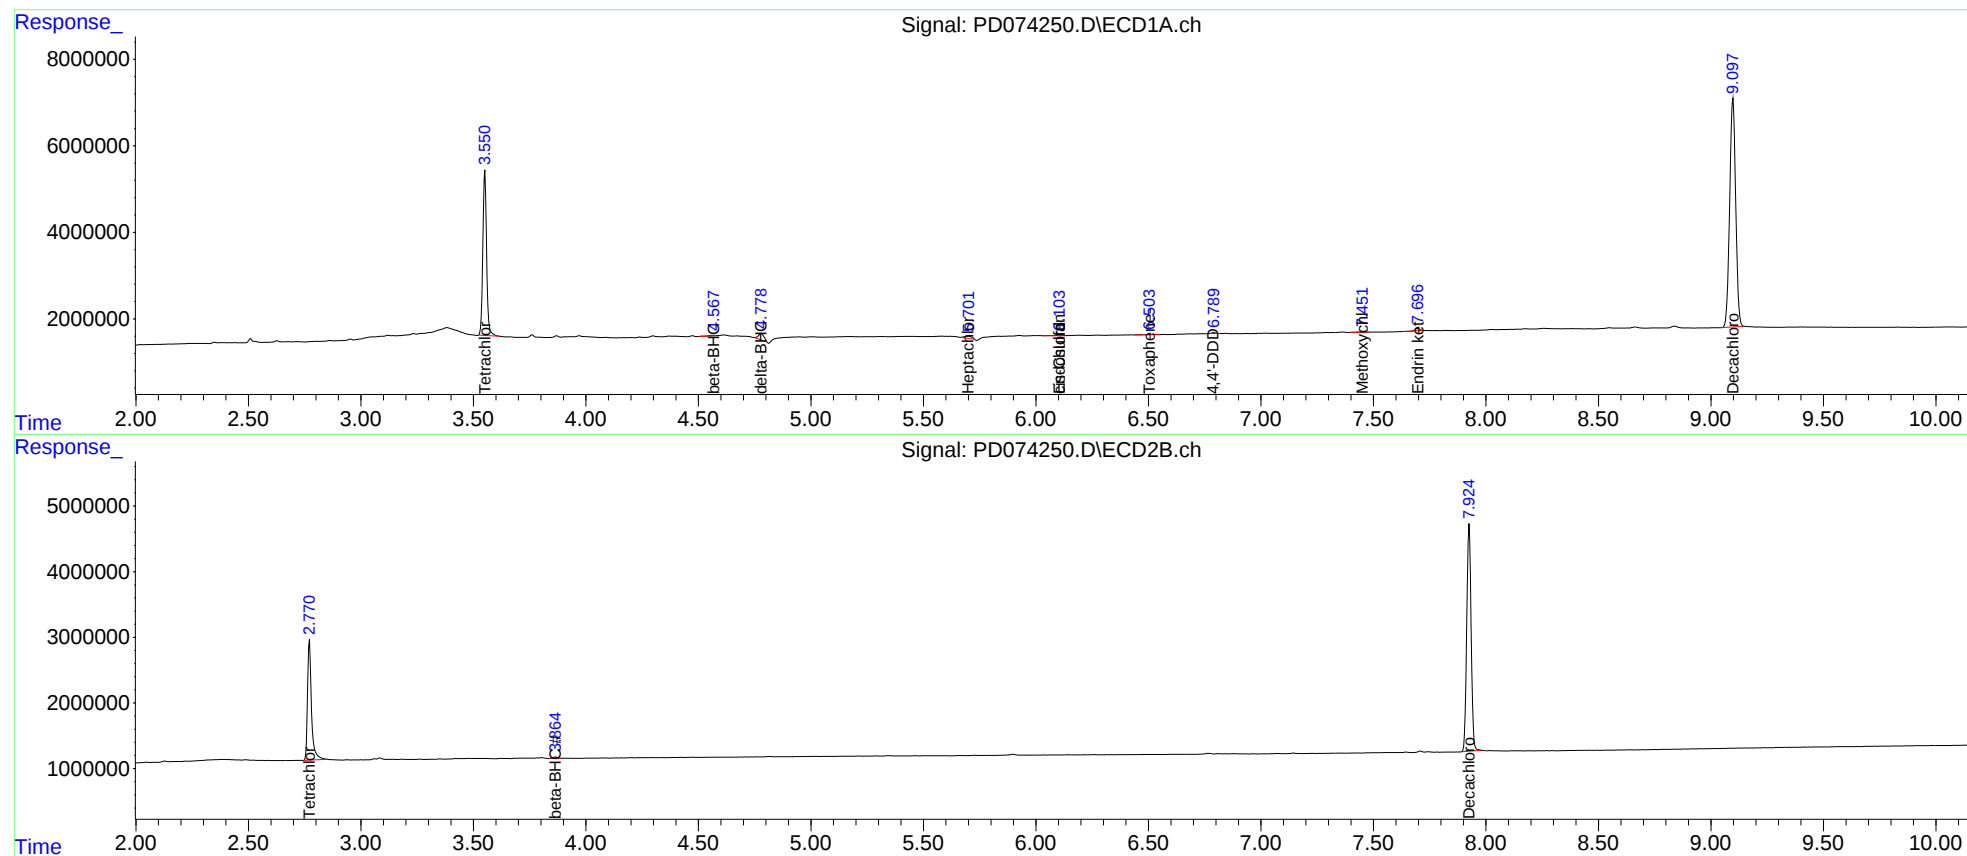

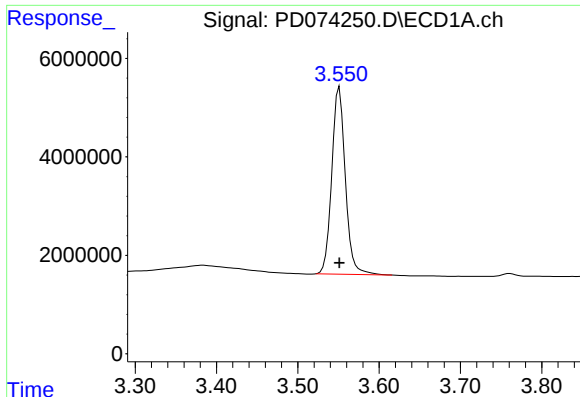


#1 Tetrachloro-m-xylene

R.T.: 3.551 min
Delta R.T.: 0.000 min
Response: 44191803
Conc: 17.79 ng/ml

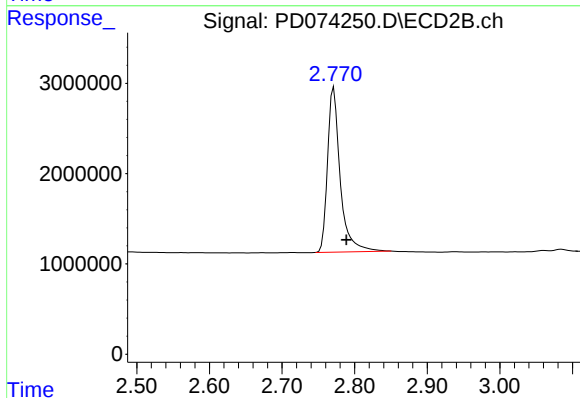


#1 Tetrachloro-m-xylene

R.T.: 2.771 min
Delta R.T.: -0.017 min
Response: 22250470
Conc: 17.69 ng/ml

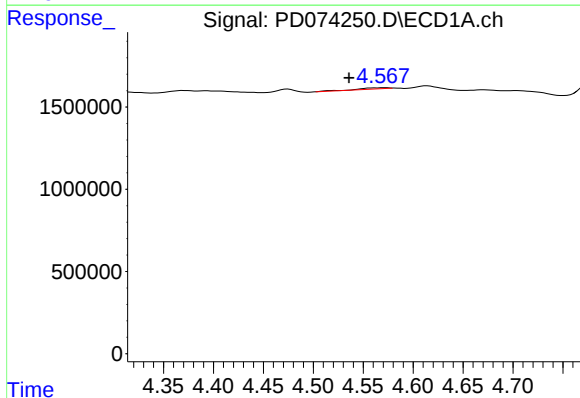


#6 beta-BHC

R.T.: 4.571 min
Delta R.T.: 0.035 min
Response: 189129
Conc: 0.11 ng/ml

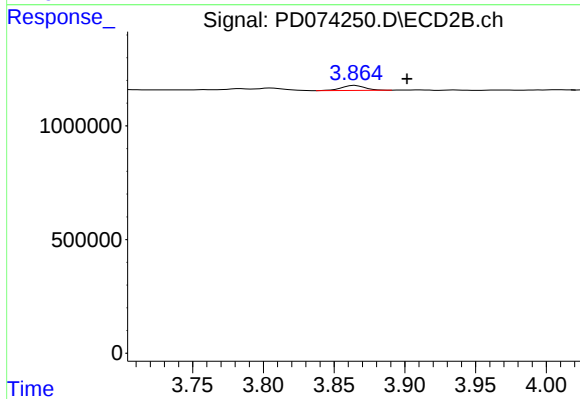


#6 beta-BHC

R.T.: 3.865 min
Delta R.T.: -0.037 min
Response: 253382
Conc: 0.31 ng/ml

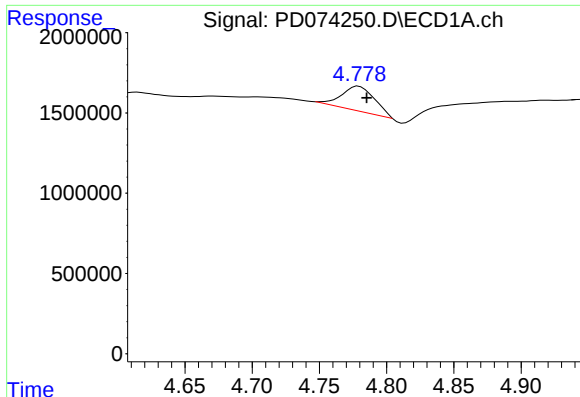


#7 delta-BHC

R.T.: 4.779 min
Delta R.T.: -0.006 min
Response: 2490751
Conc: 0.68 ng/ml

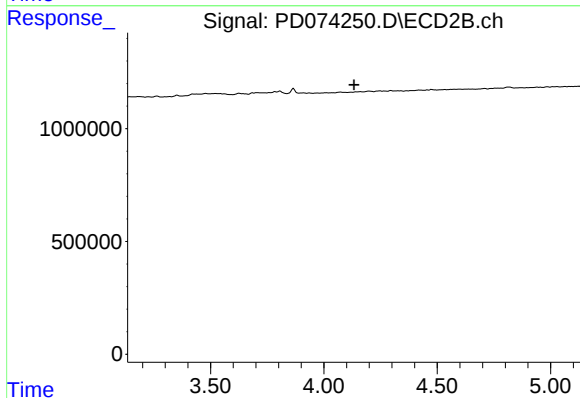


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.133 min
Response: 0
Conc: N.D.

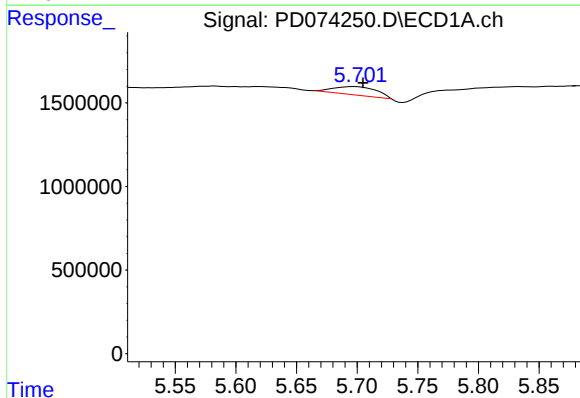


#8 Heptachlor epoxide

R.T.: 5.698 min
Delta R.T.: -0.007 min
Response: 1175319
Conc: 0.36 ng/ml

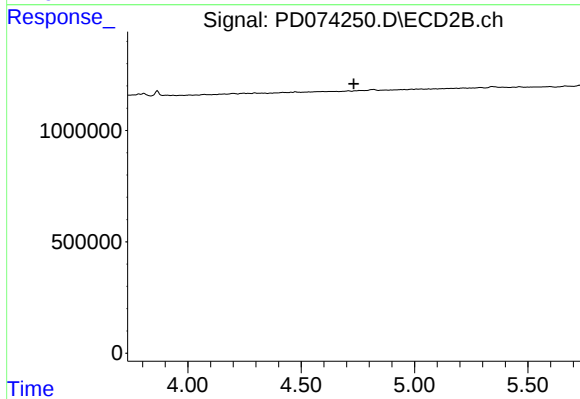


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.732 min
Response: 0
Conc: N.D.

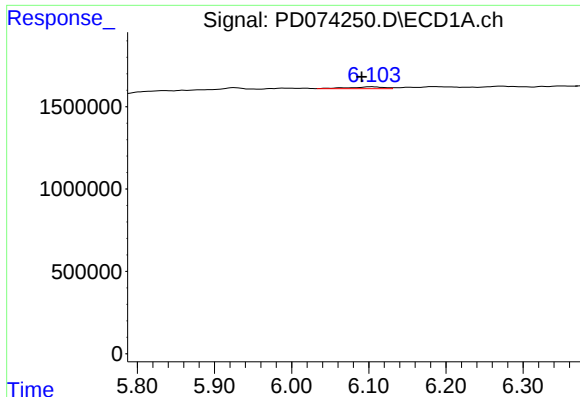


#9 Endosulfan I

R.T.: 6.104 min
Delta R.T.: 0.013 min
Response: 350277
Conc: 0.12 ng/ml

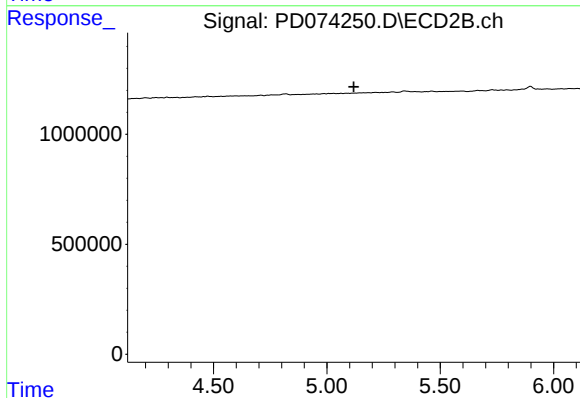


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.118 min
Response: 0
Conc: N.D.

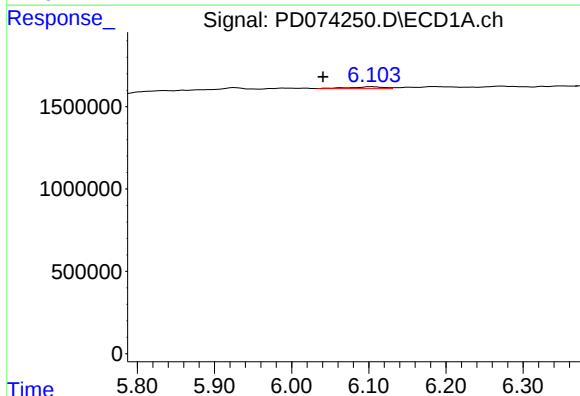


#11 cis-Chlordane

R.T.: 6.104 min
Delta R.T.: 0.063 min
Response: 350277
Conc: 0.11 ng/ml

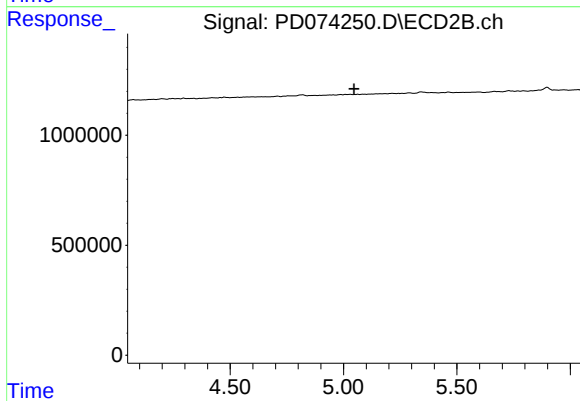


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.047 min
Response: 0
Conc: N.D.

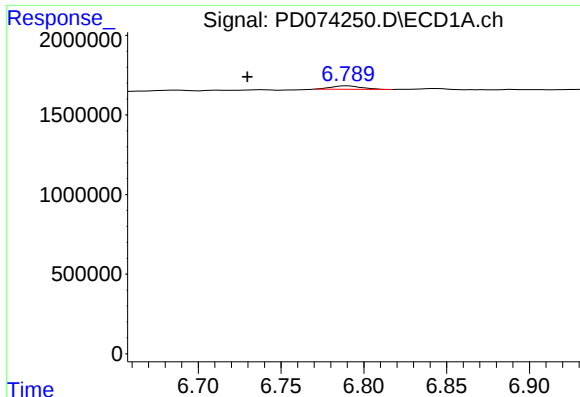


#16 4,4'-DDD

R.T.: 6.790 min
Delta R.T.: 0.060 min
Response: 266986
Conc: 0.11 ng/ml

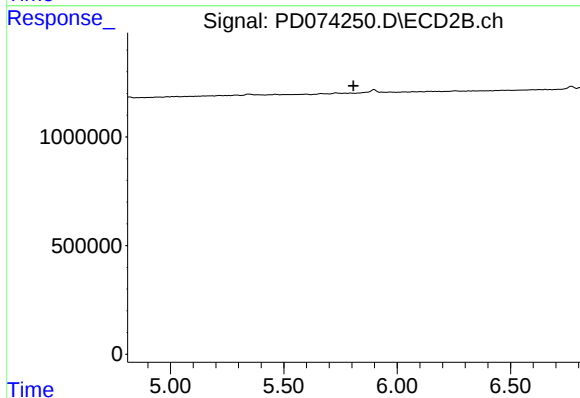


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.808 min
Response: 0
Conc: N.D.

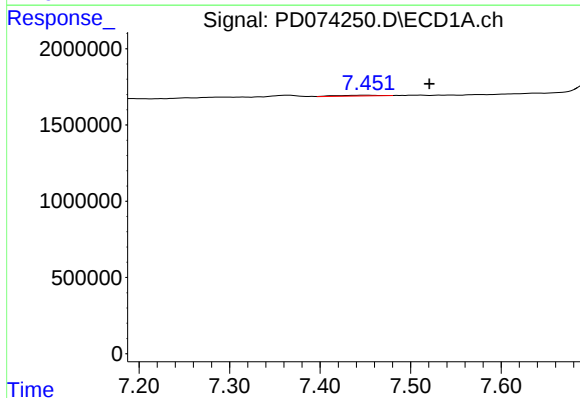


#20 Methoxychlor

R.T.: 7.452 min
Delta R.T.: -0.068 min
Response: 180198
Conc: 0.13 ng/ml

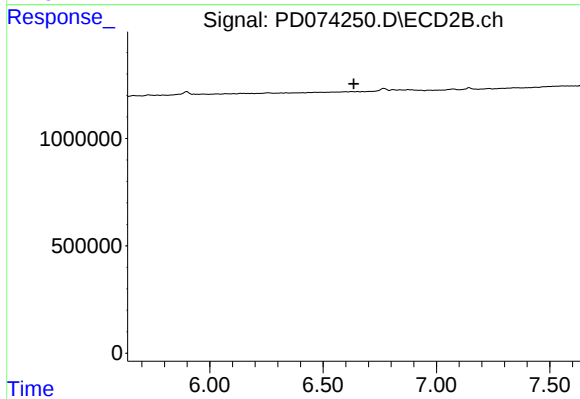


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.636 min
Response: 0
Conc: N.D.

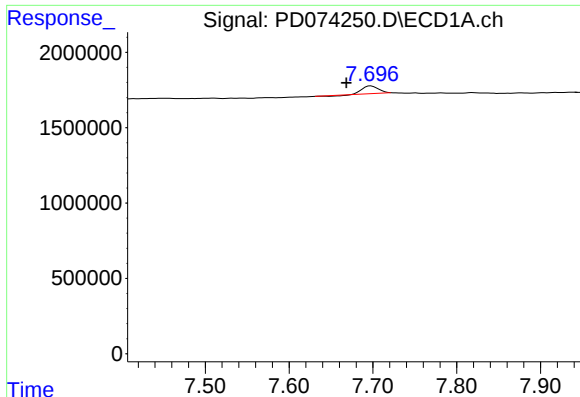


#21 Endrin ketone

R.T.: 7.698 min
Delta R.T.: 0.029 min
Response: 680909
Conc: 0.23 ng/ml

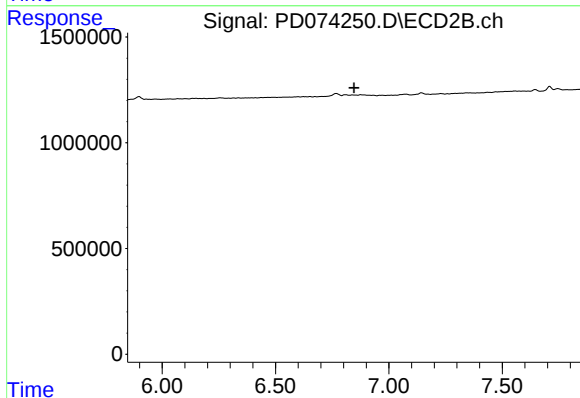


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 6.846 min
Response: 0
Conc: N.D.

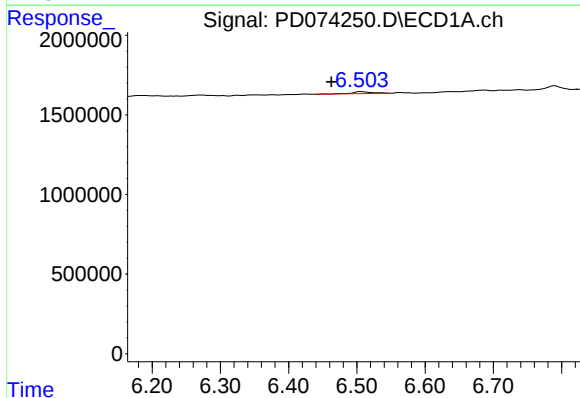


#23 Toxaphene-2

R.T.: 6.505 min
Delta R.T.: 0.043 min
Response: 259196
Conc: 8.74 ng/ml

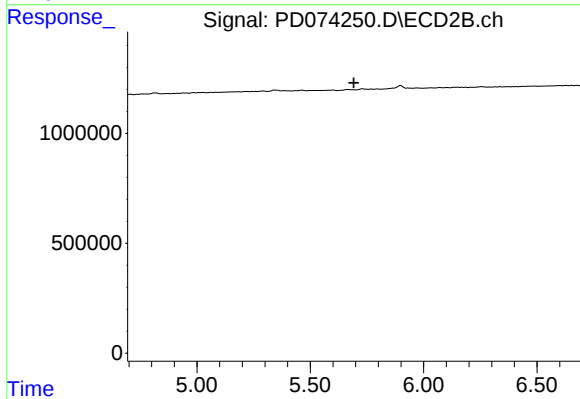


#23 Toxaphene-2

R.T.: 0.000 min
Exp R.T.: 5.692 min
Response: 0
Conc: N.D.

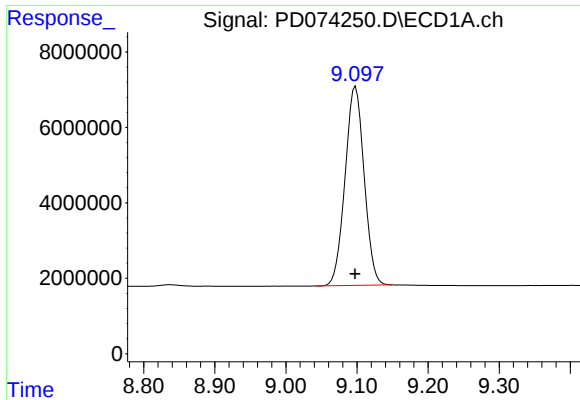

#27 Decachlorobiphenyl

R.T.: 9.098 min
Delta R.T.: 0.000 min
Response: 98276766
Conc: 35.91 ng/ml

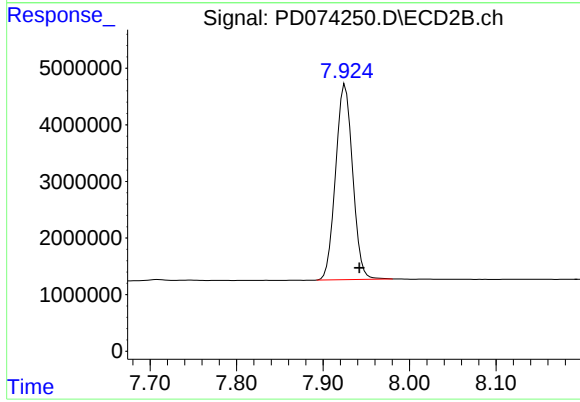

#27 Decachlorobiphenyl

R.T.: 7.926 min
Delta R.T.: -0.016 min
Response: 47070776
Conc: 39.31 ng/ml