

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031623\
 Data File : PD074253.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2023 11:59
 Operator : AR\AJ
 Sample : 01884-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CB908

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/21/2023
 Supervised By : Ankita Jodhani 03/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 21:37:20 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 14 03:05:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.557	2.771	42057052	18651813	16.929	14.825
2) SA Decachlor...	9.104	7.927	85175295	39262806	31.120	32.790
Target Compounds						
16) A 4,4'-DDD	6.732	5.792	1411227	5461475	0.597m	4.639 #
19) B Endosulfa...	7.155	6.334	2763358	1409866	1.061m	1.120
20) A Methoxychlor	7.517	6.619	1857628	3103160	1.353m	5.045m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031623\
Data File : PD074253.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2023 11:59
Operator : AR\AJ
Sample : 01884-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 21:37:20 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 14 03:05:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

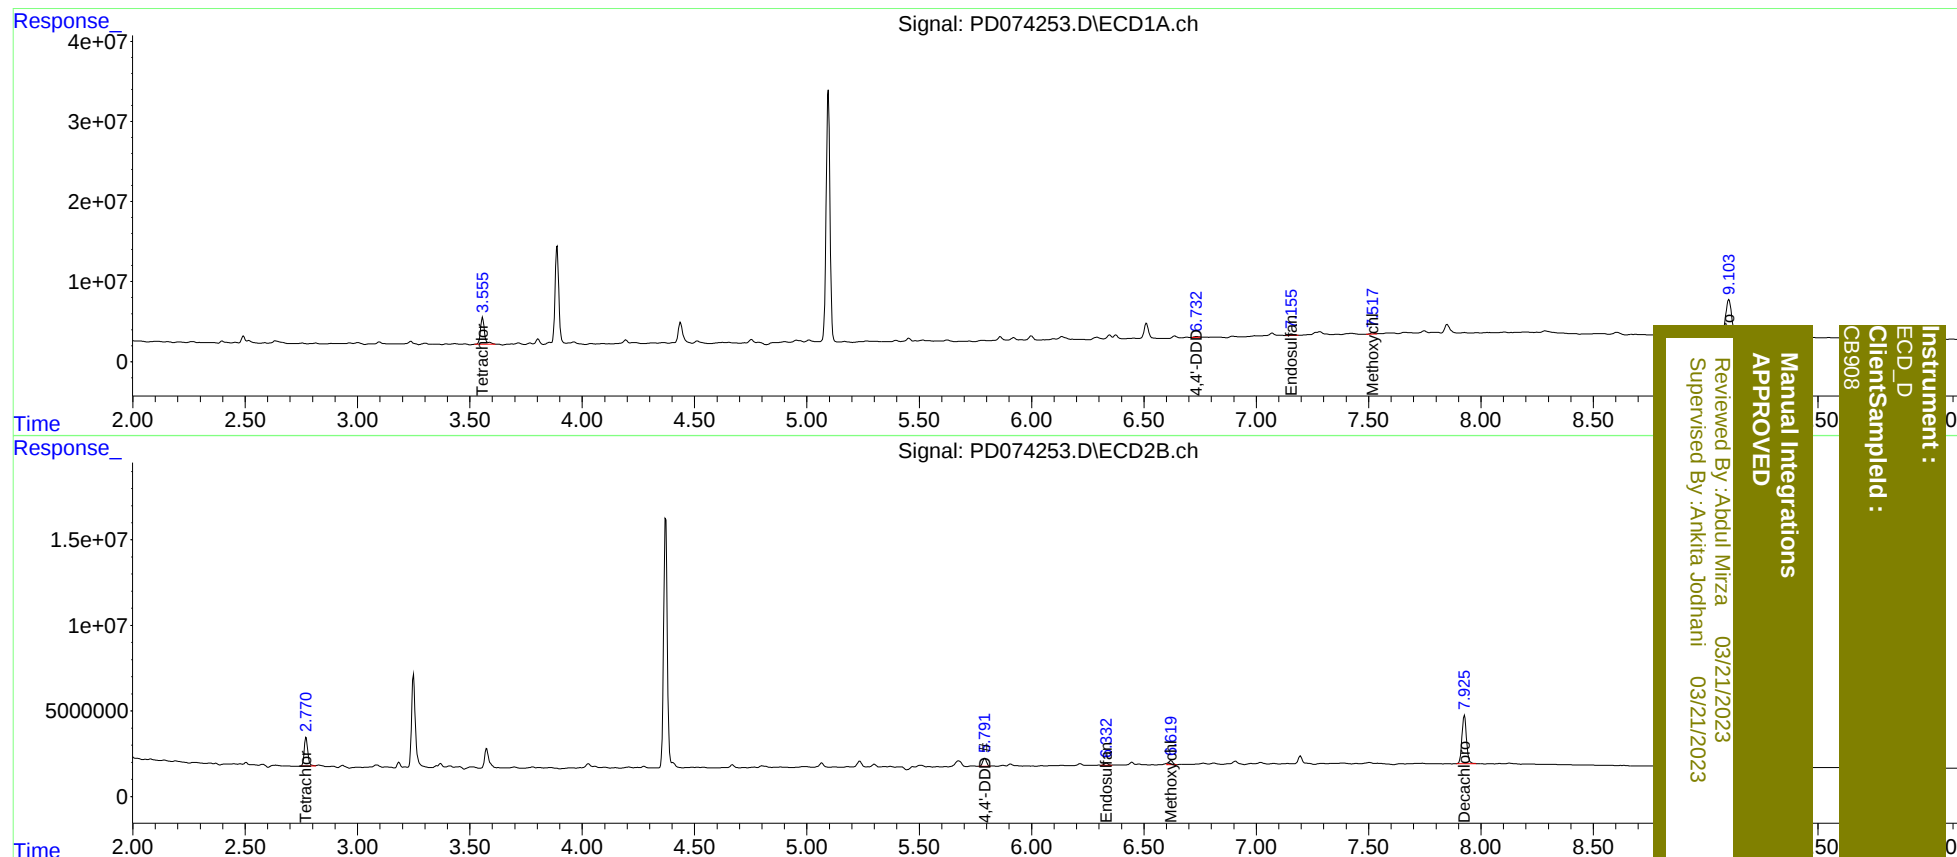

Instrument :
ECD_D
ClientSampled :
CB908

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 03/21/2023
Supervised By: Ankita Jodhani 03/21/2023