

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031623\
 Data File : PD074265.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2023 15:53
 Operator : AR\AJ
 Sample : INDA372
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA3151

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 21:39:37 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 14 03:05:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.555	2.770	46294888	23780920	18.634	18.902
2) SA Decachlor...	9.102	7.927	95618539	45065773	34.936	37.636
Target Compounds						
2) A alpha-BHC	4.012	3.274	71341197	33685032	18.282	18.849
3) MA gamma-BHC...	4.346	3.605	68920230	31898924	18.672	18.676
4) MA Heptachlor	4.938	3.947	69601005	30767857	18.385	18.556
9) A Endosulfan I	6.096	5.102	54939071	26017761	18.416	18.555
13) MA Dieldrin	6.372	5.367	119.4E6	57768945	37.650	37.263
14) MA Endrin	6.601	5.643	97295994	50774762	36.921	37.743
16) A 4,4'-DDD	6.735	5.791	90784276	45588458	38.414	38.719
17) MA 4,4'-DDT	7.050	6.043	92488054	46316015	36.857	36.970
20) A Methoxychlor	7.525	6.620	258.5E6	120.2E6	188.285	195.468

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031623\
Data File : PD074265.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2023 15:53
Operator : AR\AJ
Sample : INDA372
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 21:39:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 14 03:05:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

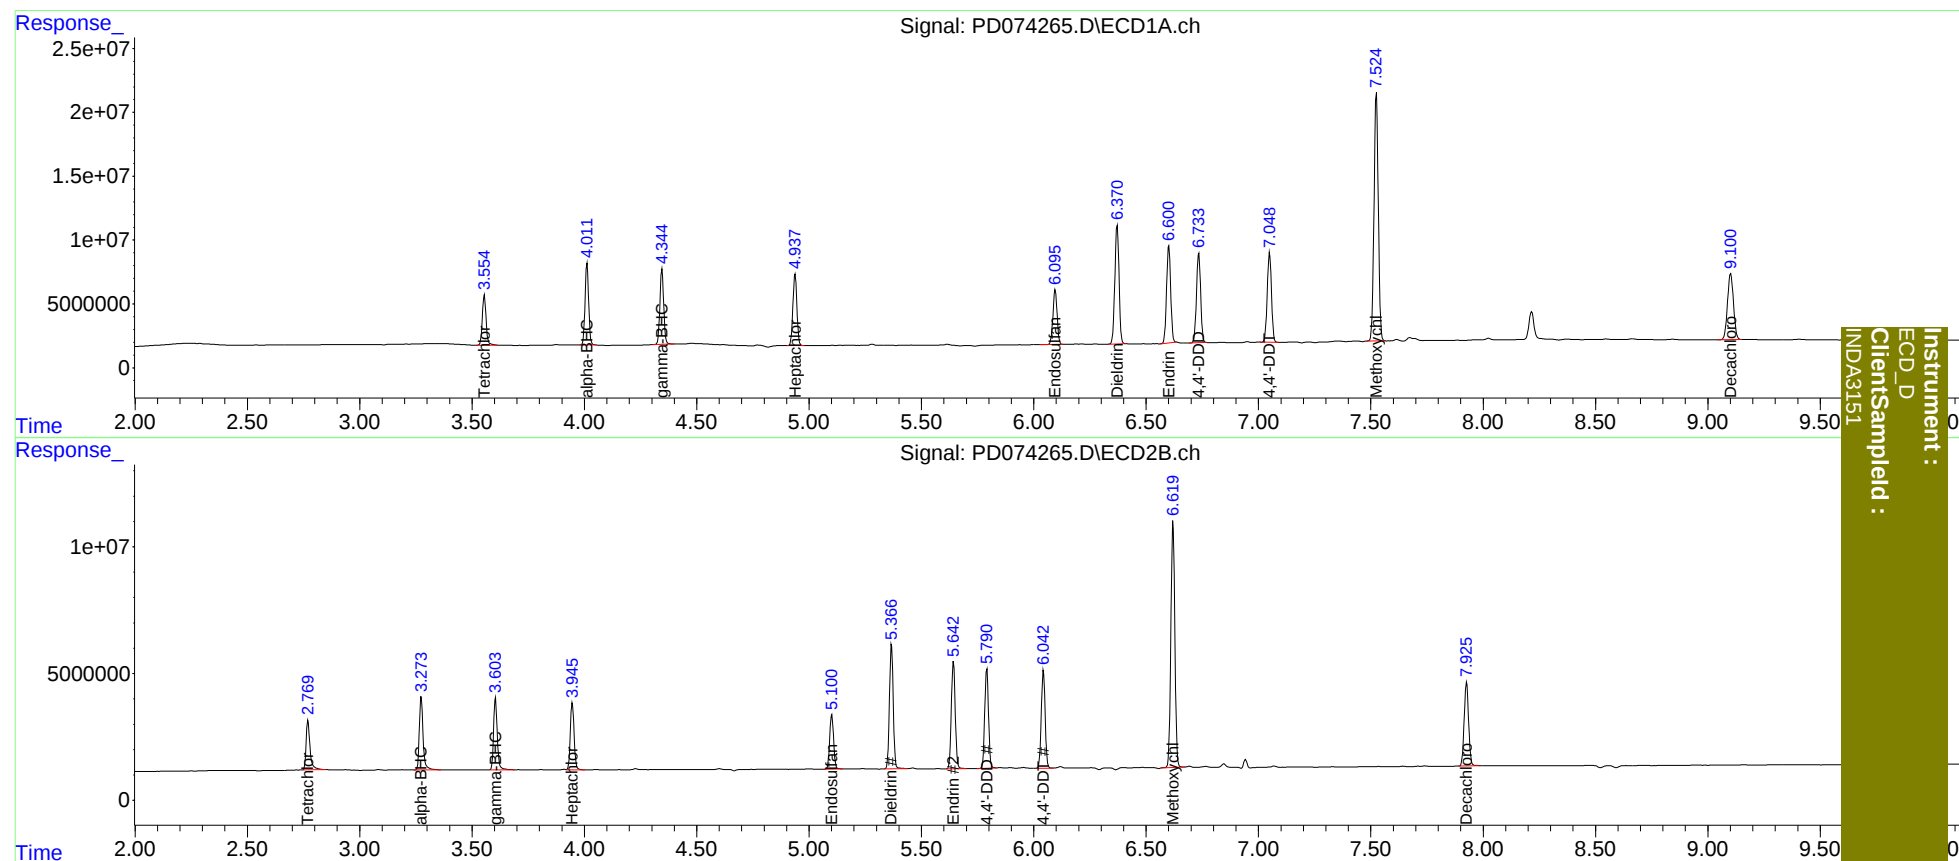

Instrument :
ECD_D
ClientSampled :
INDA3151