

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031721\
 Data File : PD061677.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Mar 2021 18:19
 Operator : AR\AJ
 Sample : PTOXICC250
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 19:02:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX031721.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 17 19:01:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.485	3.982	21104096	218.0E6	24.500	25.031
7) SA Decachlor...	8.257	9.039	30033006	227.0E6	25.042	25.908
Target Compounds						
2) Toxaphene-1	5.968	6.556	3063100	28243546	270.836	259.295
3) Toxaphene-2	6.237	7.062	2335613	22571388	255.770	239.372
4) Toxaphene-3	6.602	7.138	5007284	67722532	248.925	270.370
5) Toxaphene-4	6.746	7.224	1807057	41912201	254.344	257.918
6) Toxaphene-5	7.029	7.638	2010911	30138146	247.971	273.845

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031721\
Data File : PD061677.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Mar 2021 18:19
Operator : AR\AJ
Sample : PTOXICC250
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 19:02:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX031721.M
Quant Title : GC Extractables
QLast Update : Wed Mar 17 19:01:51 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

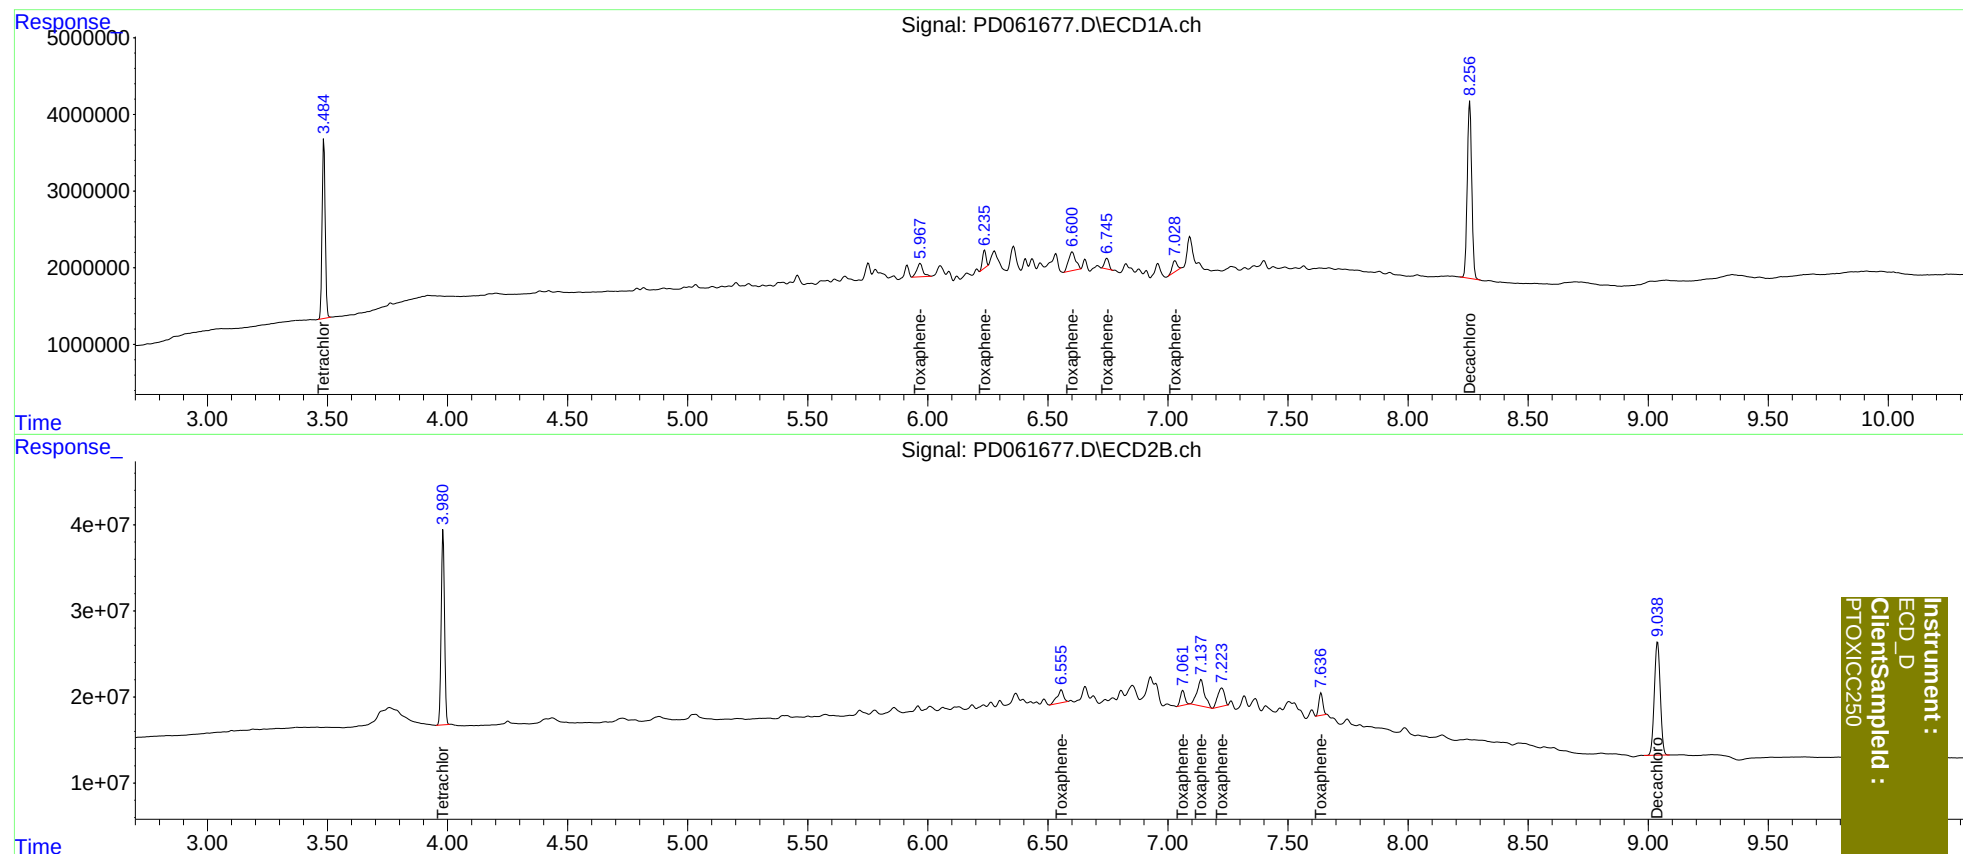

Instrument :
ECD_D
ClientSample :
PTOXICC250