

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031721\
 Data File : PD061686.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Mar 2021 20:25
 Operator : AR\AJ
 Sample : PTOXCCC500
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 18 08:27:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX031721.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 17 19:05:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.485	3.981	42325321	414.8E6	49.631	48.213
7) SA Decachlor...	8.257	9.039	58873312	421.7E6	49.243	48.397
Target Compounds						
2) Toxaphene-1	5.969	6.555	6364107	50404794	562.521	449.956
3) Toxaphene-2	6.237	7.063	4815688	44401208	515.324	499.570
4) Toxaphene-3	6.604	7.139	10171622	123.5E6	500.130	470.237
5) Toxaphene-4	6.747	7.225	3633745	77771828	486.957	483.030
6) Toxaphene-5	7.030	7.638	4698760	54530642	547.928	492.979

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031721\
Data File : PD061686.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Mar 2021 20:25
Operator : AR\AJ
Sample : PTOXCCC500
Misc :
ALS Vial : 25 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 18 08:27:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX031721.M
Quant Title : GC Extractables
QLast Update : Wed Mar 17 19:05:51 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

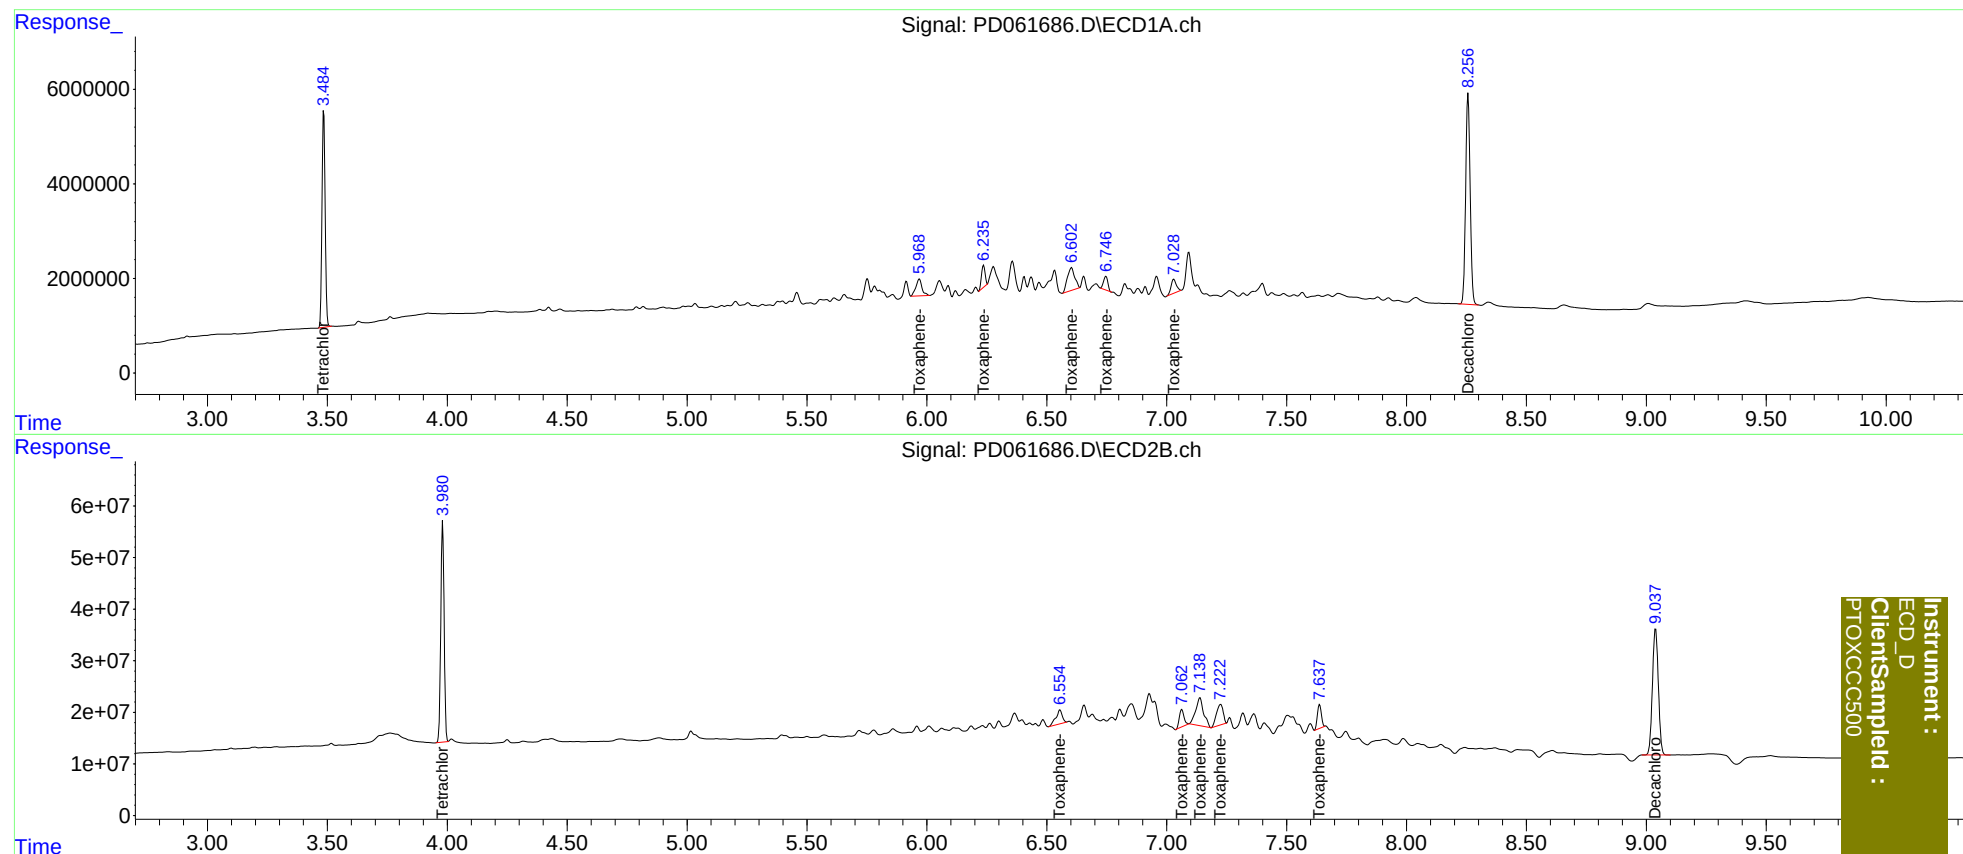

Instrument :
ECD_D
Sample :
PTOXCCC500