

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031721\
 Data File : PD061694.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Mar 2021 22:17
 Operator : AR\AJ
 Sample : M1458-09
 Misc : TOX MDL 100 PPB
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL-WATER-03-QT1-2021

Manual Integrations
 APPROVED

Ankita
 3/18/2021 4:02:51 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 18 08:28:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX031721.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 17 19:05:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.485	3.981	14886726	149.3E6	17.456	17.350
7) SA Decachlor...	8.257	9.039	21825344	155.0E6	18.255	17.793
Target Compounds						
2) Toxaphene-1	5.968	6.555	505289	4987817	44.662	44.526m
3) Toxaphene-2	6.237	7.063	480189	3452720	51.385	38.847
4) Toxaphene-3	6.601	7.138	914972	14169378	44.988	53.966
5) Toxaphene-4	6.748	7.219	312656	9345024	41.899	58.041 #
6) Toxaphene-5	7.047	7.638	792089	6770694	92.366m	61.210 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031721\
Data File : PD061694.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Mar 2021 22:17
Operator : AR\AJ
Sample : M1458-09
Misc : TOX MDL 100 PPB
ALS Vial : 33 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 18 08:28:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX031721.M
Quant Title : GC Extractables
QLast Update : Wed Mar 17 19:05:51 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

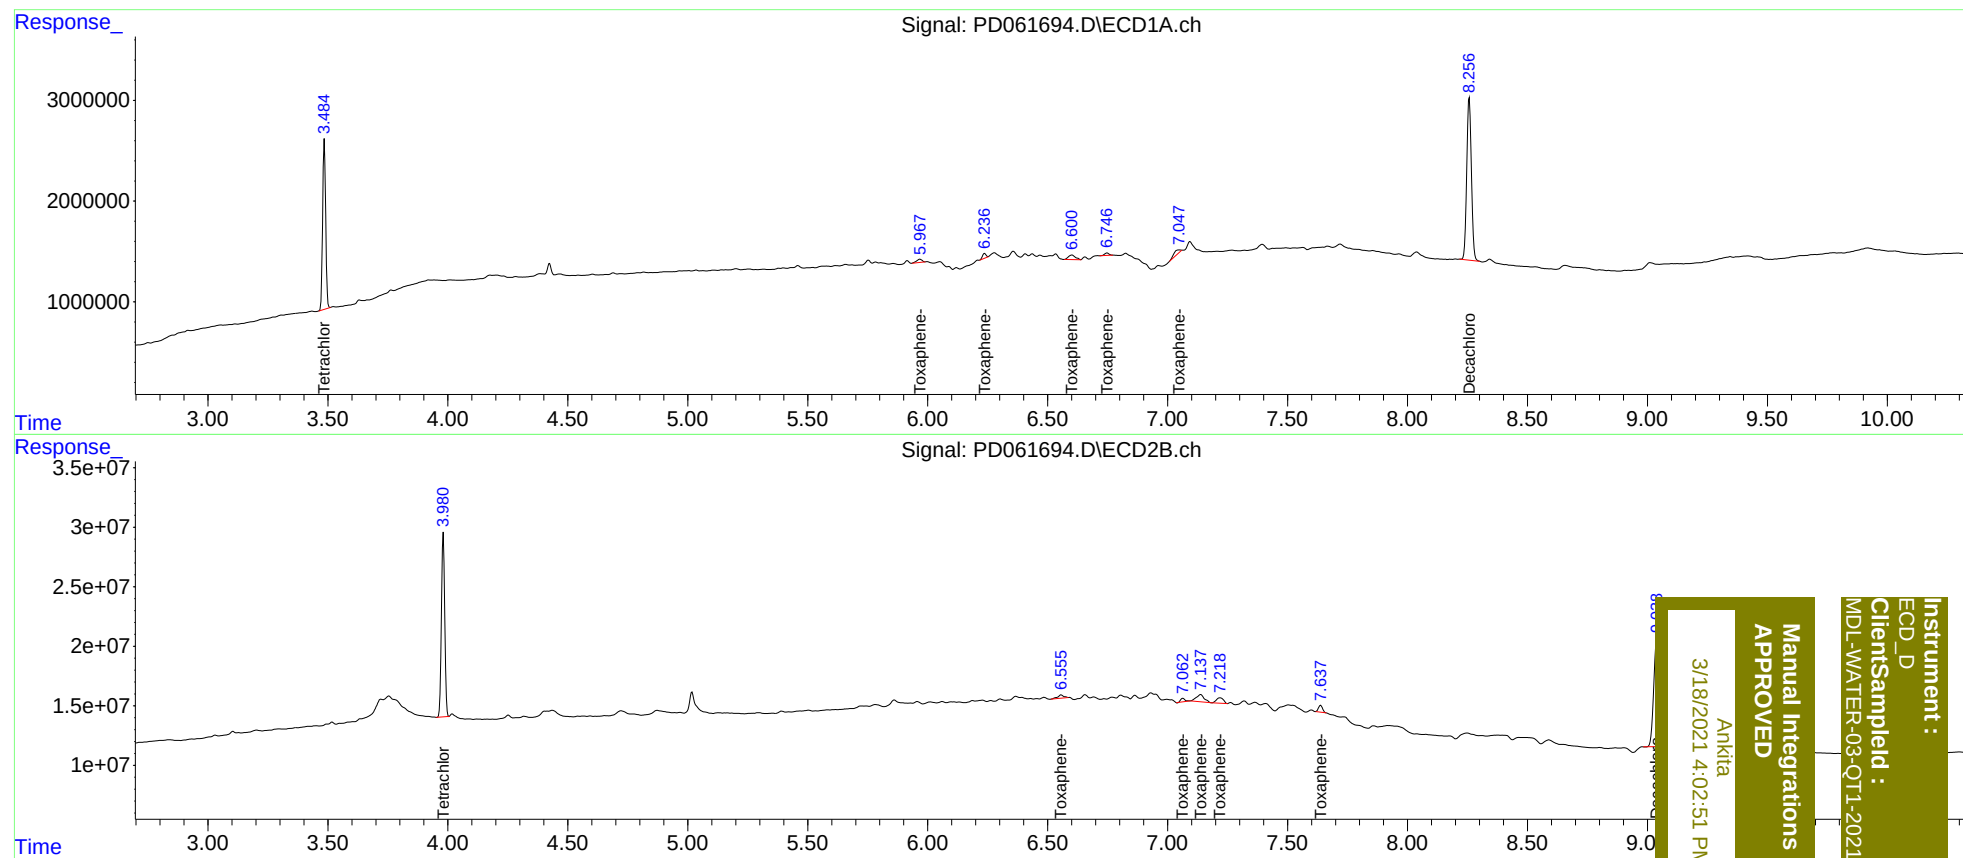

Manual Integrations
APPROVED

3/18/2021 4:02:51 PM

Ankita

Instrument :
ECD_D
ClientSample :
MDL-WATER-03-QT1-2021