

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031721\
 Data File : PD061669.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Mar 2021 16:26
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 18:01:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031721.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 17 18:01:27 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.484	3.981	98300560	800.6E6	97.757	93.352
28)	SA Decachlor...	8.257	9.039	109.2E6	793.9E6	93.025	93.565
Target Compounds							
23)	Chlordane-1	4.360	4.974	31779044	357.0E6	952.435	935.506
24)	Chlordane-2	4.863	5.441	36952470	348.9E6	916.944	911.438
25)	Chlordane-3	5.434	6.087	117.1E6	1525.4E6	965.516	942.454
26)	Chlordane-4	5.492	6.161	96458384	1745.6E6	968.135	933.689
27)	Chlordane-5	6.332	6.965	43474103	337.8E6	949.370	966.112



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031721\
Data File : PD061669.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Mar 2021 16:26
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 18:01:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031721.M
Quant Title : GC Extractables
QLast Update : Wed Mar 17 18:01:27 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

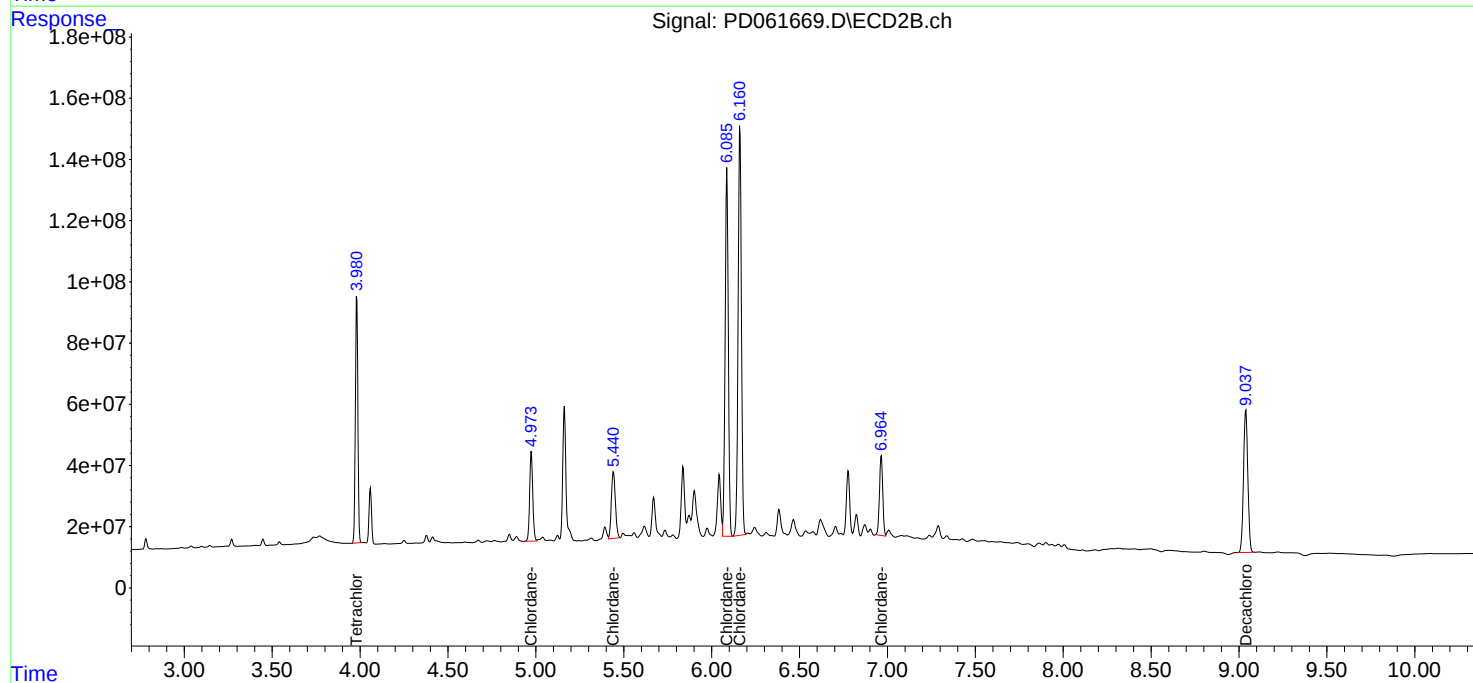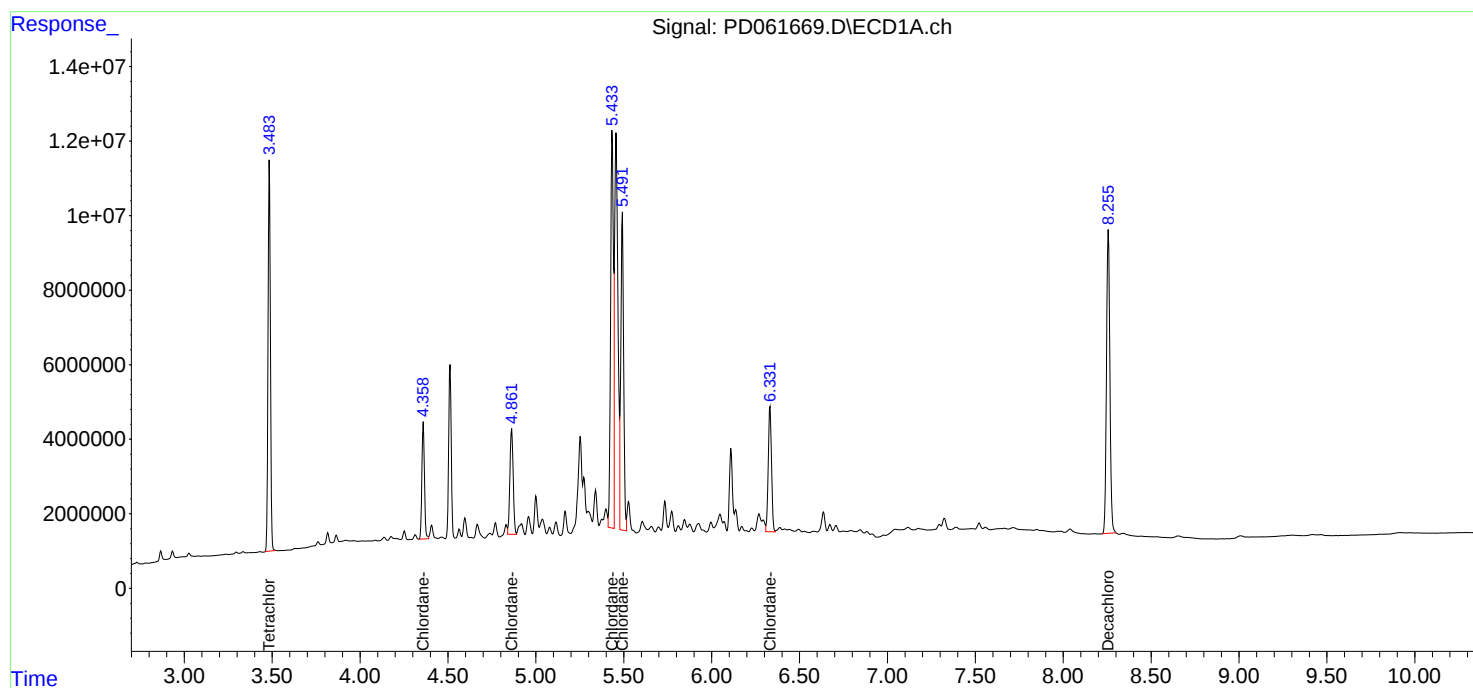


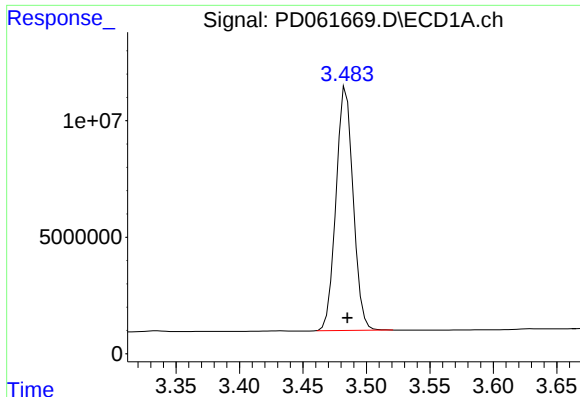

#1 Tetrachloro-m-xylene


R.T.: 3.484 min
Delta R.T.: 0.000 min
Response: 98300560
Conc: 97.76 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

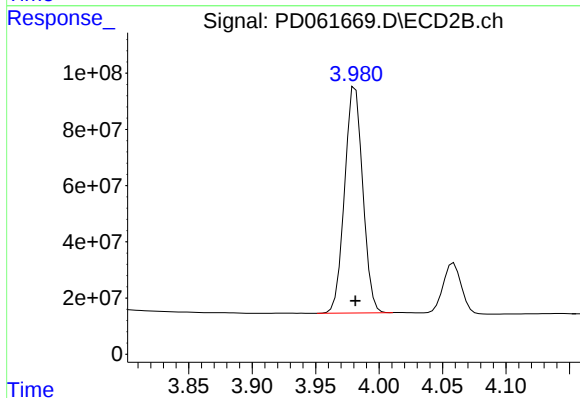


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 800640555
Conc: 93.35 ng/ml

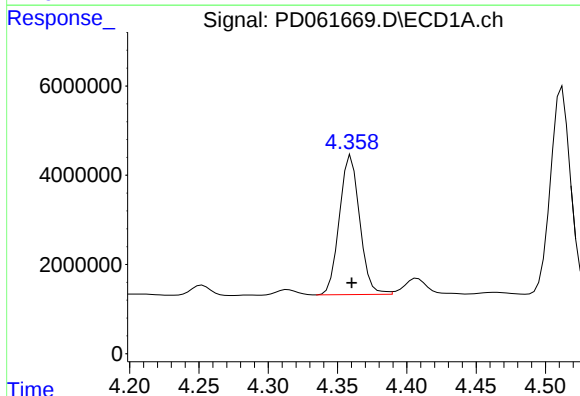


#23 Chlordane-1

R.T.: 4.360 min
Delta R.T.: 0.000 min
Response: 31779044
Conc: 952.44 ng/ml

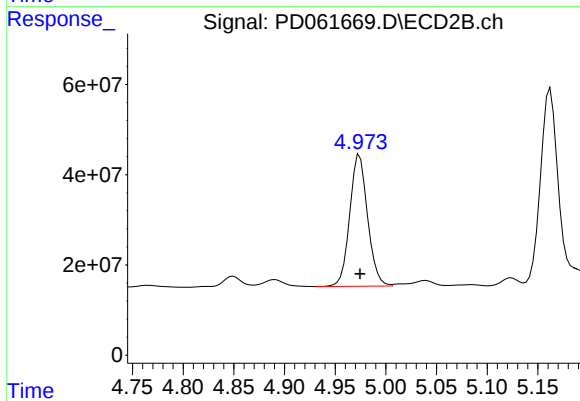

#23 Chlordane-1


R.T.: 4.974 min
Delta R.T.: 0.000 min
Response: 356960949
Conc: 935.51 ng/ml

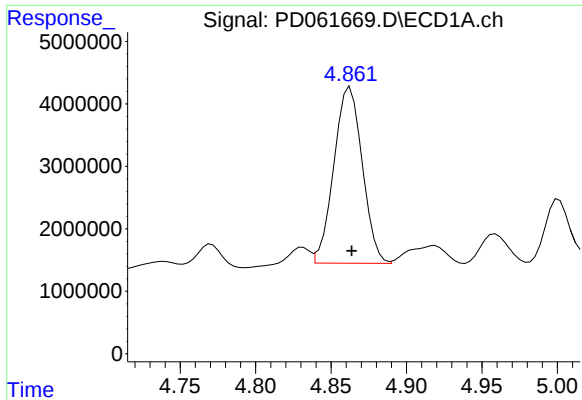

#24 Chlordane-2


R.T.: 4.863 min
Delta R.T.: -0.001 min
Response: 36952470
Conc: 916.94 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

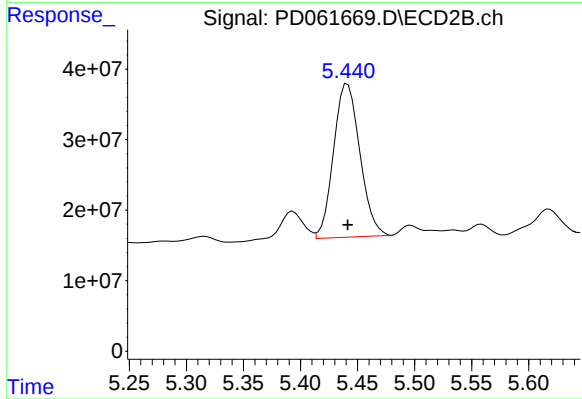


#24 Chlordane-2

R.T.: 5.441 min
Delta R.T.: 0.000 min
Response: 348923536
Conc: 911.44 ng/ml

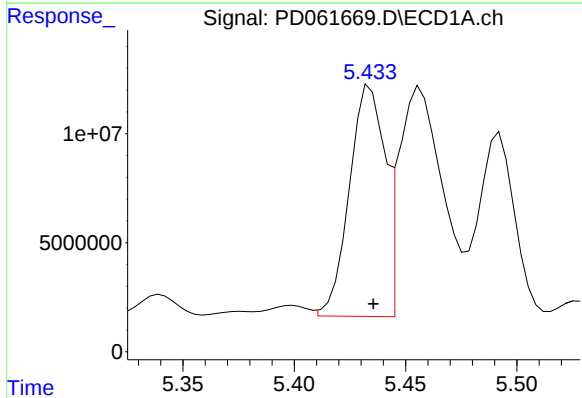


#25 Chlordane-3

R.T.: 5.434 min
Delta R.T.: -0.001 min
Response: 117097290
Conc: 965.52 ng/ml

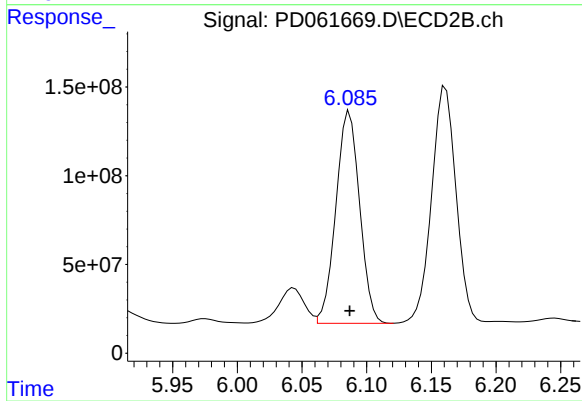

#25 Chlordane-3


R.T.: 6.087 min
Delta R.T.: 0.000 min
Response: 1525357080
Conc: 942.45 ng/ml

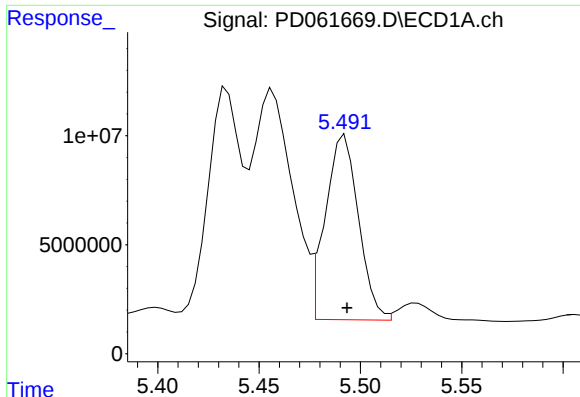

#26 Chlordane-4


R.T.: 5.492 min
Delta R.T.: -0.001 min
Response: 96458384
Conc: 968.13 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

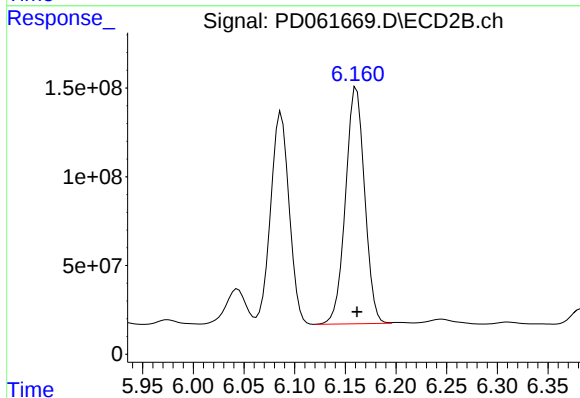


#26 Chlordane-4

R.T.: 6.161 min
Delta R.T.: 0.000 min
Response: 1745583656
Conc: 933.69 ng/ml

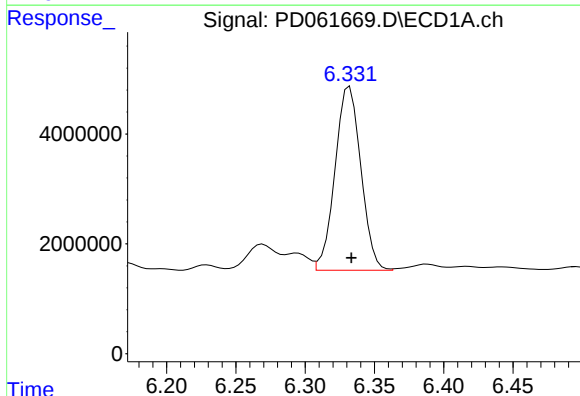


#27 Chlordane-5

R.T.: 6.332 min
Delta R.T.: -0.001 min
Response: 43474103
Conc: 949.37 ng/ml

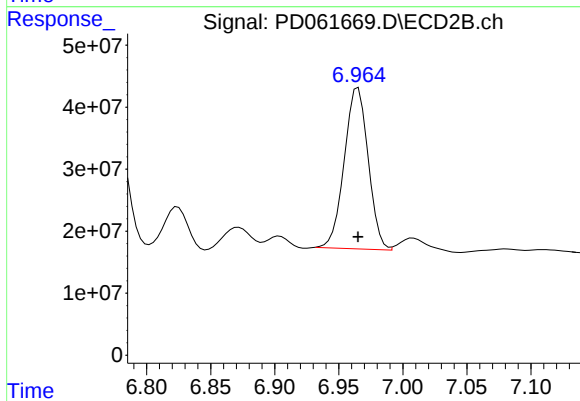

#27 Chlordane-5


R.T.: 6.965 min
Delta R.T.: 0.000 min
Response: 337784361
Conc: 966.11 ng/ml

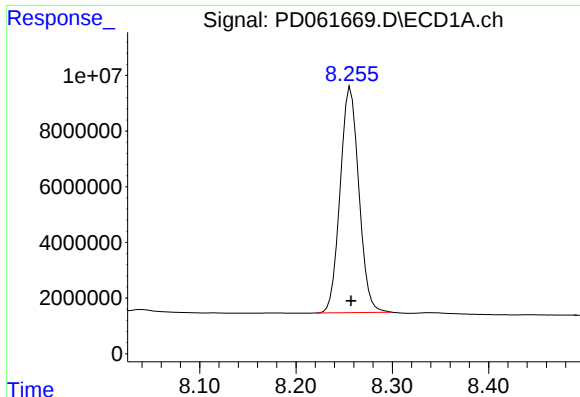

#28 Decachlorobiphenyl

R.T.: 8.257 min
Delta R.T.: 0.000 min
Response: 109220300
Conc: 93.03 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

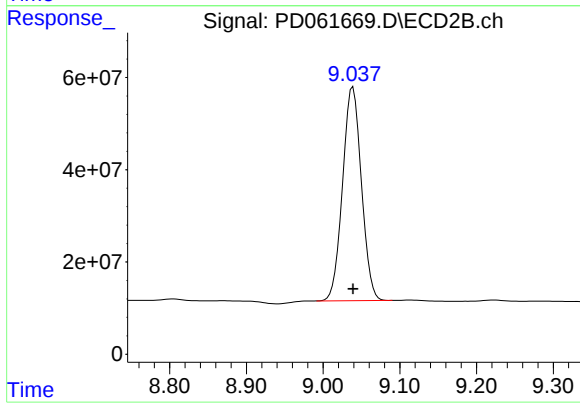

#28 Decachlorobiphenyl

R.T.: 9.039 min
Delta R.T.: 0.000 min
Response: 793873210
Conc: 93.57 ng/ml