

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031721\
 Data File : PD061680.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Mar 2021 19:01
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD031721

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 19:12:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031721.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 17 18:09:15 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	3.982	51096791	436.8E6	52.279	51.758
28)	SA Decachlor...	8.257	9.040	61289092	432.9E6	52.135	50.510
Target Compounds							
23)	Chlordane-1	4.361	4.975	17248625	199.4E6	522.171	539.461
24)	Chlordane-2	4.864	5.442	20606354	195.0E6	522.530	520.353
25)	Chlordane-3	5.436	6.087	61846063	838.5E6	524.439	524.109
26)	Chlordane-4	5.494	6.161	51112833	965.0E6	523.839	521.896
27)	Chlordane-5	6.334	6.965	23703888	181.6E6	506.467	517.651



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031721\
Data File : PD061680.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Mar 2021 19:01
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD031721

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 19:12:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031721.M
Quant Title : GC Extractables
QLast Update : Wed Mar 17 18:09:15 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

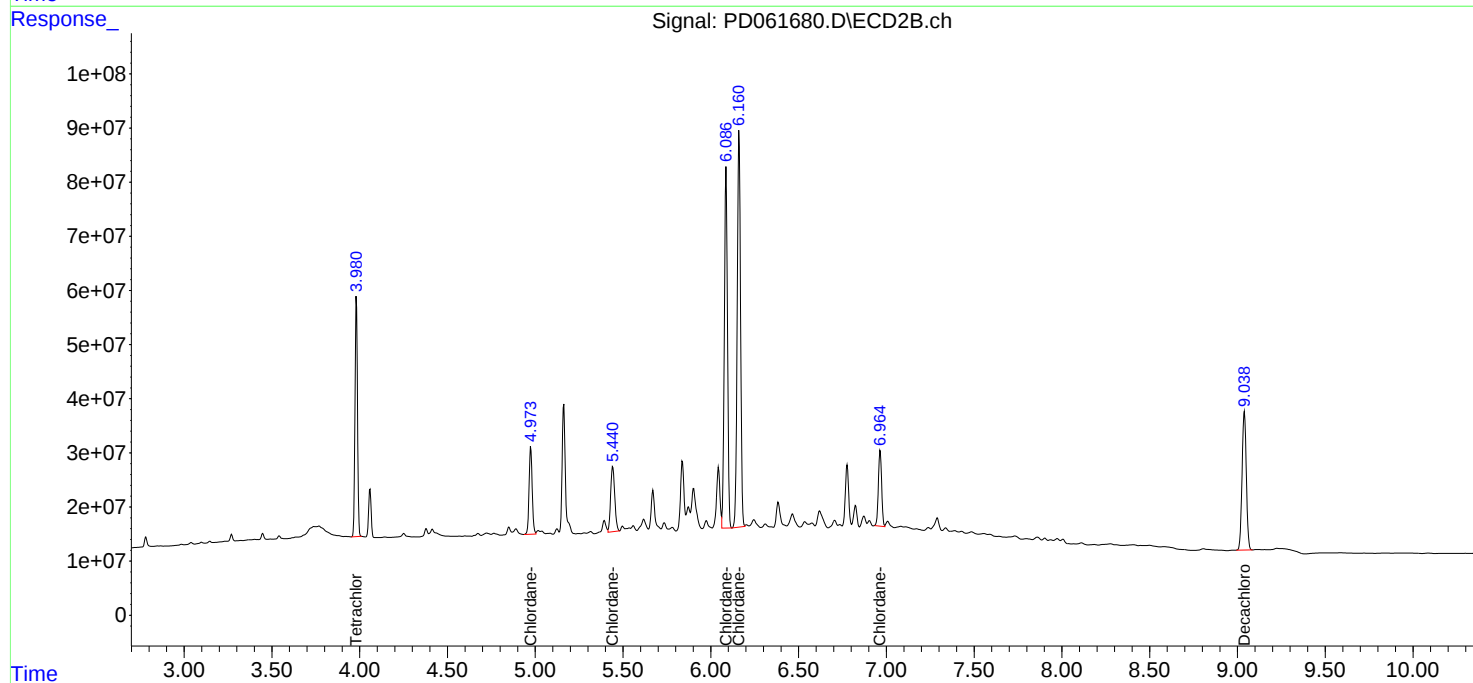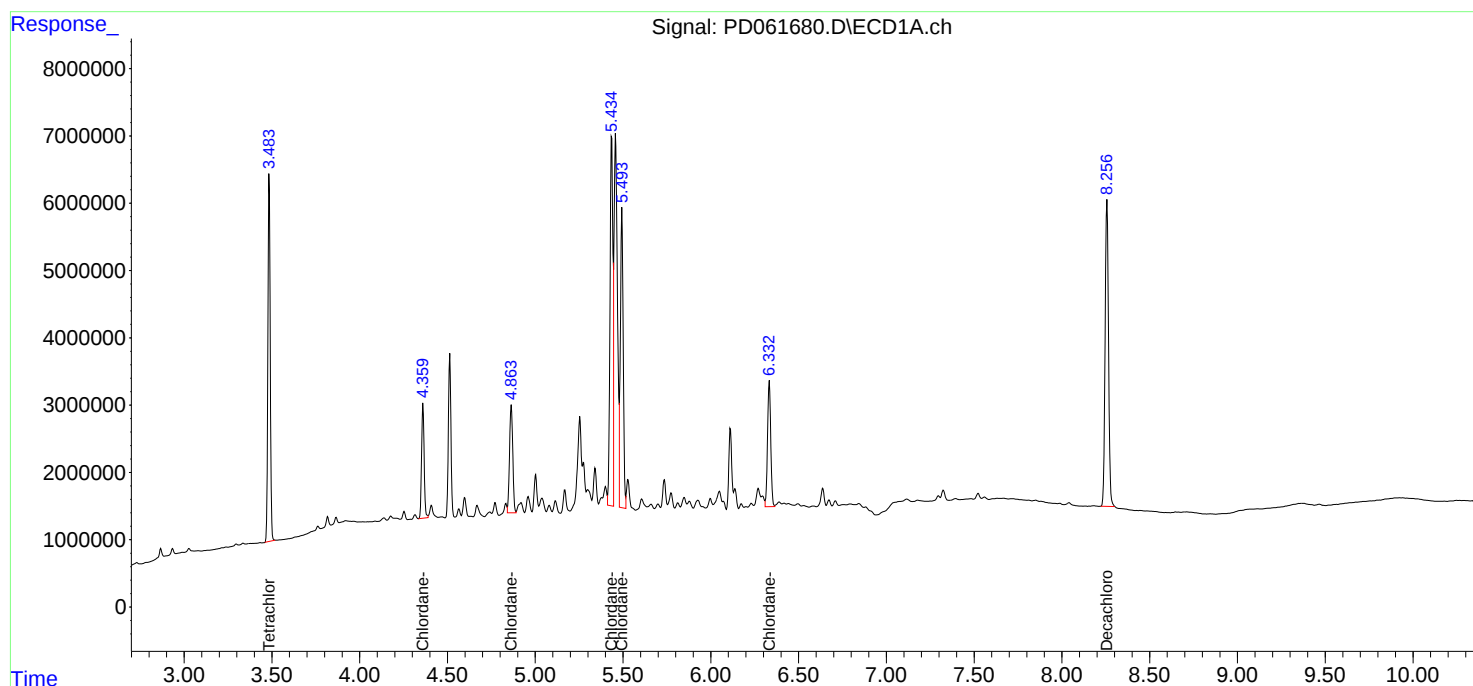


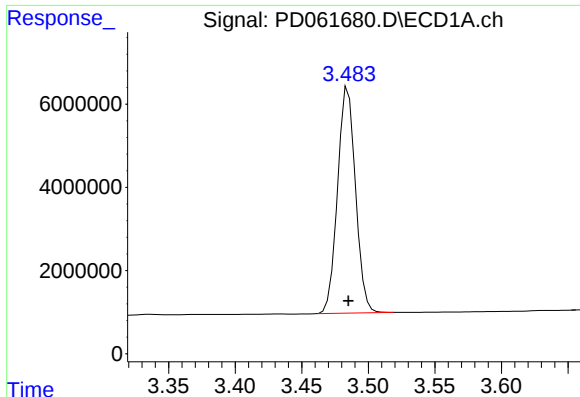

#1 Tetrachloro-m-xylene


R.T.: 3.485 min
Delta R.T.: 0.000 min
Response: 51096791
Conc: 52.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD031721

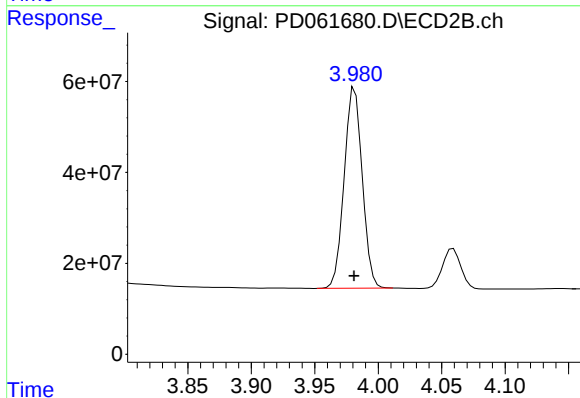


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 436798610
Conc: 51.76 ng/ml

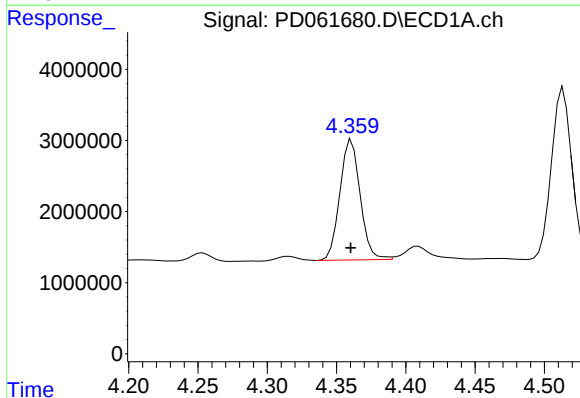


#23 Chlordane-1

R.T.: 4.361 min
Delta R.T.: 0.000 min
Response: 17248625
Conc: 522.17 ng/ml

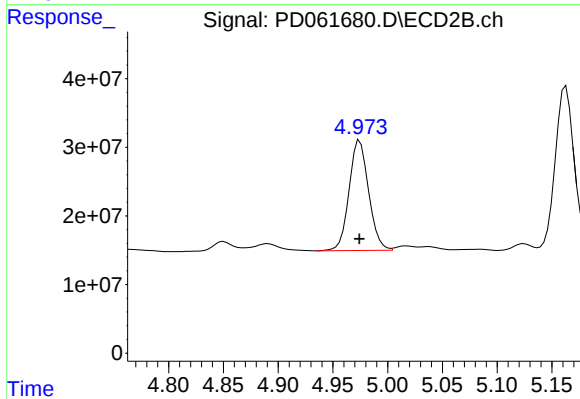

#23 Chlordane-1


R.T.: 4.975 min
Delta R.T.: 0.000 min
Response: 199366749
Conc: 539.46 ng/ml

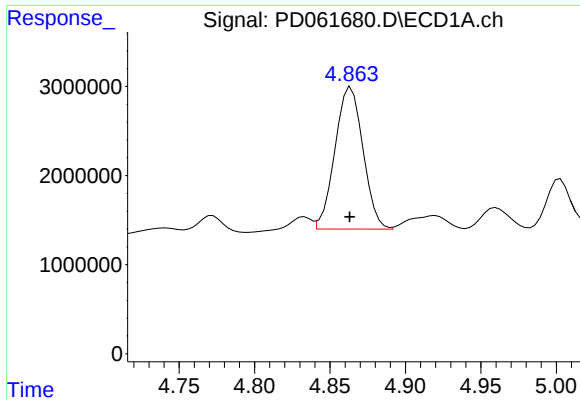

#24 Chlordane-2


R.T.: 4.864 min
Delta R.T.: 0.000 min
Response: 20606354
Conc: 522.53 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD031721

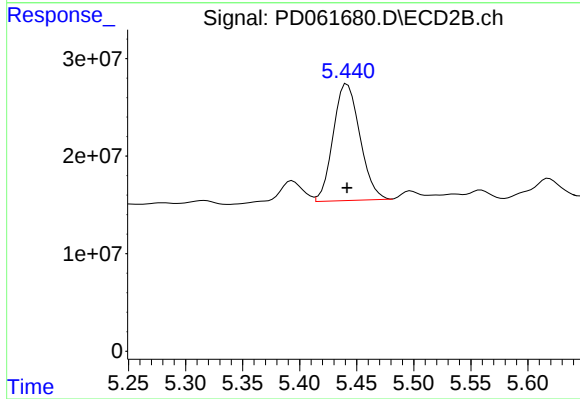


#24 Chlordane-2

R.T.: 5.442 min
Delta R.T.: 0.000 min
Response: 194968163
Conc: 520.35 ng/ml

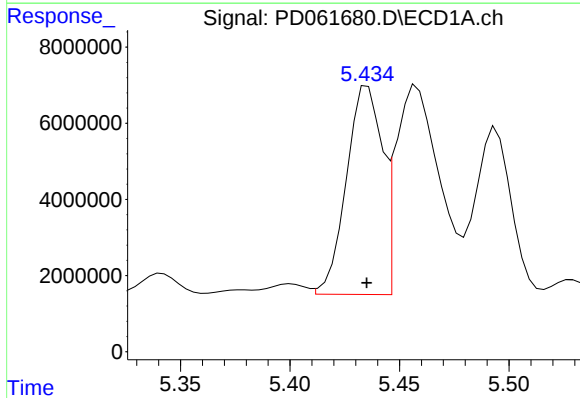


#25 Chlordane-3

R.T.: 5.436 min
Delta R.T.: 0.000 min
Response: 61846063
Conc: 524.44 ng/ml

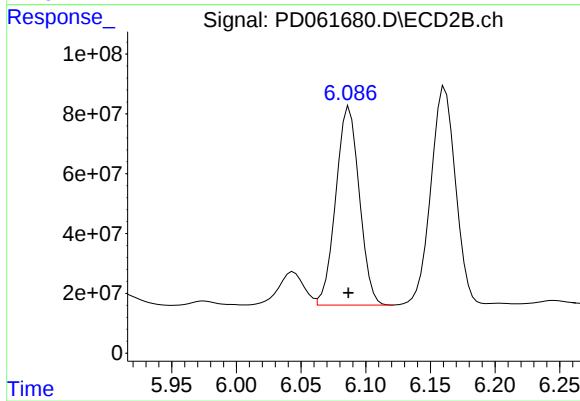

#25 Chlordane-3


R.T.: 6.087 min
Delta R.T.: 0.000 min
Response: 838547434
Conc: 524.11 ng/ml

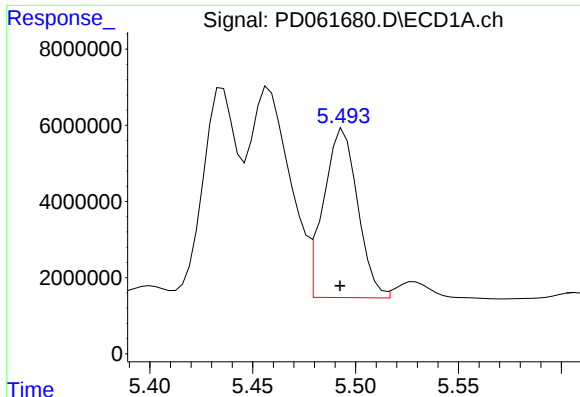

#26 Chlordane-4


R.T.: 5.494 min
Delta R.T.: 0.002 min
Response: 51112833
Conc: 523.84 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD031721

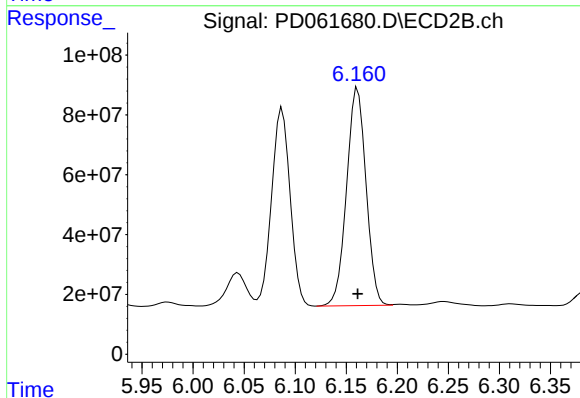


#26 Chlordane-4

R.T.: 6.161 min
Delta R.T.: 0.000 min
Response: 964992153
Conc: 521.90 ng/ml

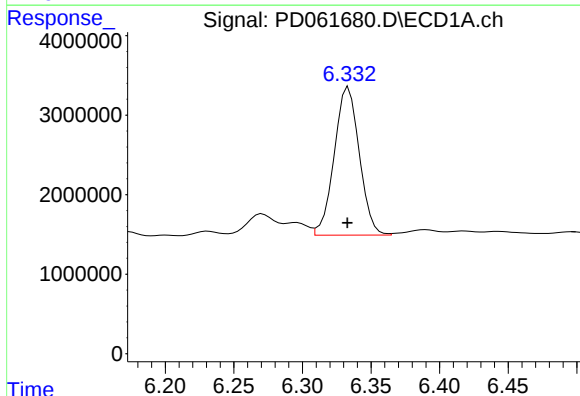


#27 Chlordane-5

R.T.: 6.334 min
Delta R.T.: 0.000 min
Response: 23703888
Conc: 506.47 ng/ml

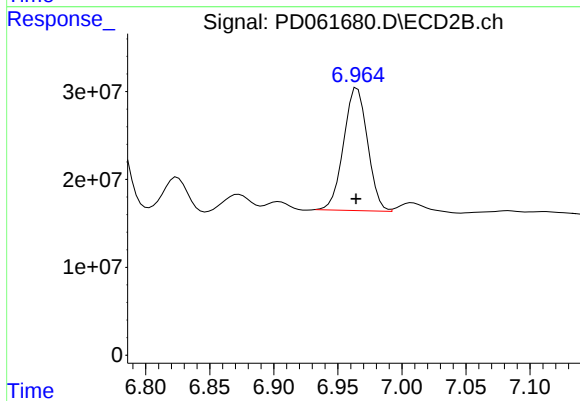

#27 Chlordane-5


R.T.: 6.965 min
Delta R.T.: 0.000 min
Response: 181620390
Conc: 517.65 ng/ml

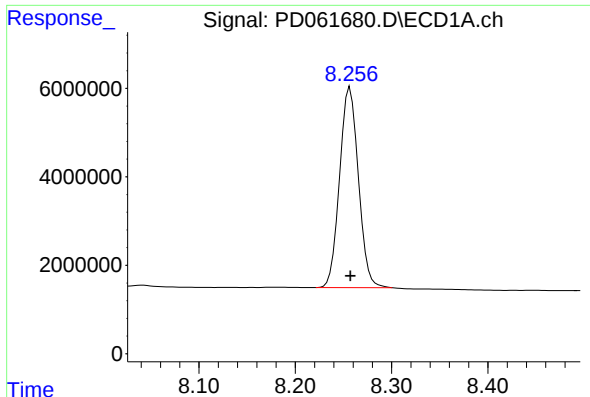

#28 Decachlorobiphenyl

R.T.: 8.257 min
Delta R.T.: 0.000 min
Response: 61289092
Conc: 52.13 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD031721

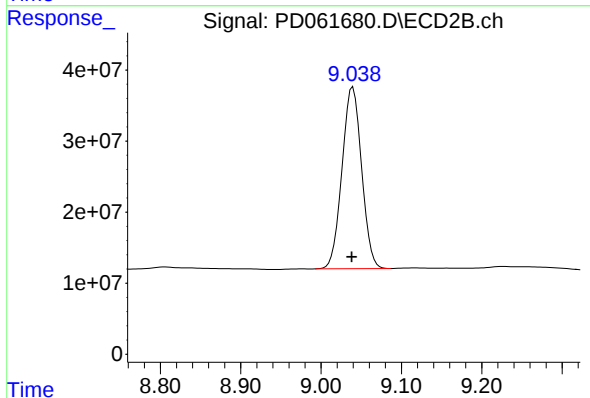

#28 Decachlorobiphenyl

R.T.: 9.040 min
Delta R.T.: 0.001 min
Response: 432872492
Conc: 50.51 ng/ml