

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031721\
 Data File : PD061685.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Mar 2021 20:11
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 18 08:14:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031721.M
 Quant Title : GC Extractables
 QLast Update : Thu Mar 18 07:52:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	3.981	50524013	432.2E6	59.109	50.377
28)	SA Decachlor...	8.257	9.040	60215953	427.6E6	49.203	49.190
Target Compounds							
23)	Chlordane-1	4.360	4.975	17128033	193.7E6	518.521	524.152
24)	Chlordane-2	4.864	5.441	20417067	189.6E6	517.730	506.144
25)	Chlordane-3	5.436	6.087	61656139	819.7E6	522.829	512.336
26)	Chlordane-4	5.493	6.161	50711151	947.7E6	519.722	512.527
27)	Chlordane-5	6.333	6.965	23004971	178.6E6	520.159	509.119



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031721\
Data File : PD061685.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Mar 2021 20:11
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleID :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 18 08:14:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031721.M
Quant Title : GC Extractables
QLast Update : Thu Mar 18 07:52:17 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

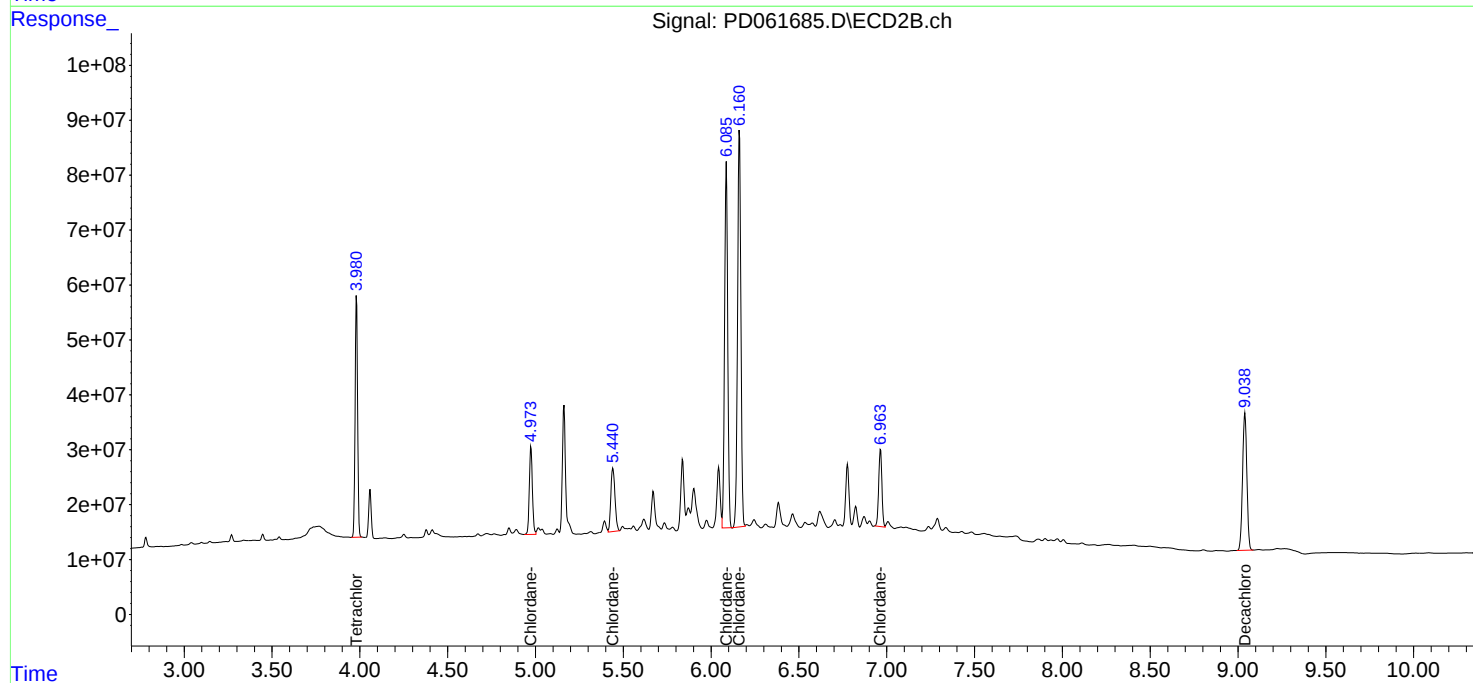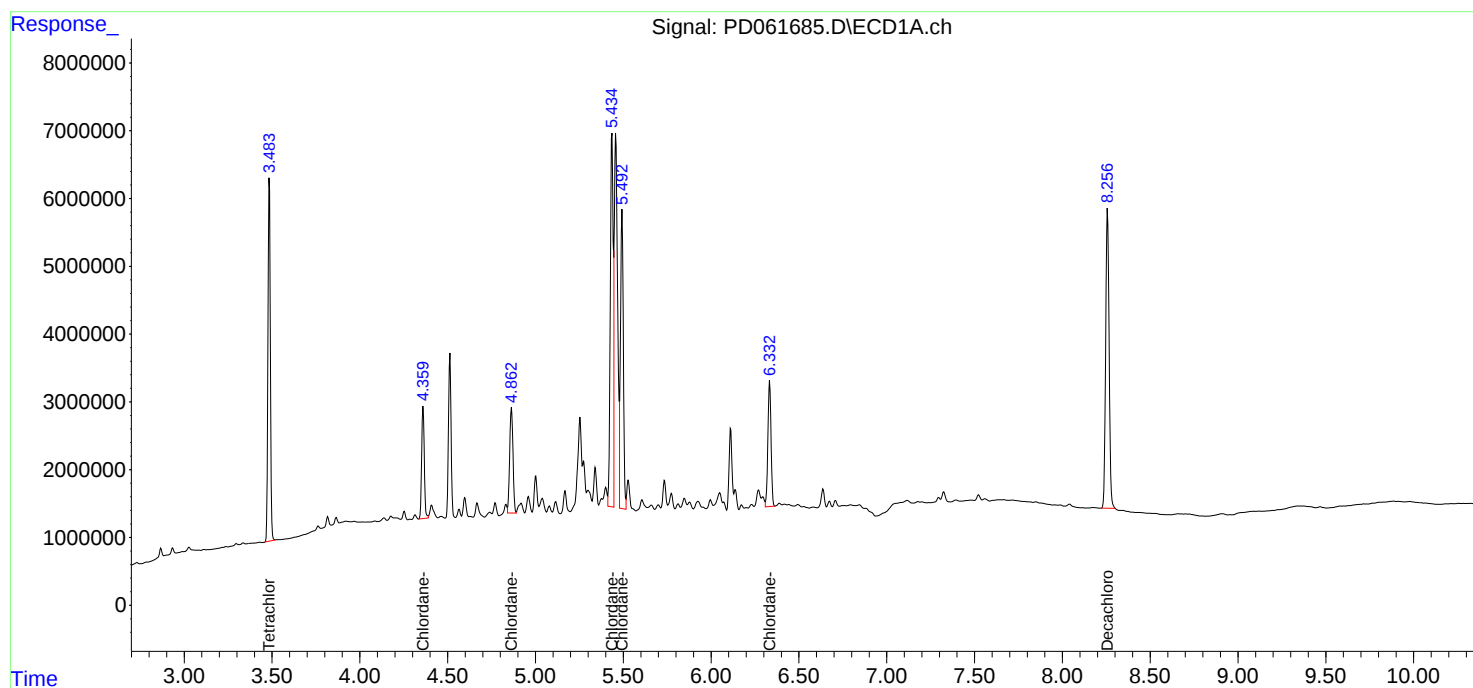


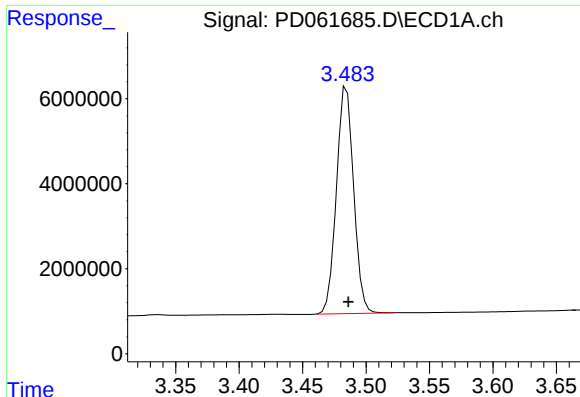

#1 Tetrachloro-m-xylene


R.T.: 3.485 min
Delta R.T.: -0.001 min
Response: 50524013
Conc: 59.11 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

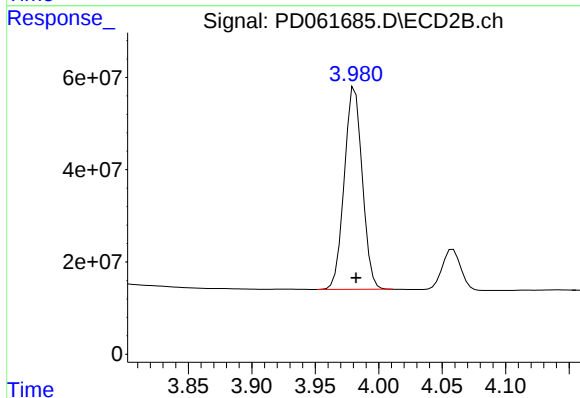


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 432198866
Conc: 50.38 ng/ml

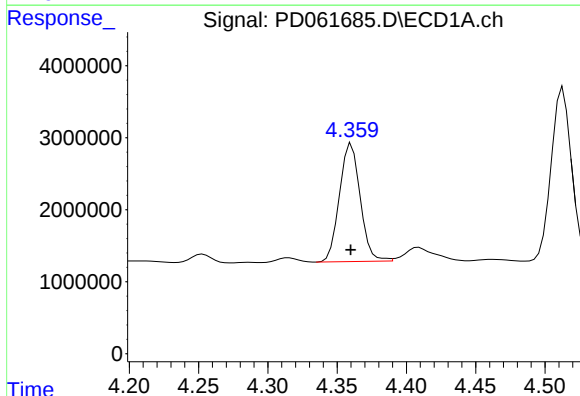


#23 Chlordane-1

R.T.: 4.360 min
Delta R.T.: 0.000 min
Response: 17128033
Conc: 518.52 ng/ml

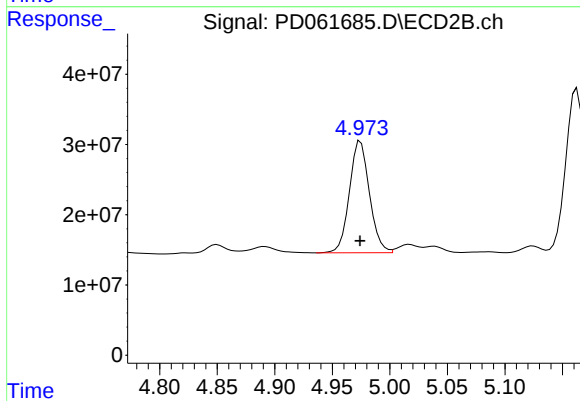

#23 Chlordane-1


R.T.: 4.975 min
Delta R.T.: 0.000 min
Response: 193709210
Conc: 524.15 ng/ml

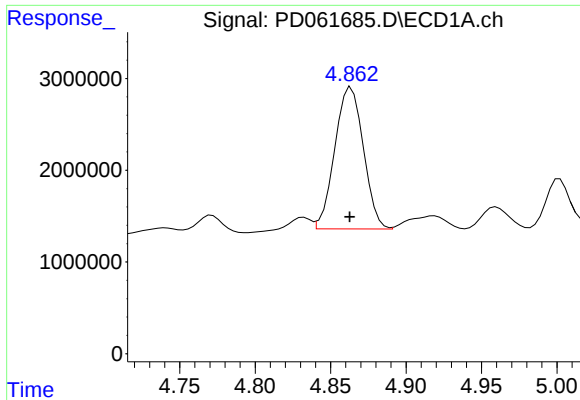

#24 Chlordane-2


R.T.: 4.864 min
Delta R.T.: 0.001 min
Response: 20417067
Conc: 517.73 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

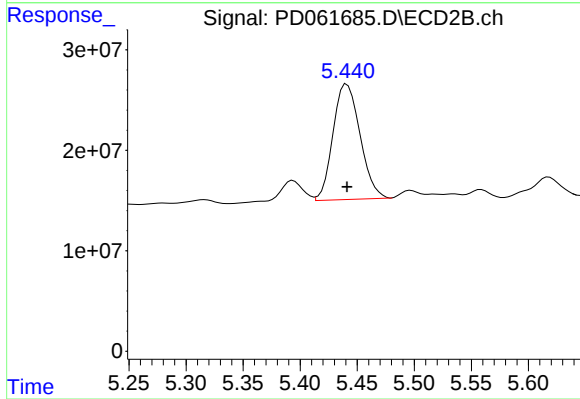


#24 Chlordane-2

R.T.: 5.441 min
Delta R.T.: 0.000 min
Response: 189644059
Conc: 506.14 ng/ml

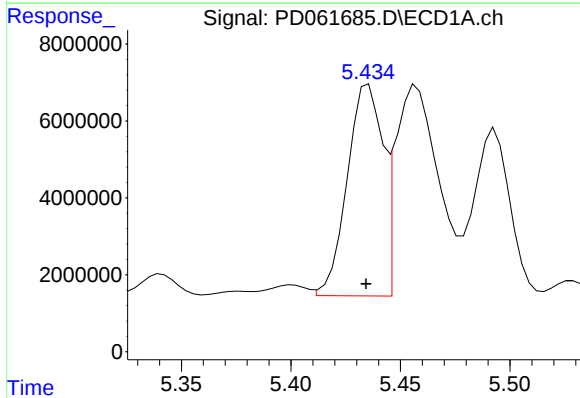


#25 Chlordane-3

R.T.: 5.436 min
Delta R.T.: 0.001 min
Response: 61656139
Conc: 522.83 ng/ml

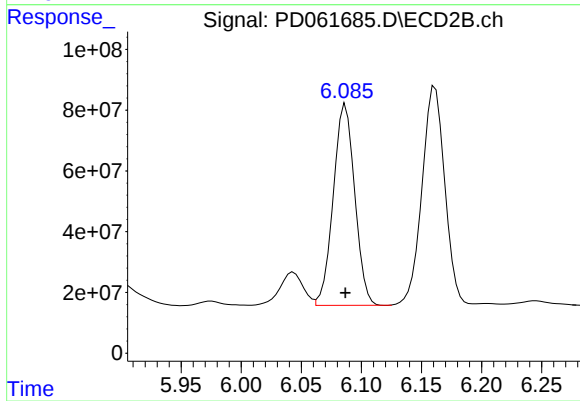

#25 Chlordane-3


R.T.: 6.087 min
Delta R.T.: 0.000 min
Response: 819710838
Conc: 512.34 ng/ml

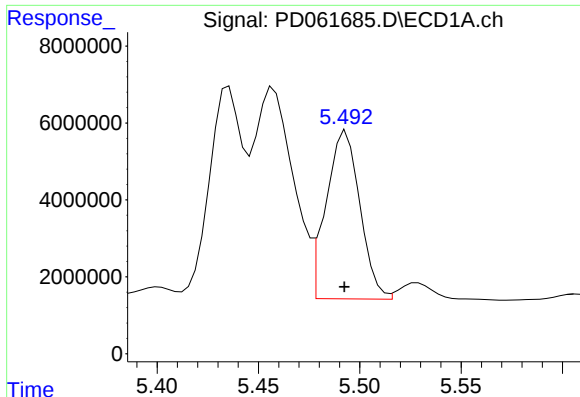

#26 Chlordane-4


R.T.: 5.493 min
Delta R.T.: 0.000 min
Response: 50711151
Conc: 519.72 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

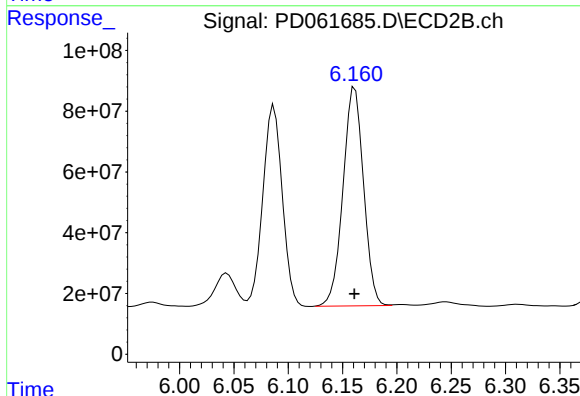


#26 Chlordane-4

R.T.: 6.161 min
Delta R.T.: 0.000 min
Response: 947669199
Conc: 512.53 ng/ml

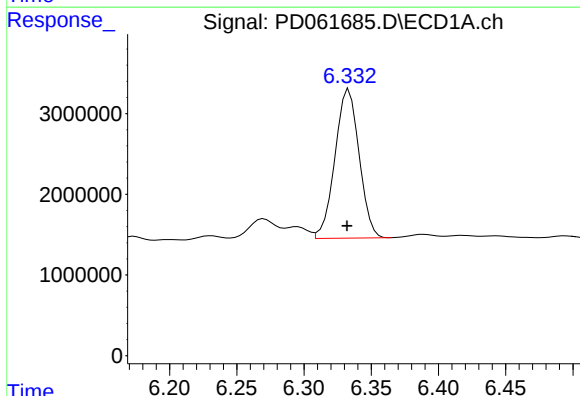


#27 Chlordane-5

R.T.: 6.333 min
Delta R.T.: 0.001 min
Response: 23004971
Conc: 520.16 ng/ml

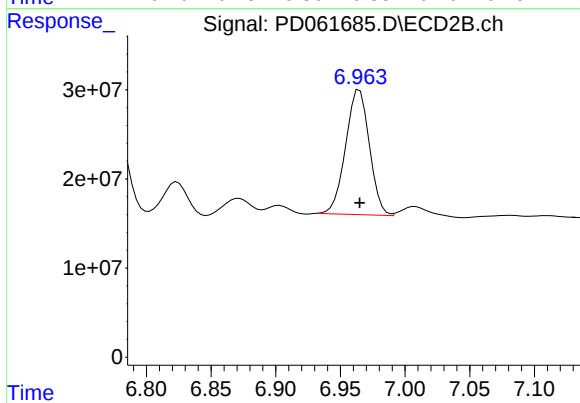

#27 Chlordane-5


R.T.: 6.965 min
Delta R.T.: 0.000 min
Response: 178626650
Conc: 509.12 ng/ml

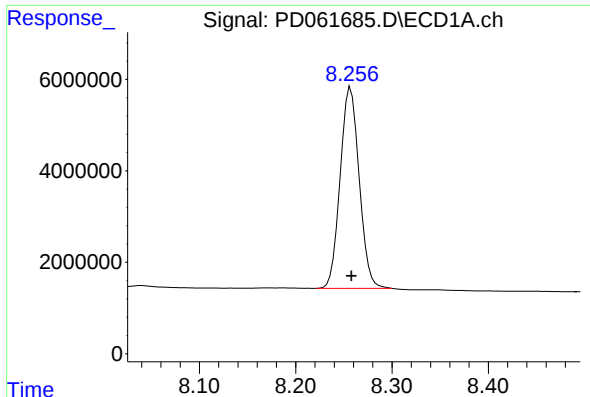

#28 Decachlorobiphenyl

R.T.: 8.257 min
Delta R.T.: 0.000 min
Response: 60215953
Conc: 49.20 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

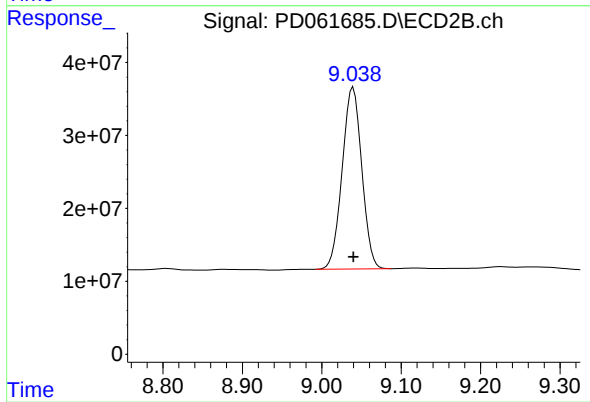

#28 Decachlorobiphenyl

R.T.: 9.040 min
Delta R.T.: 0.000 min
Response: 427612842
Conc: 49.19 ng/ml