

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031721\
 Data File : PD061697.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Mar 2021 22:59
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 18 08:26:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031721.M
 Quant Title : GC Extractables
 QLast Update : Thu Mar 18 07:52:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	3.982	49651990	410.3E6	58.089	47.828
28)	SA Decachlor...	8.257	9.039	57466907	419.1E6	46.957	48.206
Target Compounds							
23)	Chlordane-1	4.360	4.975	16804051	184.6E6	508.713	499.561
24)	Chlordane-2	4.864	5.441	20153630	178.7E6	511.050	477.004
25)	Chlordane-3	5.435	6.087	59071908	787.6E6	500.915	492.279
26)	Chlordane-4	5.493	6.161	49417151	899.2E6	506.461	486.293
27)	Chlordane-5	6.333	6.965	21726375	169.4E6	491.249	482.960



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031721\
Data File : PD061697.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Mar 2021 22:59
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 18 08:26:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031721.M
Quant Title : GC Extractables
QLast Update : Thu Mar 18 07:52:17 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

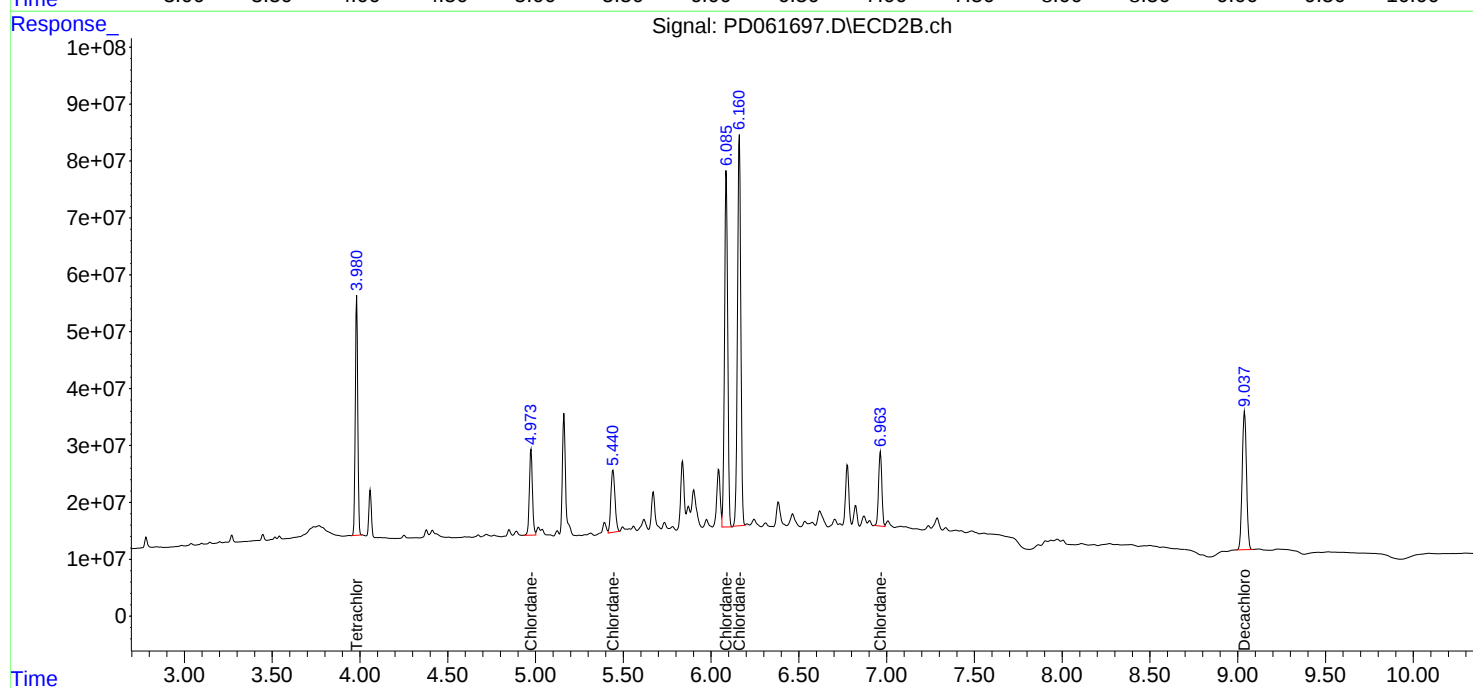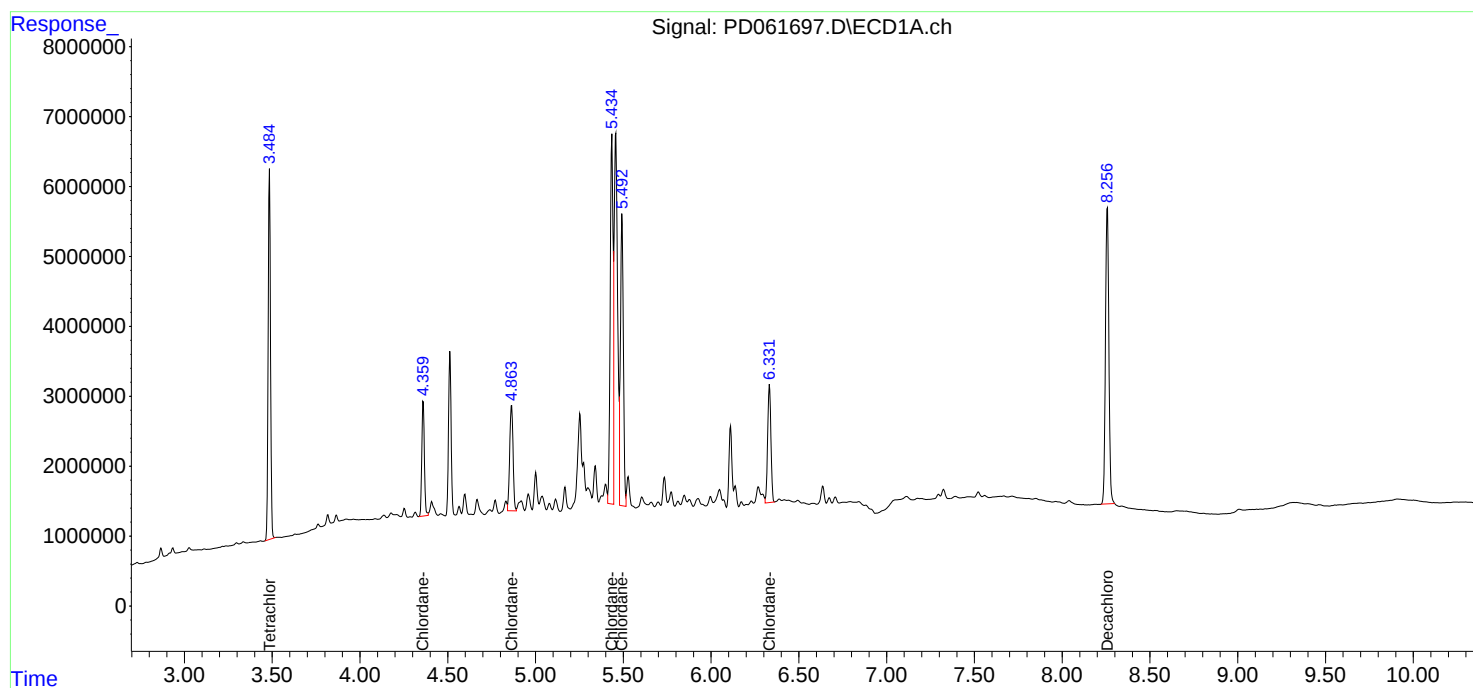


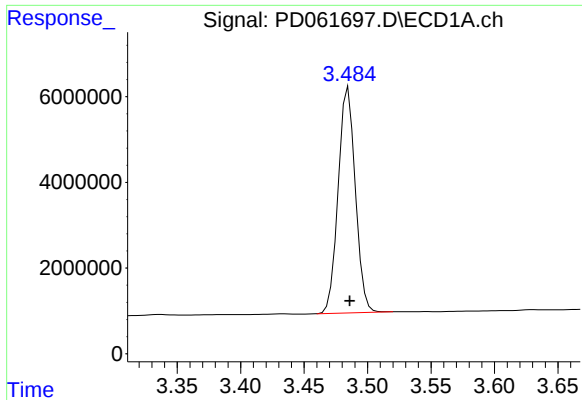

#1 Tetrachloro-m-xylene


R.T.: 3.485 min
Delta R.T.: -0.001 min
Response: 49651990
Conc: 58.09 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

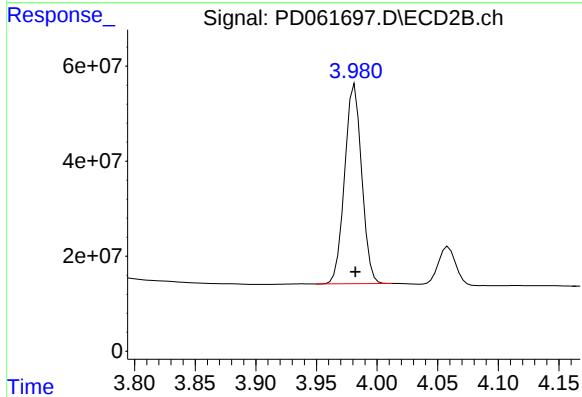


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 410330570
Conc: 47.83 ng/ml

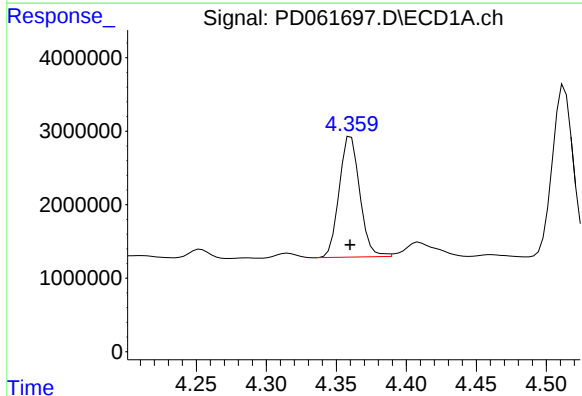


#23 Chlordane-1

R.T.: 4.360 min
Delta R.T.: 0.000 min
Response: 16804051
Conc: 508.71 ng/ml

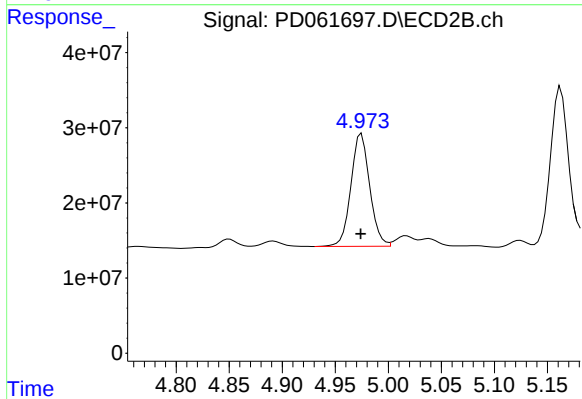

#23 Chlordane-1


R.T.: 4.975 min
Delta R.T.: 0.000 min
Response: 184621177
Conc: 499.56 ng/ml

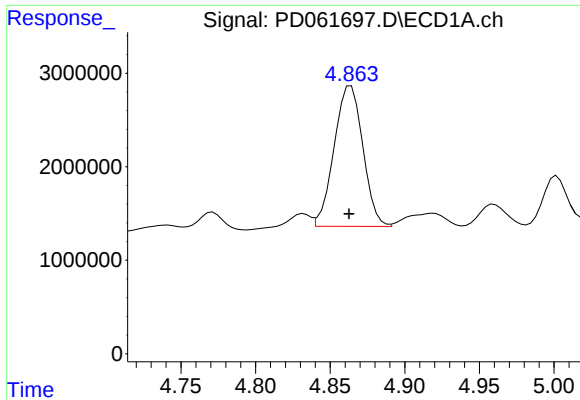

#24 Chlordane-2


R.T.: 4.864 min
Delta R.T.: 0.001 min
Response: 20153630
Conc: 511.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

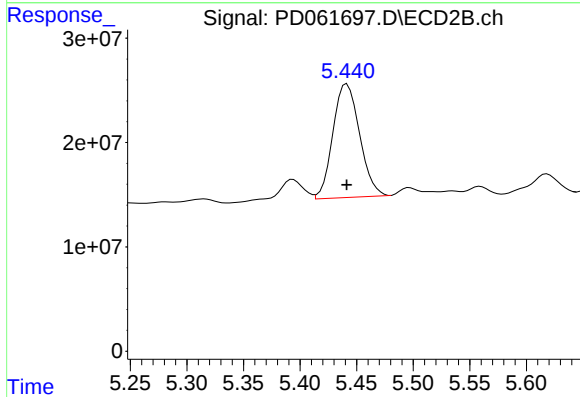


#24 Chlordane-2

R.T.: 5.441 min
Delta R.T.: 0.000 min
Response: 178725927
Conc: 477.00 ng/ml

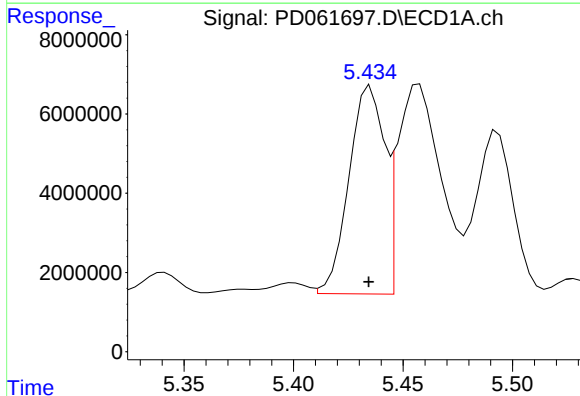


#25 Chlordane-3

R.T.: 5.435 min
Delta R.T.: 0.000 min
Response: 59071908
Conc: 500.92 ng/ml

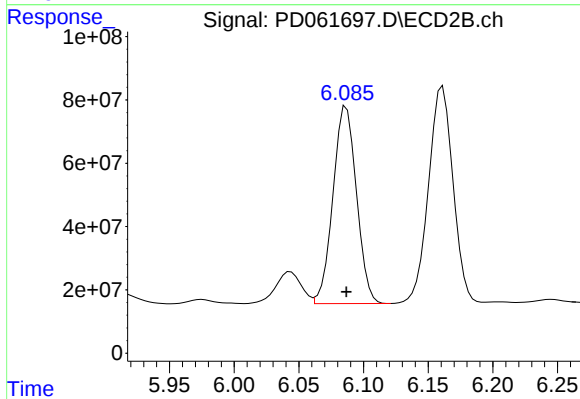

#25 Chlordane-3


R.T.: 6.087 min
Delta R.T.: 0.000 min
Response: 787620910
Conc: 492.28 ng/ml

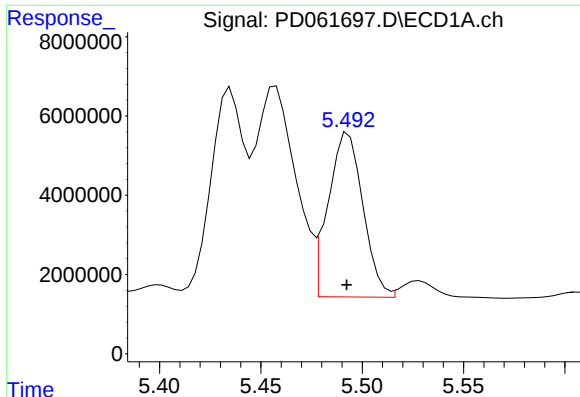

#26 Chlordane-4


R.T.: 5.493 min
Delta R.T.: 0.000 min
Response: 49417151
Conc: 506.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

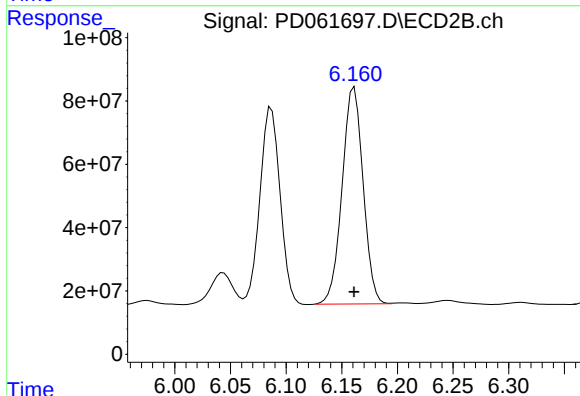


#26 Chlordane-4

R.T.: 6.161 min
Delta R.T.: 0.000 min
Response: 899162065
Conc: 486.29 ng/ml

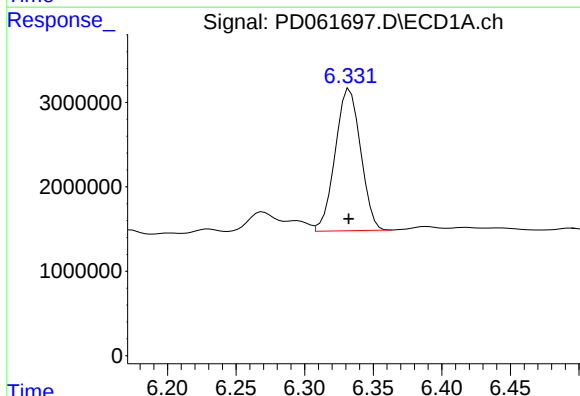


#27 Chlordane-5

R.T.: 6.333 min
Delta R.T.: 0.000 min
Response: 21726375
Conc: 491.25 ng/ml

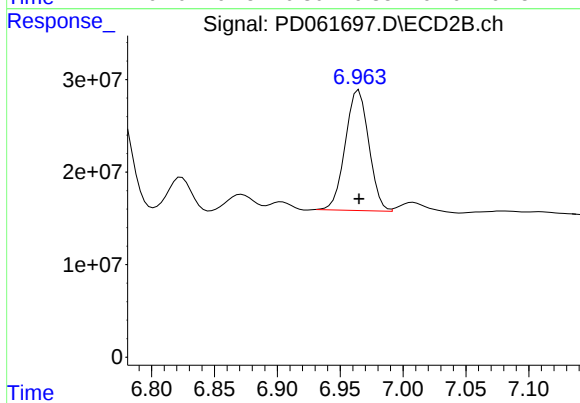

#27 Chlordane-5


R.T.: 6.965 min
Delta R.T.: 0.000 min
Response: 169448734
Conc: 482.96 ng/ml

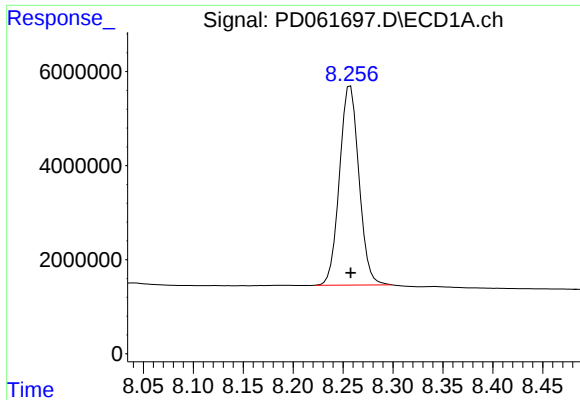

#28 Decachlorobiphenyl

R.T.: 8.257 min
Delta R.T.: 0.000 min
Response: 57466907
Conc: 46.96 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

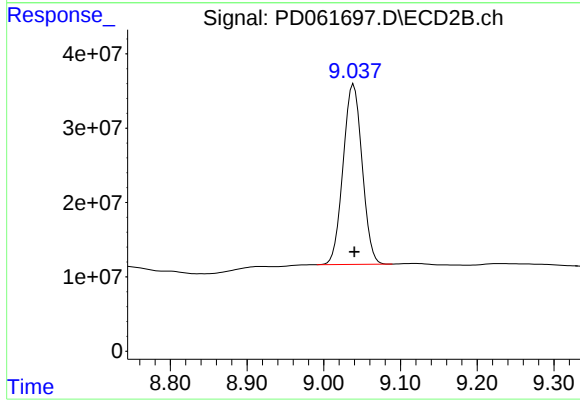

#28 Decachlorobiphenyl

R.T.: 9.039 min
Delta R.T.: -0.001 min
Response: 419065847
Conc: 48.21 ng/ml