

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031722\
 Data File : PD0684651.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2022 15:04
 Operator : AR\AJ
 Sample : PB143387BL (Sig #1); PB143397BSD (Sig #2)
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 03:14:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 03:30:32 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.456	4.176	21598403	181.7E6	17.789	19.002
28)	SA Decachlor...	8.217	9.375	24863383	116.9E6	19.680	20.637
Target Compounds							
4)	MA Heptachlor	0.000	5.395	0	178118	N.D.	0.015 #
6)	B beta-BHC	4.397f	5.041f	321519	6579160	0.432	1.198 #
7)	B delta-BHC	0.000	5.232f	0	1230048	N.D.	0.102 #
8)	B Heptachlo...	0.000	6.079	0	6009414	N.D.	0.575 #
12)	B 4,4'-DDE	0.000	6.530f	0	418198	N.D.	0.045 #
14)	MA Endrin	6.025f	0.000	189116	0	0.144	N.D. #
21)	B Endrin ke...	0.000	7.970	0	2182841	N.D.	0.282 #
23)	Chlordane-1	0.000	5.177f	0	593914	N.D.	1.505 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031722\
Data File : PD0684651.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2022 15:04
Operator : AR\AJ
Sample : PB143387BL (Sig #1); PB143397BSD (Sig #2)
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 03:14:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 03:30:32 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

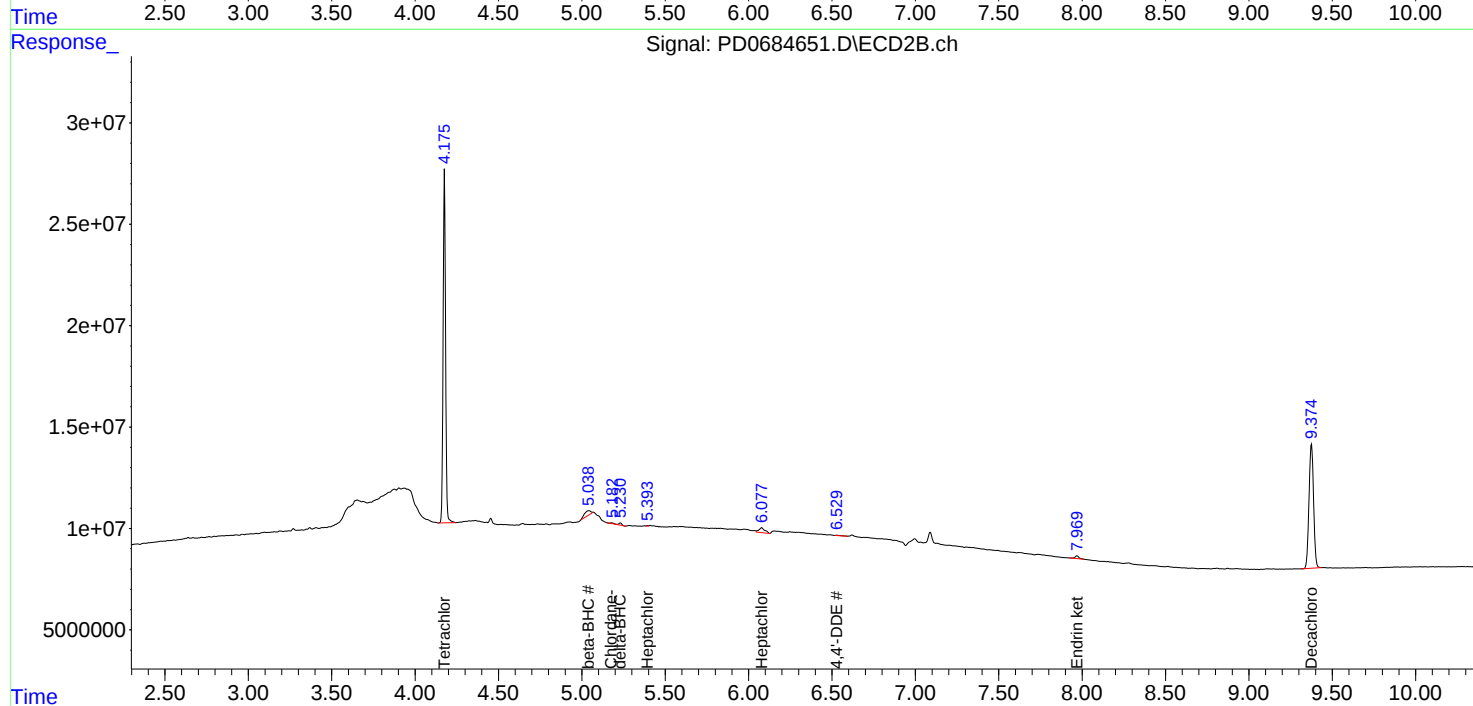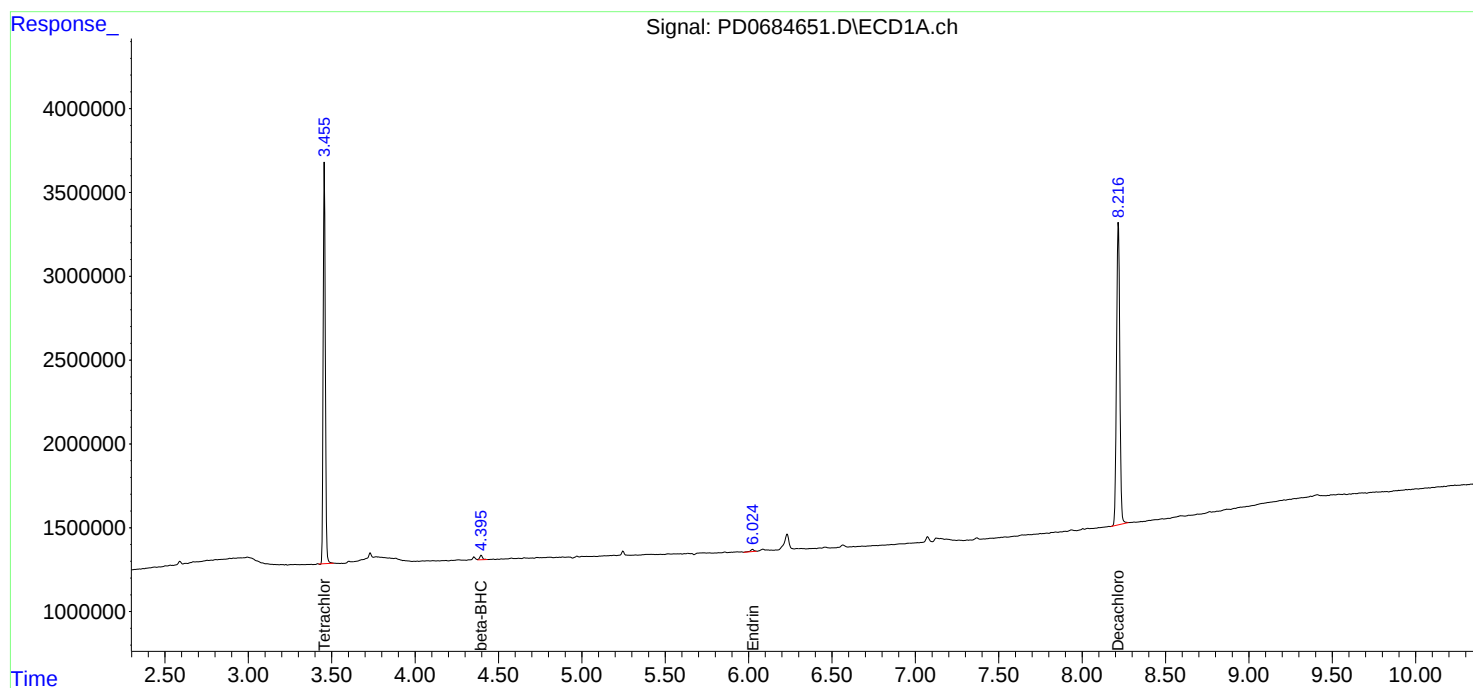


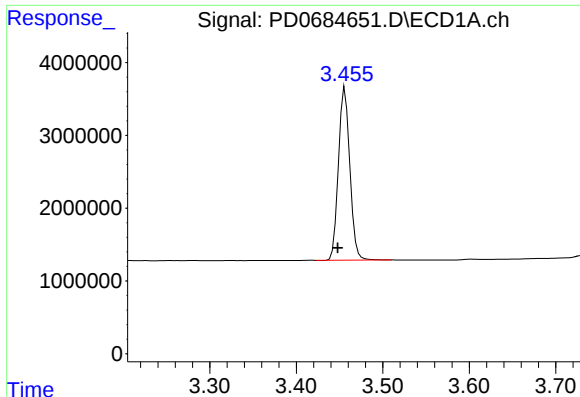

#1 Tetrachloro-m-xylene


R.T.: 3.456 min
Delta R.T.: 0.008 min
Response: 21598403
Conc: 17.79 ng/ml

Instrument :
ECD_D
ClientSampleId :

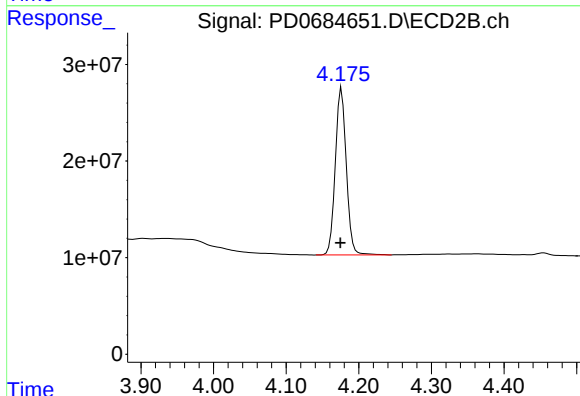


#1 Tetrachloro-m-xylene

R.T.: 4.176 min
Delta R.T.: 0.002 min
Response: 181675258
Conc: 19.00 ng/ml

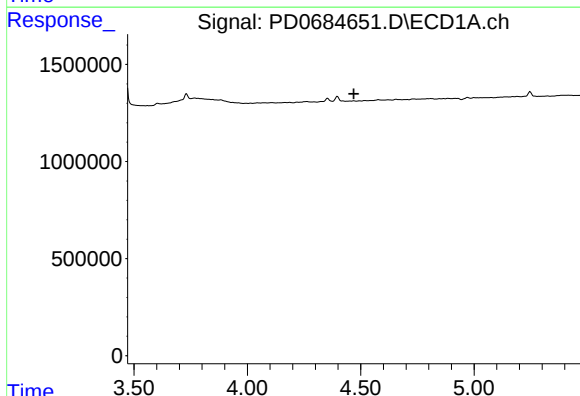


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.470 min
Response: 0
Conc: N.D.

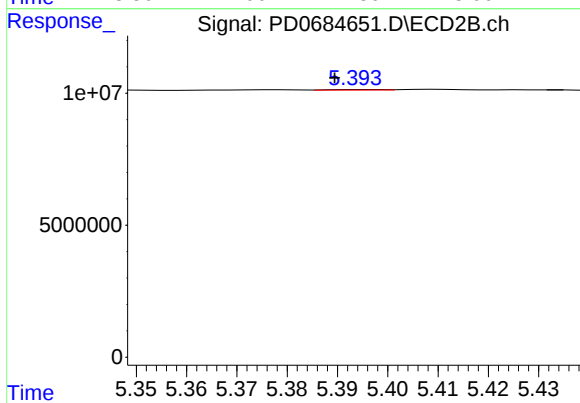

#4 Heptachlor


R.T.: 5.395 min
Delta R.T.: 0.005 min
Response: 178118
Conc: 0.01 ng/ml

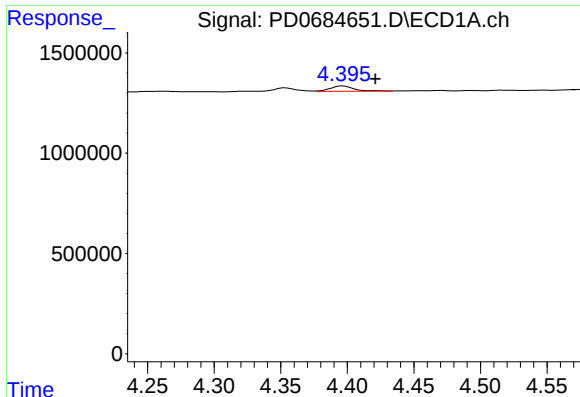

#6 beta-BHC


R.T.: 4.397 min
Delta R.T.: -0.024 min
Response: 321519
Conc: 0.43 ng/ml

Instrument :
ECD_D
ClientSampleId :

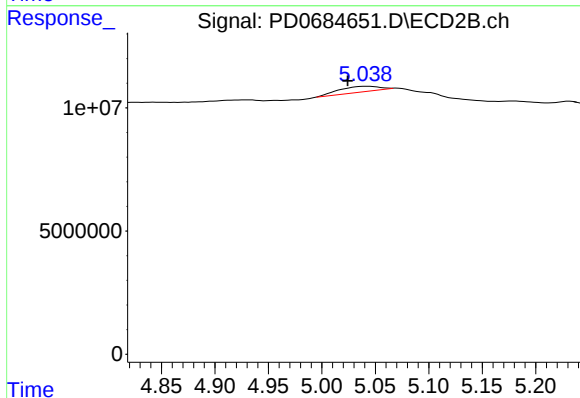


#6 beta-BHC

R.T.: 5.041 min
Delta R.T.: 0.017 min
Response: 6579160
Conc: 1.20 ng/ml

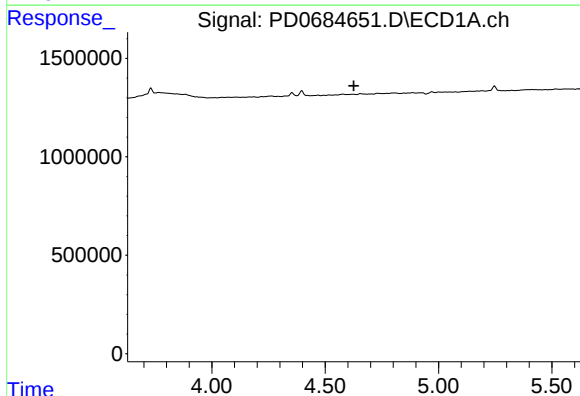


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.626 min
Response: 0
Conc: N.D.

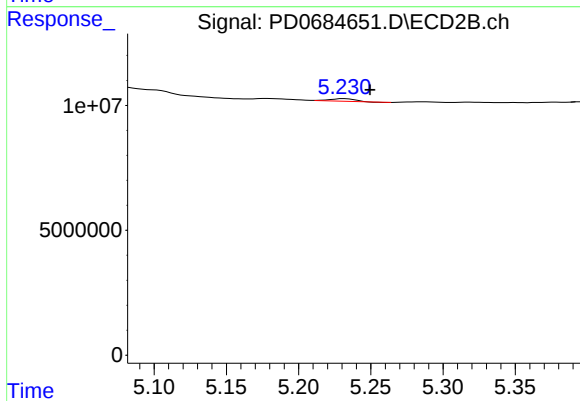

#7 delta-BHC


R.T.: 5.232 min
Delta R.T.: -0.018 min
Response: 1230048
Conc: 0.10 ng/ml

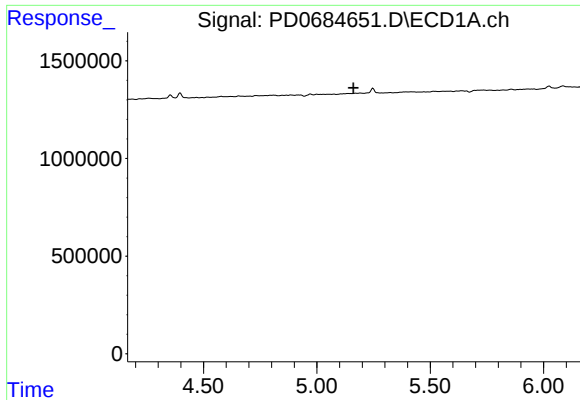

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.162 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

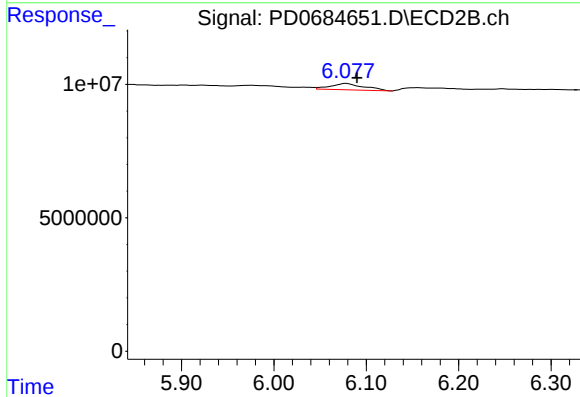


#8 Heptachlor epoxide

R.T.: 6.079 min
Delta R.T.: -0.011 min
Response: 6009414
Conc: 0.58 ng/ml

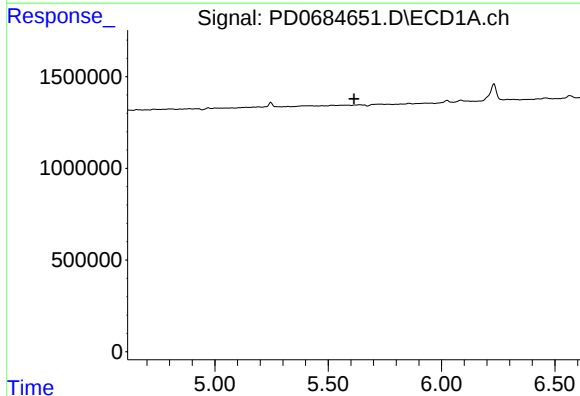


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.614 min
Response: 0
Conc: N.D.

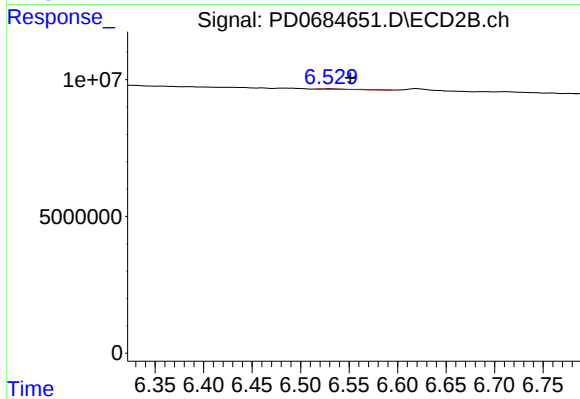

#12 4,4'-DDE


R.T.: 6.530 min
Delta R.T.: -0.021 min
Response: 418198
Conc: 0.05 ng/ml

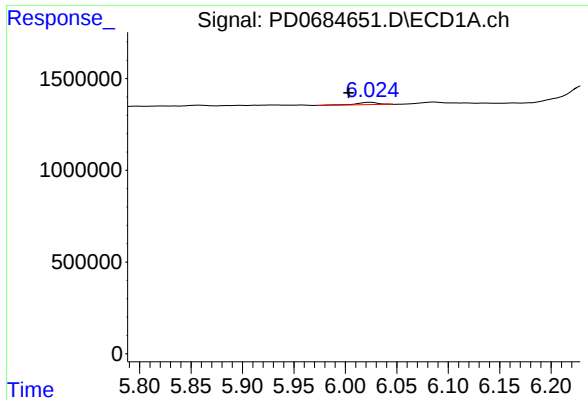

#14 Endrin


R.T.: 6.025 min
Delta R.T.: 0.022 min
Response: 189116
Conc: 0.14 ng/ml

Instrument :
ECD_D
ClientSampleId :

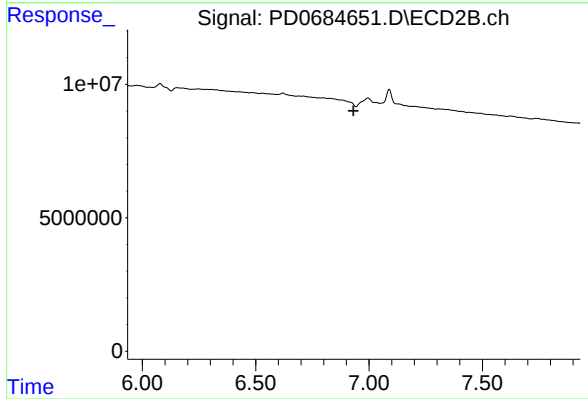


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.932 min
Response: 0
Conc: N.D.

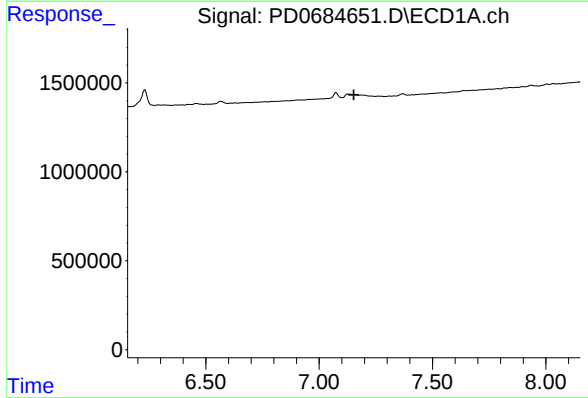


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.153 min
Response: 0
Conc: N.D.

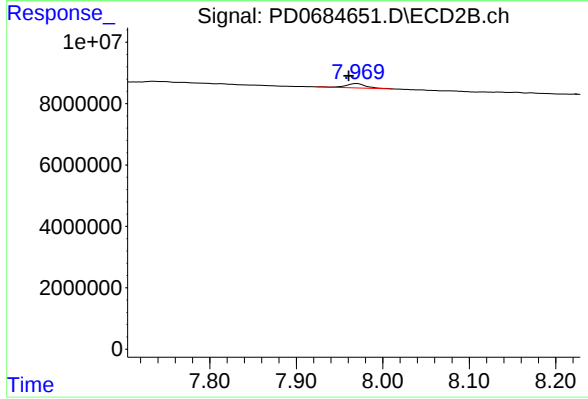

#21 Endrin ketone


R.T.: 7.970 min
Delta R.T.: 0.009 min
Response: 2182841
Conc: 0.28 ng/ml

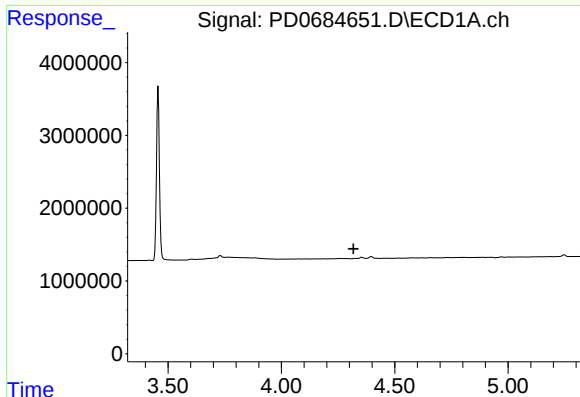

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.319 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

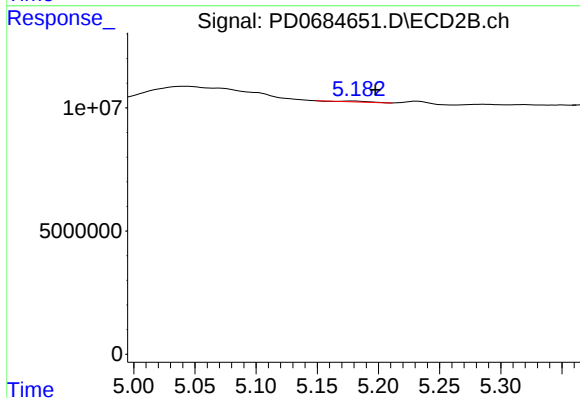


#23 Chlordane-1

R.T.: 5.177 min
Delta R.T.: -0.021 min
Response: 593914
Conc: 1.51 ng/ml

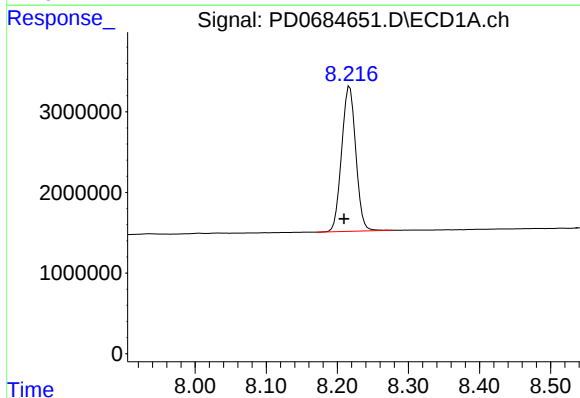

#28 Decachlorobiphenyl

R.T.: 8.217 min
Delta R.T.: 0.008 min
Response: 24863383
Conc: 19.68 ng/ml

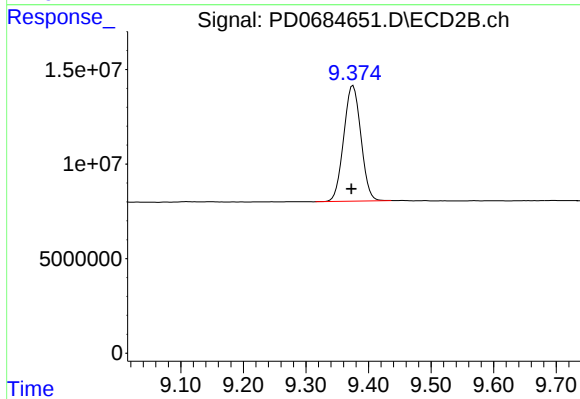

#28 Decachlorobiphenyl

R.T.: 9.375 min
Delta R.T.: 0.003 min
Response: 116945509
Conc: 20.64 ng/ml