

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031722\
 Data File : PD0684654.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2022 16:03
 Operator : AR\AJ
 Sample : N1949-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 03:15:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 03:30:32 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.449	4.175	27121745	220.2E6	22.338	23.031
28)	SA Decachlor...	8.208	9.370	25454649	120.3E6	20.148	21.222
Target Compounds							
2)	A alpha-BHC	3.878	0.000	425404	0	0.235	N.D. #
4)	MA Heptachlor	0.000	5.395	0	82174	N.D.	0.007 #
6)	B beta-BHC	0.000	5.029	0	448394	N.D.	0.082 #
7)	B delta-BHC	0.000	5.230f	0	1692480	N.D.	0.141 #
8)	B Heptachlo...	0.000	6.073f	0	2734204	N.D.	0.262 #
11)	B alpha-Chl...	0.000	6.402	0	1015537	N.D.	0.102 #
21)	B Endrin ke...	0.000	7.962	0	497334	N.D.	0.064 #
26)	Chlordane-4	0.000	6.402	0	1015537	N.D.	0.653 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031722\
Data File : PD0684654.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2022 16:03
Operator : AR\AJ
Sample : N1949-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 03:15:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 03:30:32 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

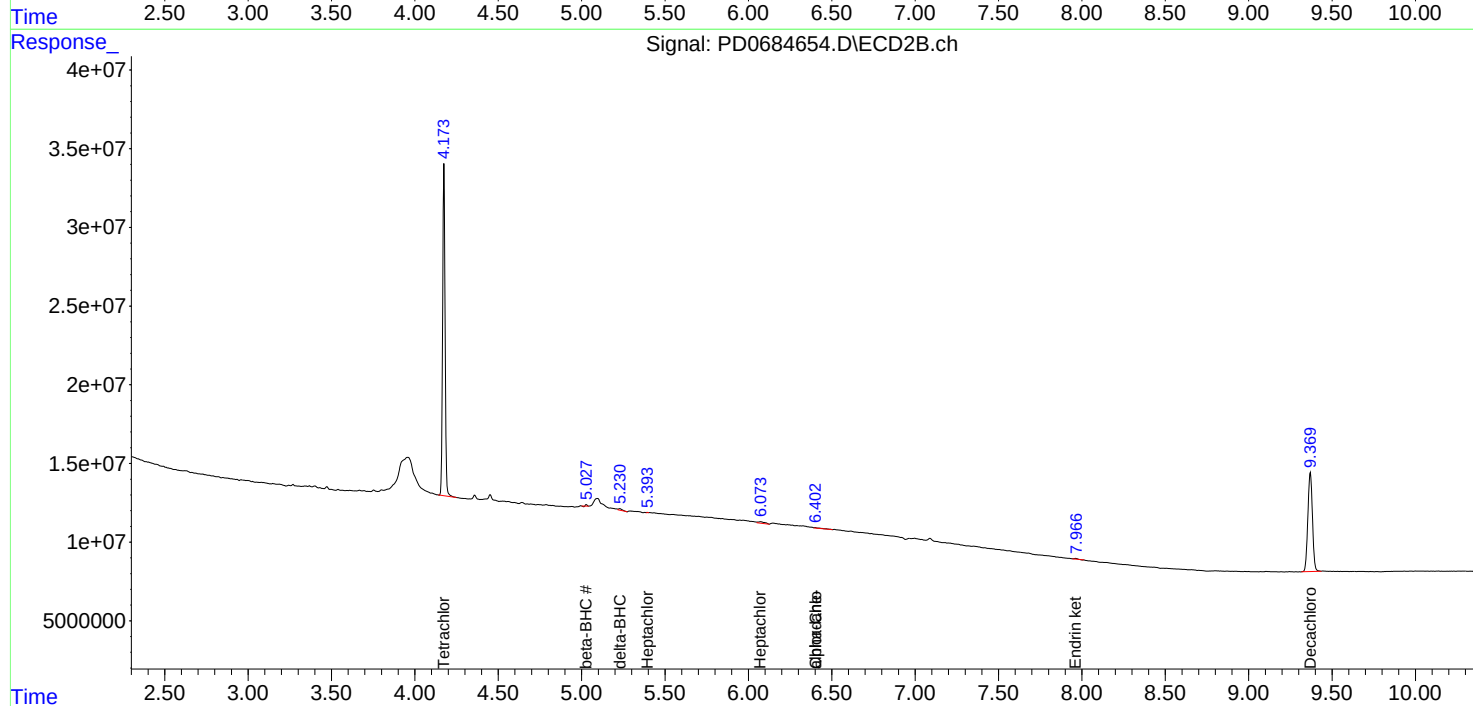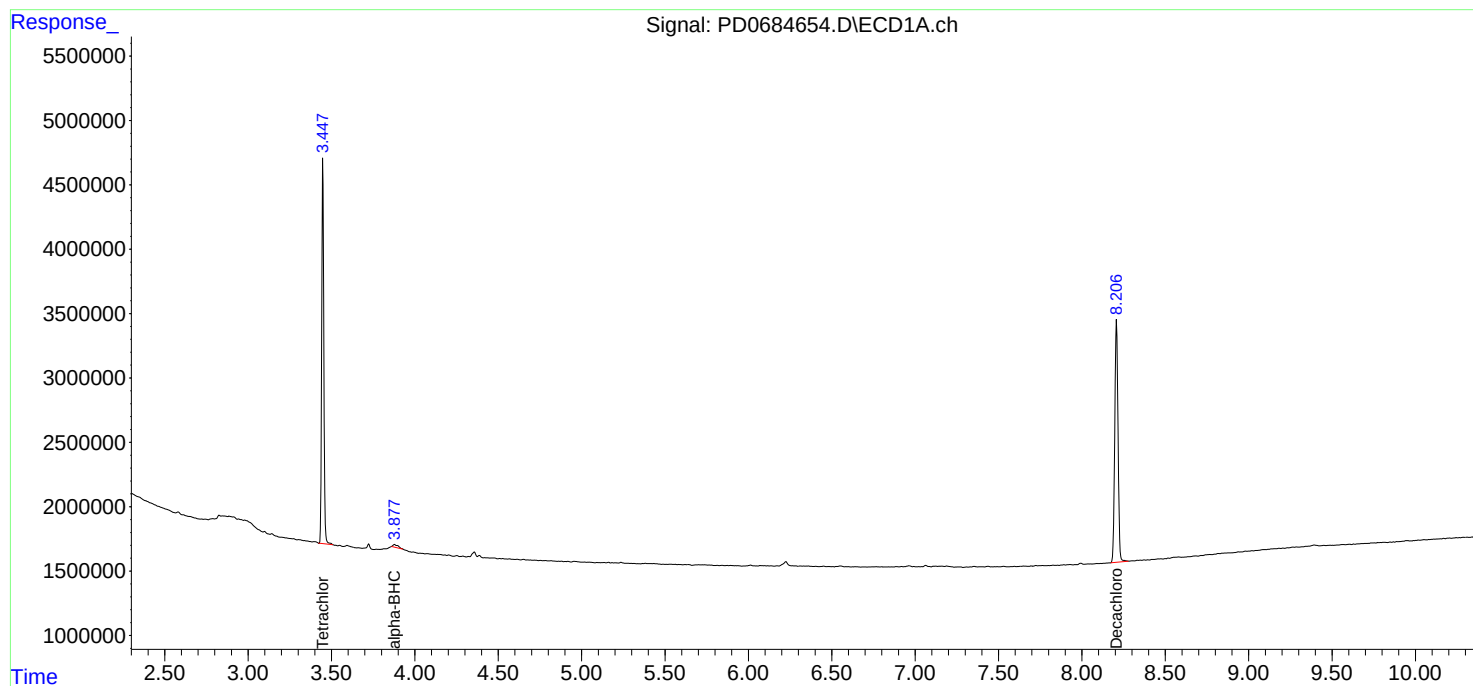


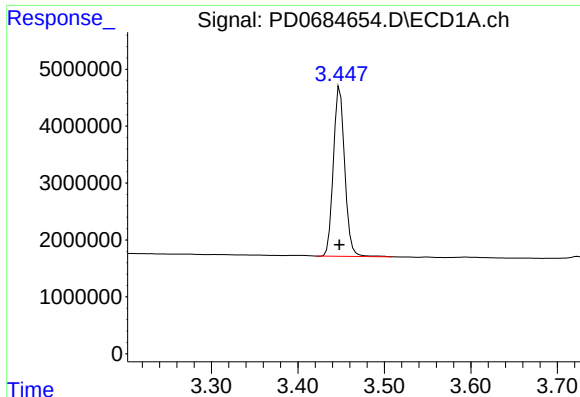

#1 Tetrachloro-m-xylene


R.T.: 3.449 min
Delta R.T.: 0.000 min
Response: 27121745
Conc: 22.34 ng/ml

Instrument :
ECD_D
ClientSampleId :

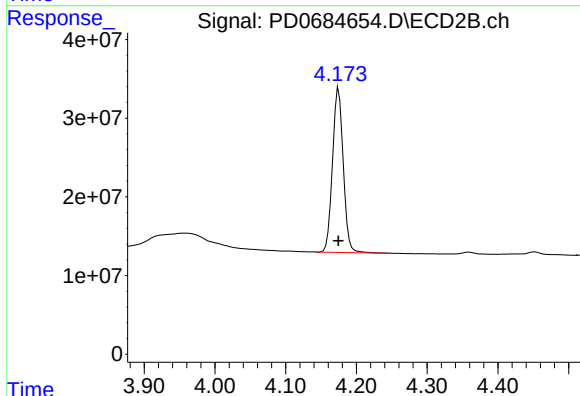


#1 Tetrachloro-m-xylene

R.T.: 4.175 min
Delta R.T.: 0.000 min
Response: 220191383
Conc: 23.03 ng/ml

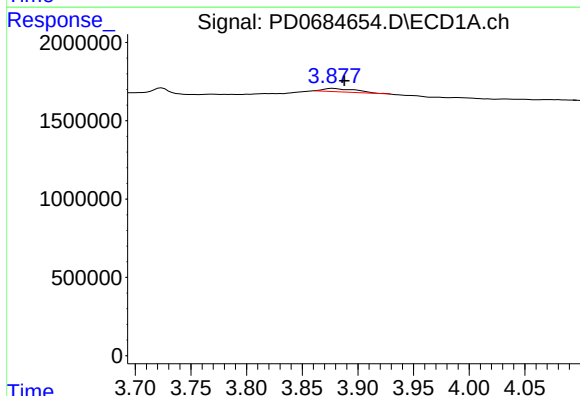


#2 alpha-BHC

R.T.: 3.878 min
Delta R.T.: -0.010 min
Response: 425404
Conc: 0.23 ng/ml

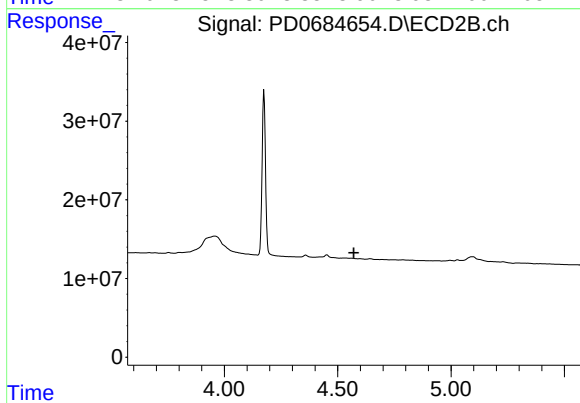

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.571 min
Response: 0
Conc: N.D.

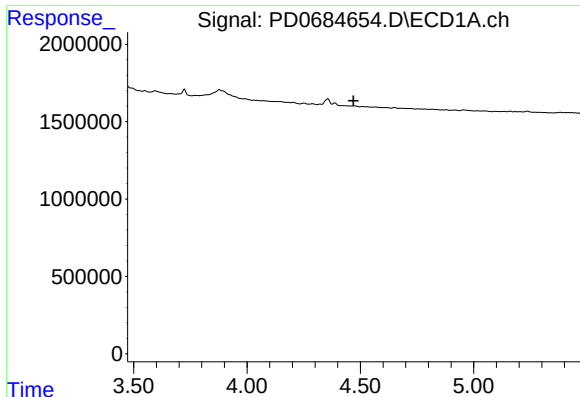

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.470 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

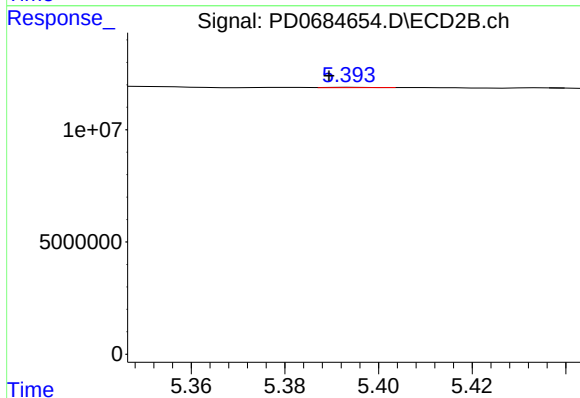


#4 Heptachlor

R.T.: 5.395 min
Delta R.T.: 0.005 min
Response: 82174
Conc: 0.01 ng/ml

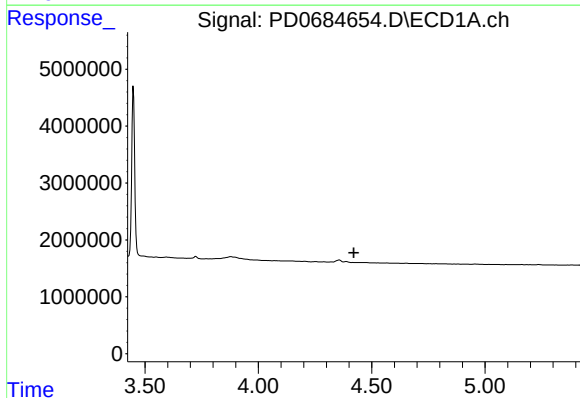


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.421 min
Response: 0
Conc: N.D.

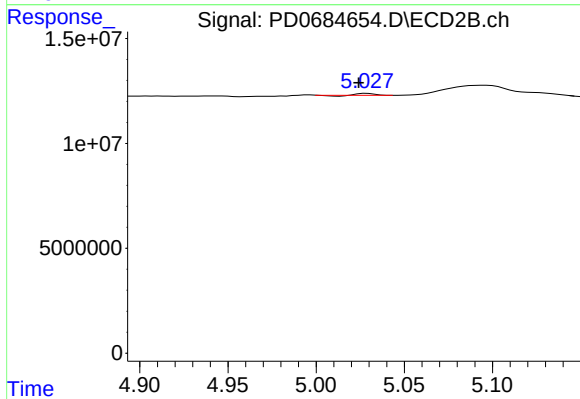

#6 beta-BHC


R.T.: 5.029 min
Delta R.T.: 0.005 min
Response: 448394
Conc: 0.08 ng/ml

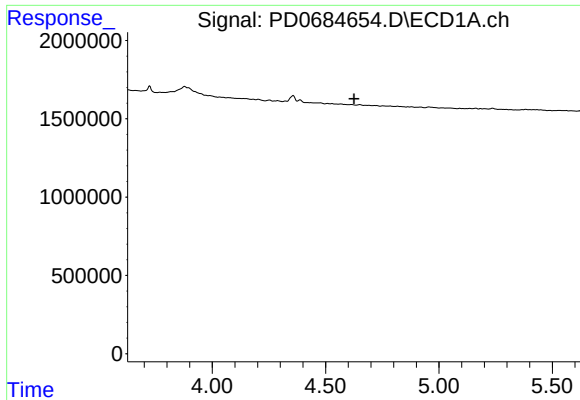

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.626 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

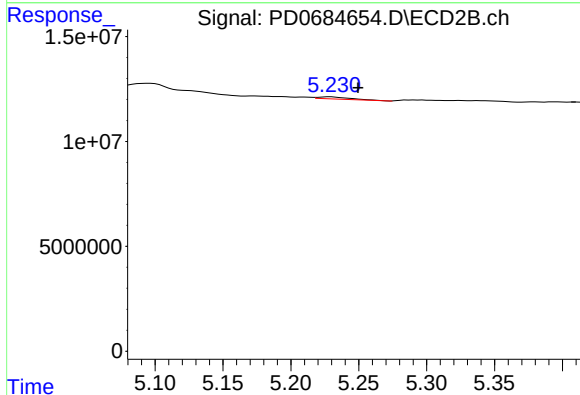


#7 delta-BHC

R.T.: 5.230 min
Delta R.T.: -0.020 min
Response: 1692480
Conc: 0.14 ng/ml

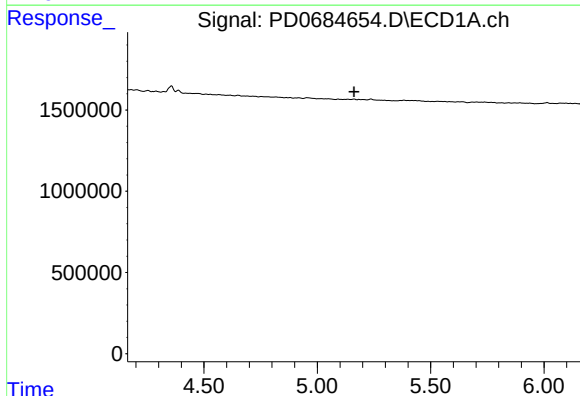


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.162 min
Response: 0
Conc: N.D.

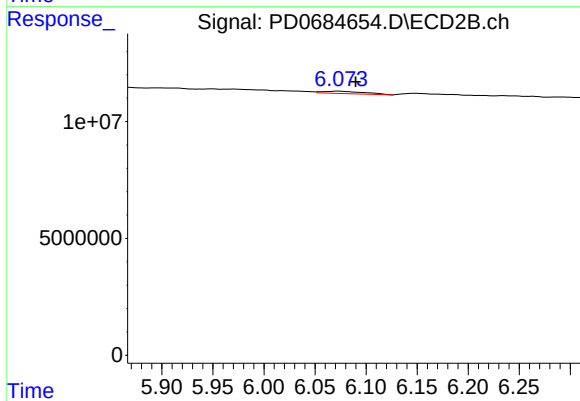

#8 Heptachlor epoxide


R.T.: 6.073 min
Delta R.T.: -0.017 min
Response: 2734204
Conc: 0.26 ng/ml

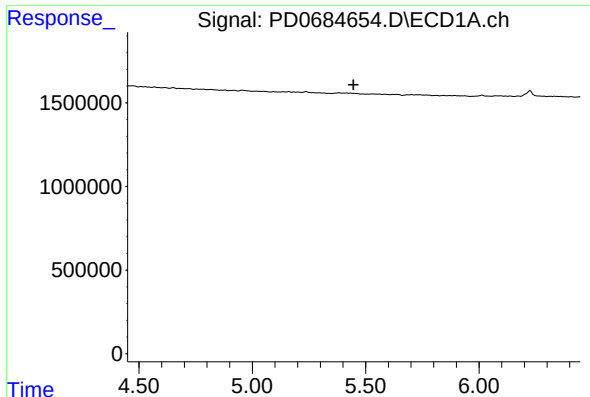

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.447 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

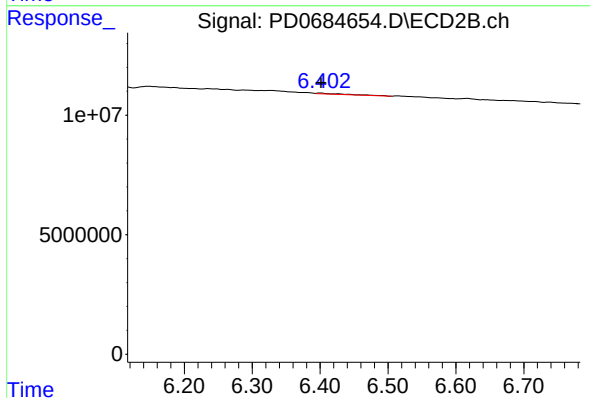


#11 alpha-Chlordane

R.T.: 6.402 min
Delta R.T.: 0.000 min
Response: 1015537
Conc: 0.10 ng/ml

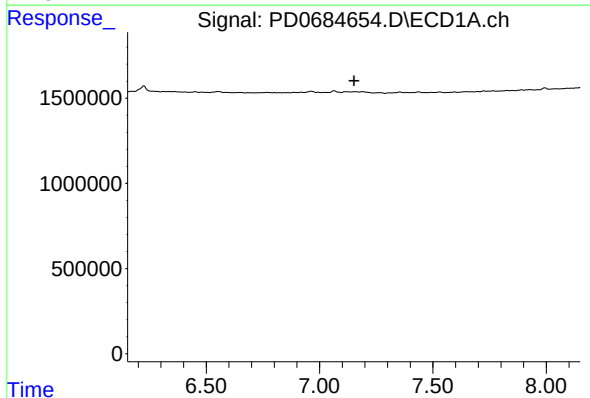


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 7.153 min
Response: 0
Conc: N.D.

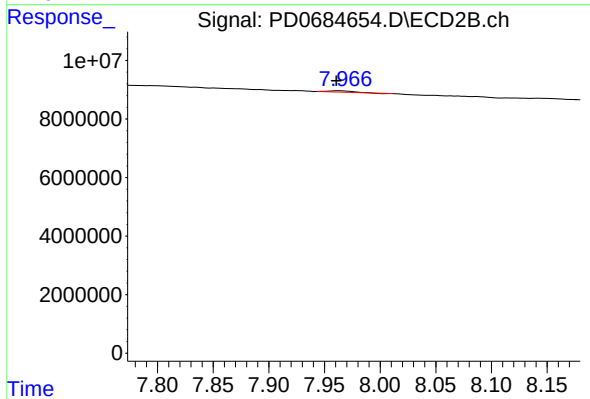

#21 Endrin ketone


R.T.: 7.962 min
Delta R.T.: 0.002 min
Response: 497334
Conc: 0.06 ng/ml

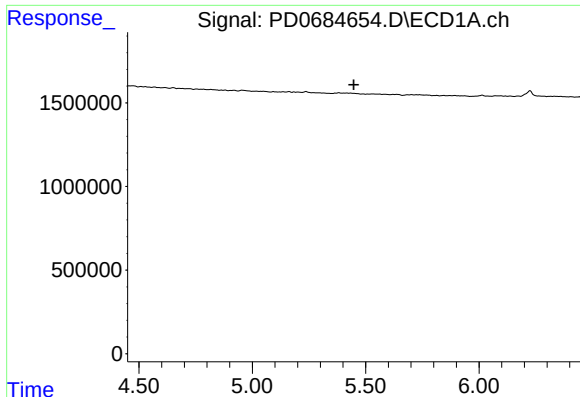

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.447 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

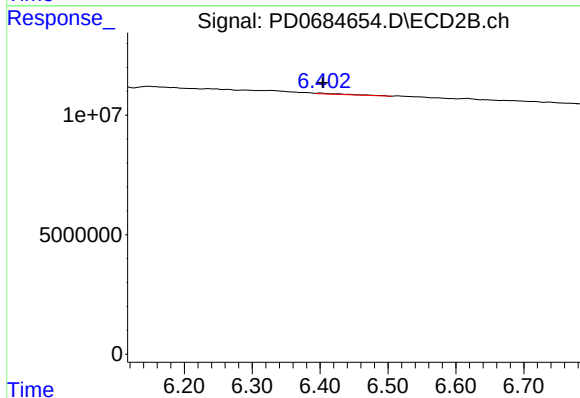


#26 Chlordane-4

R.T.: 6.402 min
Delta R.T.: -0.003 min
Response: 1015537
Conc: 0.65 ng/ml

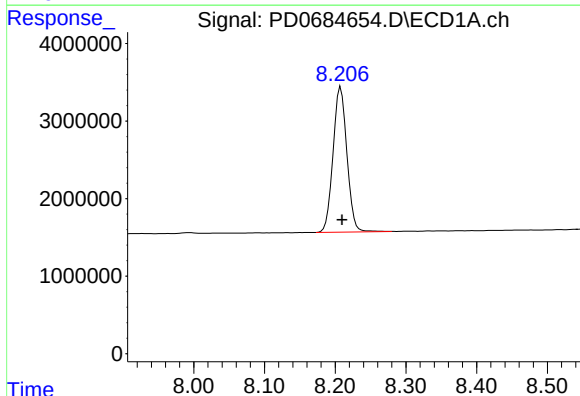

#28 Decachlorobiphenyl

R.T.: 8.208 min
Delta R.T.: -0.002 min
Response: 25454649
Conc: 20.15 ng/ml

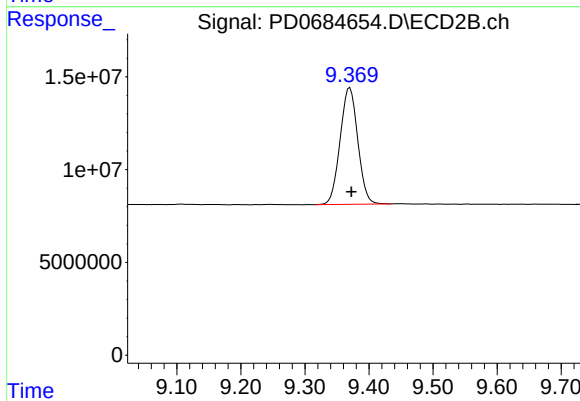

#28 Decachlorobiphenyl

R.T.: 9.370 min
Delta R.T.: -0.002 min
Response: 120261634
Conc: 21.22 ng/ml