

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031722\
 Data File : PD0684666.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2022 19:05
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 03:18:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 03:30:32 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.448	4.175	26009588	212.7E6	21.422	22.251
28)	SA Decachlor...	8.208	9.371	27875299	129.2E6	22.064	22.799
Target Compounds							
5)	MB Aldrin	0.000	5.708	0	129421	N.D.	0.011 #
7)	B delta-BHC	0.000	5.229f	0	1609973	N.D.	0.134 #
8)	B Heptachlo...	0.000	6.076	0	9999272	N.D.	0.958 #
9)	A Endosulfan I	0.000	6.467	0	190891	N.D.	0.020 #
10)	B gamma-Chl...	0.000	6.315	0	1060412	N.D.	0.103 #
14)	MA Endrin	6.013	0.000	426263	0	0.324	N.D. #
21)	B Endrin ke...	0.000	7.973	0	701762	N.D.	0.091 #
23)	Chlordane-1	4.345f	0.000	198715	0	4.683	N.D. #
25)	Chlordane-3	0.000	6.315	0	1060412	N.D.	0.789 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031722\
Data File : PD0684666.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2022 19:05
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 03:18:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 03:30:32 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

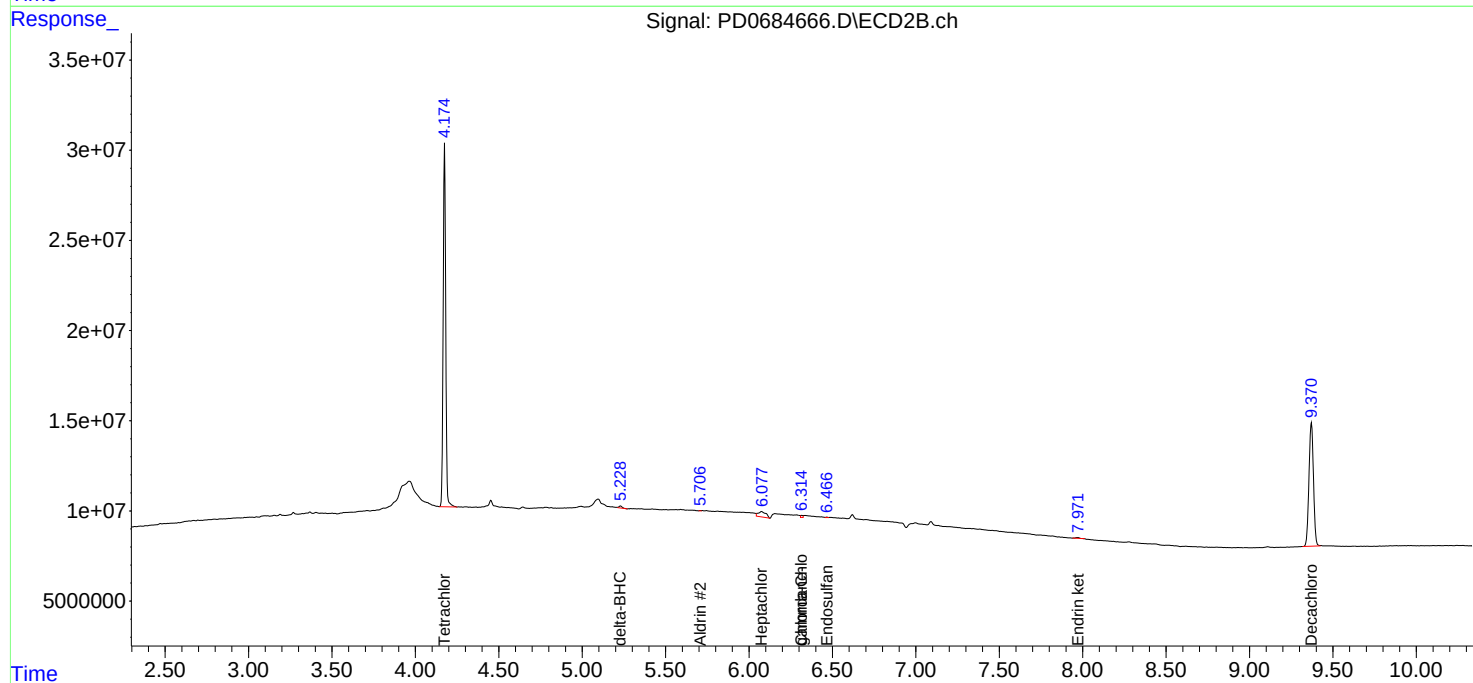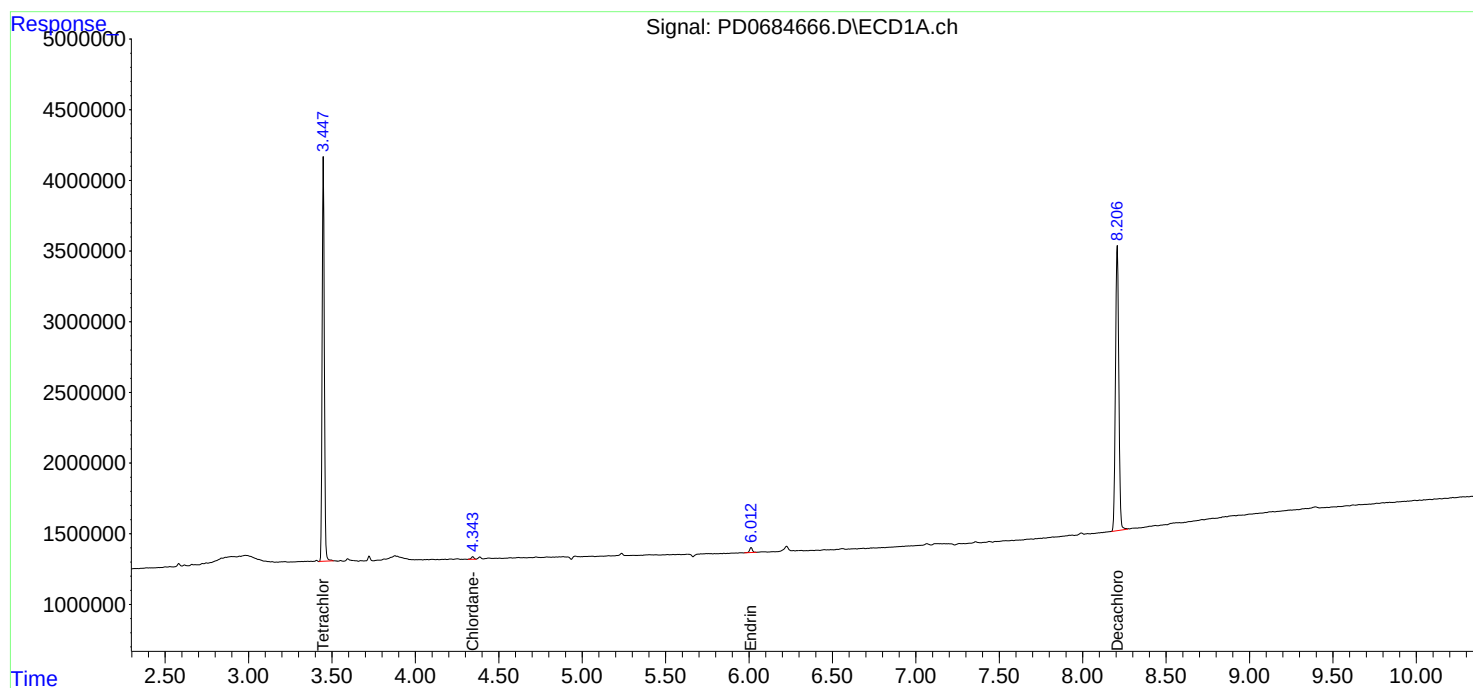


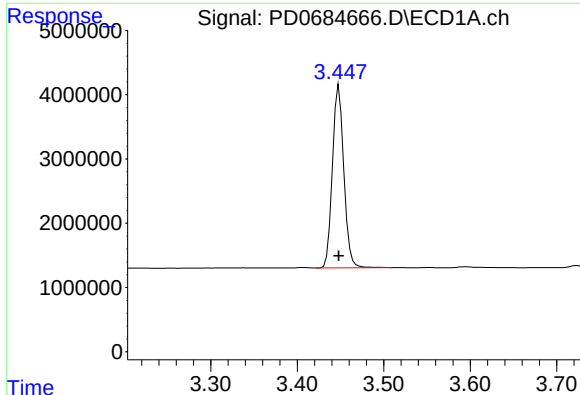

#1 Tetrachloro-m-xylene


R.T.: 3.448 min
Delta R.T.: 0.000 min
Response: 26009588
Conc: 21.42 ng/ml

Instrument :
ECD_D
ClientSampleId :

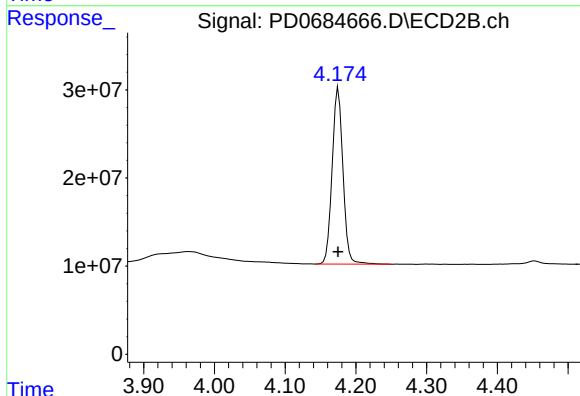


#1 Tetrachloro-m-xylene

R.T.: 4.175 min
Delta R.T.: 0.000 min
Response: 212735698
Conc: 22.25 ng/ml

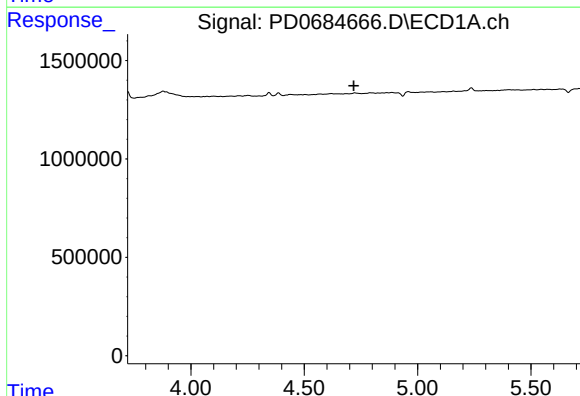


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.718 min
Response: 0
Conc: N.D.

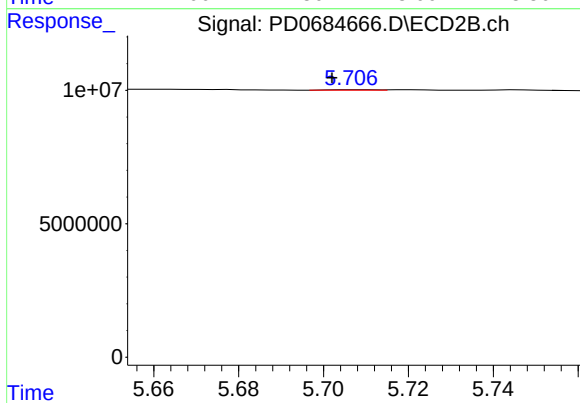

#5 Aldrin


R.T.: 5.708 min
Delta R.T.: 0.006 min
Response: 129421
Conc: 0.01 ng/ml

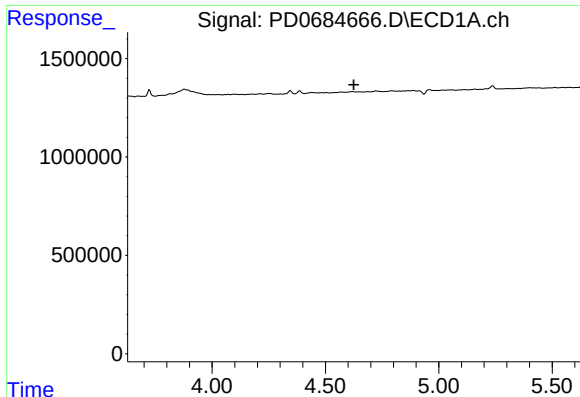

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.626 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

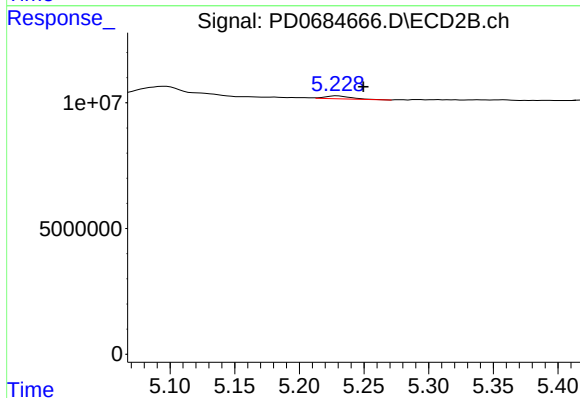


#7 delta-BHC

R.T.: 5.229 min
Delta R.T.: -0.021 min
Response: 1609973
Conc: 0.13 ng/ml

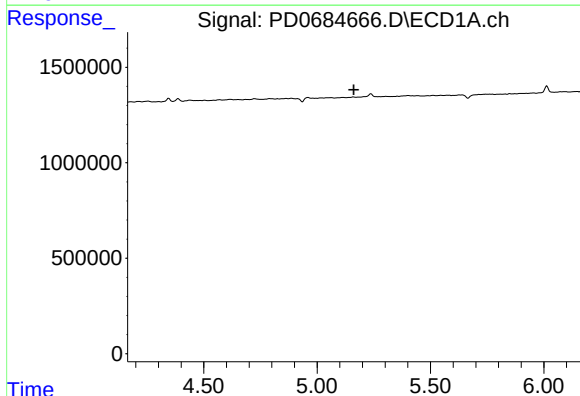


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.162 min
Response: 0
Conc: N.D.

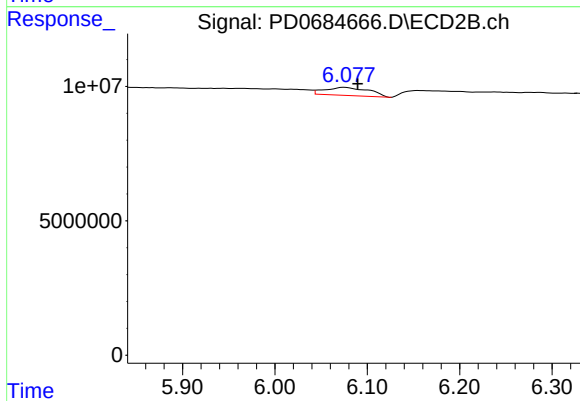

#8 Heptachlor epoxide


R.T.: 6.076 min
Delta R.T.: -0.014 min
Response: 9999272
Conc: 0.96 ng/ml

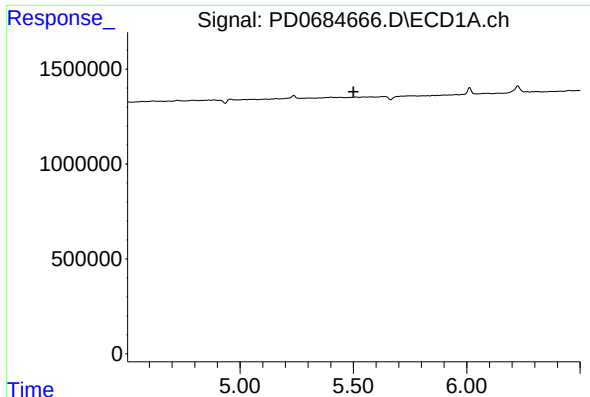

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.501 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

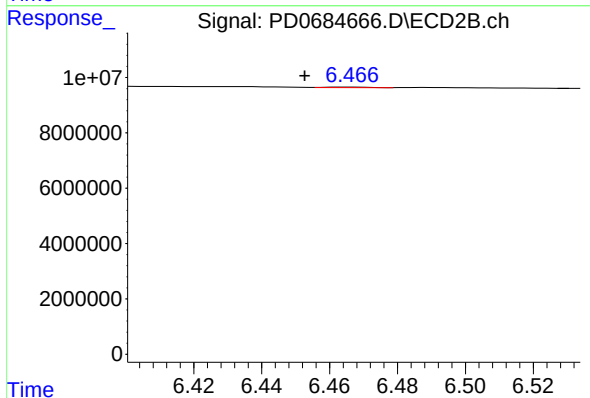


#9 Endosulfan I

R.T.: 6.467 min
Delta R.T.: 0.014 min
Response: 190891
Conc: 0.02 ng/ml

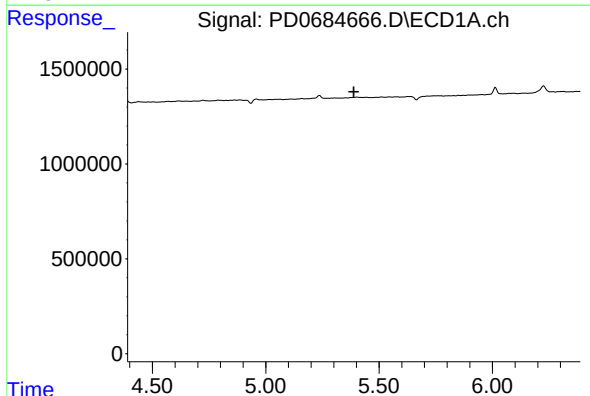


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.388 min
Response: 0
Conc: N.D.

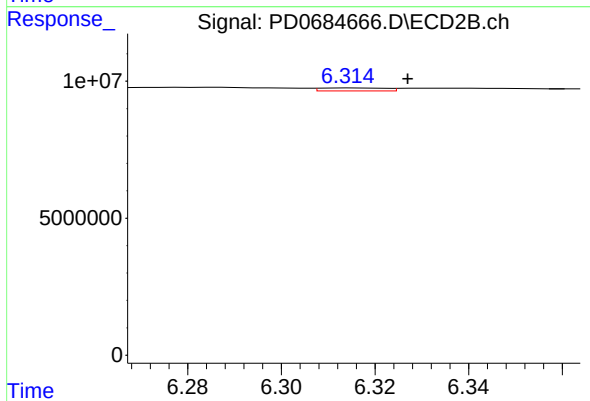

#10 gamma-Chlordane


R.T.: 6.315 min
Delta R.T.: -0.012 min
Response: 1060412
Conc: 0.10 ng/ml

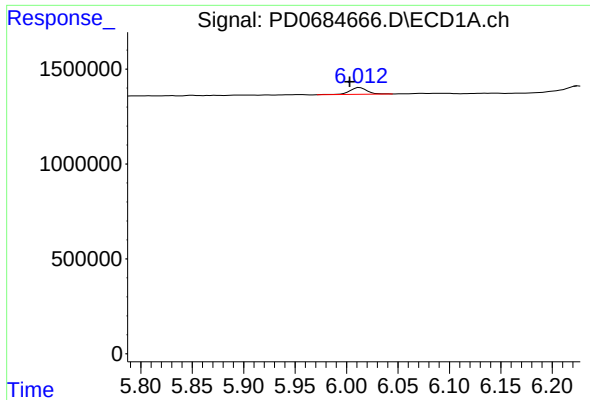

#14 Endrin


R.T.: 6.013 min
Delta R.T.: 0.010 min
Response: 426263
Conc: 0.32 ng/ml

Instrument :
ECD_D
ClientSampleId :

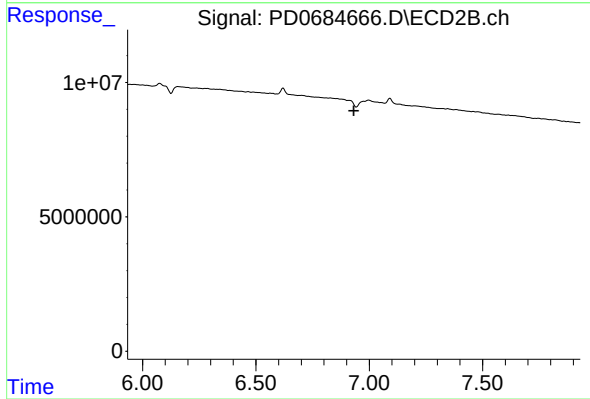


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.932 min
Response: 0
Conc: N.D.

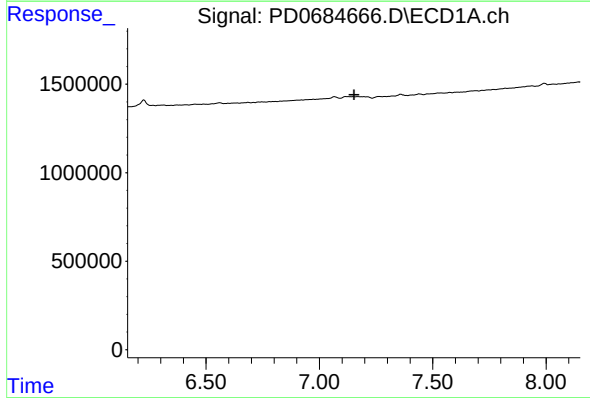


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.153 min
Response: 0
Conc: N.D.

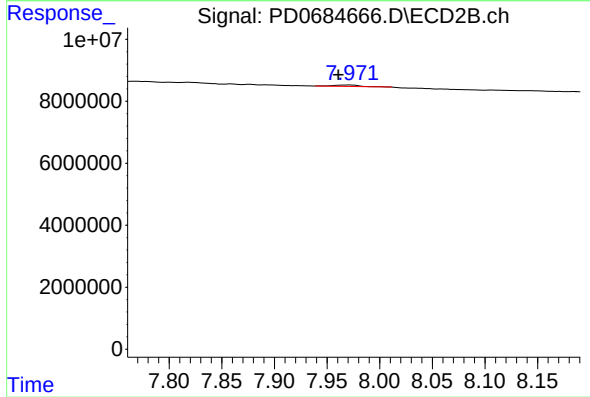

#21 Endrin ketone


R.T.: 7.973 min
Delta R.T.: 0.012 min
Response: 701762
Conc: 0.09 ng/ml

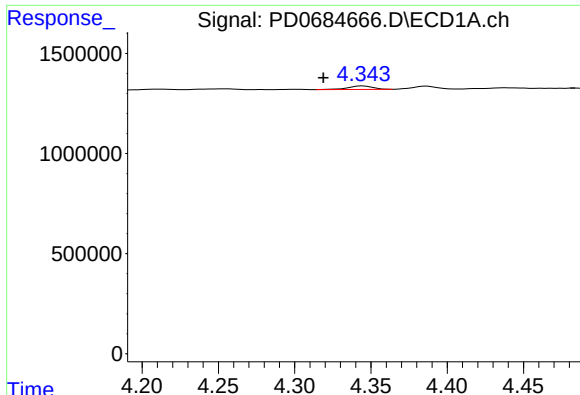

#23 Chlordane-1


R.T.: 4.345 min
Delta R.T.: 0.026 min
Response: 198715
Conc: 4.68 ng/ml

Instrument :
ECD_D
ClientSampleId :

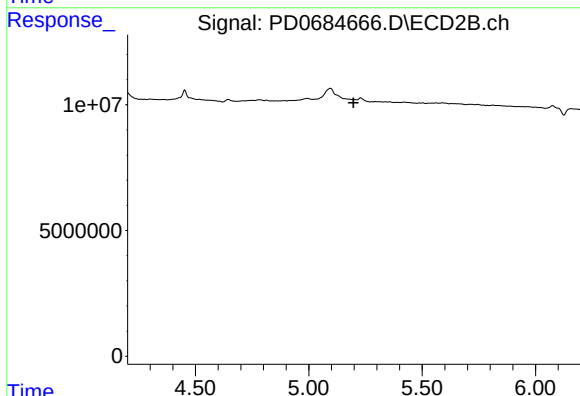


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.198 min
Response: 0
Conc: N.D.

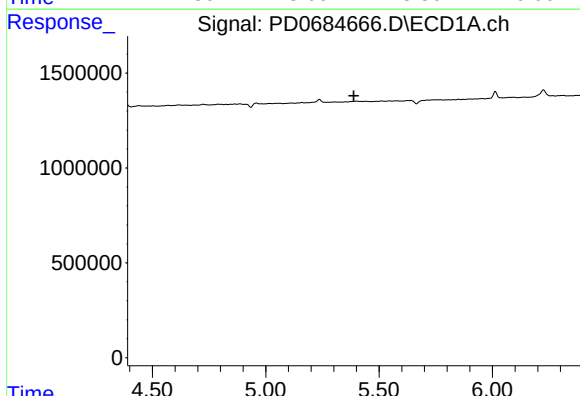


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.389 min
Response: 0
Conc: N.D.

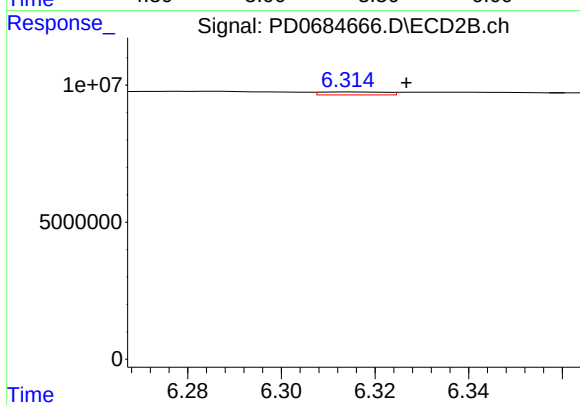

#25 Chlordane-3


R.T.: 6.315 min
Delta R.T.: -0.012 min
Response: 1060412
Conc: 0.79 ng/ml

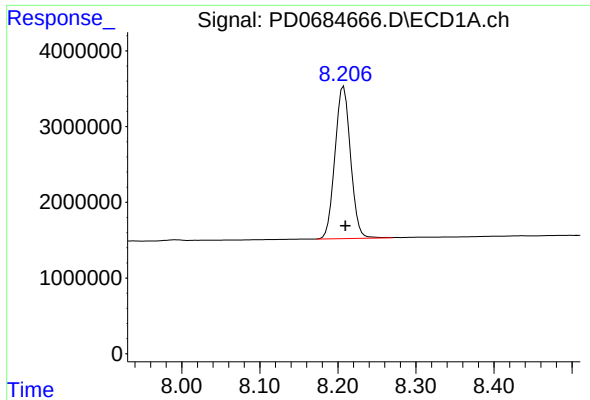

#28 Decachlorobiphenyl

R.T.: 8.208 min
Delta R.T.: -0.002 min
Response: 27875299
Conc: 22.06 ng/ml

Instrument :
ECD_D
ClientSampleId :

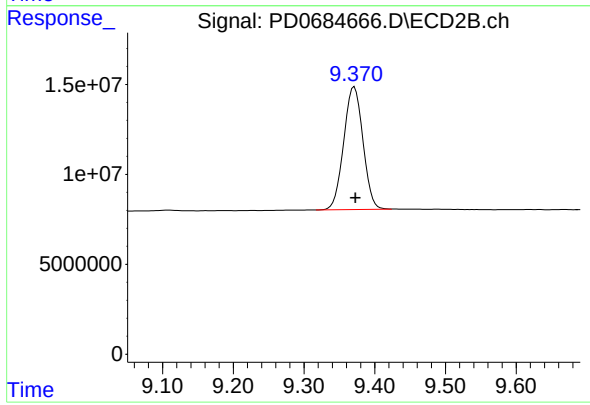

#28 Decachlorobiphenyl

R.T.: 9.371 min
Delta R.T.: -0.001 min
Response: 129196753
Conc: 22.80 ng/ml