

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031722\
 Data File : PD068670.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2022 21:11
 Operator : AR\AJ
 Sample : N1954-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CL-02-031522

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/17/2022
 Supervised By : Ankita Jodhani 03/17/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 03:20:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 03:30:32 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.446	4.175	14882035	122.0E6	12.257m	12.763
28) SA Decachlor...	8.206	9.370	17238906	89271311	13.645	15.754

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031722\
Data File : PD068670.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2022 21:11
Operator : AR\AJ
Sample : N1954-01
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
CL-02-031522


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/17/2022
Supervised By :Ankita Jodhani 03/17/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 03:20:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 03:30:32 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

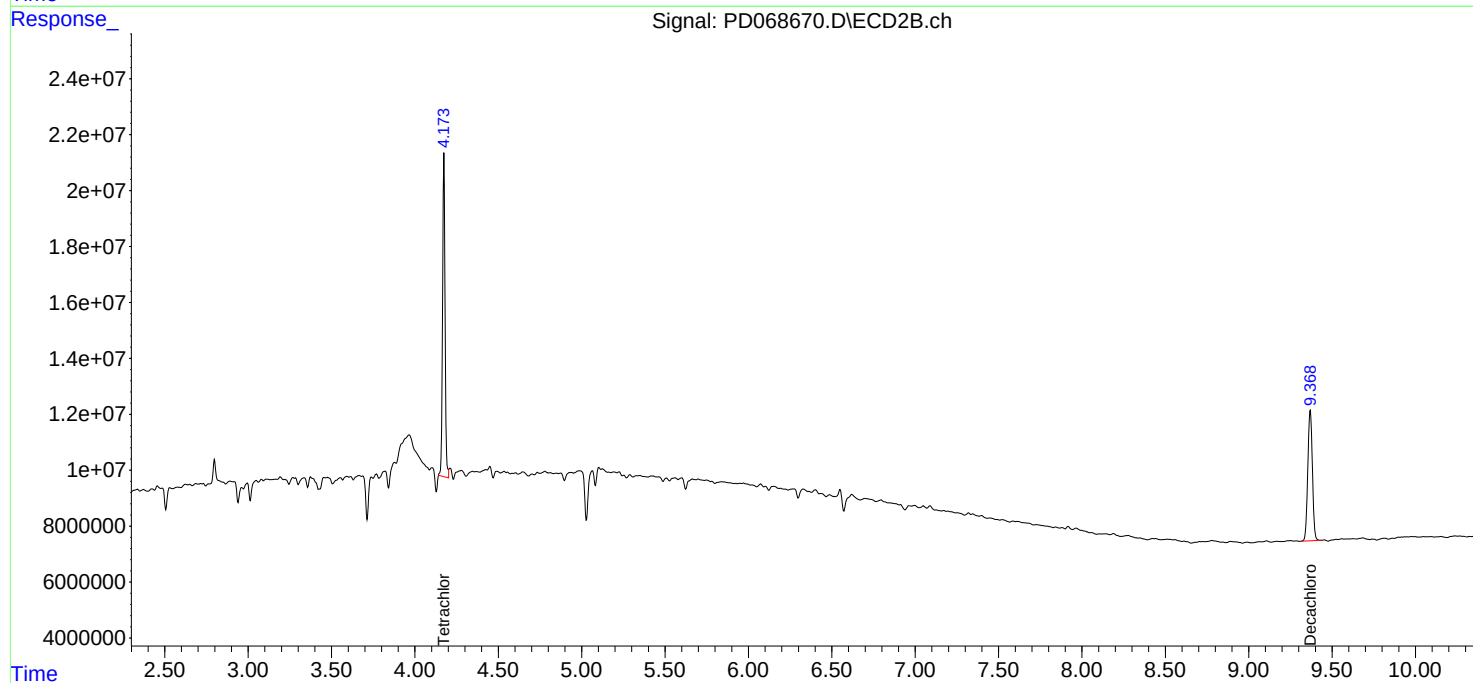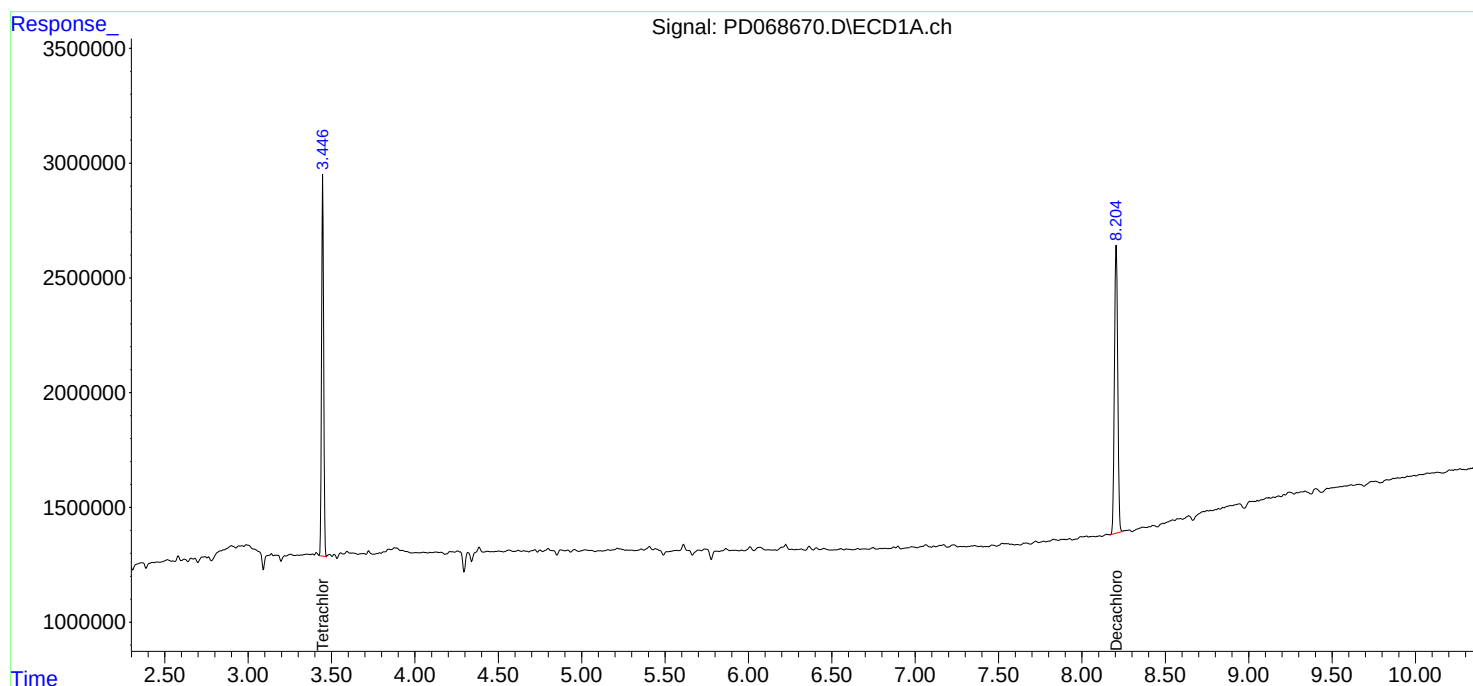

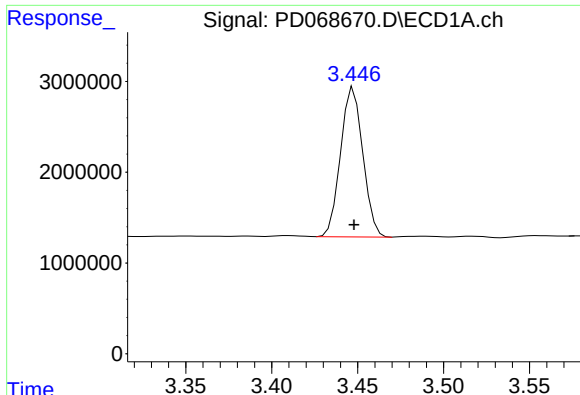


#1 Tetrachloro-m-xylene

R.T.: 3.446 min
Delta R.T.: -0.002 min
Response: 14882035
Conc: 12.26 ng/ml

Instrument :
ECD_D
ClientSampleId :
CL-02-031522


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/17/2022
Supervised By :Ankita Jodhani 03/17/2022

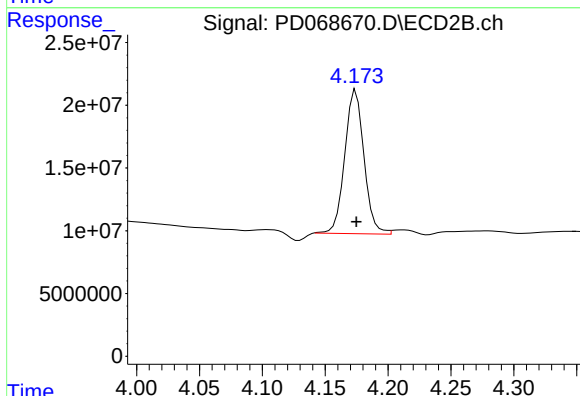


#1 Tetrachloro-m-xylene

R.T.: 4.175 min
Delta R.T.: 0.000 min
Response: 122024977
Conc: 12.76 ng/ml

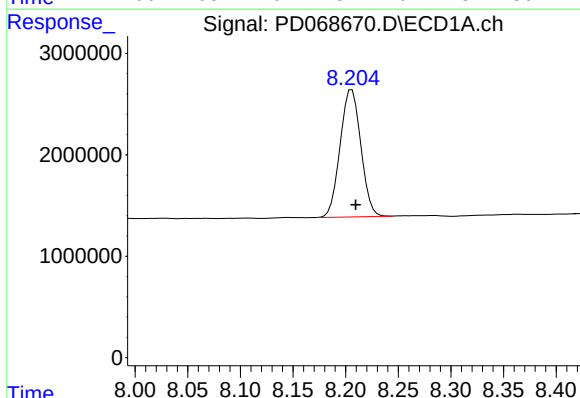

#28 Decachlorobiphenyl

R.T.: 8.206 min
Delta R.T.: -0.004 min
Response: 17238906
Conc: 13.65 ng/ml

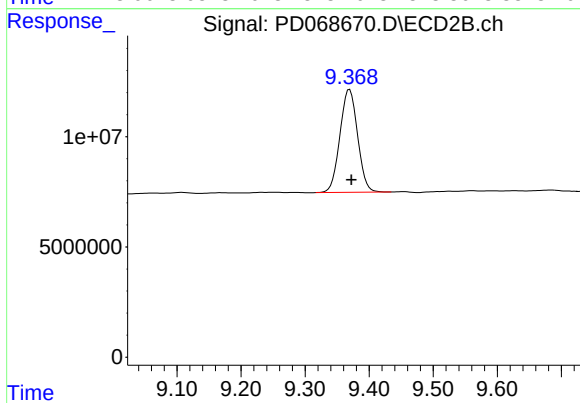

#28 Decachlorobiphenyl

R.T.: 9.370 min
Delta R.T.: -0.003 min
Response: 89271311
Conc: 15.75 ng/ml