

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD031722\  
 Data File : PD068675.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 16 Mar 2022 22:21  
 Operator : AR\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_D  
 ClientSampleId :  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 17 03:21:38 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD031222.M  
 Quant Title : GC Extractables  
 QLast Update : Mon Mar 14 03:30:32 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

|                             | Compound        | RT#1  | RT#2  | Resp#1   | Resp#2  | ng/ml  | ng/ml  |
|-----------------------------|-----------------|-------|-------|----------|---------|--------|--------|
| -----                       |                 |       |       |          |         |        |        |
| System Monitoring Compounds |                 |       |       |          |         |        |        |
| 1)                          | SA Tetrachlo... | 3.449 | 4.175 | 26821147 | 212.8E6 | 22.090 | 22.255 |
| 28)                         | SA Decachlor... | 8.207 | 9.370 | 23868021 | 117.8E6 | 18.892 | 20.792 |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD031722\  
Data File : PD068675.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 16 Mar 2022 22:21  
Operator : AR\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
I.BLK

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Mar 17 03:21:38 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD031222.M  
Quant Title : GC Extractables  
QLast Update : Mon Mar 14 03:30:32 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

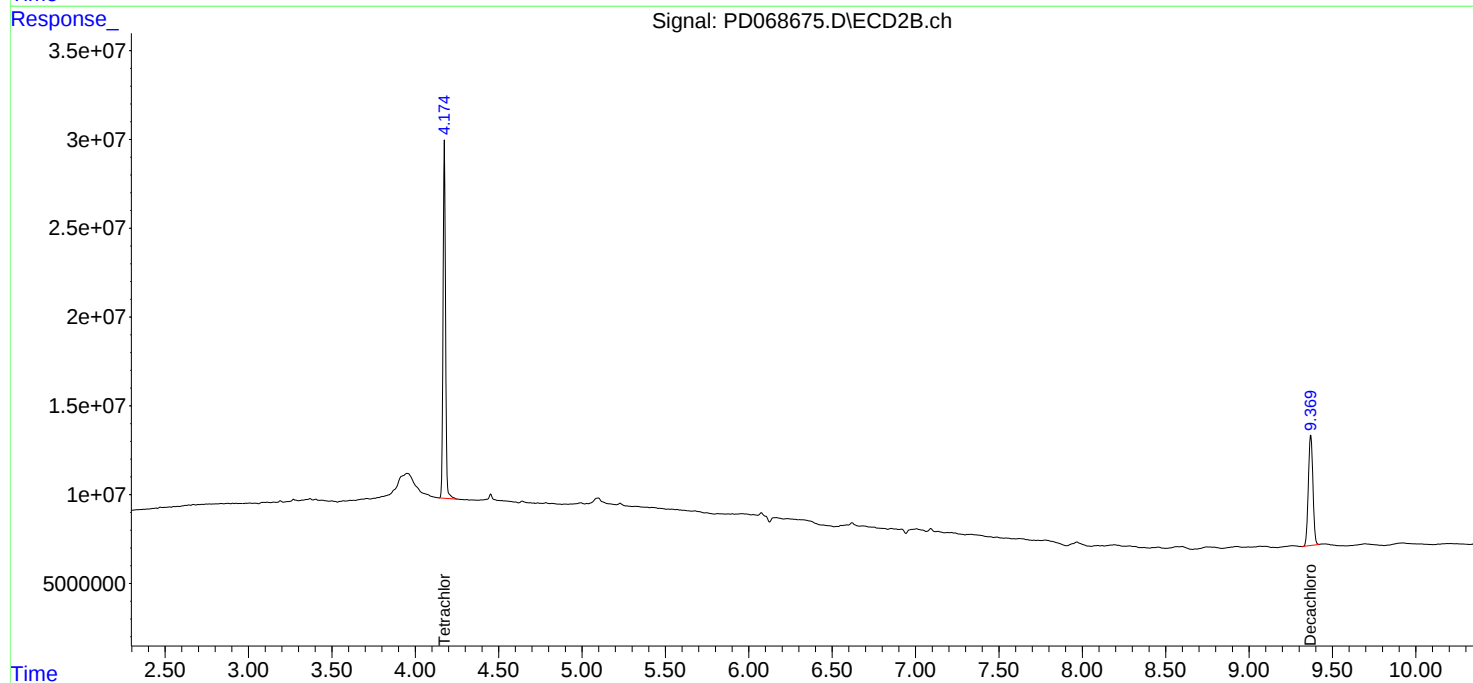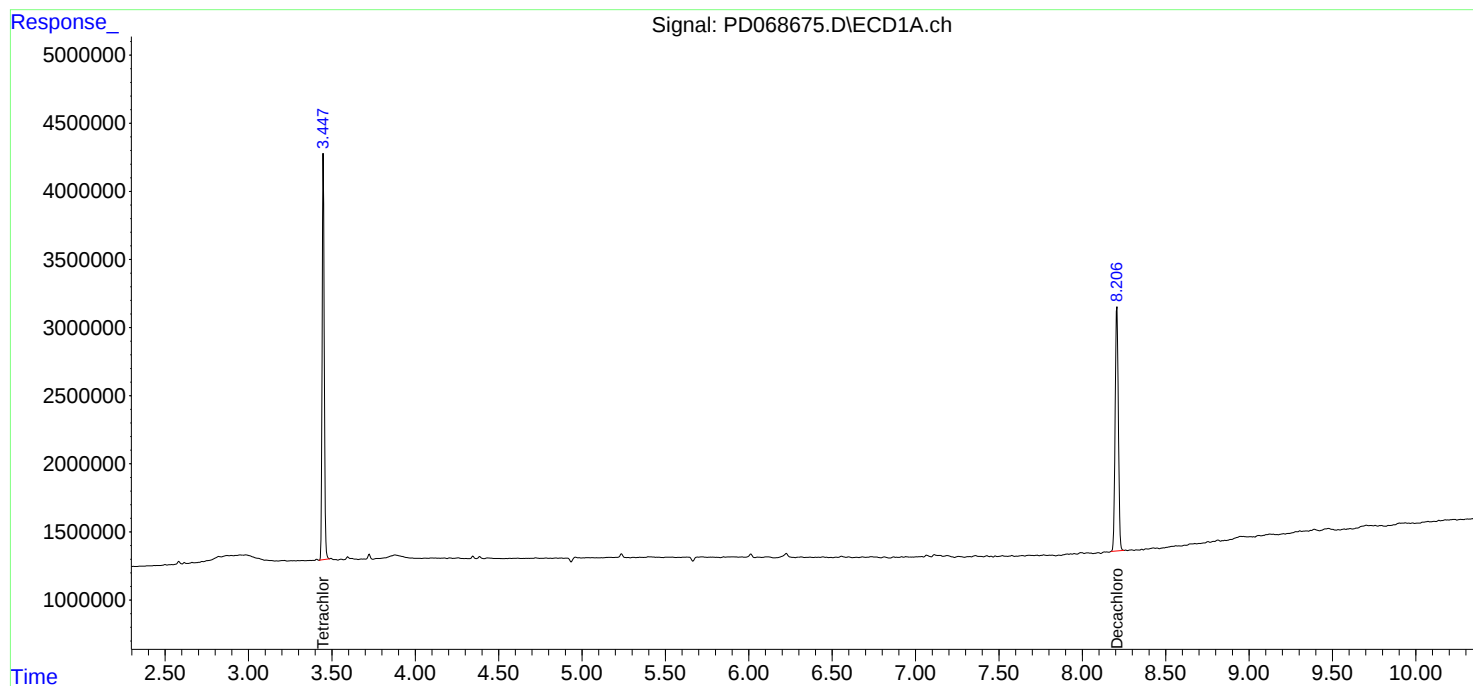


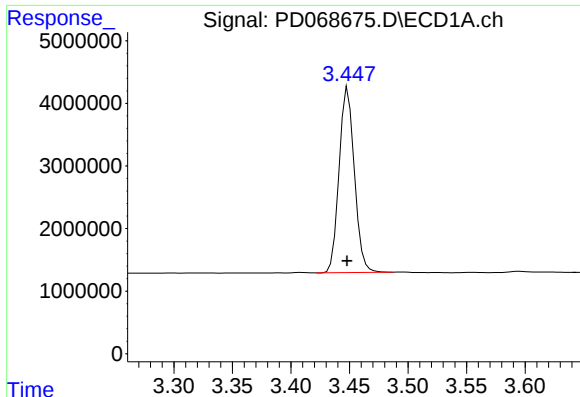

#1 Tetrachloro-m-xylene


R.T.: 3.449 min  
Delta R.T.: 0.000 min  
Response: 26821147  
Conc: 22.09 ng/ml

Instrument :  
ECD\_D  
ClientSampleId :  
I.BLK

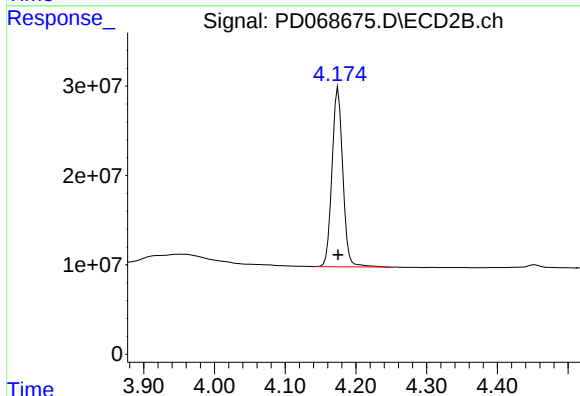


#1 Tetrachloro-m-xylene

R.T.: 4.175 min  
Delta R.T.: 0.000 min  
Response: 212773344  
Conc: 22.25 ng/ml

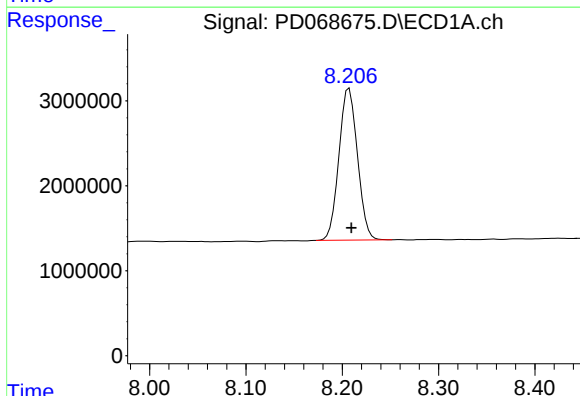

#28 Decachlorobiphenyl

R.T.: 8.207 min  
Delta R.T.: -0.002 min  
Response: 23868021  
Conc: 18.89 ng/ml

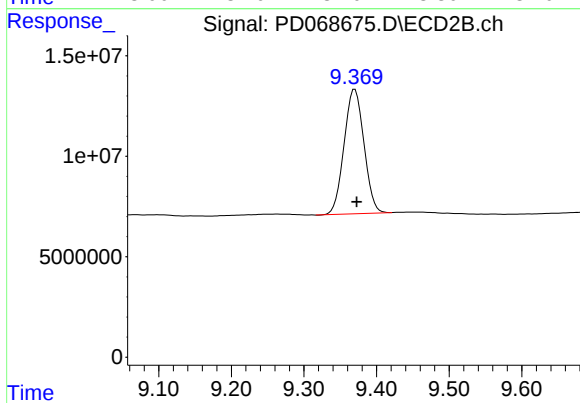

#28 Decachlorobiphenyl

R.T.: 9.370 min  
Delta R.T.: -0.002 min  
Response: 117823742  
Conc: 20.79 ng/ml