

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031819\
 Data File : PD051867.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Mar 2019 20:50
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 02:40:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 01 23:43:17 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.223	4.044	29342870	613.1E6	22.130	21.380
28)	SA Decachlor...	7.821	9.155	23908609	373.2E6	21.034	20.431
Target Compounds							
3)	MA gamma-BHC...	3.918	0.000	1914079	0	0.916	N.D. #
4)	MA Heptachlor	0.000	5.245	0	2939202	N.D.	0.077 #
7)	B delta-BHC	0.000	5.086f	0	21988789	N.D.	0.640 #
8)	B Heptachlo...	4.873f	5.922	775970	12146074	0.395	0.379
9)	A Endosulfan I	0.000	6.284	0	21478895	N.D.	0.725 #
10)	B gamma-Chl...	0.000	6.167	0	33552410	N.D.	1.049 #
15)	B Endosulfa...	0.000	6.982	0	921783	N.D.	0.036 #
17)	MA 4,4'-DDT	0.000	7.196	0	647671	N.D.	0.032 #
25)	Chlordane-3	0.000	6.167	0	33552410	N.D.	7.535 #
27)	Chlordane-5	0.000	7.032f	0	406186	N.D.	0.401 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031819\
Data File : PD051867.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Mar 2019 20:50
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 02:40:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 01 23:43:17 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

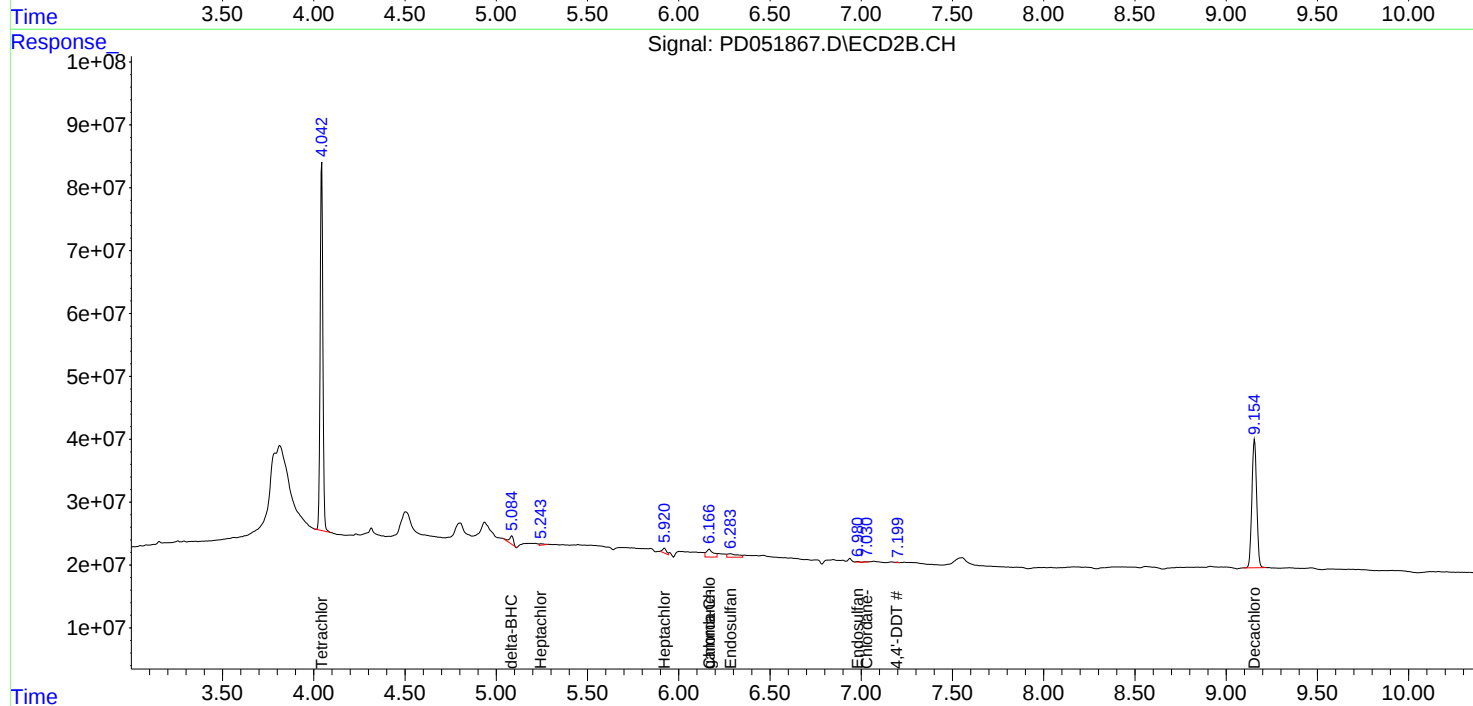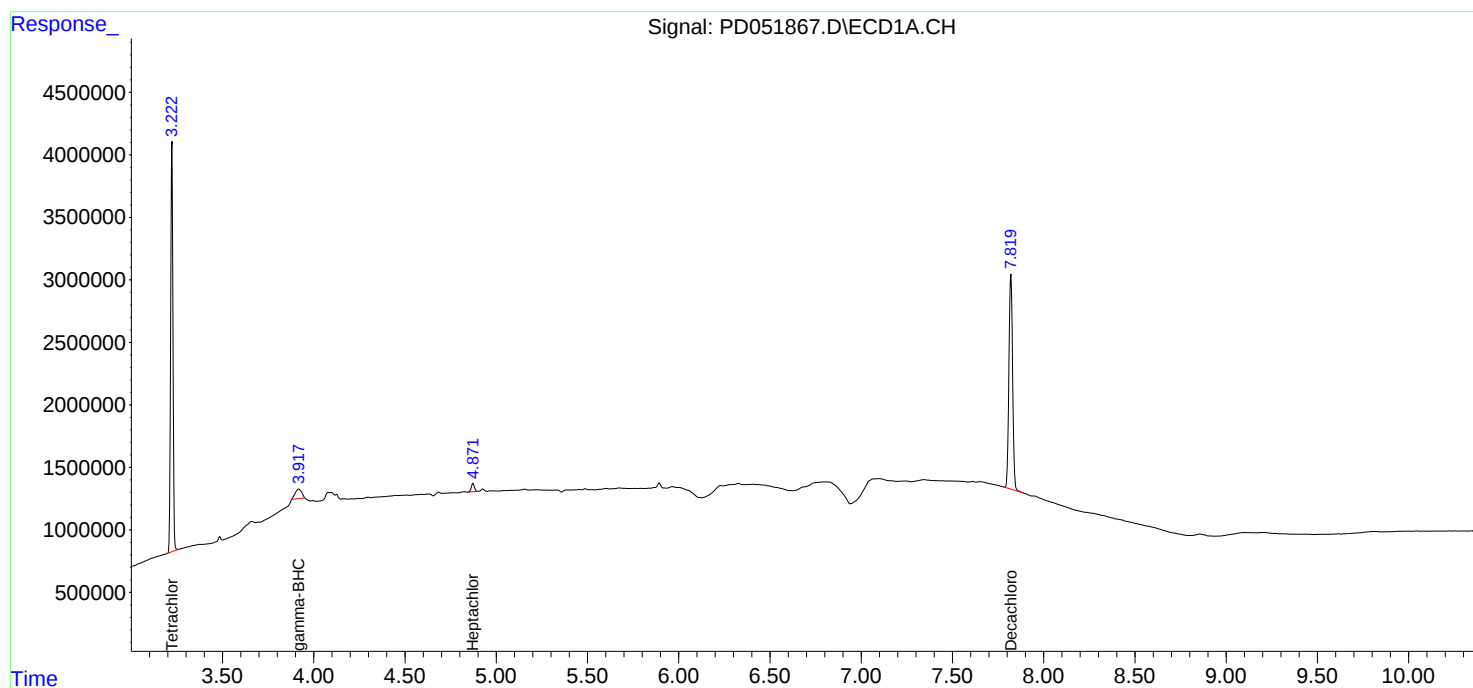


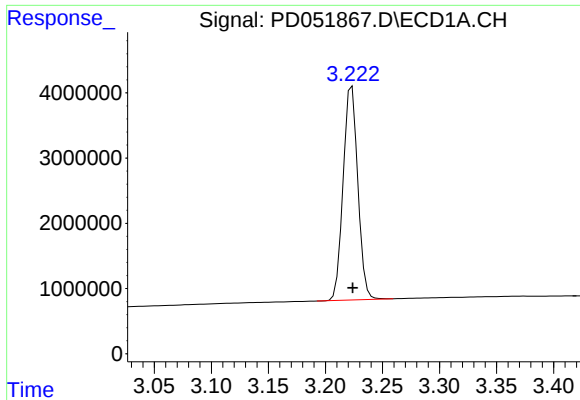

#1 Tetrachloro-m-xylene


R.T.: 3.223 min
Delta R.T.: 0.000 min
Response: 29342870
Conc: 22.13 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

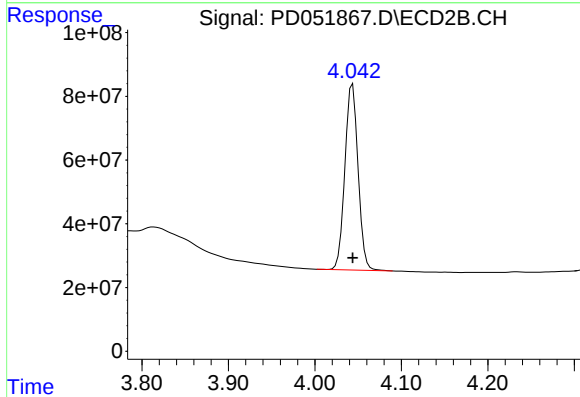


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 613116498
Conc: 21.38 ng/ml

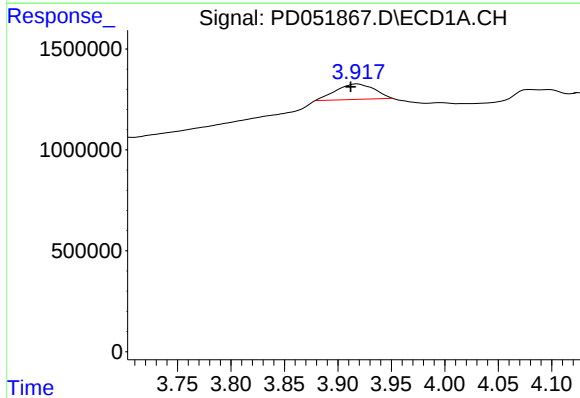


#3 gamma-BHC (Lindane)

R.T.: 3.918 min
Delta R.T.: 0.006 min
Response: 1914079
Conc: 0.92 ng/ml

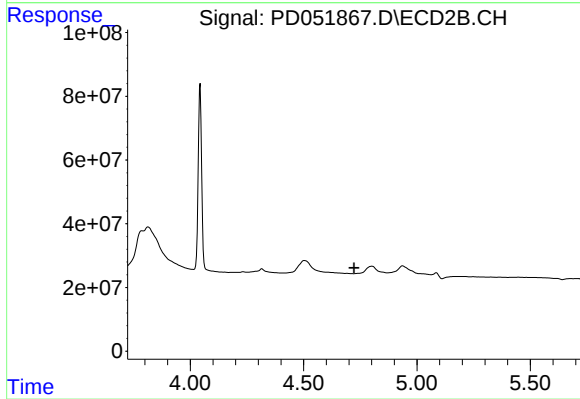

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.723 min
Response: 0
Conc: N.D.

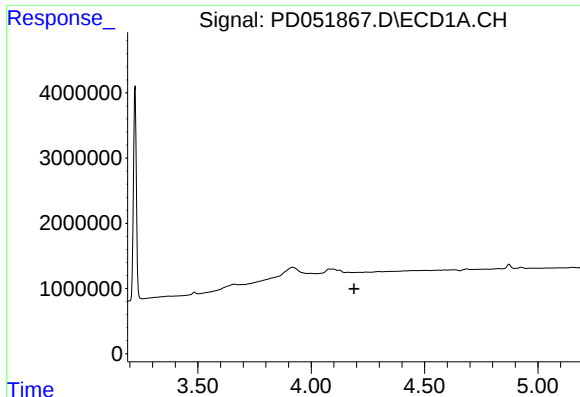

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.190 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

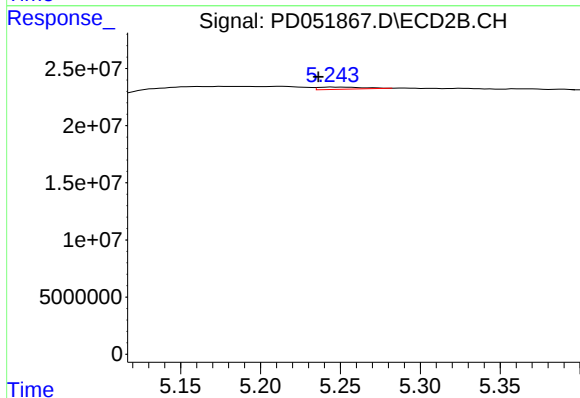


#4 Heptachlor

R.T.: 5.245 min
Delta R.T.: 0.009 min
Response: 2939202
Conc: 0.08 ng/ml

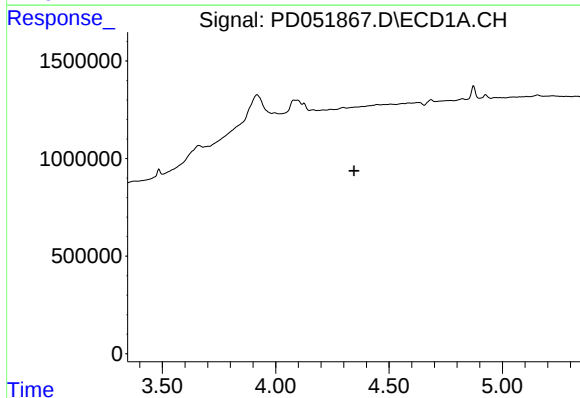


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.346 min
Response: 0
Conc: N.D.

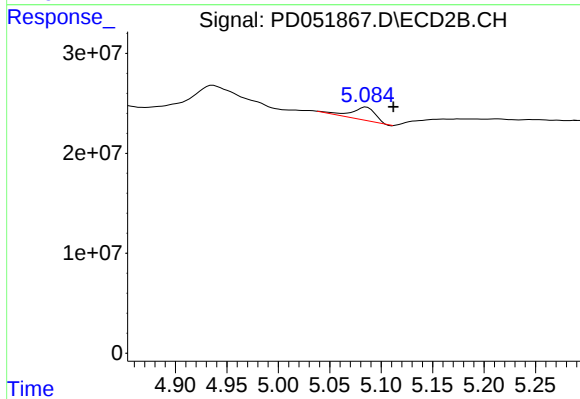

#7 delta-BHC


R.T.: 5.086 min
Delta R.T.: -0.026 min
Response: 21988789
Conc: 0.64 ng/ml

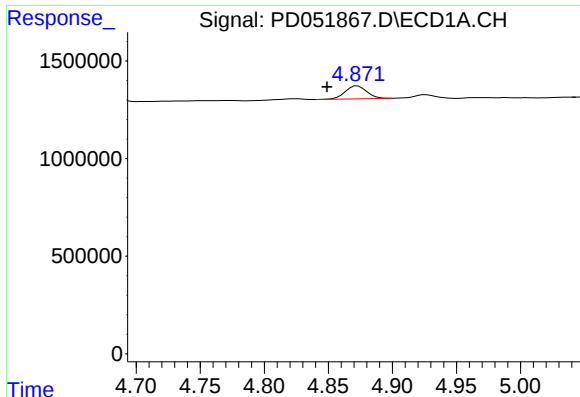

#8 Heptachlor epoxide


R.T.: 4.873 min
Delta R.T.: 0.024 min
Response: 775970
Conc: 0.39 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

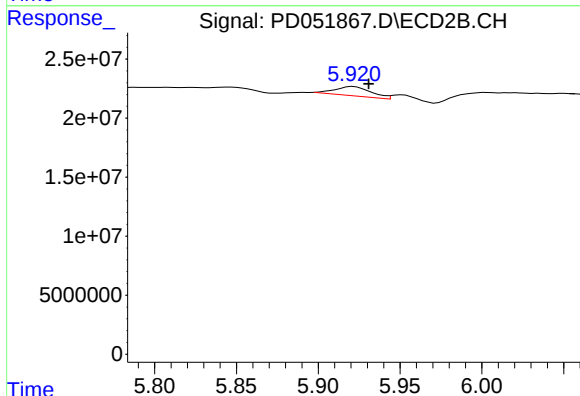


#8 Heptachlor epoxide

R.T.: 5.922 min
Delta R.T.: -0.009 min
Response: 12146074
Conc: 0.38 ng/ml

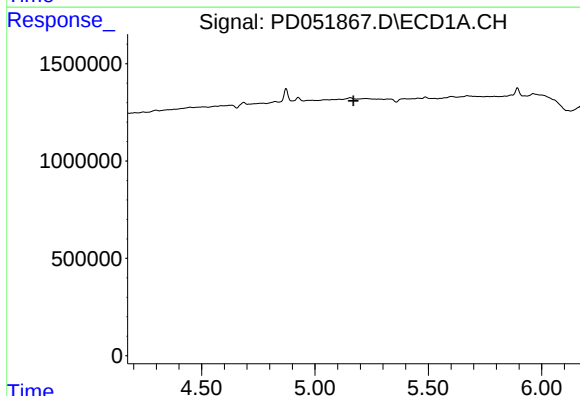


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.170 min
Response: 0
Conc: N.D.

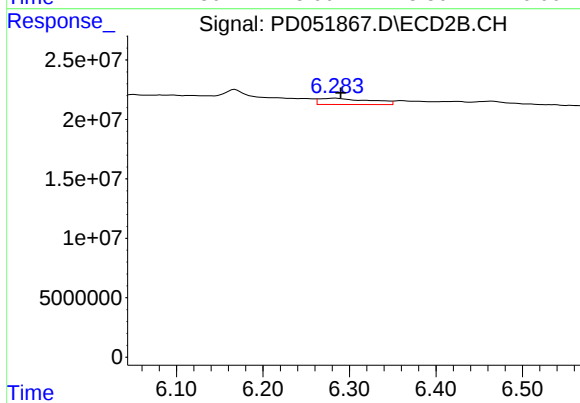

#9 Endosulfan I


R.T.: 6.284 min
Delta R.T.: -0.006 min
Response: 21478895
Conc: 0.72 ng/ml

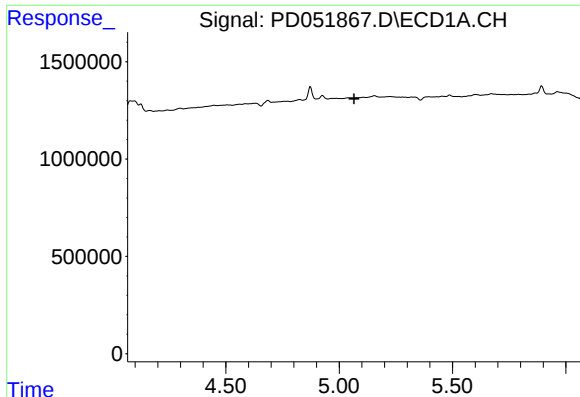

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.066 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

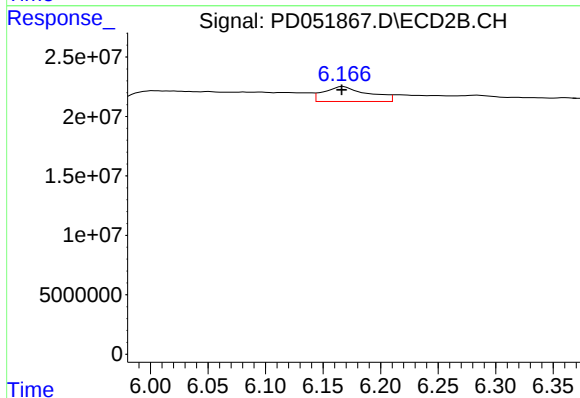


#10 gamma-Chlordane

R.T.: 6.167 min
Delta R.T.: 0.001 min
Response: 33552410
Conc: 1.05 ng/ml

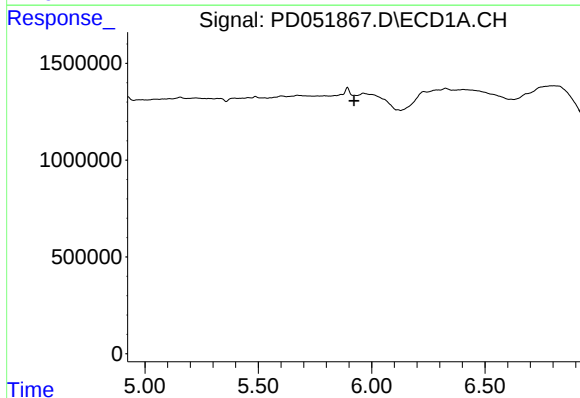


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 5.923 min
Response: 0
Conc: N.D.

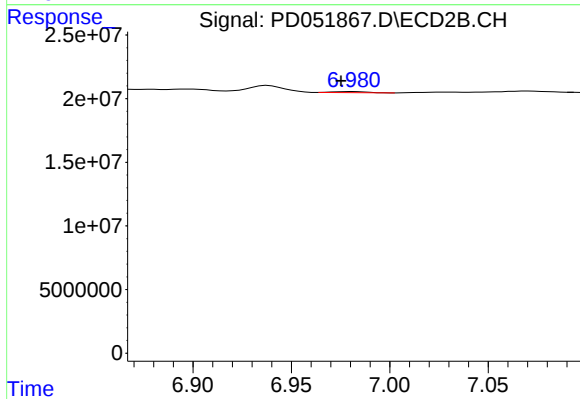

#15 Endosulfan II


R.T.: 6.982 min
Delta R.T.: 0.006 min
Response: 921783
Conc: 0.04 ng/ml

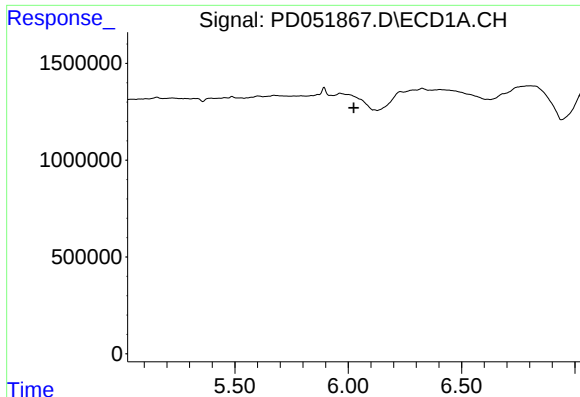

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.024 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

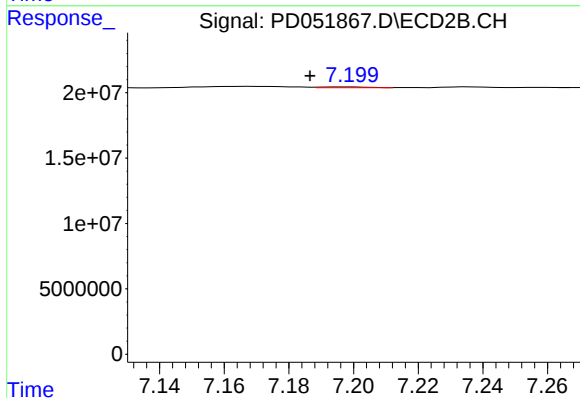


#17 4,4'-DDT

R.T.: 7.196 min
Delta R.T.: 0.009 min
Response: 647671
Conc: 0.03 ng/ml

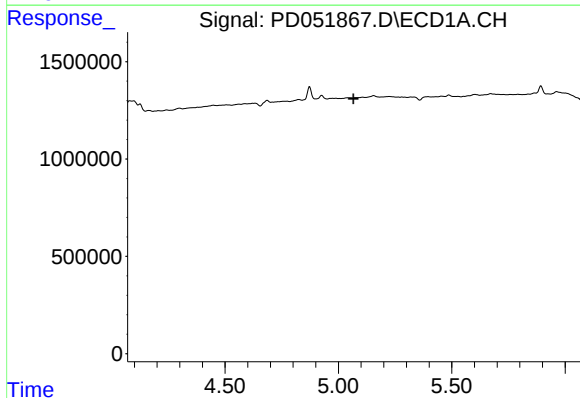


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.067 min
Response: 0
Conc: N.D.

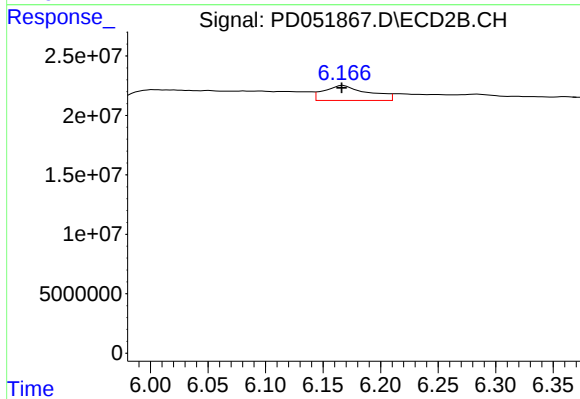

#25 Chlordane-3


R.T.: 6.167 min
Delta R.T.: 0.001 min
Response: 33552410
Conc: 7.53 ng/ml

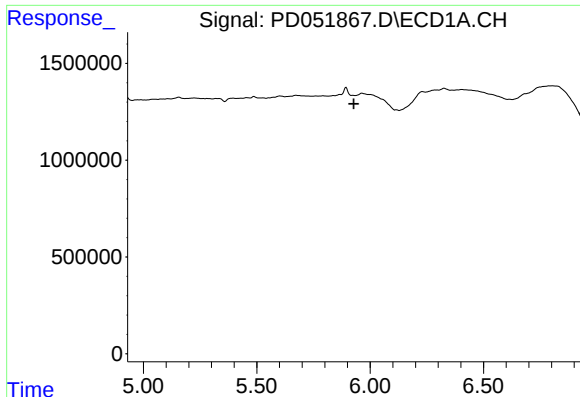

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 5.927 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

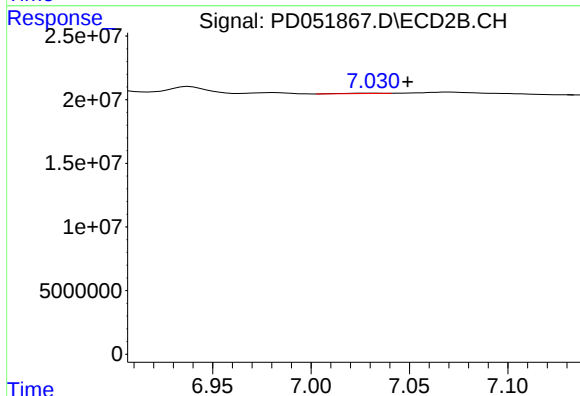


#27 Chlordane-5

R.T.: 7.032 min
Delta R.T.: -0.018 min
Response: 406186
Conc: 0.40 ng/ml

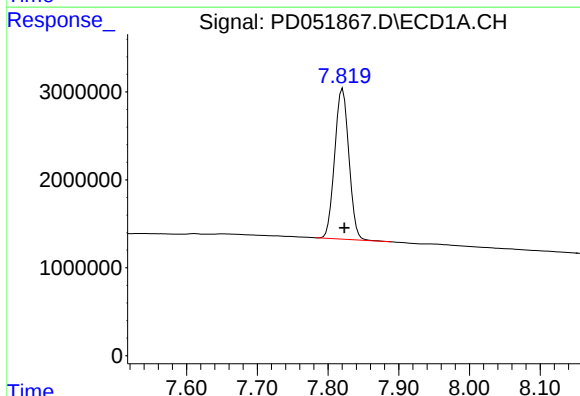

#28 Decachlorobiphenyl

R.T.: 7.821 min
Delta R.T.: -0.003 min
Response: 23908609
Conc: 21.03 ng/ml

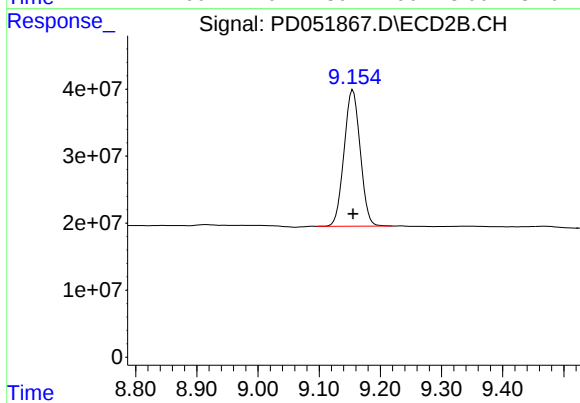

#28 Decachlorobiphenyl

R.T.: 9.155 min
Delta R.T.: 0.000 min
Response: 373205260
Conc: 20.43 ng/ml