

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031819\
 Data File : PD051865.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Mar 2019 20:22
 Operator : AJ\SJ
 Sample : K1948-12
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PST-025-SW079-031319

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 02:40:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 01 23:43:17 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.223	4.044	28305193	582.2E6	21.347	20.301
28)	SA Decachlor...	7.821	9.155	19209892	306.0E6	16.900	16.751

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031819\
Data File : PD051865.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Mar 2019 20:22
Operator : AJ\SJ
Sample : K1948-12
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PST-025-SW079-031319

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 02:40:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 01 23:43:17 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

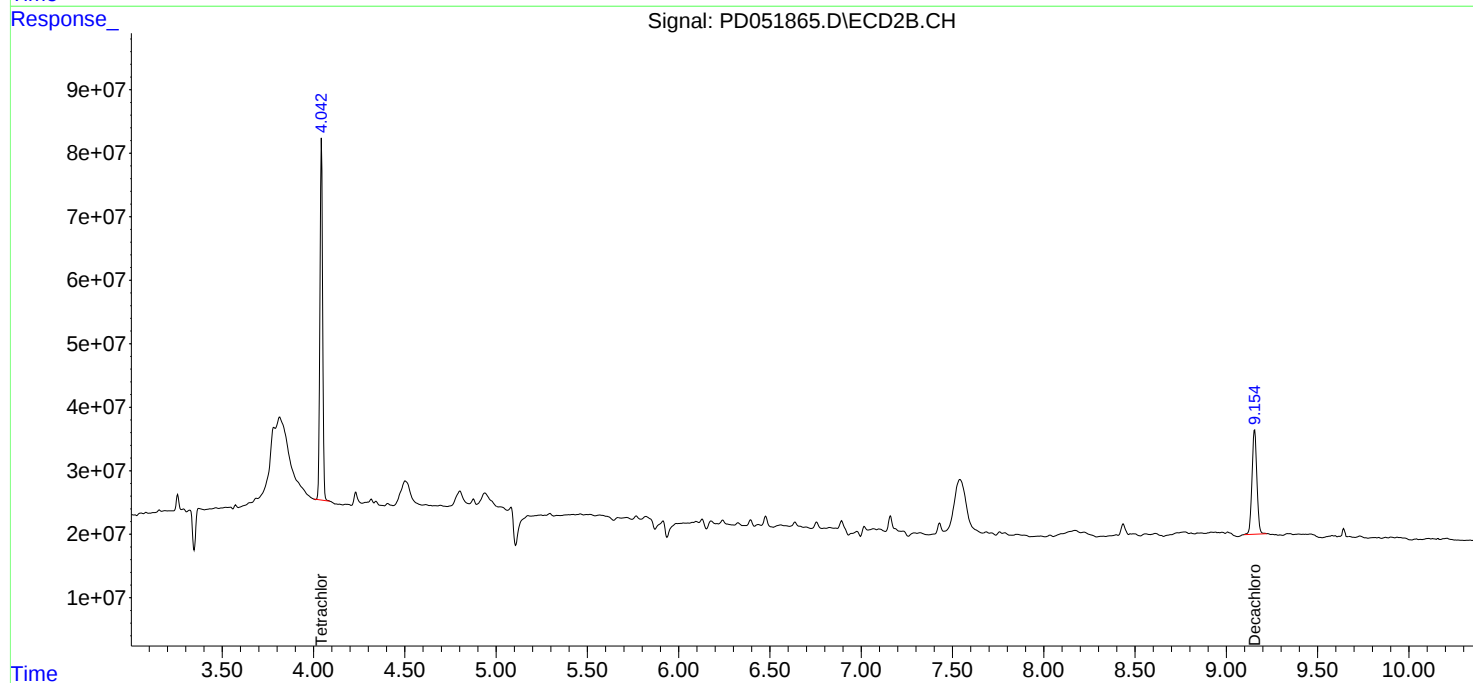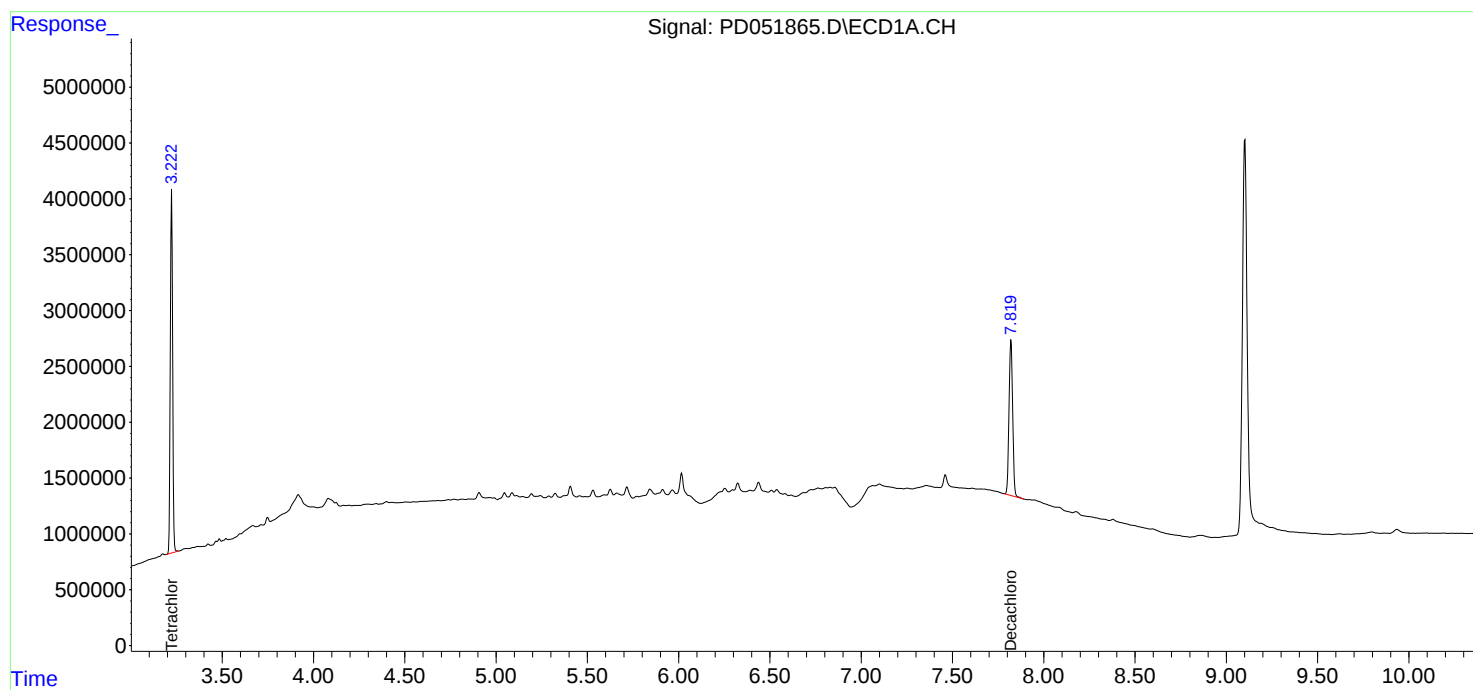


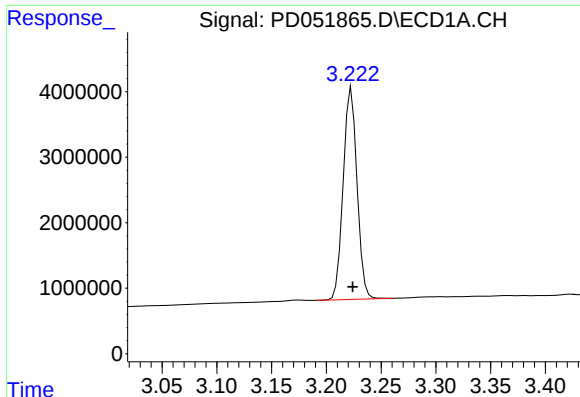

#1 Tetrachloro-m-xylene


R.T.: 3.223 min
Delta R.T.: -0.001 min
Response: 28305193
Conc: 21.35 ng/ml

Instrument :
ECD_D
ClientSampleId :
PST-025-SW079-031319

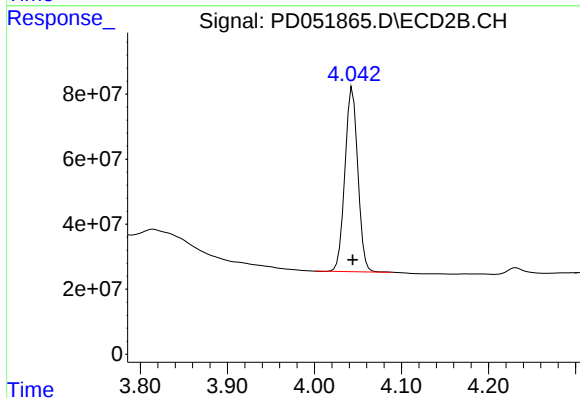


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 582174441
Conc: 20.30 ng/ml

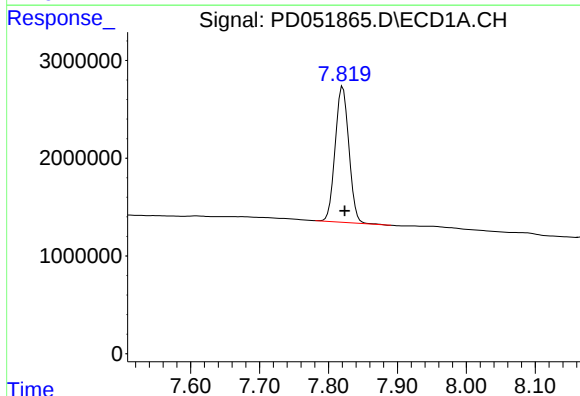

#28 Decachlorobiphenyl

R.T.: 7.821 min
Delta R.T.: -0.003 min
Response: 19209892
Conc: 16.90 ng/ml

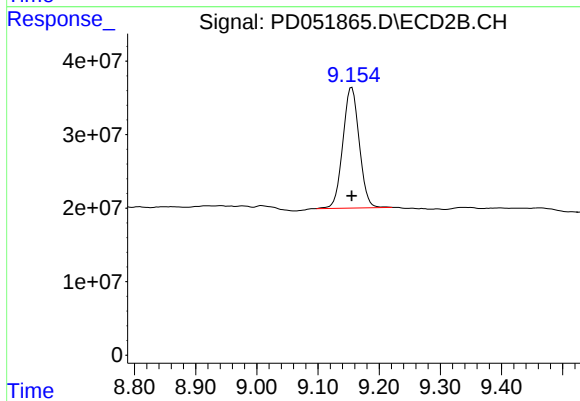

#28 Decachlorobiphenyl

R.T.: 9.155 min
Delta R.T.: 0.000 min
Response: 305990095
Conc: 16.75 ng/ml