

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031821\
 Data File : PD061727.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2021 15:50
 Operator : AR\AJ
 Sample : M1713-03
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TP-7A

Manual Integrations
 APPROVED

Ankita
 3/19/2021 10:24:05 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 06:34:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031721.M
 Quant Title : GC Extractables
 QLast Update : Thu Mar 18 07:52:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	3.982	13277585	128.6E6	15.534	14.993
28)	SA Decachlor...	8.259	9.042	17233100	127.7E6	14.081	14.689
Target Compounds							
12)	B 4,4'-DDE	5.666	6.309	1857181	6660267	1.636m	0.600 #
15)	B Endosulfa...	6.330	6.903	646485	8885385	0.626	0.958 #
17)	MA 4,4'-DDT	6.419	7.120	841551	19453593	0.837m	1.973 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031821\
Data File : PD061727.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2021 15:50
Operator : AR\AJ
Sample : M1713-03
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
TP-7A


Manual Integrations
APPROVED

Ankita
3/19/2021 10:24:05 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 06:34:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031721.M
Quant Title : GC Extractables
QLast Update : Thu Mar 18 07:52:17 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

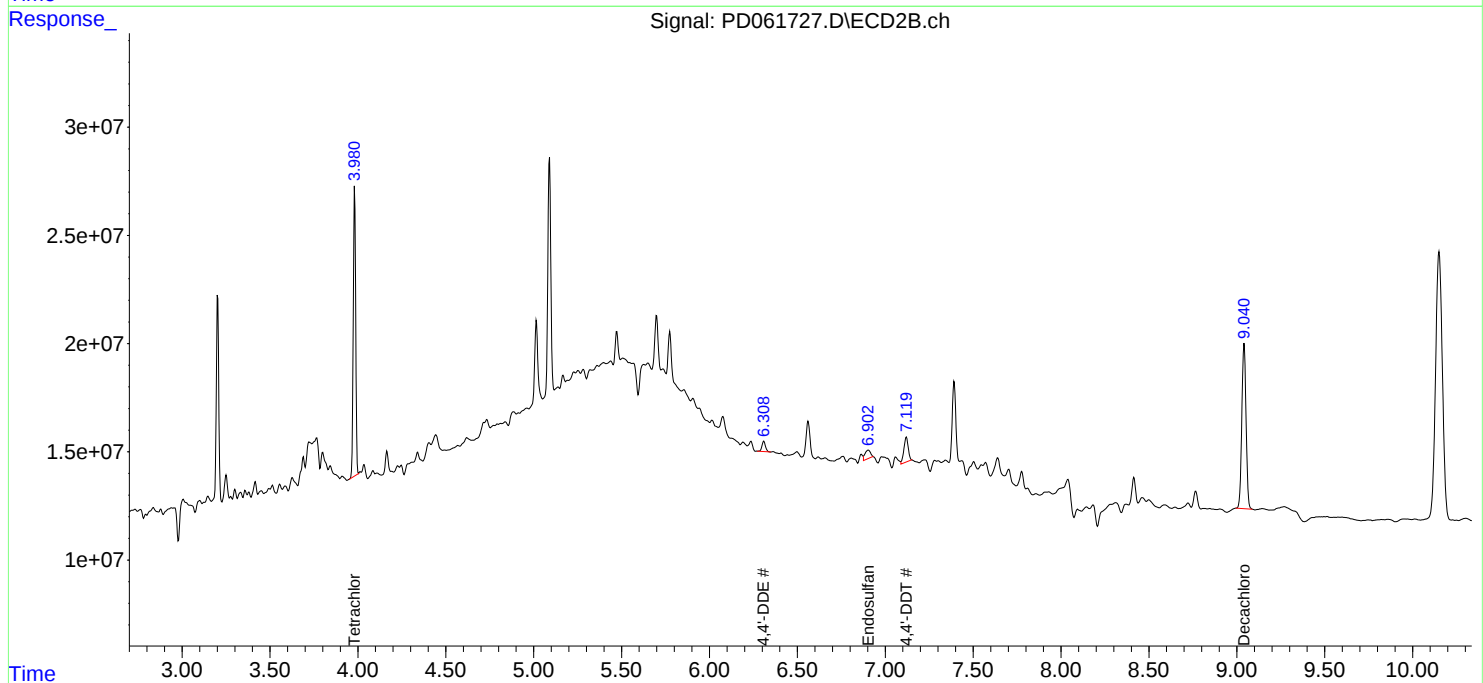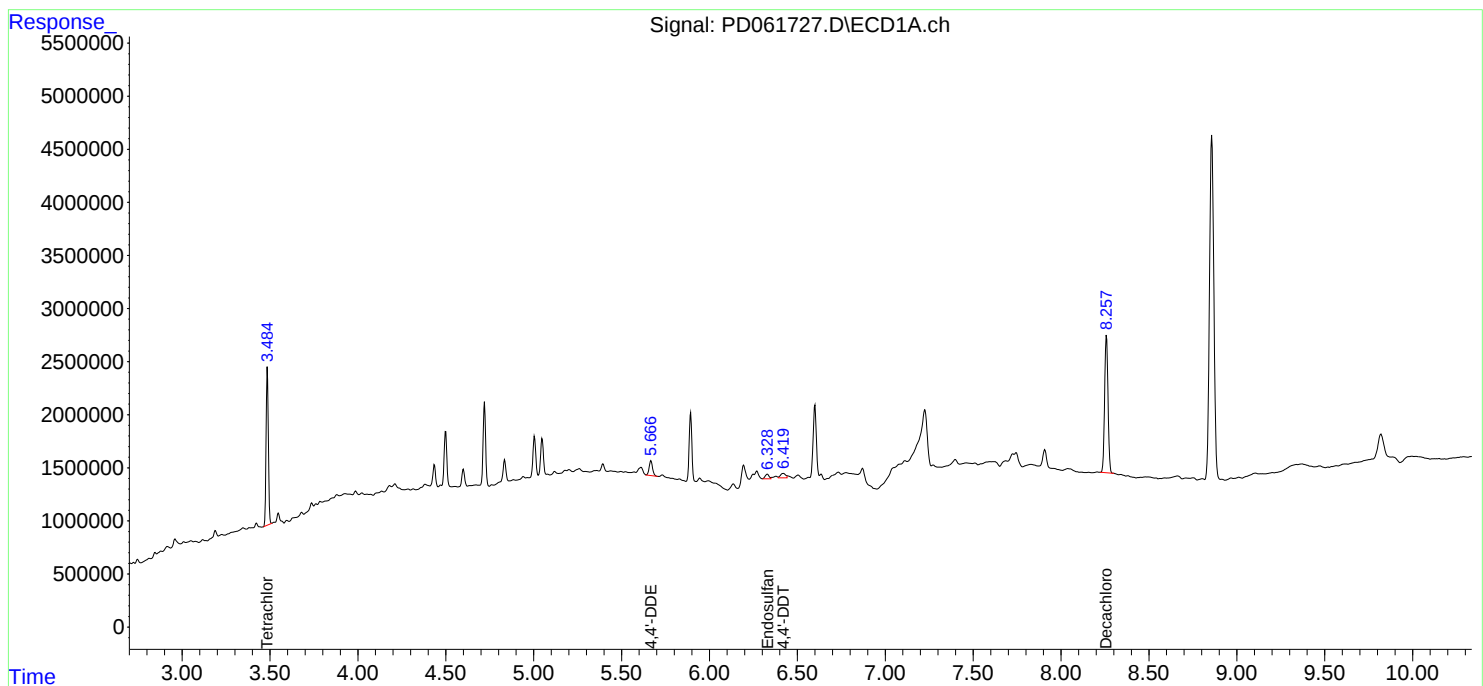

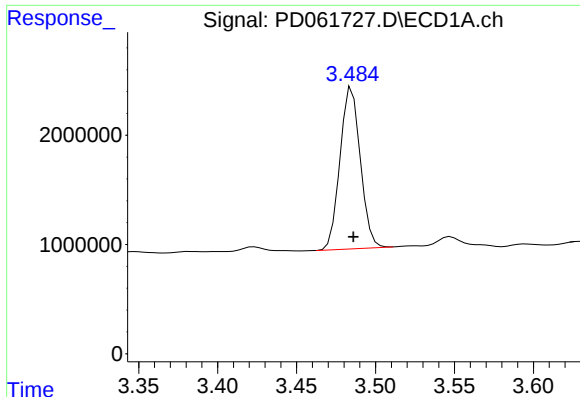


#1 Tetrachloro-m-xylene

R.T.: 3.485 min
Delta R.T.: 0.000 min
Response: 13277585
Conc: 15.53 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-7A


Manual Integrations
APPROVED

Ankita
3/19/2021 10:24:05 AM

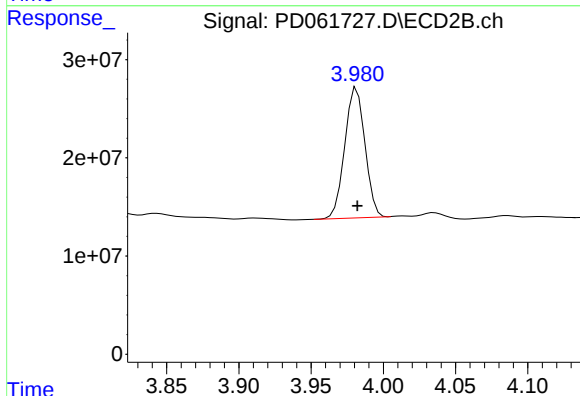


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 128629137
Conc: 14.99 ng/ml

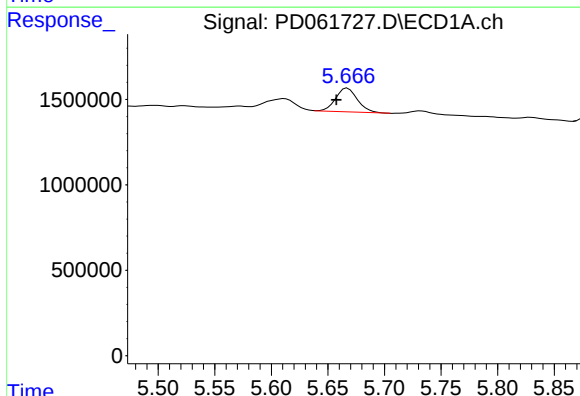


#12 4,4'-DDE

R.T.: 5.666 min
Delta R.T.: 0.009 min
Response: 1857181
Conc: 1.64 ng/ml m

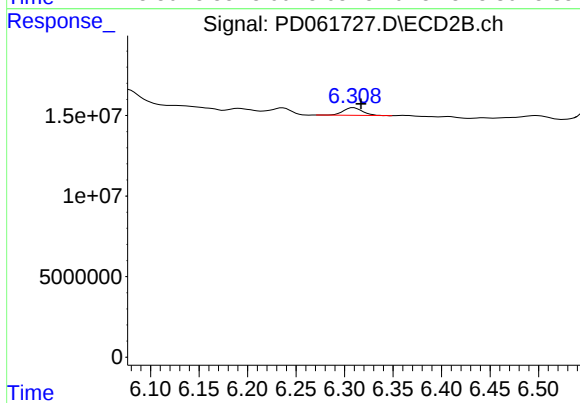

#12 4,4'-DDE

R.T.: 6.309 min
Delta R.T.: -0.008 min
Response: 6660267
Conc: 0.60 ng/ml

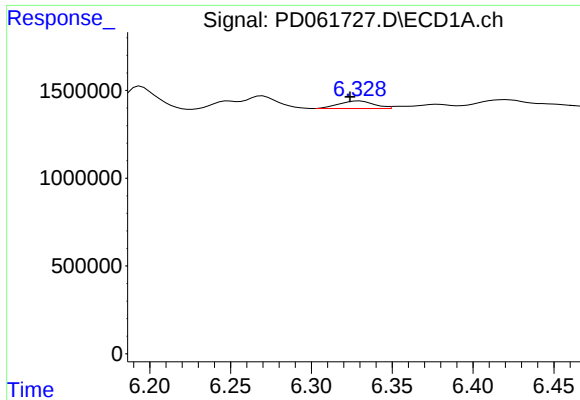


#15 Endosulfan II

R.T.: 6.330 min
Delta R.T.: 0.006 min
Response: 646485
Conc: 0.63 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-7A


Manual Integrations
APPROVED

Ankita
3/19/2021 10:24:05 AM

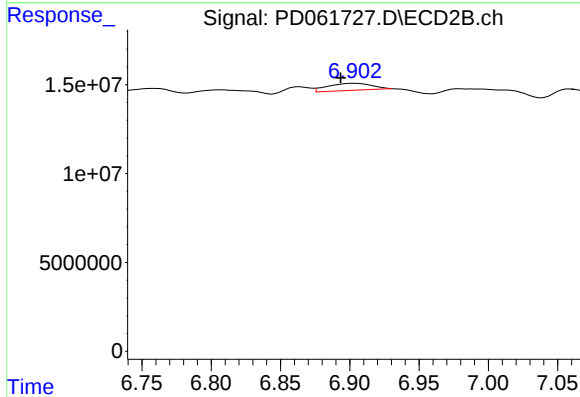


#15 Endosulfan II

R.T.: 6.903 min
Delta R.T.: 0.010 min
Response: 8885385
Conc: 0.96 ng/ml

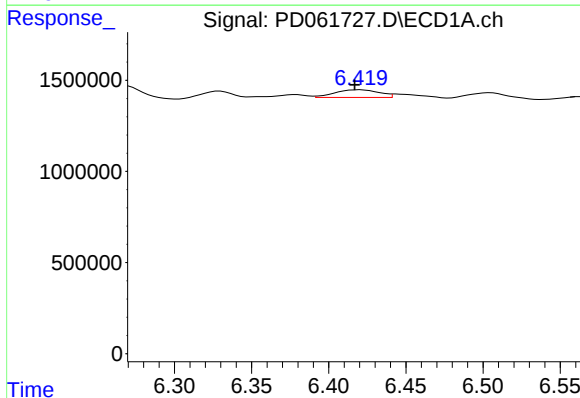


#17 4,4'-DDT

R.T.: 6.419 min
Delta R.T.: 0.003 min
Response: 841551
Conc: 0.84 ng/ml m

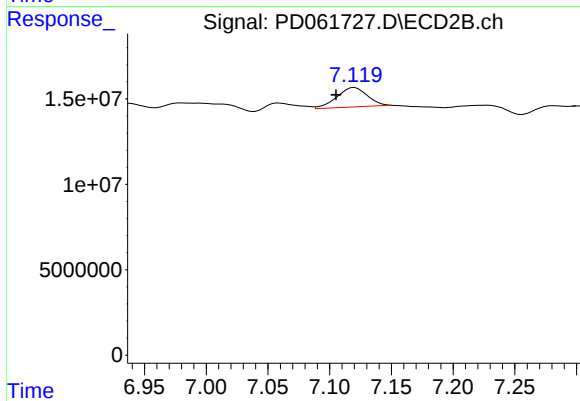

#17 4,4'-DDT

R.T.: 7.120 min
Delta R.T.: 0.015 min
Response: 19453593
Conc: 1.97 ng/ml

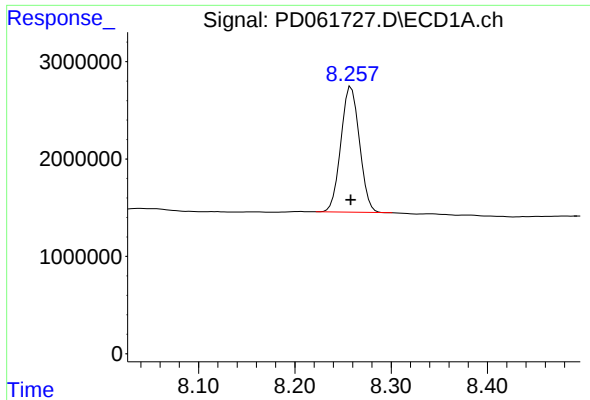


#28 Decachlorobiphenyl

R.T.: 8.259 min
Delta R.T.: 0.000 min
Response: 17233100
Conc: 14.08 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-7A

Manual Integrations
APPROVED

Ankita
3/19/2021 10:24:05 AM

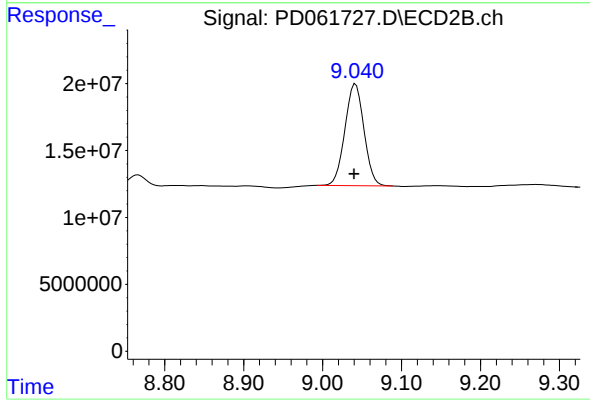

#28 Decachlorobiphenyl

R.T.: 9.042 min
Delta R.T.: 0.002 min
Response: 127696546
Conc: 14.69 ng/ml