

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031821\
 Data File : PD061745.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2021 20:58
 Operator : AR\AJ
 Sample : M1712-24
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 YELLOW-WALL-COMP

Manual Integrations
 APPROVED

Ankita
 3/19/2021 10:24:09 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 06:38:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031721.M
 Quant Title : GC Extractables
 QLast Update : Thu Mar 18 07:52:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.486	3.980	21470777	192.3E6	25.119	22.411m
28)	SA Decachlor...	8.260	9.043	27037281	195.3E6	22.093	22.467

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031821\
Data File : PD061745.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2021 20:58
Operator : AR\AJ
Sample : M1712-24
Misc :
ALS Vial : 40 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
YELLOW-WALL-COMP


Manual Integrations
APPROVED

Ankita
3/19/2021 10:24:09 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 06:38:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031721.M
Quant Title : GC Extractables
QLast Update : Thu Mar 18 07:52:17 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

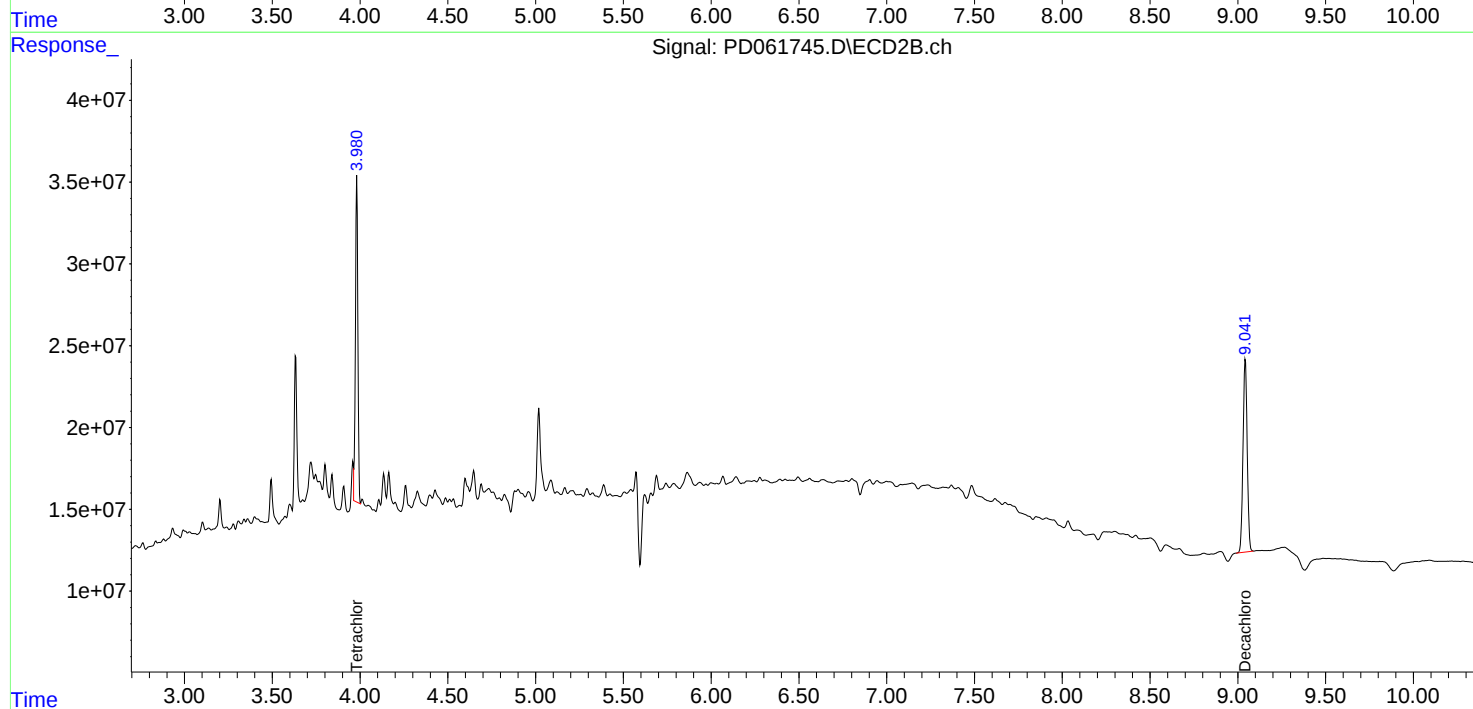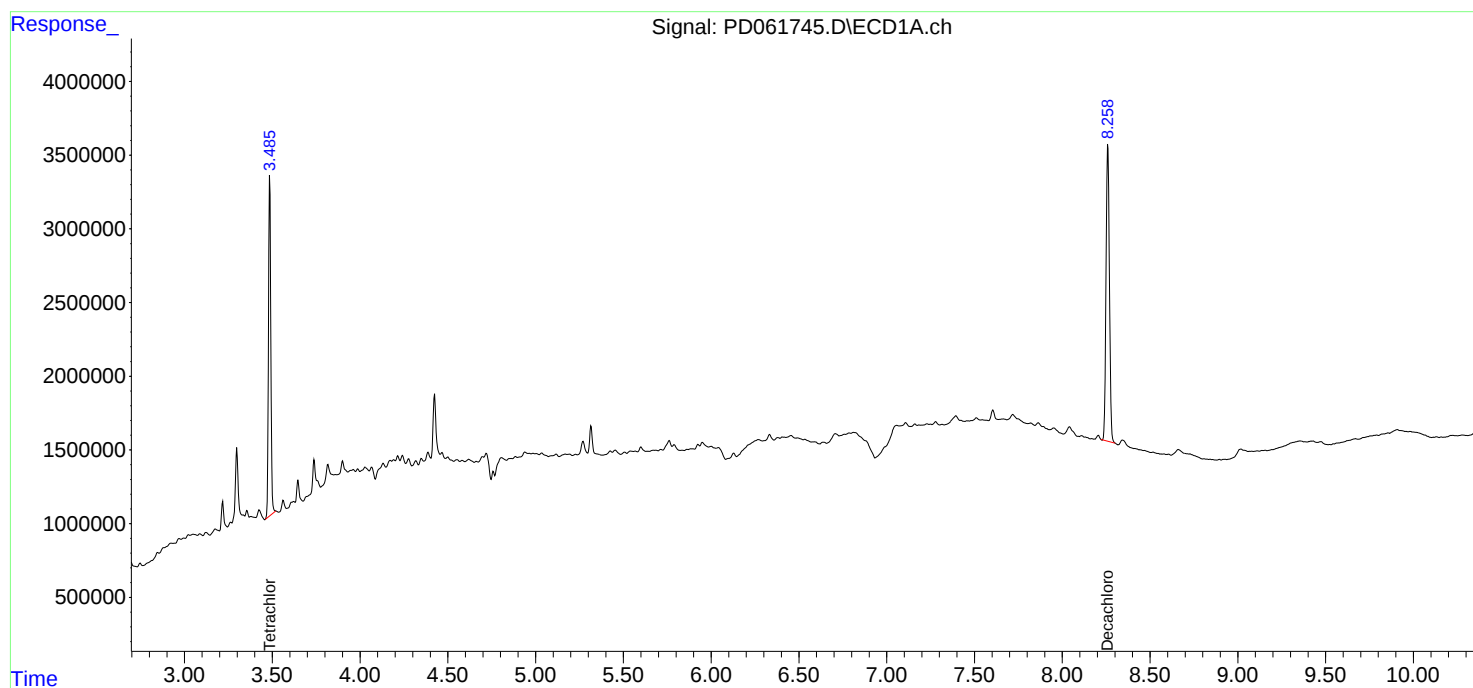

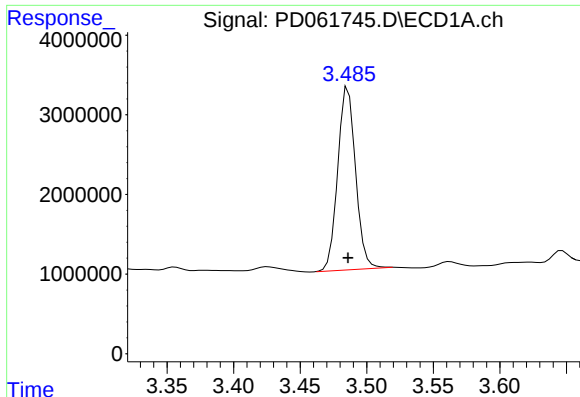


#1 Tetrachloro-m-xylene

R.T.: 3.486 min
Delta R.T.: 0.000 min
Response: 21470777
Conc: 25.12 ng/ml

Instrument :
ECD_D
ClientSampleId :
YELLOW-WALL-COMP


Manual Integrations
APPROVED

Ankita
3/19/2021 10:24:09 AM

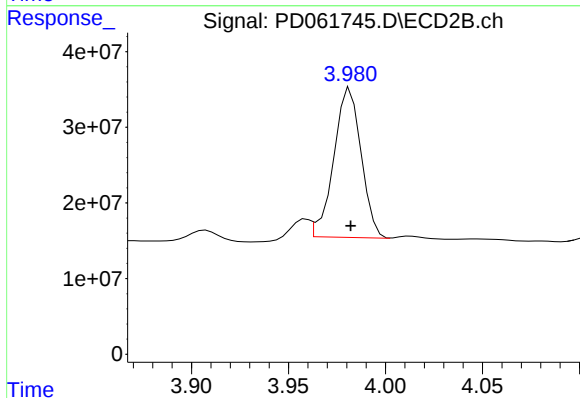


#1 Tetrachloro-m-xylene

R.T.: 3.980 min
Delta R.T.: -0.002 min
Response: 192268011
Conc: 22.41 ng/ml m

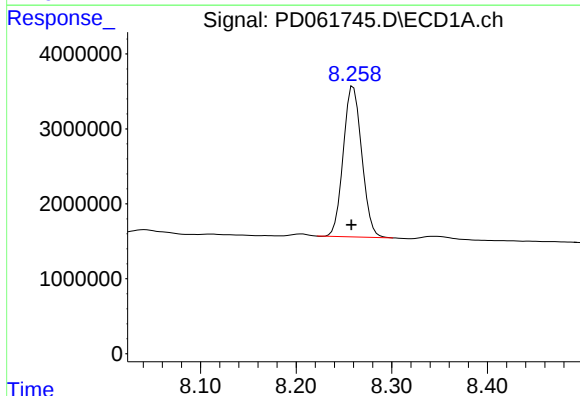

#28 Decachlorobiphenyl

R.T.: 8.260 min
Delta R.T.: 0.002 min
Response: 27037281
Conc: 22.09 ng/ml

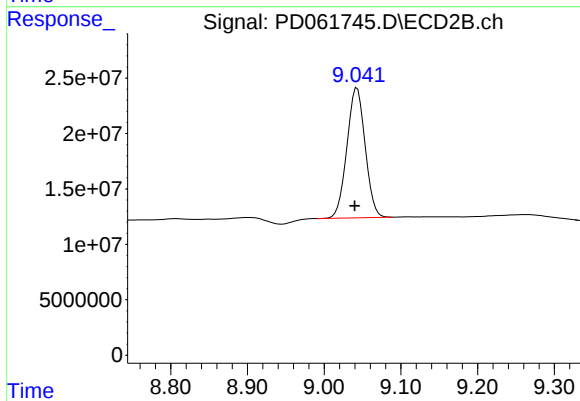

#28 Decachlorobiphenyl

R.T.: 9.043 min
Delta R.T.: 0.003 min
Response: 195311225
Conc: 22.47 ng/ml