

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031824\
 Data File : PD082163.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2024 21:24
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA2057

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 05:04:58 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031824CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 19 05:02:34 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.567	2.777	14784573	22111757	10.222	10.140
27)	SA Decachlor...	9.122	7.913	37294012	37773998	20.960	20.287
Target Compounds							
2)	A alpha-BHC	4.024	3.277	22981036	30228813	9.638	9.866
3)	MA gamma-BHC...	4.358	3.606	22592118	27927001	9.808	9.844
4)	MA Heptachlor	4.951	3.946	23642667	26006929	10.089	9.983
9)	A Endosulfan I	6.110	5.097	20646426	22258781	10.132	10.007
13)	MA Dieldrin	6.386	5.362	40841961	47280472	19.671	19.580
14)	MA Endrin	6.616	5.636	32207394	39296602	19.735	19.840
16)	A 4,4'-DDD	6.749	5.784	28472064	36055693	19.539	19.822
17)	MA 4,4'-DDT	7.064	6.035	28670749	35923372	19.485	19.495
20)	A Methoxychlor	7.540	6.611	77116522	102.5E6	101.213	103.390


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031824\
Data File : PD082163.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2024 21:24
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 05:04:58 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031824CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 19 05:02:34 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

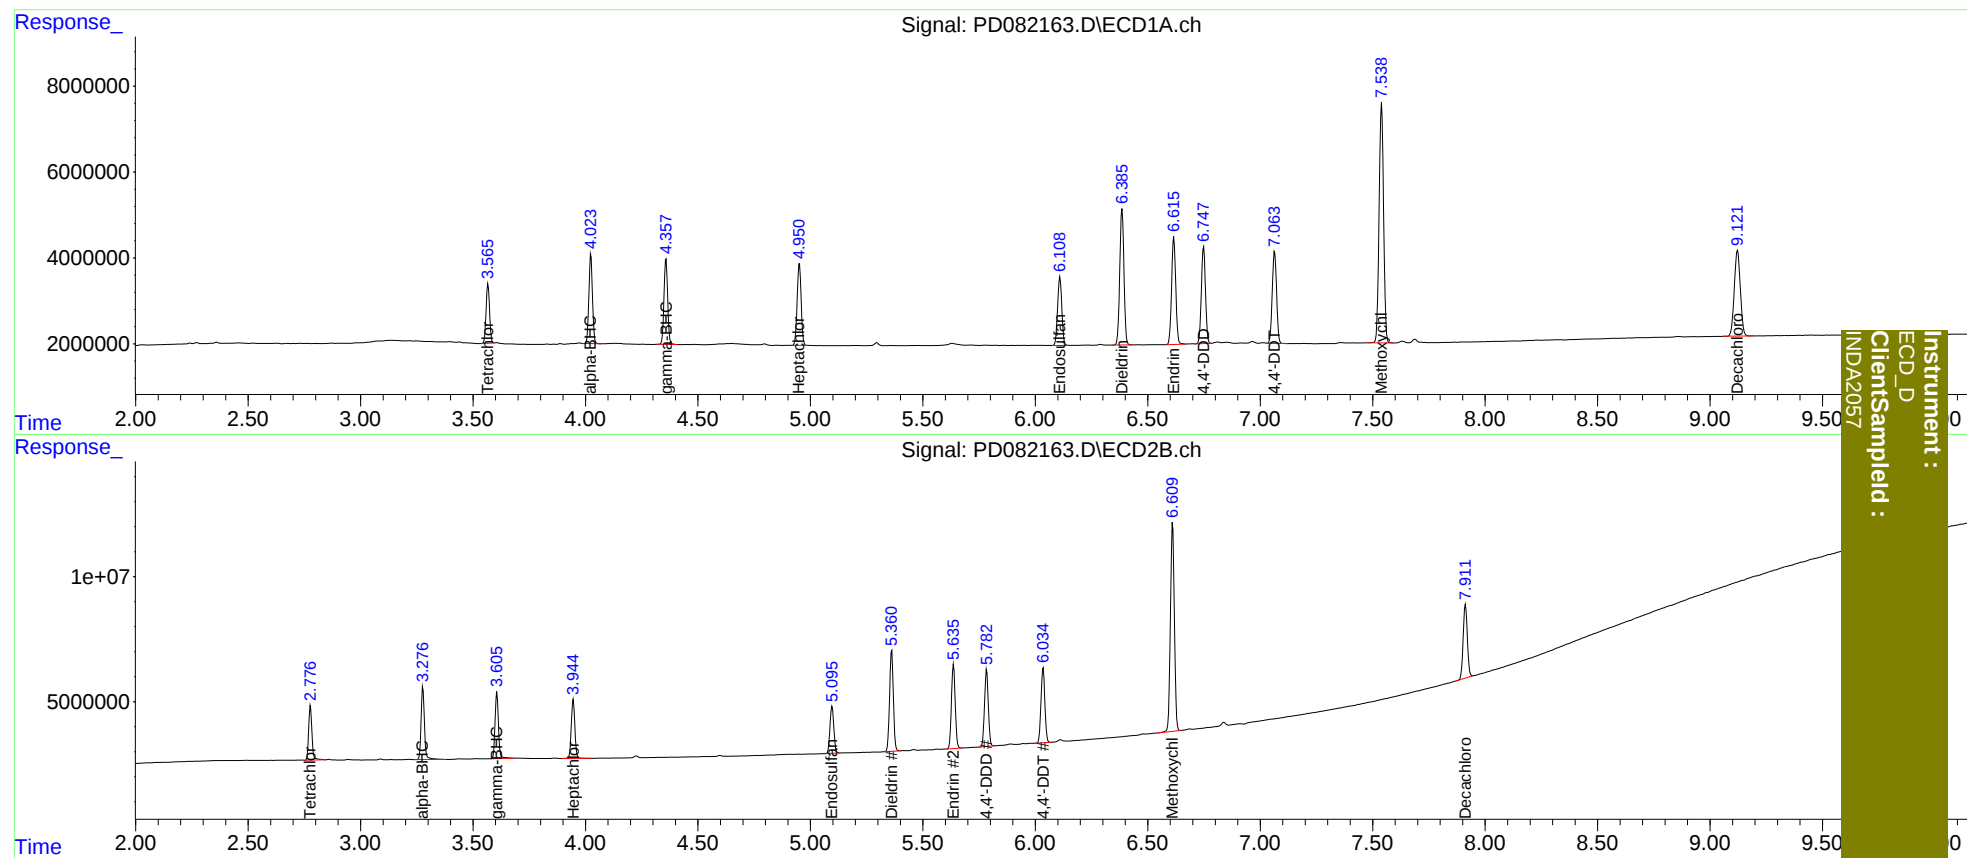


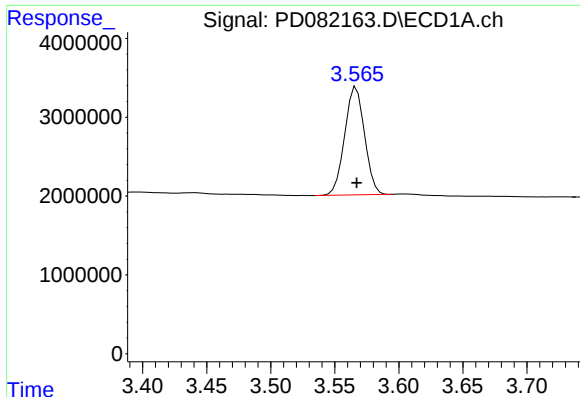

#1 Tetrachloro-m-xylene


R.T.: 3.567 min
Delta R.T.: 0.000 min
Response: 14784573
Conc: 10.22 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA2057

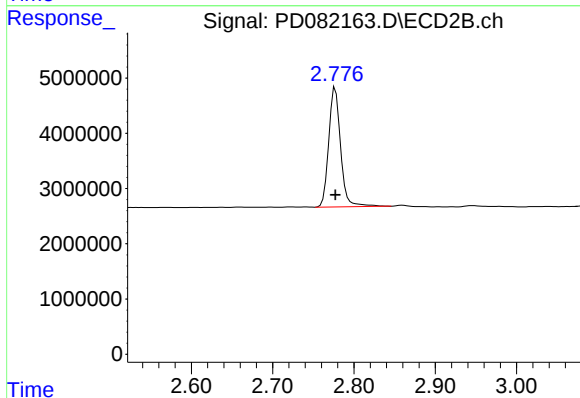


#1 Tetrachloro-m-xylene

R.T.: 2.777 min
Delta R.T.: 0.000 min
Response: 22111757
Conc: 10.14 ng/ml

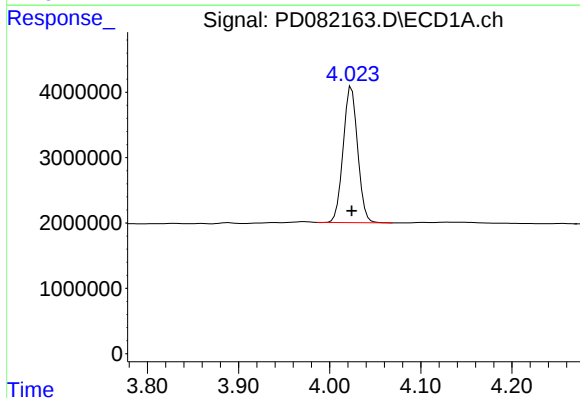


#2 alpha-BHC

R.T.: 4.024 min
Delta R.T.: 0.000 min
Response: 22981036
Conc: 9.64 ng/ml

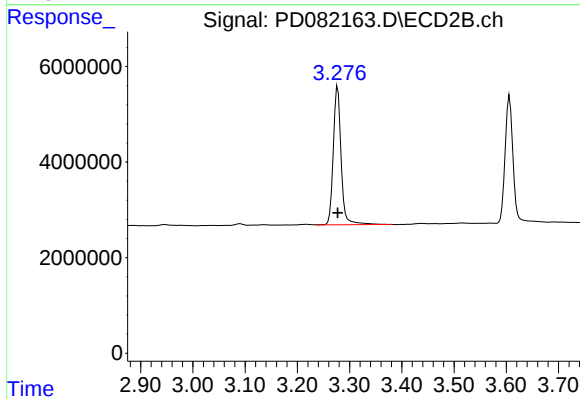

#2 alpha-BHC


R.T.: 3.277 min
Delta R.T.: 0.000 min
Response: 30228813
Conc: 9.87 ng/ml

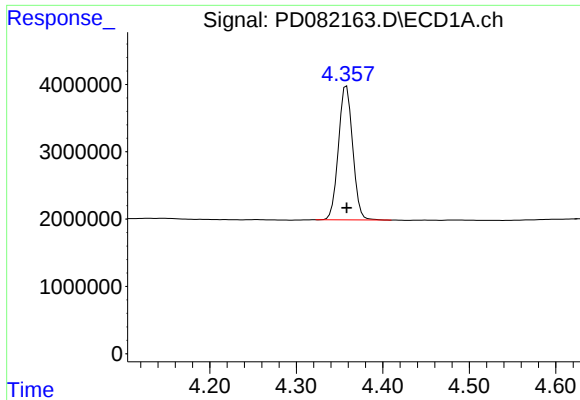

#3 gamma-BHC (Lindane)


R.T.: 4.358 min
Delta R.T.: 0.000 min
Response: 22592118
Conc: 9.81 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA2057

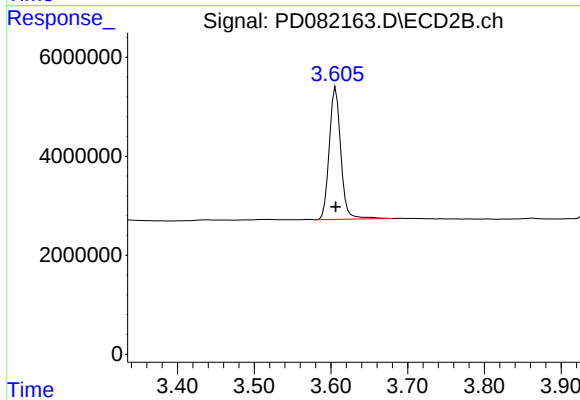


#3 gamma-BHC (Lindane)

R.T.: 3.606 min
Delta R.T.: 0.000 min
Response: 27927001
Conc: 9.84 ng/ml

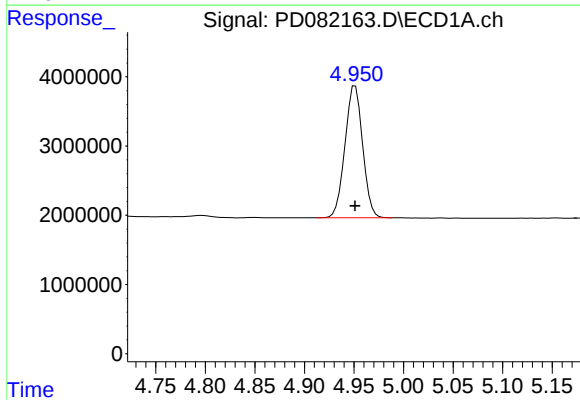


#4 Heptachlor

R.T.: 4.951 min
Delta R.T.: 0.000 min
Response: 23642667
Conc: 10.09 ng/ml

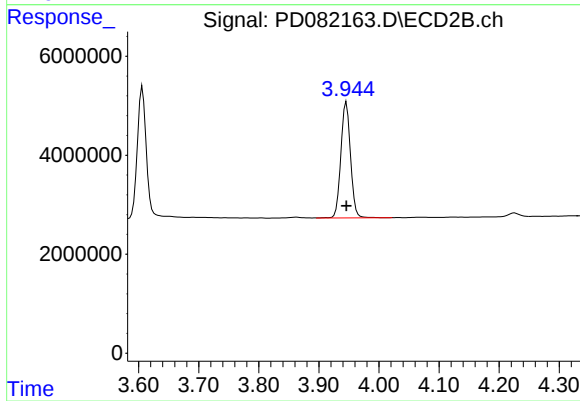

#4 Heptachlor


R.T.: 3.946 min
Delta R.T.: 0.000 min
Response: 26006929
Conc: 9.98 ng/ml

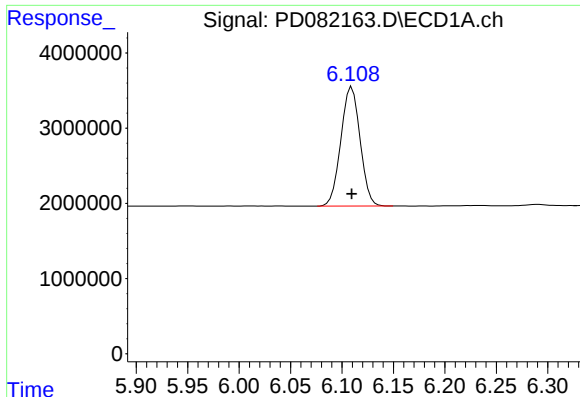

#9 Endosulfan I


R.T.: 6.110 min
Delta R.T.: 0.000 min
Response: 20646426
Conc: 10.13 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA2057

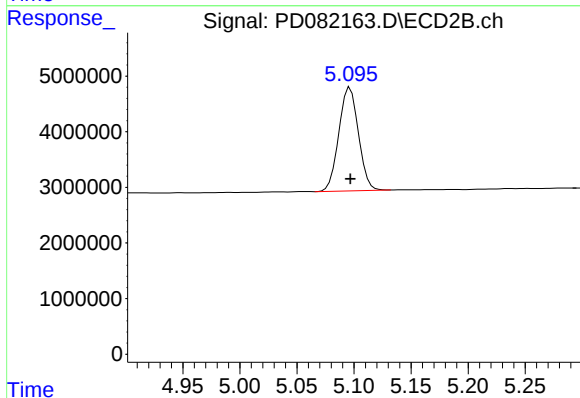


#9 Endosulfan I

R.T.: 5.097 min
Delta R.T.: 0.000 min
Response: 22258781
Conc: 10.01 ng/ml

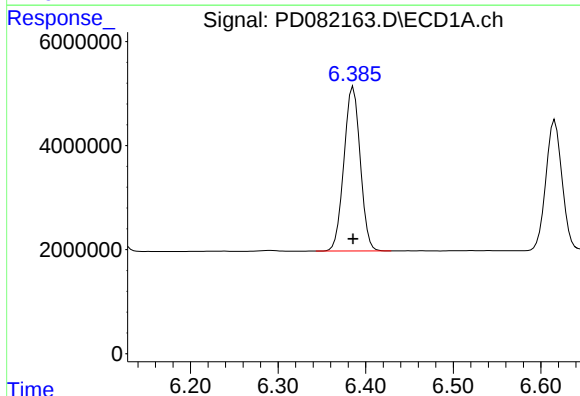


#13 Dieldrin

R.T.: 6.386 min
Delta R.T.: 0.000 min
Response: 40841961
Conc: 19.67 ng/ml

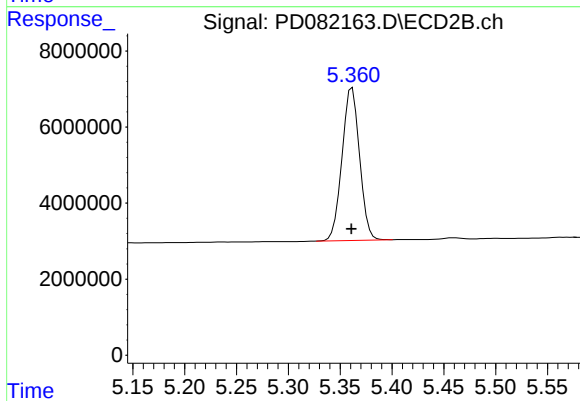

#13 Dieldrin


R.T.: 5.362 min
Delta R.T.: 0.000 min
Response: 47280472
Conc: 19.58 ng/ml

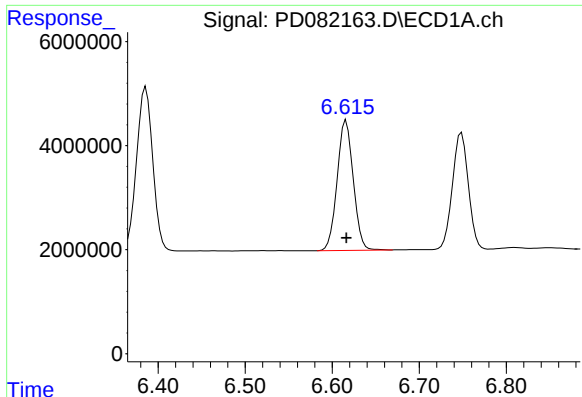

#14 Endrin


R.T.: 6.616 min
Delta R.T.: 0.000 min
Response: 32207394
Conc: 19.74 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA2057

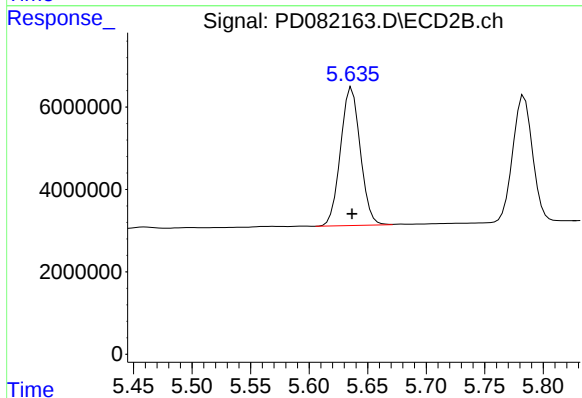


#14 Endrin

R.T.: 5.636 min
Delta R.T.: 0.000 min
Response: 39296602
Conc: 19.84 ng/ml

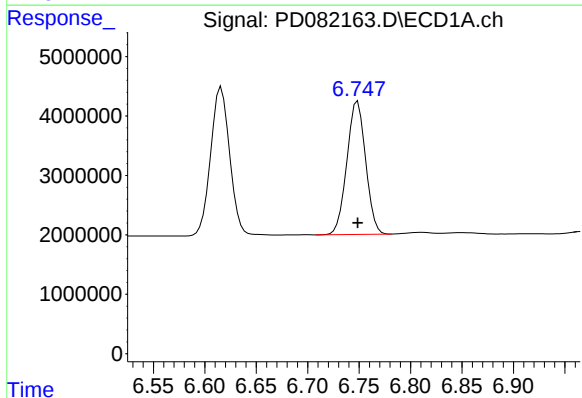


#16 4,4'-DDD

R.T.: 6.749 min
Delta R.T.: 0.000 min
Response: 28472064
Conc: 19.54 ng/ml

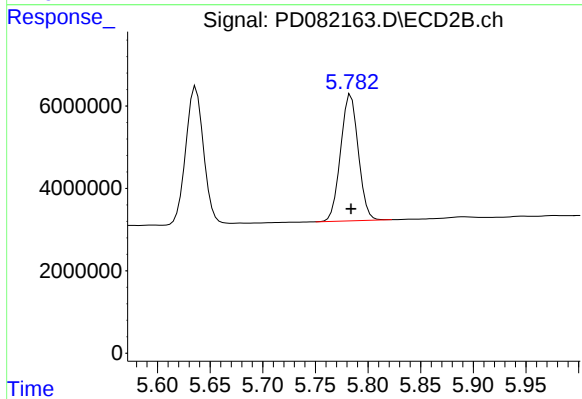

#16 4,4'-DDD


R.T.: 5.784 min
Delta R.T.: 0.000 min
Response: 36055693
Conc: 19.82 ng/ml

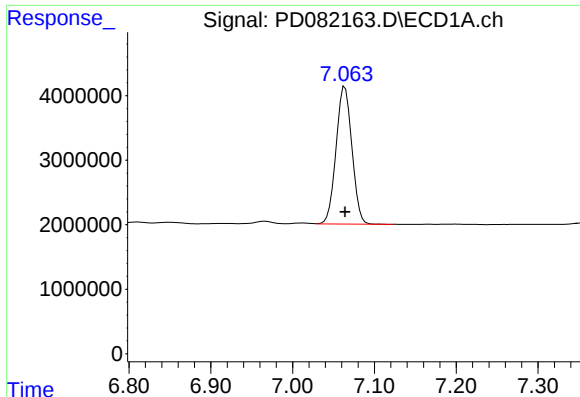

#17 4,4'-DDT


R.T.: 7.064 min
Delta R.T.: 0.000 min
Response: 28670749
Conc: 19.48 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA2057

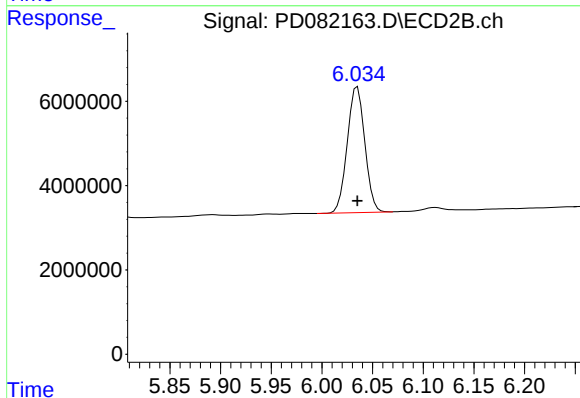


#17 4,4'-DDT

R.T.: 6.035 min
Delta R.T.: 0.000 min
Response: 35923372
Conc: 19.49 ng/ml

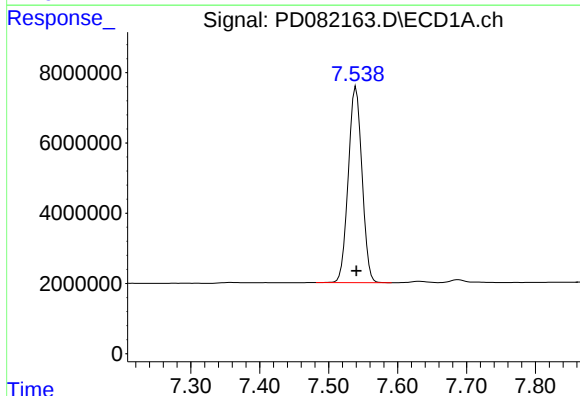


#20 Methoxychlor

R.T.: 7.540 min
Delta R.T.: 0.000 min
Response: 77116522
Conc: 101.21 ng/ml

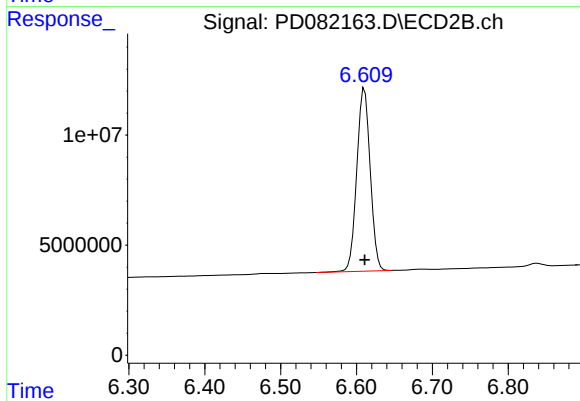

#20 Methoxychlor


R.T.: 6.611 min
Delta R.T.: 0.000 min
Response: 102461294
Conc: 103.39 ng/ml

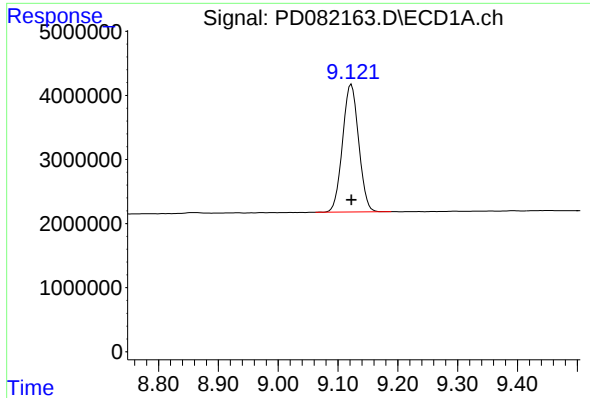

#27 Decachlorobiphenyl

R.T.: 9.122 min
Delta R.T.: 0.000 min
Response: 37294012
Conc: 20.96 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA2057

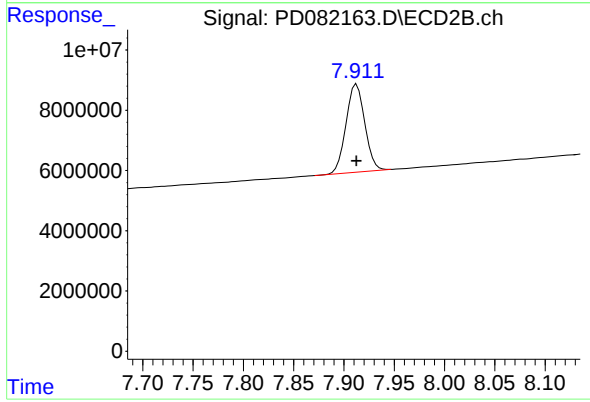

#27 Decachlorobiphenyl

R.T.: 7.913 min
Delta R.T.: 0.000 min
Response: 37773998
Conc: 20.29 ng/ml