

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031824\
 Data File : PD082165.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2024 21:50
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA3059

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 05:05:12 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031824CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 19 05:02:34 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.567	2.777	28926538	43612822	20.000	20.000
27)	SA Decachlor...	9.123	7.912	71173097	74477458	40.000	40.000
Target Compounds							
2)	A alpha-BHC	4.024	3.278	47687789	61279361	20.000	20.000
3)	MA gamma-BHC...	4.358	3.606	46070827	56741480	20.000	20.000
4)	MA Heptachlor	4.951	3.946	46867481	52103874	20.000	20.000
9)	A Endosulfan I	6.109	5.097	40755127	44486310	20.000	20.000
13)	MA Dieldrin	6.386	5.361	83049762	96587272	40.000	40.000
14)	MA Endrin	6.616	5.637	65279382	79228627	40.000	40.000
16)	A 4,4'-DDD	6.749	5.784	58289091	72759222	40.000	40.000
17)	MA 4,4'-DDT	7.064	6.035	58858316	73708811	40.000	40.000
20)	A Methoxychlor	7.540	6.611	152.4E6	198.2E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031824\
Data File : PD082165.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2024 21:50
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 05:05:12 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031824CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 19 05:02:34 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

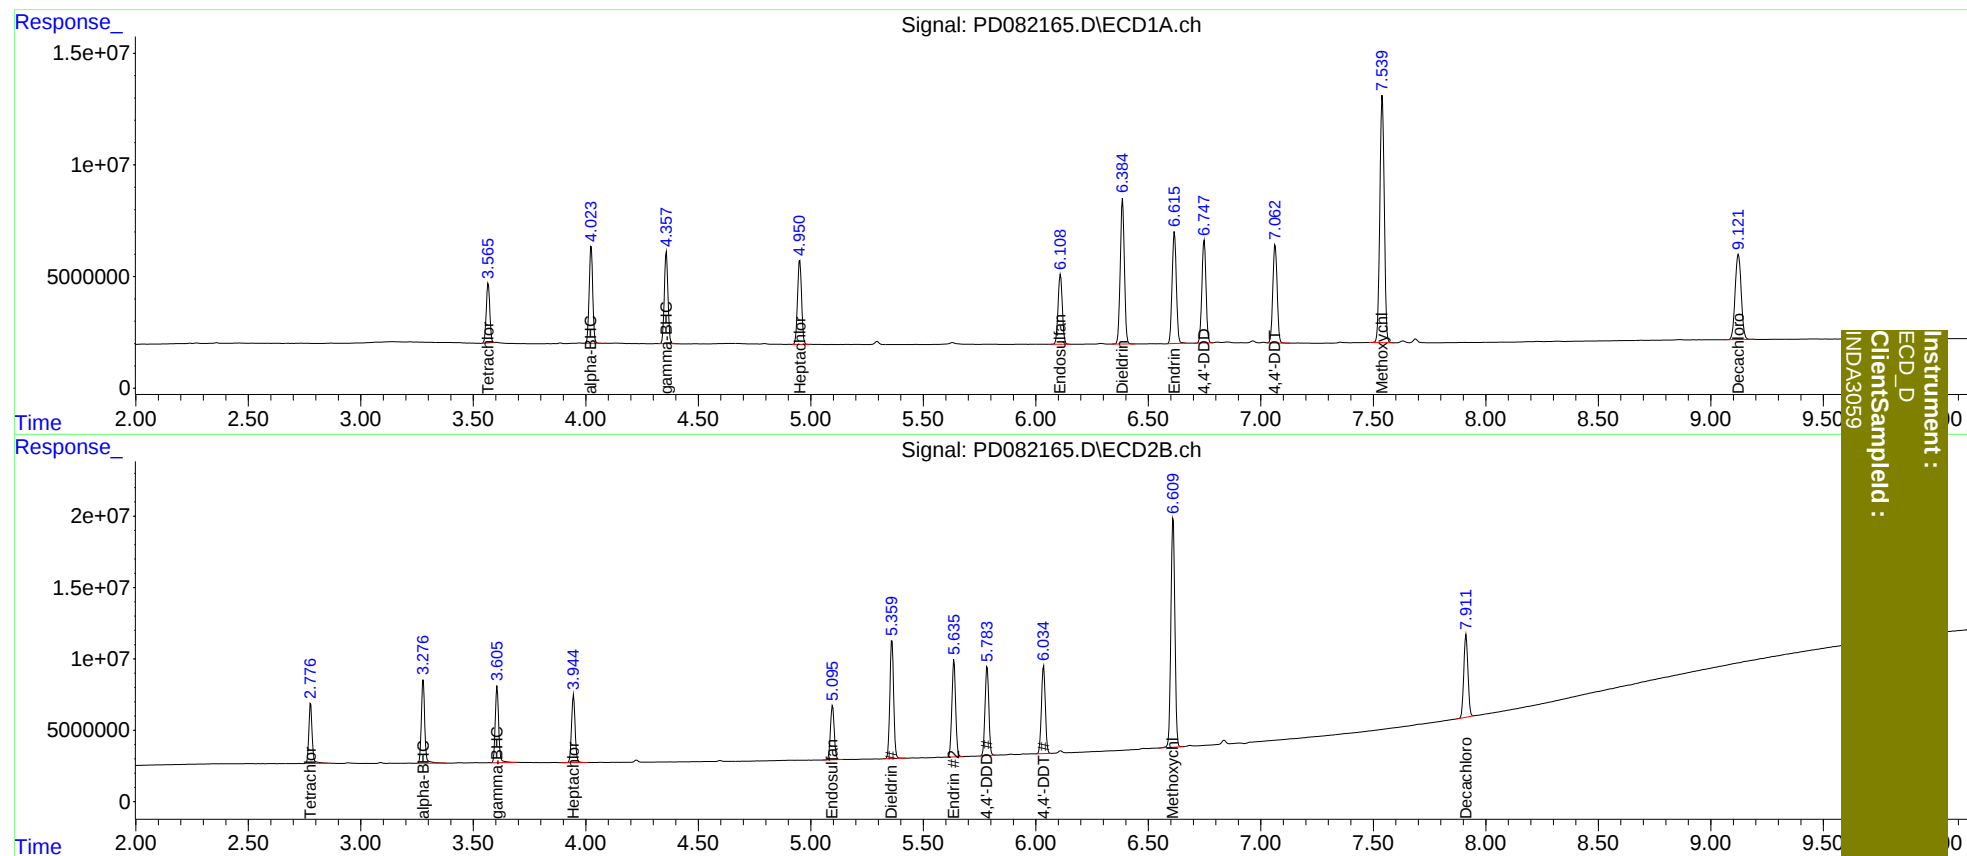


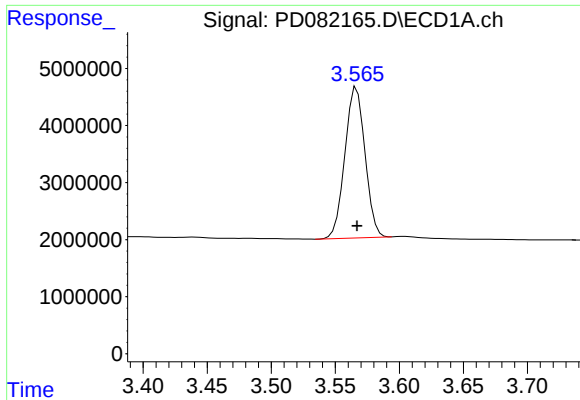

#1 Tetrachloro-m-xylene


R.T.: 3.567 min
Delta R.T.: 0.000 min
Response: 28926538
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3059

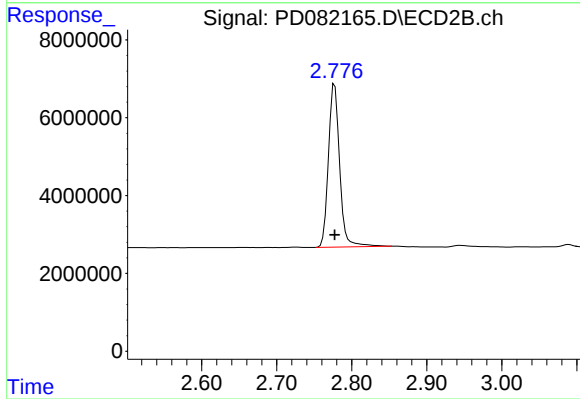


#1 Tetrachloro-m-xylene

R.T.: 2.777 min
Delta R.T.: 0.000 min
Response: 43612822
Conc: 20.00 ng/ml

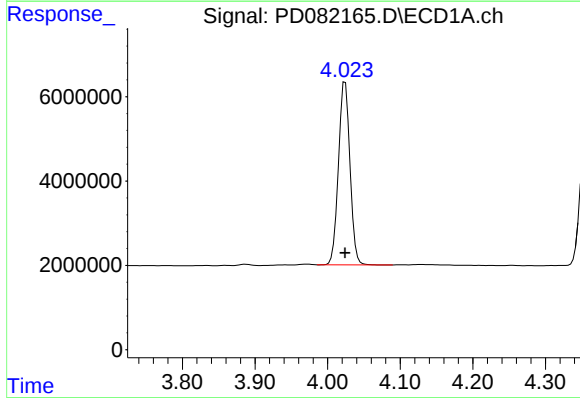


#2 alpha-BHC

R.T.: 4.024 min
Delta R.T.: 0.000 min
Response: 47687789
Conc: 20.00 ng/ml

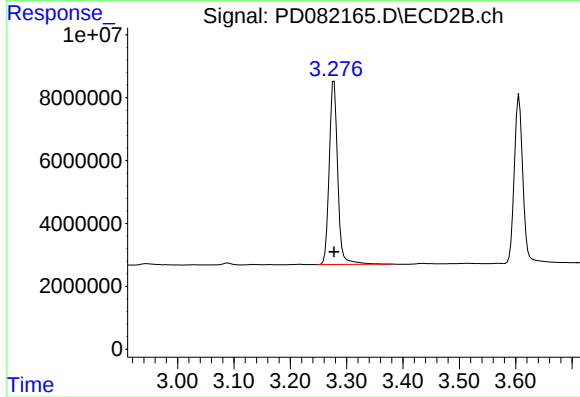

#2 alpha-BHC


R.T.: 3.278 min
Delta R.T.: 0.000 min
Response: 61279361
Conc: 20.00 ng/ml

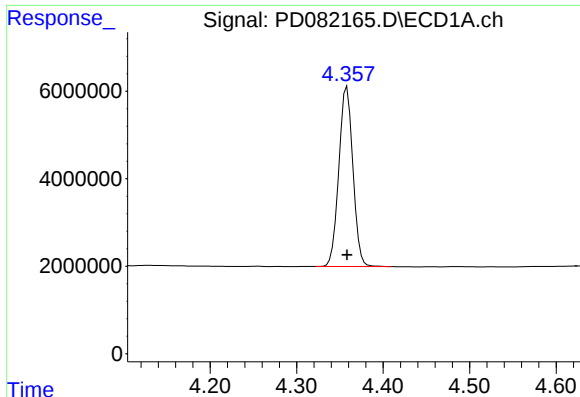

#3 gamma-BHC (Lindane)


R.T.: 4.358 min
Delta R.T.: 0.000 min
Response: 46070827
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3059

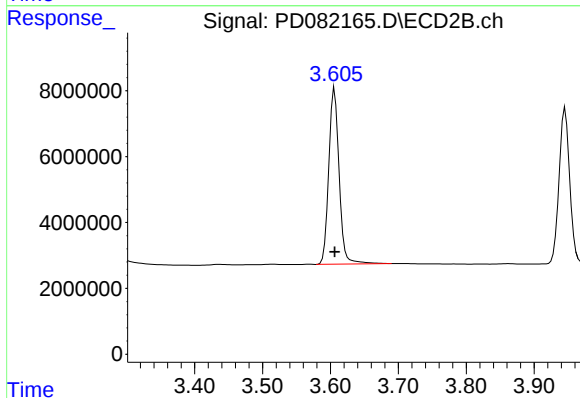


#3 gamma-BHC (Lindane)

R.T.: 3.606 min
Delta R.T.: 0.000 min
Response: 56741480
Conc: 20.00 ng/ml

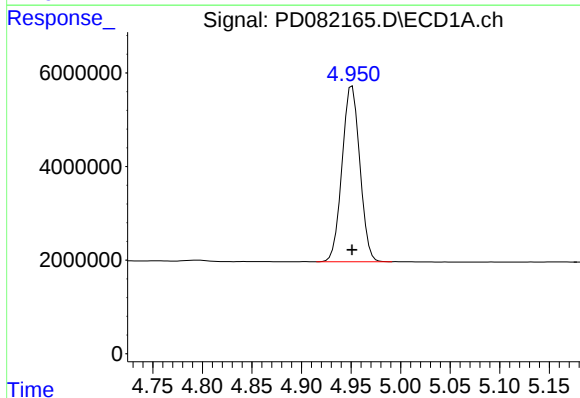


#4 Heptachlor

R.T.: 4.951 min
Delta R.T.: 0.000 min
Response: 46867481
Conc: 20.00 ng/ml

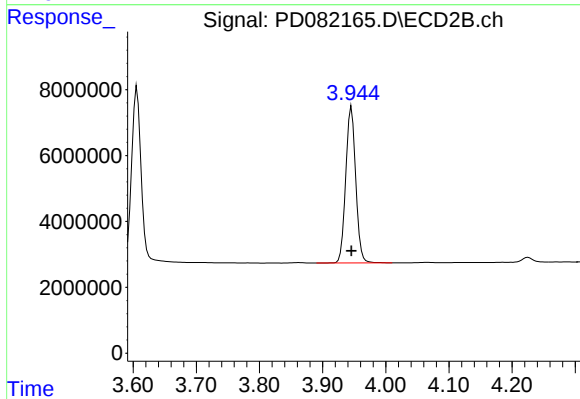

#4 Heptachlor


R.T.: 3.946 min
Delta R.T.: 0.000 min
Response: 52103874
Conc: 20.00 ng/ml

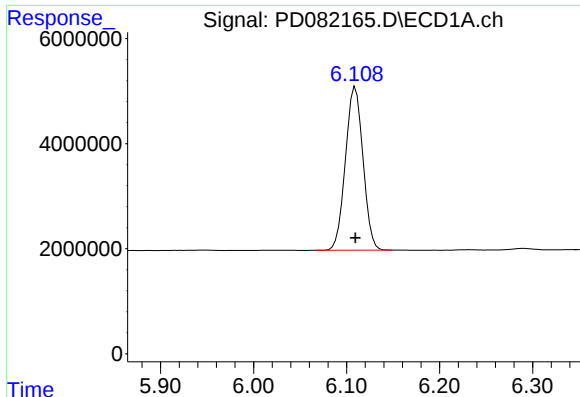

#9 Endosulfan I


R.T.: 6.109 min
Delta R.T.: 0.000 min
Response: 40755127
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3059

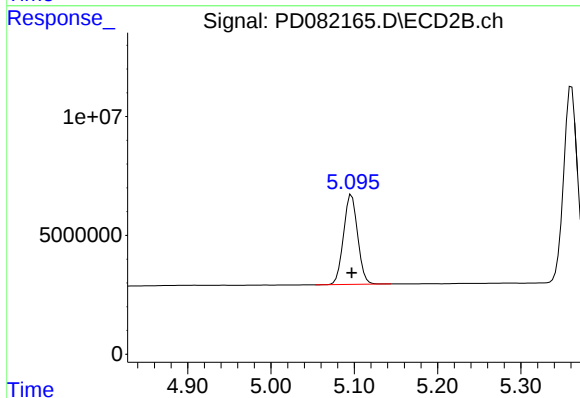


#9 Endosulfan I

R.T.: 5.097 min
Delta R.T.: 0.000 min
Response: 44486310
Conc: 20.00 ng/ml

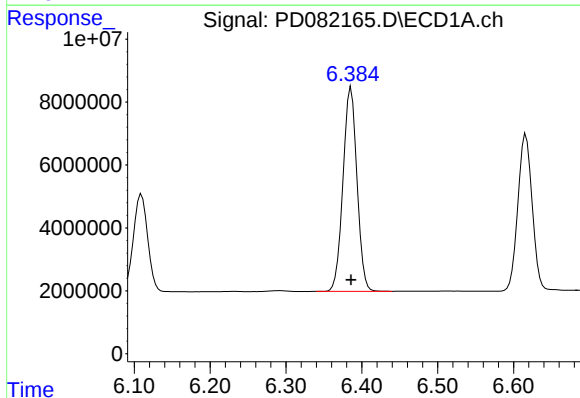


#13 Dieldrin

R.T.: 6.386 min
Delta R.T.: 0.000 min
Response: 83049762
Conc: 40.00 ng/ml

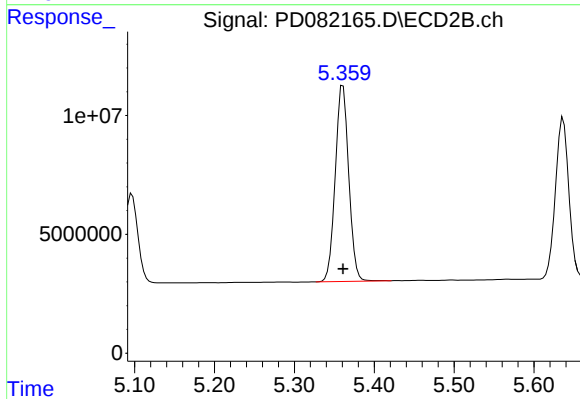

#13 Dieldrin


R.T.: 5.361 min
Delta R.T.: 0.000 min
Response: 96587272
Conc: 40.00 ng/ml

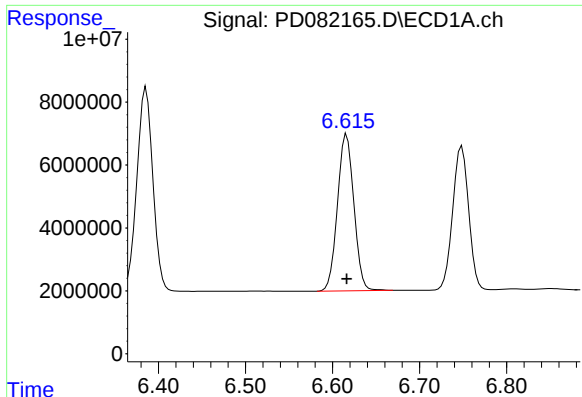

#14 Endrin


R.T.: 6.616 min
Delta R.T.: 0.000 min
Response: 65279382
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3059

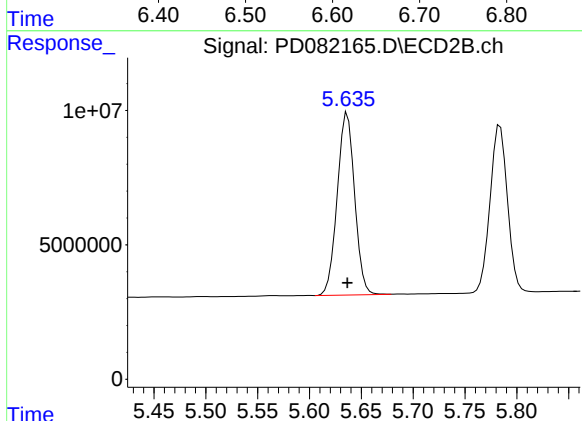


#14 Endrin

R.T.: 5.637 min
Delta R.T.: 0.000 min
Response: 79228627
Conc: 40.00 ng/ml

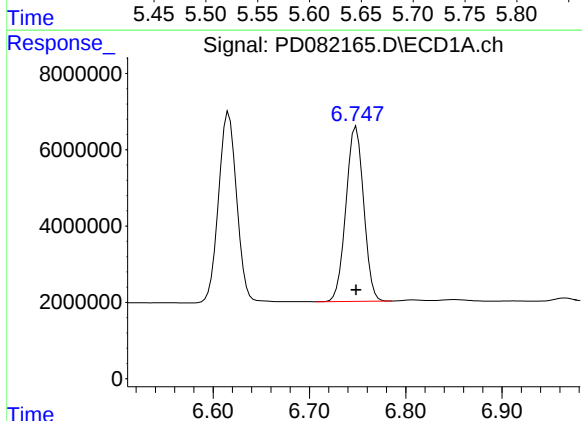


#16 4,4'-DDD

R.T.: 6.749 min
Delta R.T.: 0.000 min
Response: 58289091
Conc: 40.00 ng/ml

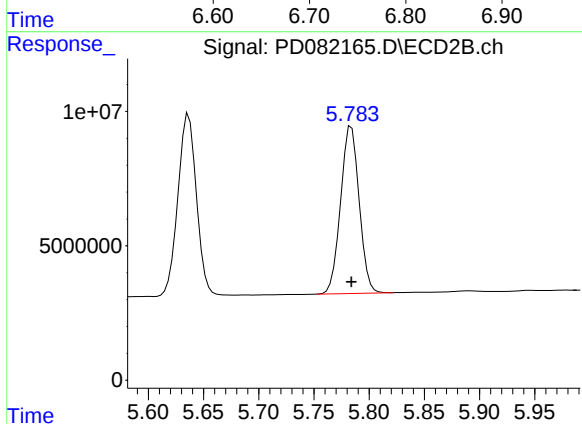

#16 4,4'-DDD


R.T.: 5.784 min
Delta R.T.: 0.000 min
Response: 72759222
Conc: 40.00 ng/ml

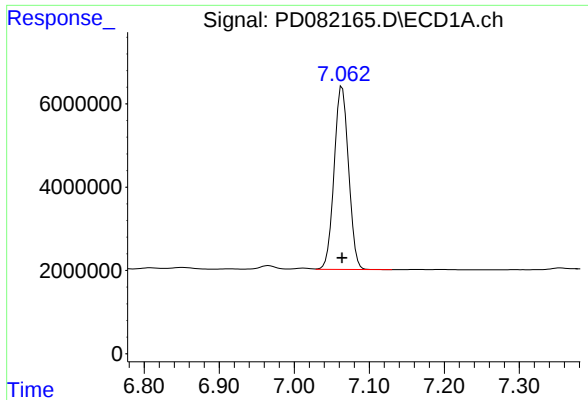

#17 4,4'-DDT


R.T.: 7.064 min
Delta R.T.: 0.000 min
Response: 58858316
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3059

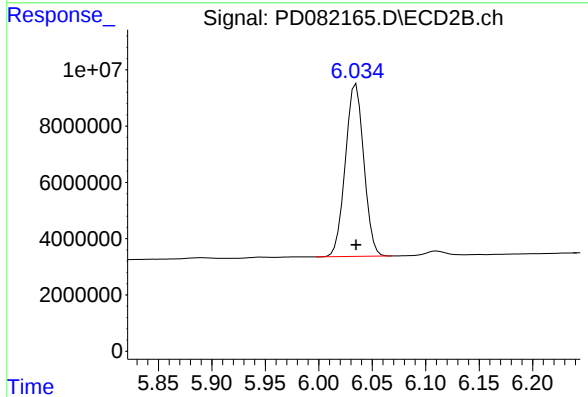


#17 4,4'-DDT

R.T.: 6.035 min
Delta R.T.: 0.000 min
Response: 73708811
Conc: 40.00 ng/ml

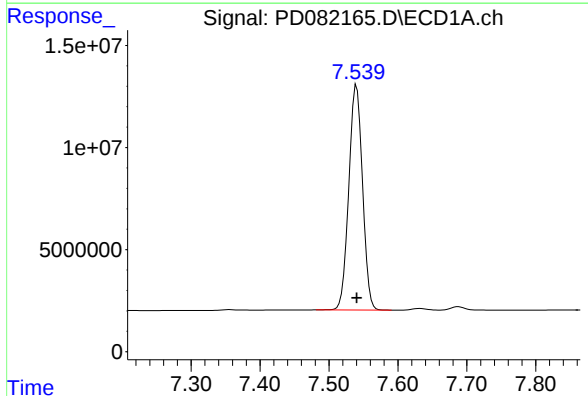


#20 Methoxychlor

R.T.: 7.540 min
Delta R.T.: 0.000 min
Response: 152384474
Conc: 200.00 ng/ml

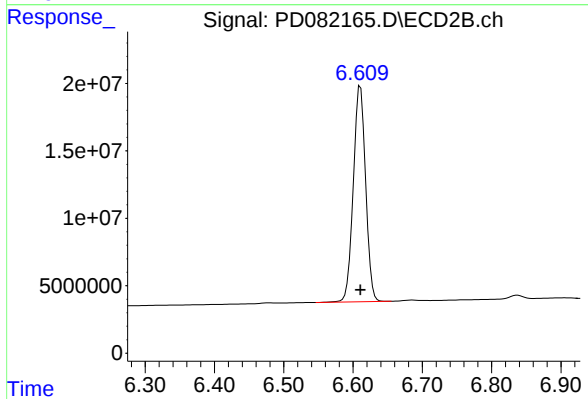

#20 Methoxychlor


R.T.: 6.611 min
Delta R.T.: 0.000 min
Response: 198204379
Conc: 200.00 ng/ml

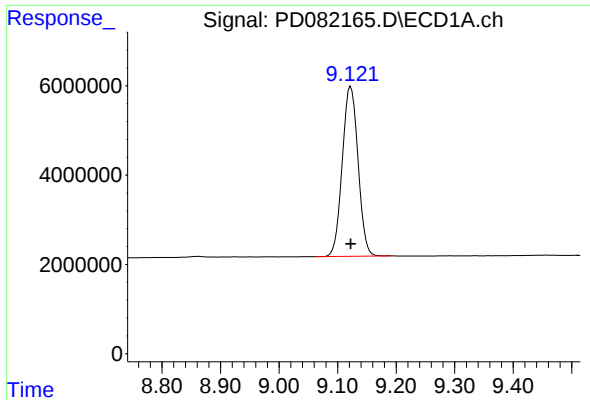

#27 Decachlorobiphenyl

R.T.: 9.123 min
Delta R.T.: 0.000 min
Response: 71173097
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3059

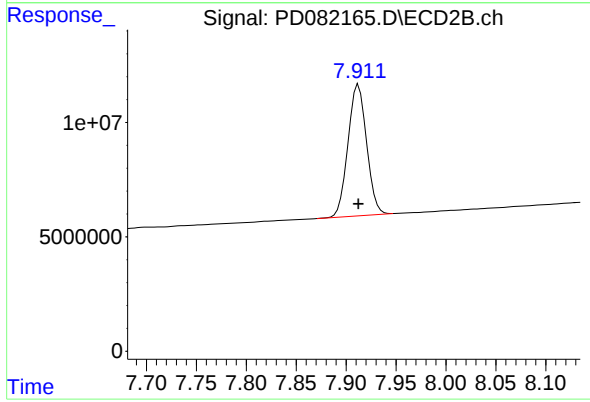

#27 Decachlorobiphenyl

R.T.: 7.912 min
Delta R.T.: 0.000 min
Response: 74477458
Conc: 40.00 ng/ml