

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031824\
 Data File : PD082167.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2024 22:17
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA4061

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 05:05:23 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031824CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 19 05:02:34 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.567	2.777	57296253	85115461	39.615	39.032
27)	SA Decachlor...	9.123	7.913	136.8E6	146.8E6	76.869	78.843
Target Compounds							
2)	A alpha-BHC	4.024	3.278	100.8E6	125.1E6	42.276	40.837
3)	MA gamma-BHC...	4.358	3.607	95555912	114.0E6	41.482	40.181
4)	MA Heptachlor	4.951	3.946	95501331	103.9E6	40.754	39.863
9)	A Endosulfan I	6.110	5.097	81099360	87086457	39.798	39.152
13)	MA Dieldrin	6.386	5.362	170.8E6	193.0E6	82.250	79.921
14)	MA Endrin	6.617	5.637	135.2E6	158.9E6	82.814	80.230
16)	A 4,4'-DDD	6.748	5.784	120.7E6	145.9E6	82.862	80.206
17)	MA 4,4'-DDT	7.065	6.035	122.3E6	150.6E6	83.105	81.738
20)	A Methoxychlor	7.540	6.610	304.5E6	379.8E6	399.616	383.272


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031824\
Data File : PD082167.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2024 22:17
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 05:05:23 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031824CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 19 05:02:34 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

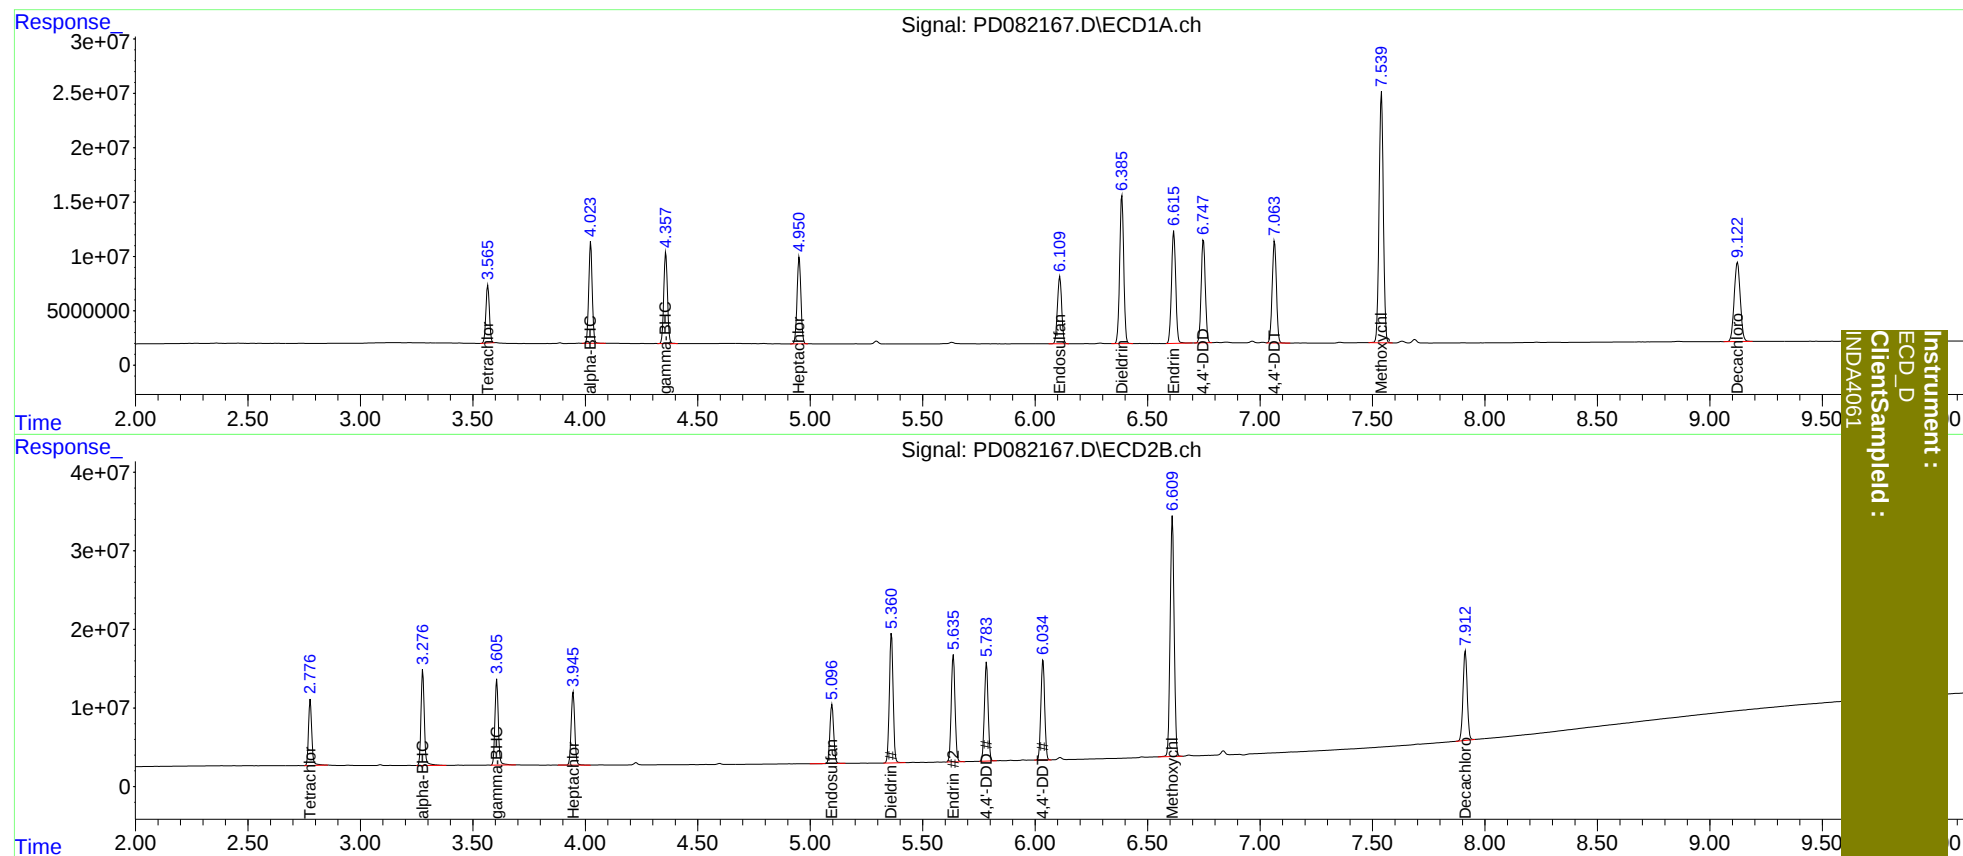


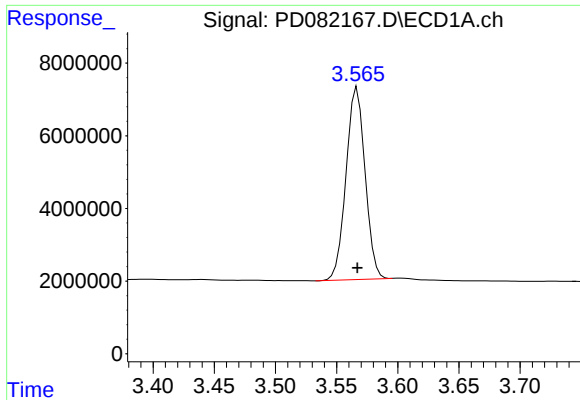

#1 Tetrachloro-m-xylene


R.T.: 3.567 min
Delta R.T.: 0.000 min
Response: 57296253
Conc: 39.62 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4061

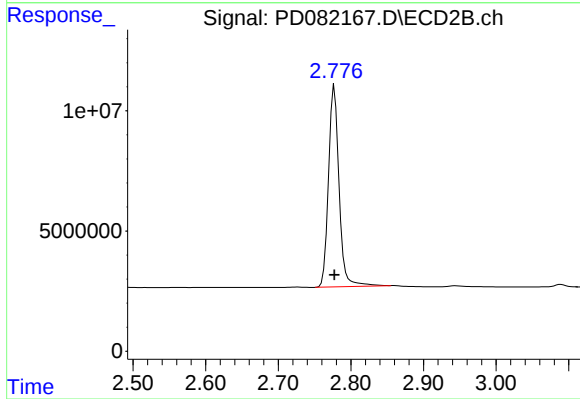


#1 Tetrachloro-m-xylene

R.T.: 2.777 min
Delta R.T.: 0.000 min
Response: 85115461
Conc: 39.03 ng/ml

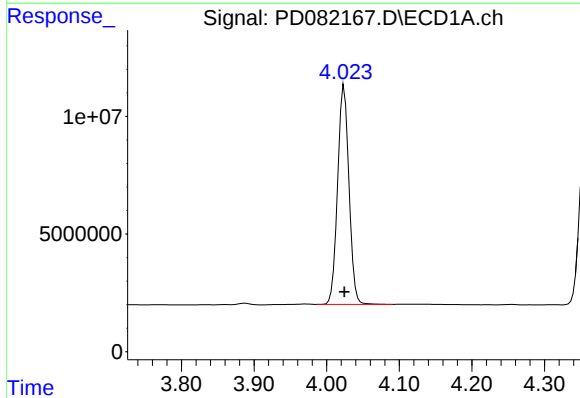


#2 alpha-BHC

R.T.: 4.024 min
Delta R.T.: 0.000 min
Response: 100801446
Conc: 42.28 ng/ml

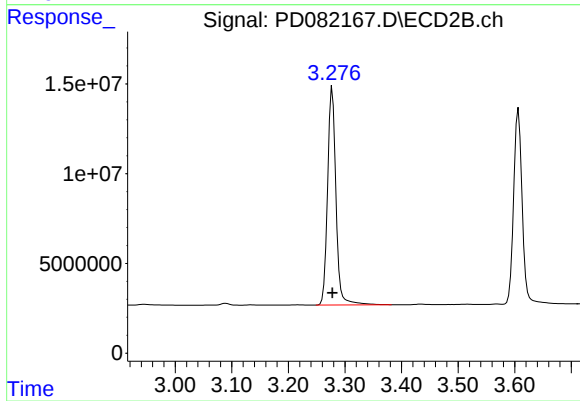

#2 alpha-BHC


R.T.: 3.278 min
Delta R.T.: 0.000 min
Response: 125121731
Conc: 40.84 ng/ml

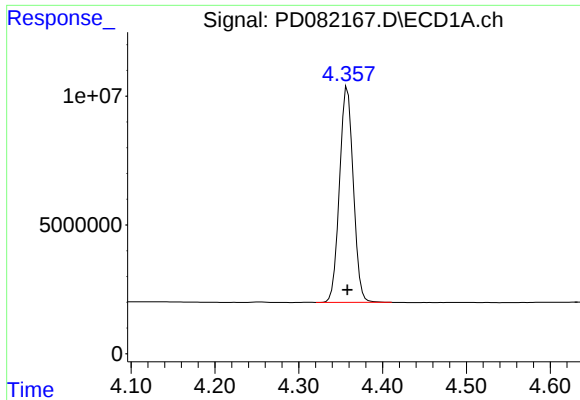

#3 gamma-BHC (Lindane)


R.T.: 4.358 min
Delta R.T.: 0.000 min
Response: 95555912
Conc: 41.48 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4061

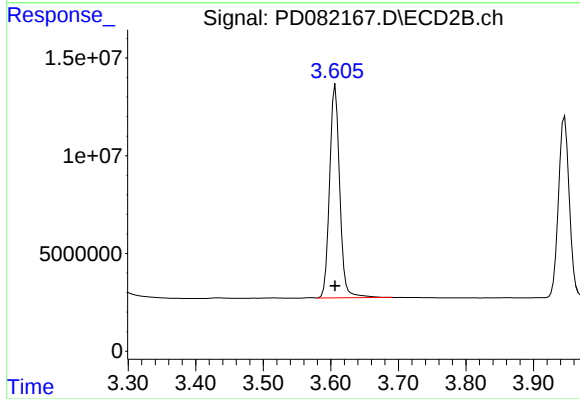


#3 gamma-BHC (Lindane)

R.T.: 3.607 min
Delta R.T.: 0.000 min
Response: 113995651
Conc: 40.18 ng/ml

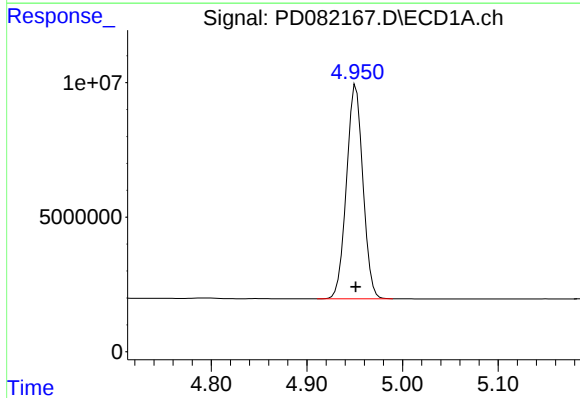


#4 Heptachlor

R.T.: 4.951 min
Delta R.T.: 0.000 min
Response: 95501331
Conc: 40.75 ng/ml

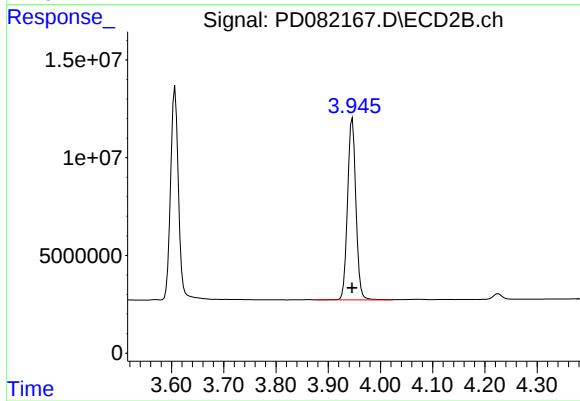

#4 Heptachlor


R.T.: 3.946 min
Delta R.T.: 0.000 min
Response: 103850336
Conc: 39.86 ng/ml

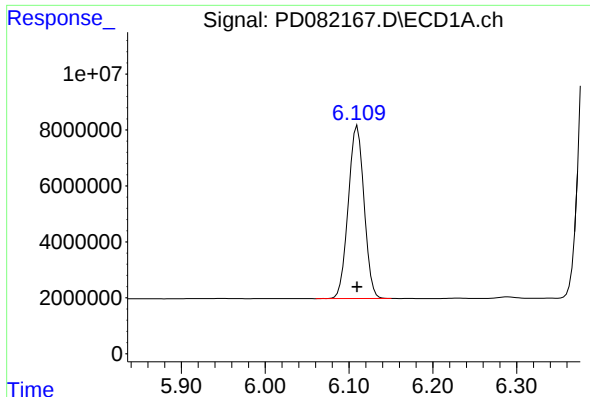

#9 Endosulfan I


R.T.: 6.110 min
Delta R.T.: 0.000 min
Response: 81099360
Conc: 39.80 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4061

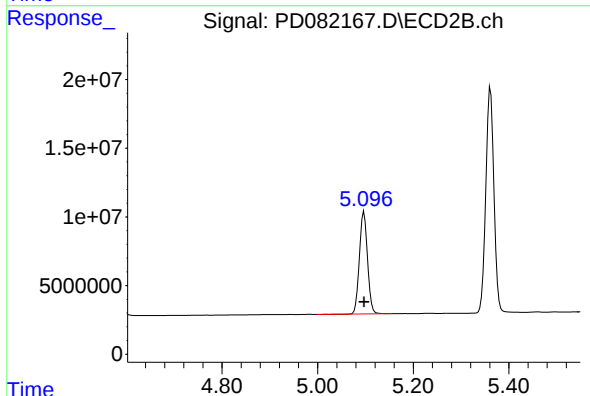


#9 Endosulfan I

R.T.: 5.097 min
Delta R.T.: 0.000 min
Response: 87086457
Conc: 39.15 ng/ml

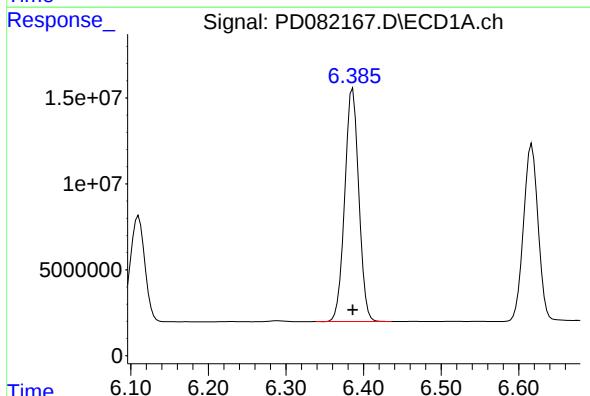


#13 Dieldrin

R.T.: 6.386 min
Delta R.T.: 0.000 min
Response: 170771695
Conc: 82.25 ng/ml

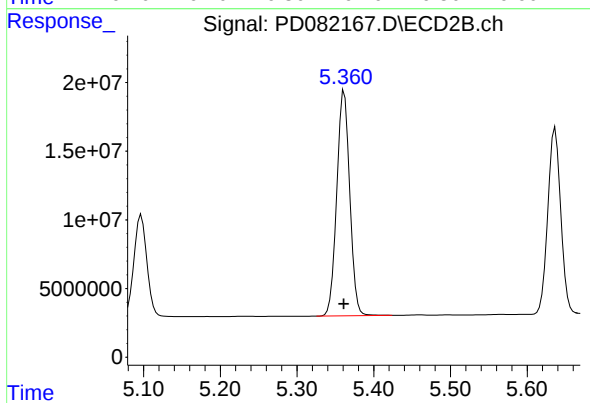

#13 Dieldrin


R.T.: 5.362 min
Delta R.T.: 0.000 min
Response: 192982757
Conc: 79.92 ng/ml

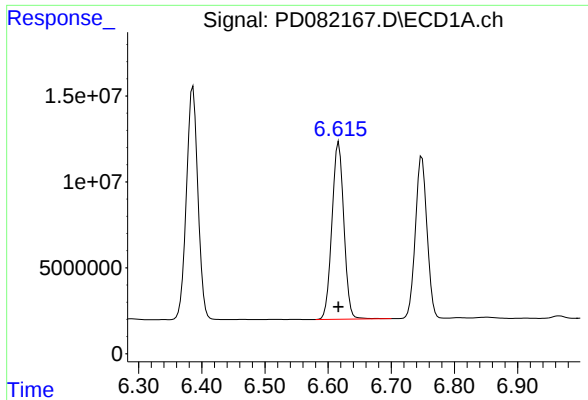

#14 Endrin


R.T.: 6.617 min
Delta R.T.: 0.000 min
Response: 135151378
Conc: 82.81 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4061

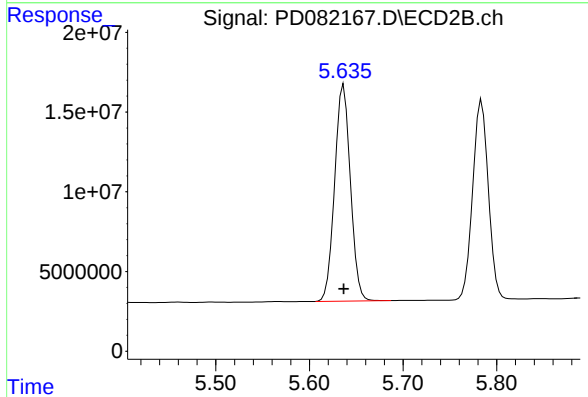


#14 Endrin

R.T.: 5.637 min
Delta R.T.: 0.000 min
Response: 158913400
Conc: 80.23 ng/ml

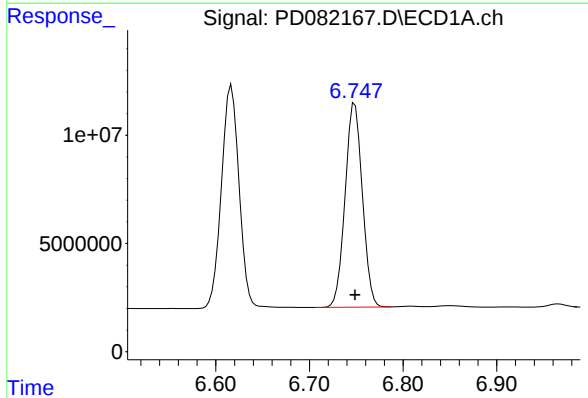


#16 4,4'-DDD

R.T.: 6.748 min
Delta R.T.: 0.000 min
Response: 120749124
Conc: 82.86 ng/ml

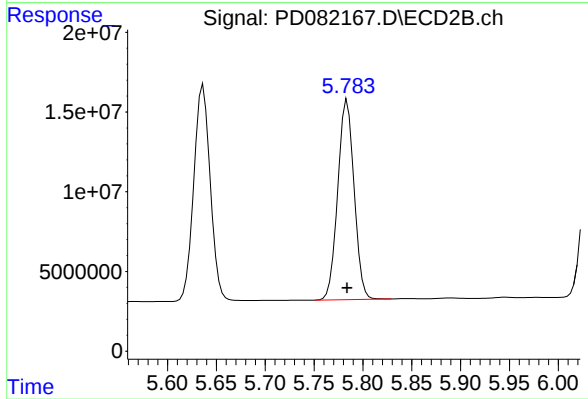

#16 4,4'-DDD


R.T.: 5.784 min
Delta R.T.: 0.000 min
Response: 145894026
Conc: 80.21 ng/ml

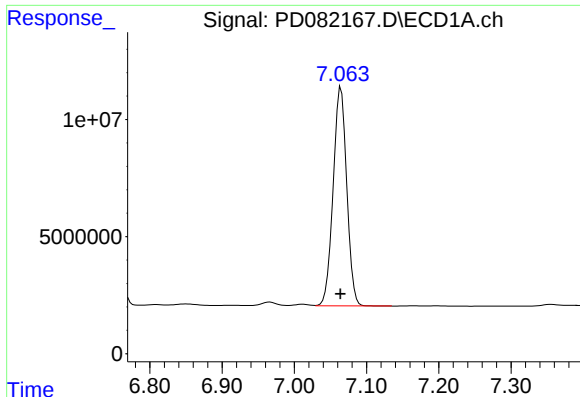

#17 4,4'-DDT


R.T.: 7.065 min
Delta R.T.: 0.000 min
Response: 122286243
Conc: 83.11 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4061

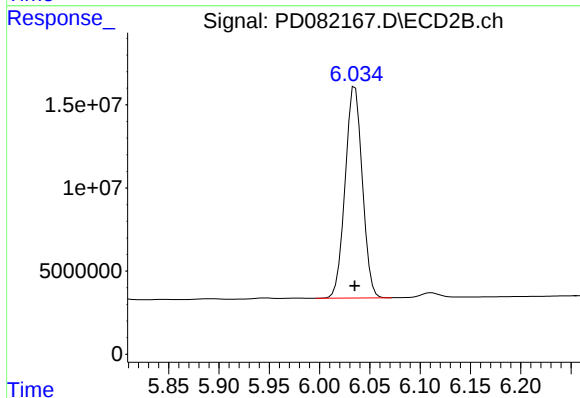


#17 4,4'-DDT

R.T.: 6.035 min
Delta R.T.: 0.000 min
Response: 150619570
Conc: 81.74 ng/ml

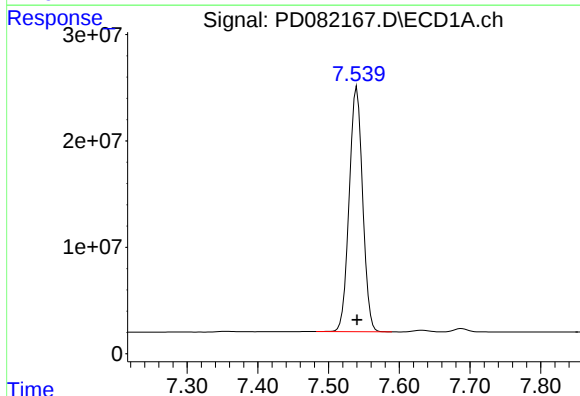


#20 Methoxychlor

R.T.: 7.540 min
Delta R.T.: 0.000 min
Response: 304476510
Conc: 399.62 ng/ml

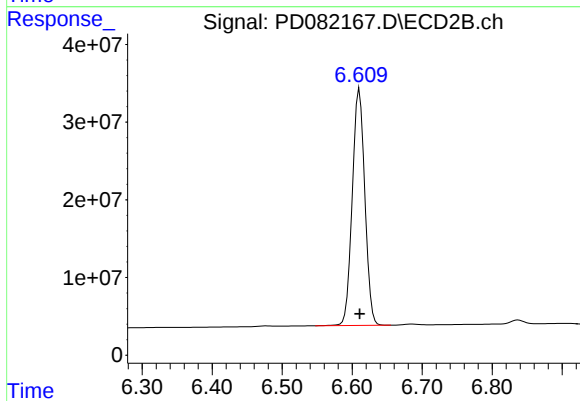

#20 Methoxychlor


R.T.: 6.610 min
Delta R.T.: 0.000 min
Response: 379831111
Conc: 383.27 ng/ml

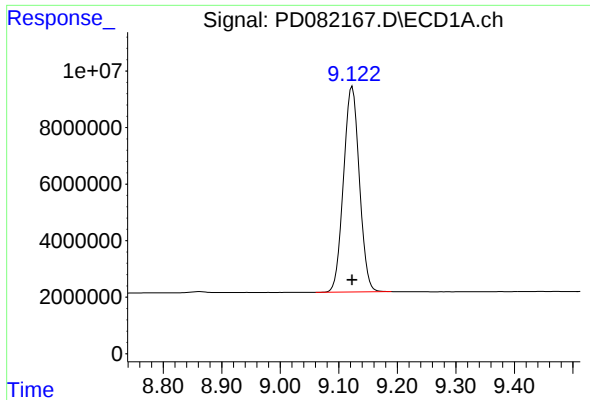

#27 Decachlorobiphenyl

R.T.: 9.123 min
Delta R.T.: 0.000 min
Response: 136774660
Conc: 76.87 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4061

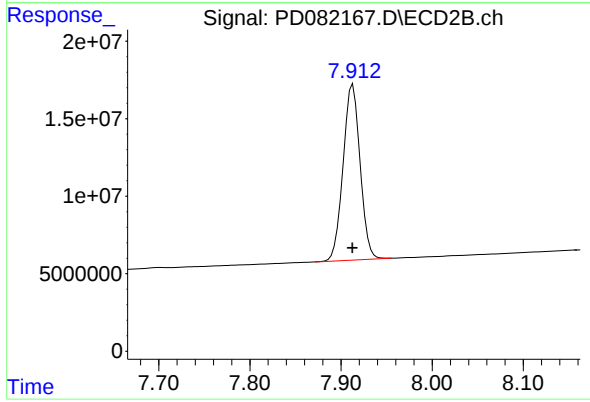

#27 Decachlorobiphenyl

R.T.: 7.913 min
Delta R.T.: 0.000 min
Response: 146801426
Conc: 78.84 ng/ml