

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031824\
 Data File : PD082169.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2024 22:43
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA5063

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 05:05:35 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031824CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 19 05:02:34 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.567	2.777	117.1E6	176.2E6	80.972	80.800
27)	SA Decachlor...	9.123	7.912	270.9E6	301.7E6	152.255	162.049
Target Compounds							
2)	A alpha-BHC	4.024	3.277	219.7E6	270.3E6	92.158	88.230
3)	MA gamma-BHC...	4.358	3.606	204.9E6	244.3E6	88.951	86.125
4)	MA Heptachlor	4.951	3.946	199.5E6	218.9E6	85.122	84.041
9)	A Endosulfan I	6.109	5.097	165.3E6	183.6E6	81.106	82.547
13)	MA Dieldrin	6.385	5.361	358.8E6	407.9E6	172.799	168.919
14)	MA Endrin	6.616	5.636	280.9E6	330.9E6	172.097	167.037
16)	A 4,4'-DDD	6.748	5.784	254.7E6	308.0E6	174.764	169.346
17)	MA 4,4'-DDT	7.064	6.035	258.2E6	319.9E6	175.504	173.590
20)	A Methoxychlor	7.539	6.610	616.4E6	738.8E6	809.013	745.527

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031824\
Data File : PD082169.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2024 22:43
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 05:05:35 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031824CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 19 05:02:34 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

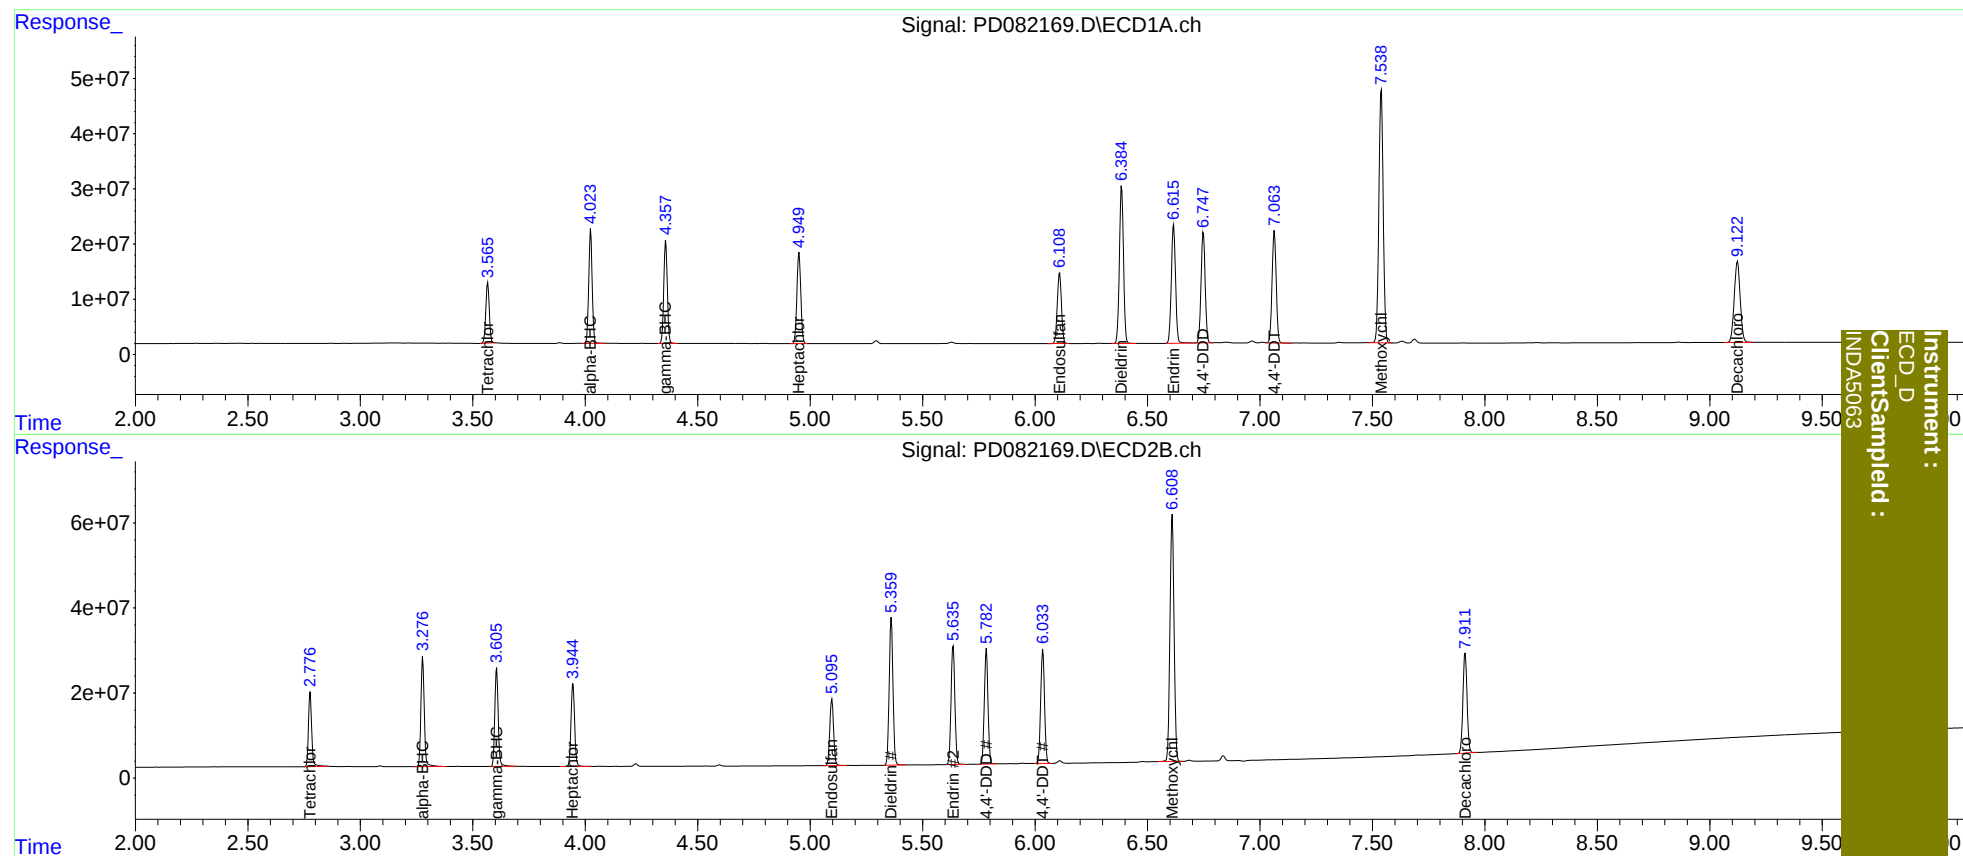


Instrument :
ECD_D
ClientSampled :
INDA5063

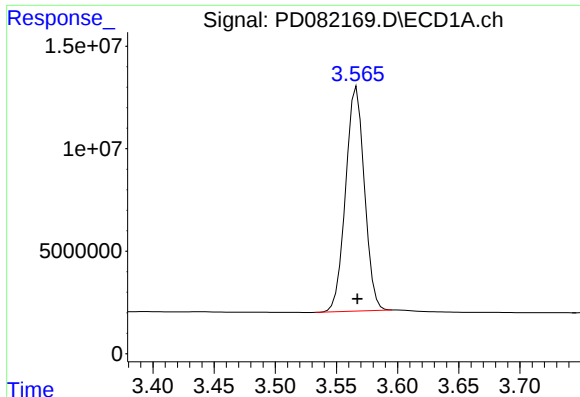

#1 Tetrachloro-m-xylene


R.T.: 3.567 min
Delta R.T.: 0.000 min
Response: 117111758
Conc: 80.97 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5063

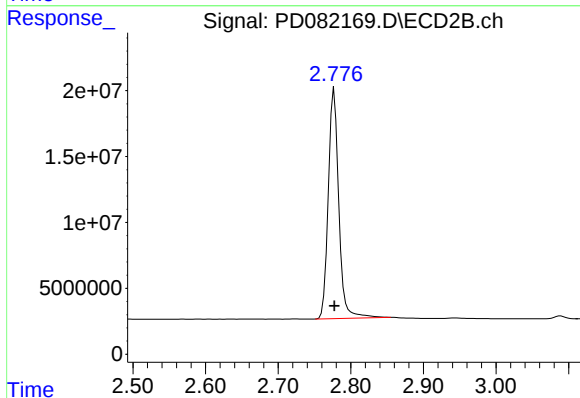


#1 Tetrachloro-m-xylene

R.T.: 2.777 min
Delta R.T.: 0.000 min
Response: 176195322
Conc: 80.80 ng/ml

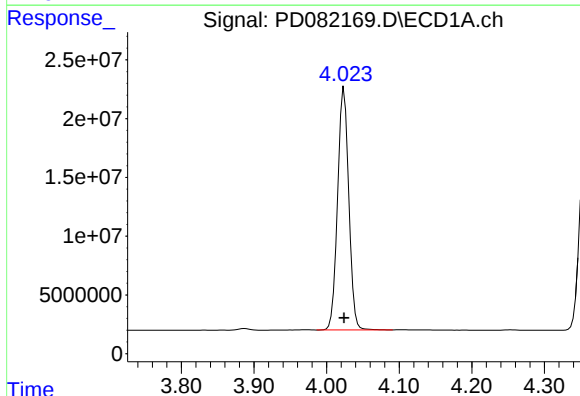


#2 alpha-BHC

R.T.: 4.024 min
Delta R.T.: 0.000 min
Response: 219740252
Conc: 92.16 ng/ml

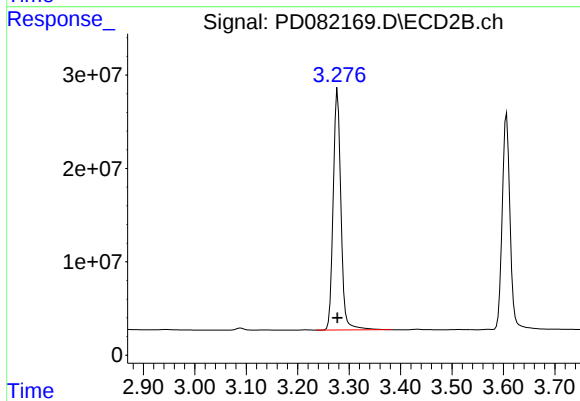

#2 alpha-BHC


R.T.: 3.277 min
Delta R.T.: 0.000 min
Response: 270334189
Conc: 88.23 ng/ml

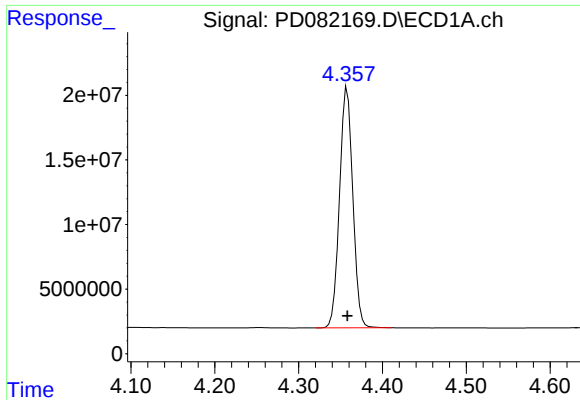

#3 gamma-BHC (Lindane)


R.T.: 4.358 min
Delta R.T.: 0.000 min
Response: 204901574
Conc: 88.95 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5063

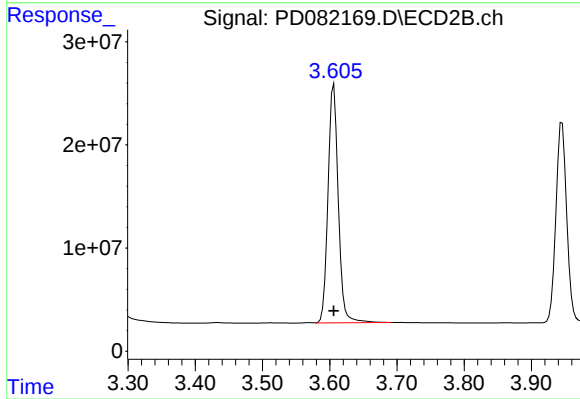


#3 gamma-BHC (Lindane)

R.T.: 3.606 min
Delta R.T.: 0.000 min
Response: 244342942
Conc: 86.12 ng/ml

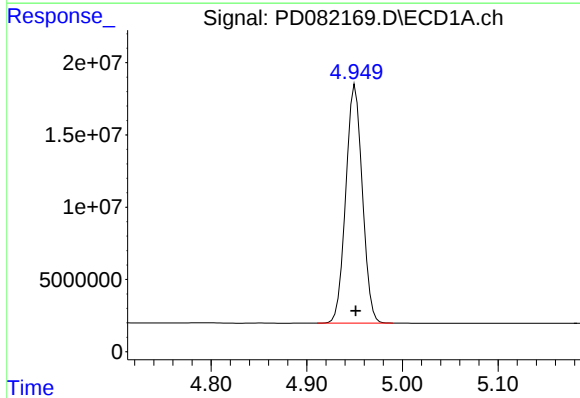


#4 Heptachlor

R.T.: 4.951 min
Delta R.T.: 0.000 min
Response: 199472266
Conc: 85.12 ng/ml

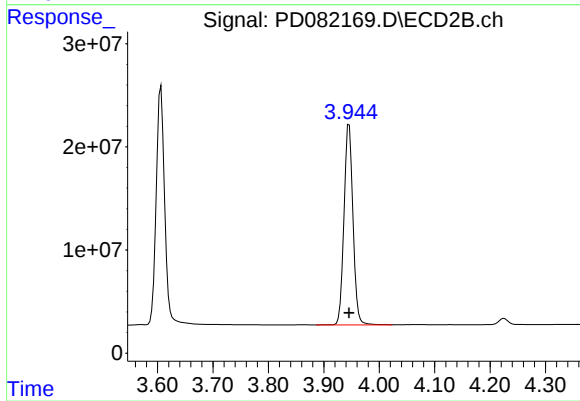

#4 Heptachlor


R.T.: 3.946 min
Delta R.T.: 0.000 min
Response: 218942492
Conc: 84.04 ng/ml

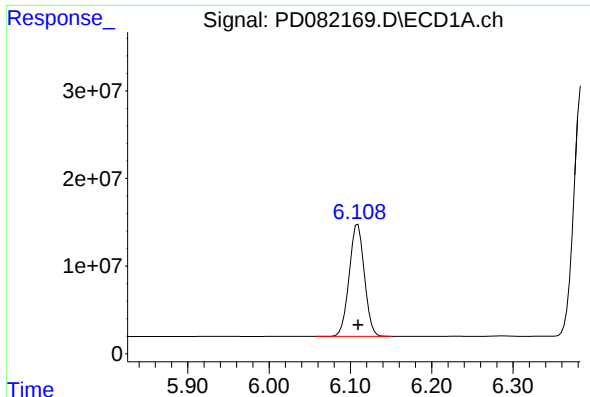

#9 Endosulfan I


R.T.: 6.109 min
Delta R.T.: 0.000 min
Response: 165273706
Conc: 81.11 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5063

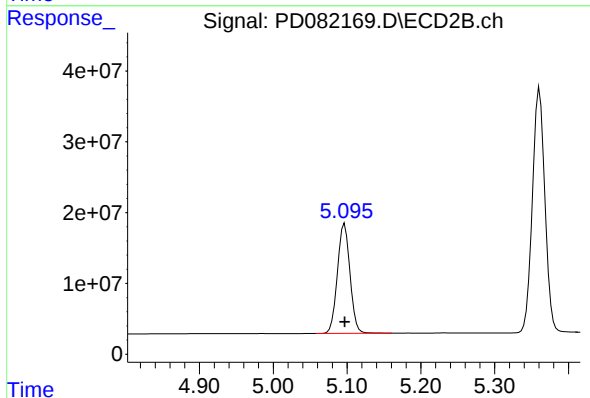


#9 Endosulfan I

R.T.: 5.097 min
Delta R.T.: 0.000 min
Response: 183610844
Conc: 82.55 ng/ml

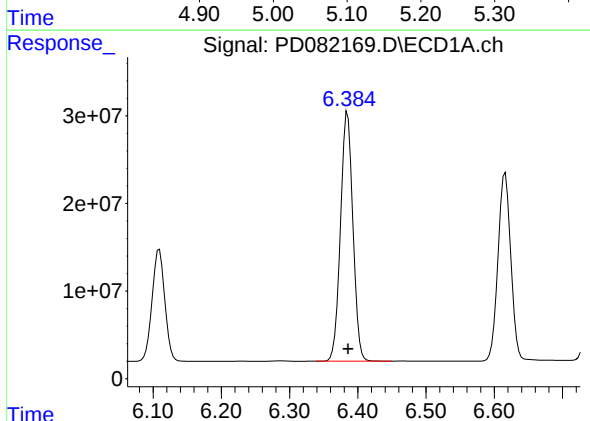


#13 Dieldrin

R.T.: 6.385 min
Delta R.T.: 0.000 min
Response: 358773297
Conc: 172.80 ng/ml

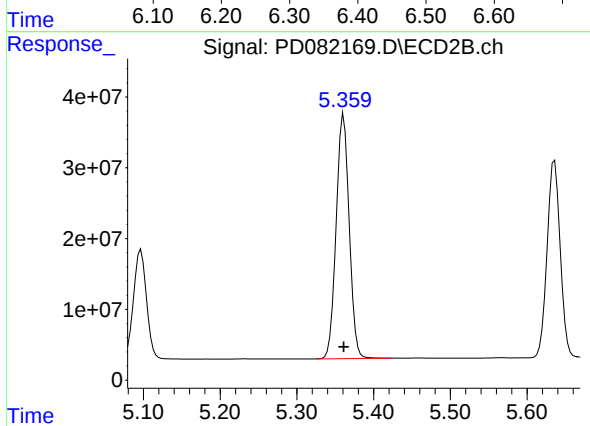

#13 Dieldrin


R.T.: 5.361 min
Delta R.T.: 0.000 min
Response: 407884949
Conc: 168.92 ng/ml

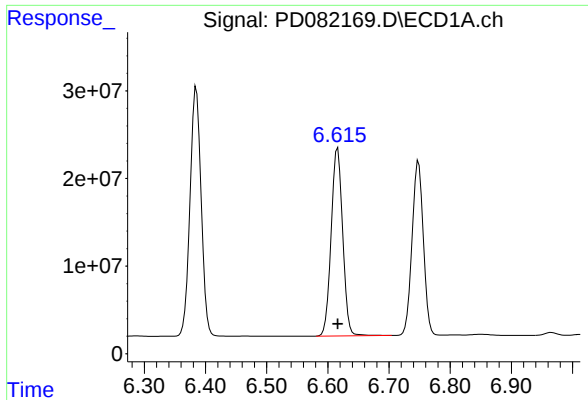

#14 Endrin


R.T.: 6.616 min
Delta R.T.: 0.000 min
Response: 280860286
Conc: 172.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5063

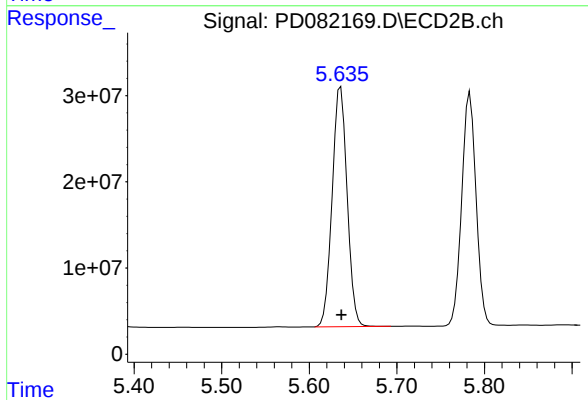


#14 Endrin

R.T.: 5.636 min
Delta R.T.: 0.000 min
Response: 330852750
Conc: 167.04 ng/ml

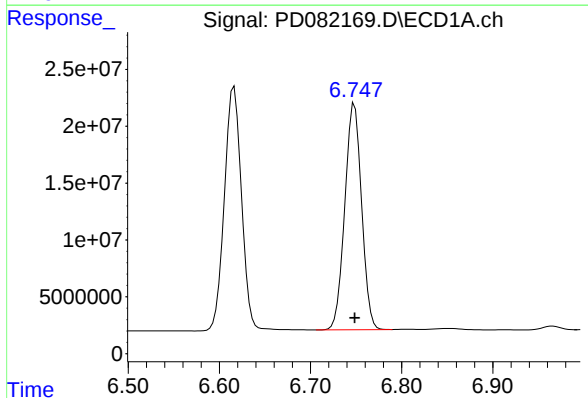


#16 4,4'-DDD

R.T.: 6.748 min
Delta R.T.: 0.000 min
Response: 254670688
Conc: 174.76 ng/ml

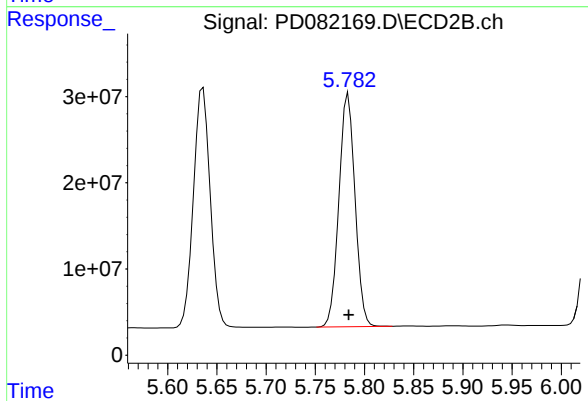

#16 4,4'-DDD


R.T.: 5.784 min
Delta R.T.: 0.000 min
Response: 308036523
Conc: 169.35 ng/ml

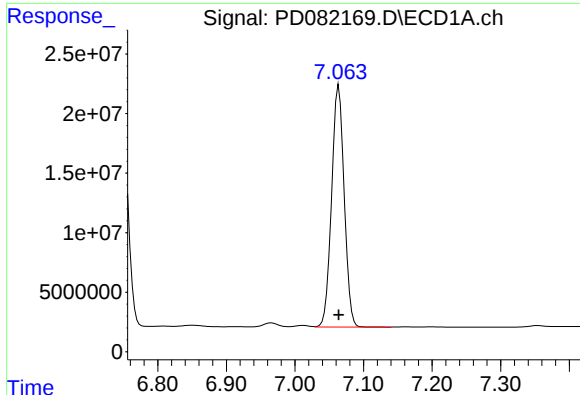

#17 4,4'-DDT


R.T.: 7.064 min
Delta R.T.: 0.000 min
Response: 258246733
Conc: 175.50 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5063

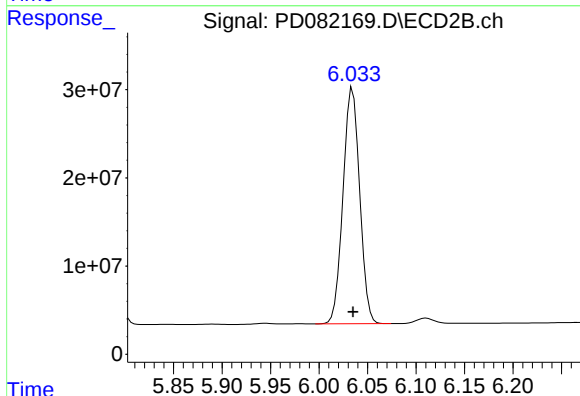


#17 4,4'-DDT

R.T.: 6.035 min
Delta R.T.: 0.000 min
Response: 319878122
Conc: 173.59 ng/ml

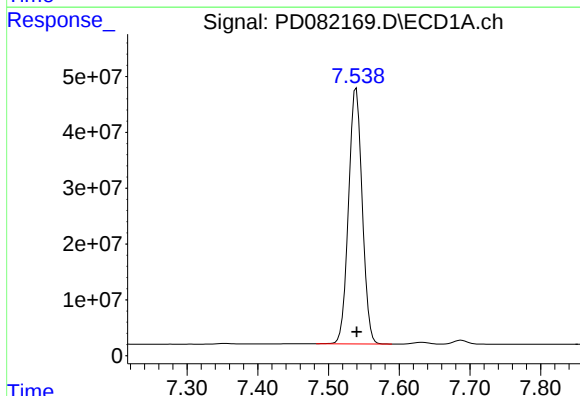


#20 Methoxychlor

R.T.: 7.539 min
Delta R.T.: 0.000 min
Response: 616405061
Conc: 809.01 ng/ml

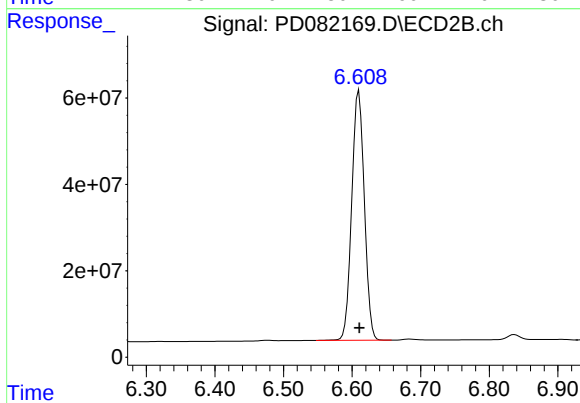

#20 Methoxychlor


R.T.: 6.610 min
Delta R.T.: 0.000 min
Response: 738833714
Conc: 745.53 ng/ml

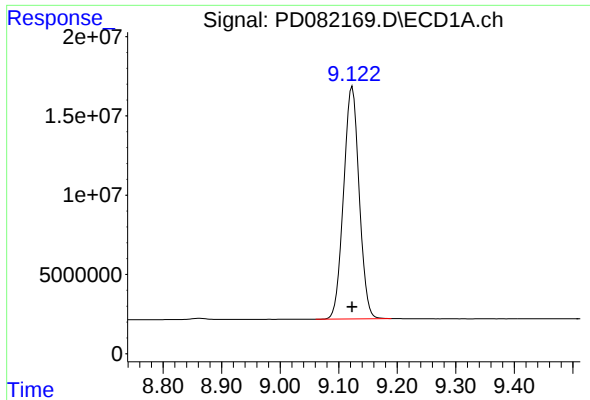

#27 Decachlorobiphenyl

R.T.: 9.123 min
Delta R.T.: 0.000 min
Response: 270911511
Conc: 152.26 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5063

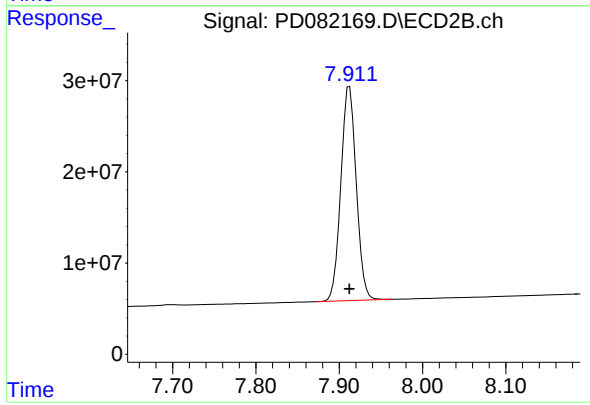

#27 Decachlorobiphenyl

R.T.: 7.912 min
Delta R.T.: 0.000 min
Response: 301724887
Conc: 162.05 ng/ml